

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011110.D
 Acq On : 26 Jul 2022 15:03
 Operator : CG/JU
 Sample : N3809-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBE69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	10	rBV	67883	89448	0.75%	0.072%
2	3.164	10	13	21	rVB	154417	192871	1.62%	0.156%
3	3.440	57	60	64	rBV	39849	48479	0.41%	0.039%
4	3.575	80	83	110	rVB	643368	936892	7.85%	0.758%
5	3.793	115	120	125	rVB	68642	97196	0.81%	0.079%
6	3.881	131	135	141	rBV	131839	165624	1.39%	0.134%
7	4.252	195	198	204	rVB5	10922	14174	0.12%	0.011%
8	4.399	219	223	227	rBV	59026	72529	0.61%	0.059%
9	4.793	286	290	293	rBV4	12462	20204	0.17%	0.016%
10	5.264	364	370	374	rBV3	8050	14647	0.12%	0.012%
11	5.387	387	391	395	rBV	18477	24471	0.21%	0.020%
12	6.840	630	638	654	rVB	622228	979042	8.21%	0.792%
13	7.005	660	666	676	rBV	2138433	3326156	27.88%	2.690%
14	7.105	679	683	691	rVB	8796	17766	0.15%	0.014%
15	7.193	691	698	710	rBV	2050061	3226851	27.05%	2.610%
16	7.287	710	714	718	rVB3	11272	16405	0.14%	0.013%
17	7.663	770	778	786	rBV	1836077	2768450	23.21%	2.239%
18	7.740	786	791	797	rVB3	17869	32800	0.27%	0.027%
19	8.381	892	900	916	rBV	1725742	2824888	23.68%	2.285%
20	8.828	968	976	986	rBV	2574213	4207649	35.27%	3.403%
21	9.240	1042	1046	1050	rVB2	9462	13337	0.11%	0.011%
22	9.546	1090	1098	1115	rBV	2050320	3324357	27.87%	2.689%
23	10.081	1181	1189	1208	rBV	2852796	4690925	39.32%	3.794%
24	10.457	1245	1253	1262	rBV	2607712	4336116	36.35%	3.507%
25	10.605	1269	1278	1294	rBV	2634815	4459124	37.38%	3.607%
26	11.116	1360	1365	1372	rVB10	6826	13623	0.11%	0.011%
27	11.740	1466	1471	1475	rBV4	9055	16307	0.14%	0.013%
28	12.057	1519	1525	1533	rBV2	49805	87099	0.73%	0.070%
29	12.681	1622	1631	1636	rBV8	9014	18857	0.16%	0.015%
30	12.934	1670	1674	1680	rBV5	11705	17006	0.14%	0.014%
31	13.046	1688	1693	1699	rBV9	6126	13745	0.12%	0.011%
32	13.151	1706	1711	1718	rBV4	11608	19486	0.16%	0.016%
33	13.293	1729	1735	1739	rBV3	10178	18308	0.15%	0.015%
34	13.751	1805	1813	1823	rBV	6196278	8411331	70.51%	6.804%
35	14.016	1848	1858	1870	rBV	6584247	9557164	80.12%	7.731%
36	14.234	1890	1895	1900	rVB	30095	41398	0.35%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011110.D
 Acq On : 26 Jul 2022 15:03
 Operator : CG/JU
 Sample : N3809-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBE69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	14.328	1904	1911	1920	rBV	3923147	5687684	47.68%	4.601%
38	14.545	1937	1948	1966	rBV	351122	699947	5.87%	0.566%
39	14.763	1982	1985	1991	rVB7	18654	26397	0.22%	0.021%
40	14.863	1997	2002	2009	rVB7	9565	20988	0.18%	0.017%
41	14.975	2017	2021	2025	rVB7	7441	13607	0.11%	0.011%
42	15.140	2046	2049	2052	rBV	19722	29197	0.24%	0.024%
43	15.193	2056	2058	2063	rVB	34803	41048	0.34%	0.033%
44	15.328	2074	2081	2096	rBV	8474302	11905020	99.80%	9.630%
45	15.451	2096	2102	2117	rBV	2720480	3707007	31.08%	2.998%
46	15.569	2117	2122	2128	rVV2	92340	138669	1.16%	0.112%
47	15.663	2133	2138	2142	rVV4	11702	22678	0.19%	0.018%
48	15.710	2143	2146	2149	rVV5	10283	13868	0.12%	0.011%
49	16.022	2195	2199	2202	rBV6	13770	26092	0.22%	0.021%
50	16.063	2203	2206	2212	rVV2	36328	64501	0.54%	0.052%
51	16.122	2212	2216	2223	rVB3	34791	55679	0.47%	0.045%
52	16.245	2230	2237	2244	rBV3	9060	24598	0.21%	0.020%
53	16.481	2273	2277	2280	rBV5	10858	15858	0.13%	0.013%
54	16.639	2302	2304	2310	rVB6	11430	14498	0.12%	0.012%
55	16.769	2320	2326	2331	rBV8	18860	32465	0.27%	0.026%
56	16.869	2339	2343	2347	rBV2	36597	54402	0.46%	0.044%
57	17.092	2375	2381	2391	rBV	4213901	6048158	50.70%	4.892%
58	17.192	2392	2398	2412	rVV2	8359883	11928911	100.00%	9.649%
59	17.404	2430	2434	2439	rVB3	12878	20655	0.17%	0.017%
60	17.610	2466	2469	2473	rBV3	21582	27646	0.23%	0.022%
61	17.786	2494	2499	2503	rBV	182968	212690	1.78%	0.172%
62	17.898	2515	2518	2522	rVB5	22474	25086	0.21%	0.020%
63	18.004	2532	2536	2541	rBV2	68528	99030	0.83%	0.080%
64	18.075	2545	2548	2552	rVB	16408	24639	0.21%	0.020%
65	18.292	2581	2585	2589	rBV2	25322	35932	0.30%	0.029%
66	18.904	2687	2689	2692	rBV3	15218	18300	0.15%	0.015%
67	19.022	2705	2709	2714	rBV3	103158	134639	1.13%	0.109%
68	19.092	2717	2721	2726	rVV	90704	117549	0.99%	0.095%
69	19.398	2770	2773	2776	rBV3	29290	28163	0.24%	0.023%
70	19.451	2776	2782	2789	rBV	9103290	11660592	97.75%	9.432%
71	20.945	3032	3036	3044	rBV3	277157	509040	4.27%	0.412%
72	21.210	3077	3081	3087	rBV	3365972	4174925	35.00%	3.377%
73	23.404	3447	3454	3461	rBV2	4354633	8064032	67.60%	6.523%
74	23.551	3473	3479	3489	rVB2	1891184	3790005	31.77%	3.066%

Sum of corrected areas: 123628920




Instrument :
BNA_P
ClientSampleId :
YBE69

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011110.D
Acq On : 26 Jul 2022 15:03
Operator : CG/JU
Sample : N3809-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBE69

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

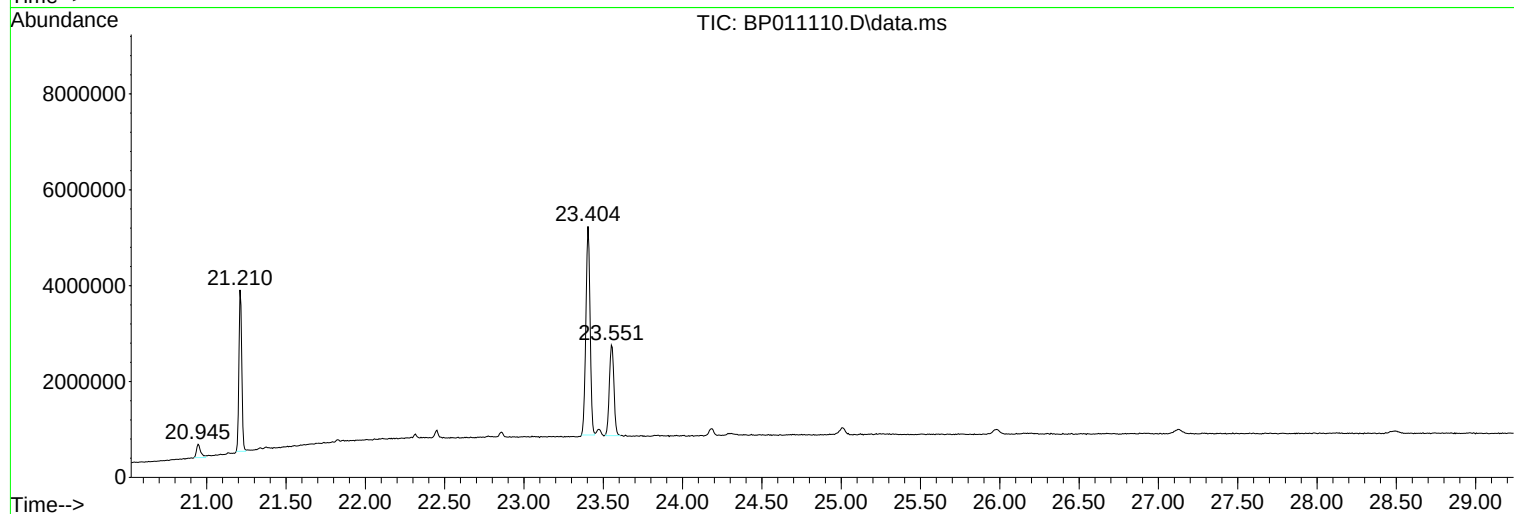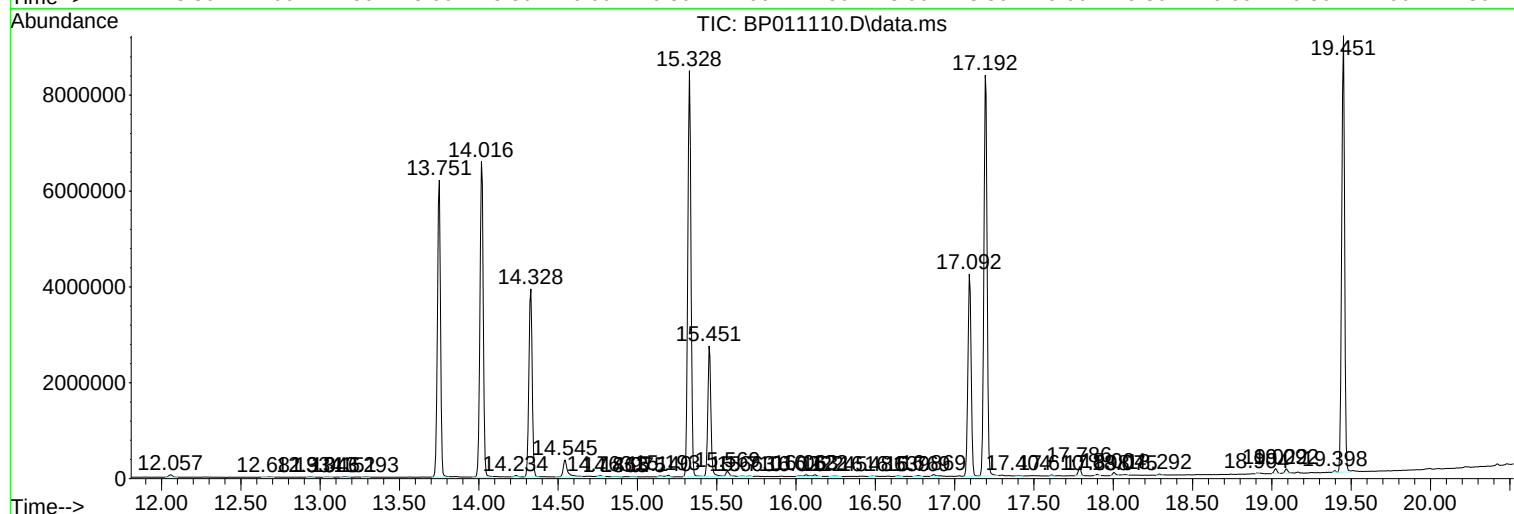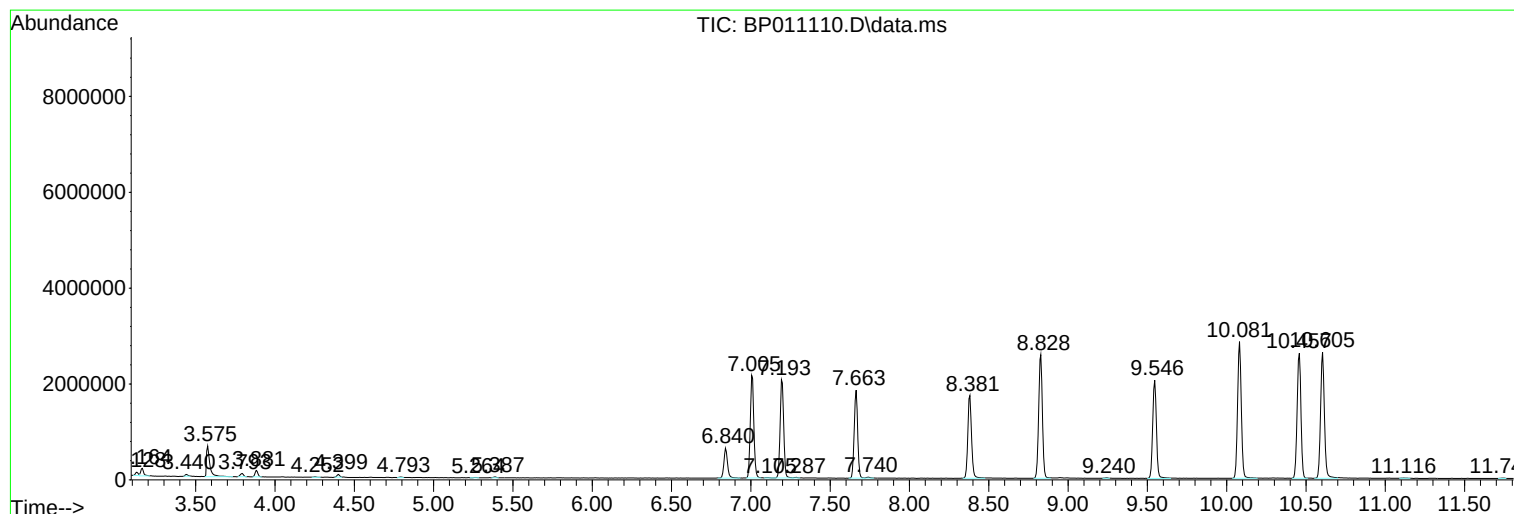

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011110.D
Acq On : 26 Jul 2022 15:03
Operator : CG/JU
Sample : N3809-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBE69










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Tetracosanol-1 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.945	2.44 ng/ul	509040	Chrysene-d12	21.210

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Tetracosanol-1	354	C24H50O	000506-51-4	91
2			Behenic alcohol	326	C22H46O	000661-19-8	91
3			Cyclooctacosane	392	C28H56	000297-24-5	91
4			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	91
5			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	91

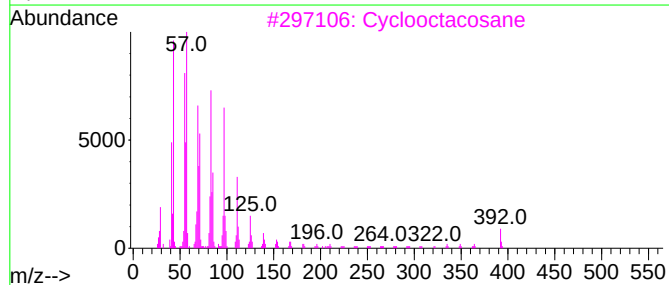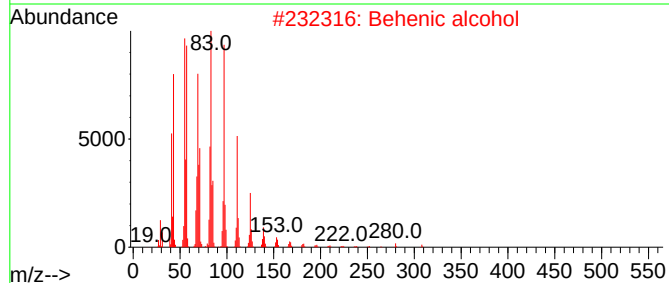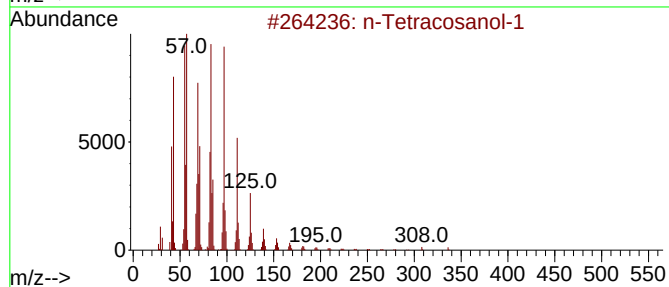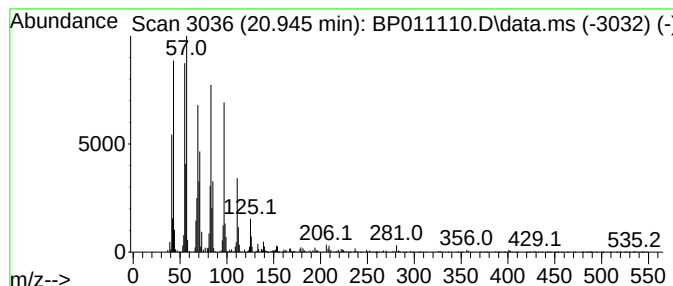

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011110.D
Acq On : 26 Jul 2022 15:03
Operator : CG/JU
Sample : N3809-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBE69

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Tetracosanol-1	20.945	2.4	ng/ul	509040	5	21.210	4174930	20.0