

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011111.D
 Acq On : 26 Jul 2022 15:38
 Operator : CG/JU
 Sample : N3801-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	10	rBV	231687	273985	3.19%	0.289%
2	3.164	10	13	20	rVB	127348	157272	1.83%	0.166%
3	3.575	80	83	98	rBV	633014	873640	10.17%	0.920%
4	3.793	115	120	126	rVB	60538	91851	1.07%	0.097%
5	3.881	131	135	140	rBV	35045	42839	0.50%	0.045%
6	4.399	220	223	226	rVB5	11254	13002	0.15%	0.014%
7	4.793	286	290	294	rVB4	9348	12820	0.15%	0.014%
8	5.387	387	391	396	rVB	14852	23315	0.27%	0.025%
9	6.840	632	638	650	rVB	405630	648368	7.55%	0.683%
10	7.005	660	666	680	rBV	1818312	2803651	32.65%	2.952%
11	7.193	691	698	710	rBV	1651064	2575846	29.99%	2.713%
12	7.287	711	714	718	rVB3	11301	14827	0.17%	0.016%
13	7.663	770	778	787	rBV	1660139	2555479	29.76%	2.691%
14	8.375	892	899	914	rBV	1210946	2058159	23.97%	2.167%
15	8.822	967	975	990	rBV	2091097	3460810	40.30%	3.644%
16	9.240	1041	1046	1051	rBV	24063	35033	0.41%	0.037%
17	9.546	1090	1098	1116	rBV	1605343	2640600	30.75%	2.781%
18	10.081	1177	1189	1206	rBV	2297650	3757018	43.75%	3.956%
19	10.457	1245	1253	1266	rVB	2379301	3887001	45.26%	4.093%
20	10.604	1268	1278	1296	rBV	2143581	3713523	43.24%	3.911%
21	11.128	1363	1367	1374	rVB8	5735	12900	0.15%	0.014%
22	11.740	1463	1471	1477	rVB2	31057	50633	0.59%	0.053%
23	12.057	1519	1525	1533	rVB	38345	67118	0.78%	0.071%
24	12.675	1625	1630	1635	rBV6	11059	22550	0.26%	0.024%
25	12.934	1668	1674	1681	rBV4	15767	27469	0.32%	0.029%
26	13.045	1688	1693	1699	rVB8	5889	10115	0.12%	0.011%
27	13.228	1720	1724	1729	rBV3	10170	15622	0.18%	0.016%
28	13.292	1731	1735	1739	rVB5	5951	9178	0.11%	0.010%
29	13.751	1805	1813	1824	rBV	4355320	6148433	71.59%	6.475%
30	13.845	1825	1829	1834	rVB7	7495	15192	0.18%	0.016%
31	14.016	1848	1858	1875	rBV	5031449	7188877	83.71%	7.570%
32	14.328	1904	1911	1921	rBV	3273631	4635637	53.98%	4.882%
33	14.545	1941	1948	1962	rBV2	125277	289243	3.37%	0.305%
34	14.763	1983	1985	1991	rVB7	6951	10738	0.13%	0.011%
35	15.145	2045	2050	2053	rBV	48813	69485	0.81%	0.073%
36	15.328	2074	2081	2091	rBV	6239513	8587820	100.00%	9.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011111.D
 Acq On : 26 Jul 2022 15:38
 Operator : CG/JU
 Sample : N3801-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.451	2096	2102	2117	rVV	1713967	2308541	26.88%	2.431%
38	15.569	2117	2122	2128	rVB	71195	108034	1.26%	0.114%
39	15.904	2173	2179	2183	rBV9	11820	21314	0.25%	0.022%
40	15.945	2183	2186	2193	rVB5	27505	39015	0.45%	0.041%
41	16.045	2200	2203	2209	rVV2	17596	33900	0.39%	0.036%
42	16.110	2209	2214	2221	rVB6	30021	57769	0.67%	0.061%
43	16.569	2286	2292	2298	rBV4	47373	70614	0.82%	0.074%
44	16.769	2320	2326	2331	rVB10	10524	19792	0.23%	0.021%
45	16.875	2338	2344	2348	rBV6	17936	29436	0.34%	0.031%
46	17.092	2374	2381	2389	rBV	3290630	4459075	51.92%	4.696%
47	17.192	2392	2398	2421	rVB2	5693399	8003810	93.20%	8.429%
48	17.398	2430	2433	2437	rVB	17188	21402	0.25%	0.023%
49	18.075	2545	2548	2554	rBV	26771	27977	0.33%	0.029%
50	18.263	2576	2580	2583	rBV5	12147	20287	0.24%	0.021%
51	19.022	2705	2709	2713	rBV	66107	91116	1.06%	0.096%
52	19.092	2718	2721	2726	rVB	58596	77210	0.90%	0.081%
53	19.451	2776	2782	2789	rBV	5996713	7938329	92.44%	8.360%
54	21.210	3077	3081	3088	rBV	2776979	3590890	41.81%	3.781%
55	23.404	3447	3454	3462	rBV2	3886708	7378833	85.92%	7.770%
56	23.557	3473	3480	3489	rVB2	1973068	3862956	44.98%	4.068%




Sum of corrected areas: 94960349

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011111.D
Acq On : 26 Jul 2022 15:38
Operator : CG/JU
Sample : N3801-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

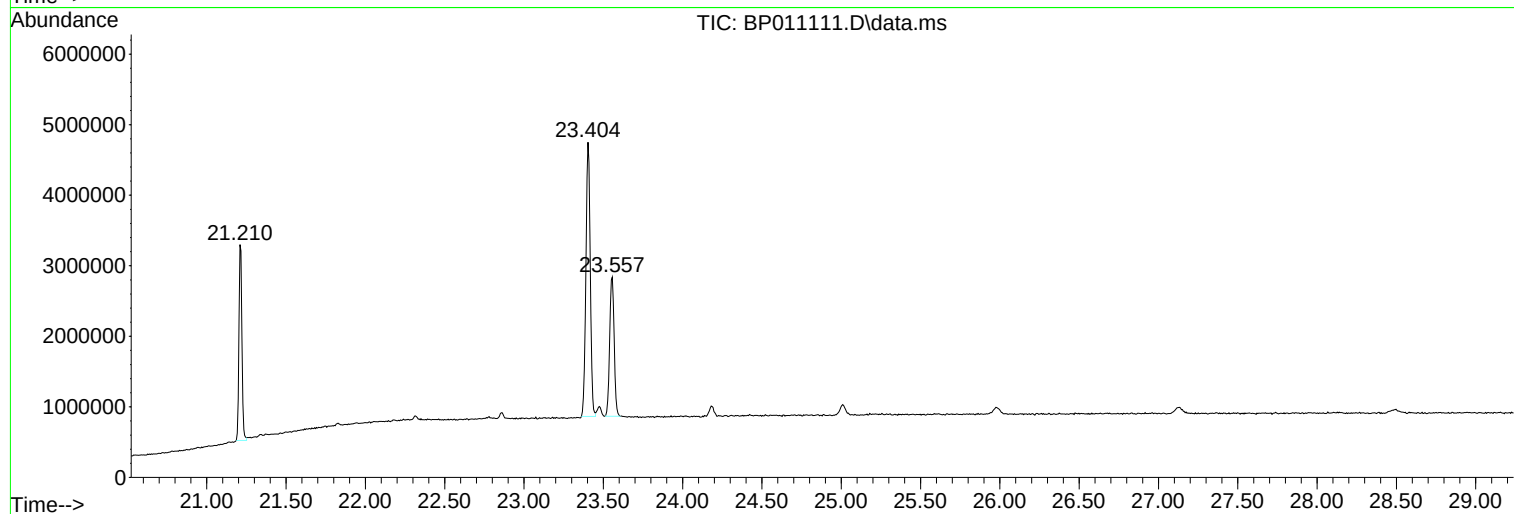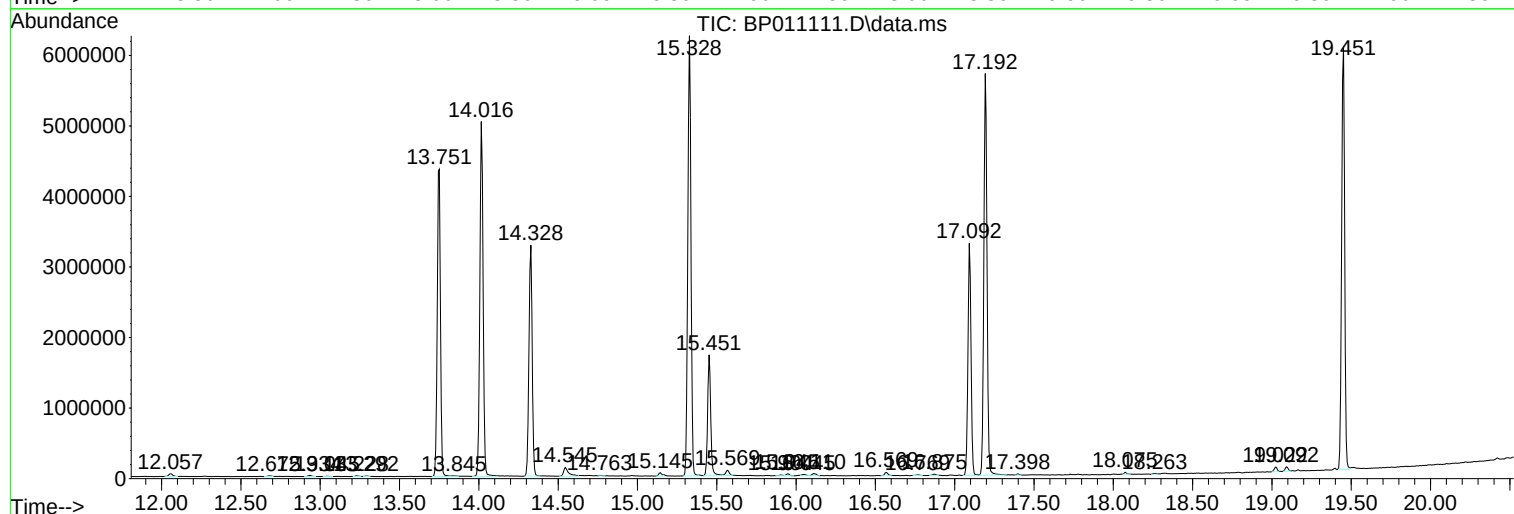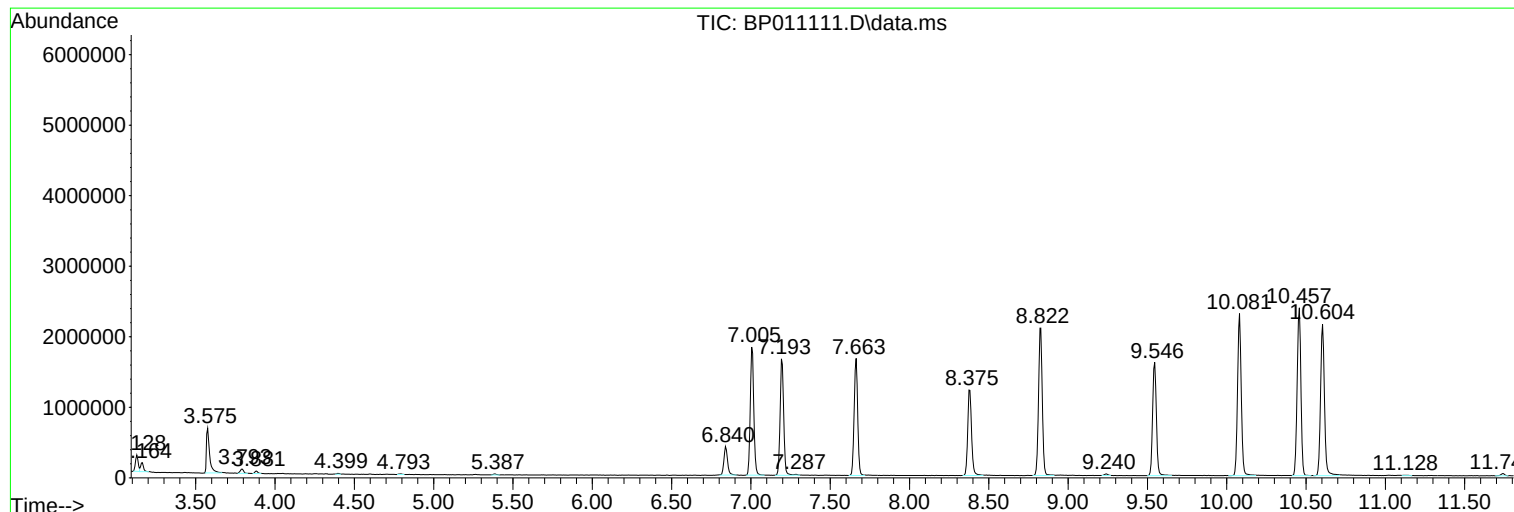

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011111.D
Acq On : 26 Jul 2022 15:38
Operator : CG/JU
Sample : N3801-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011111.D
Acq On : 26 Jul 2022 15:38
Operator : CG/JU
Sample : N3801-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc