




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021175.D
Acq On : 26 Jul 2024 18:03
Operator : MA/JU
Sample : P3329-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E85

Manual IntegrationsAPPROVED

Quant Time: Jul 26 22:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

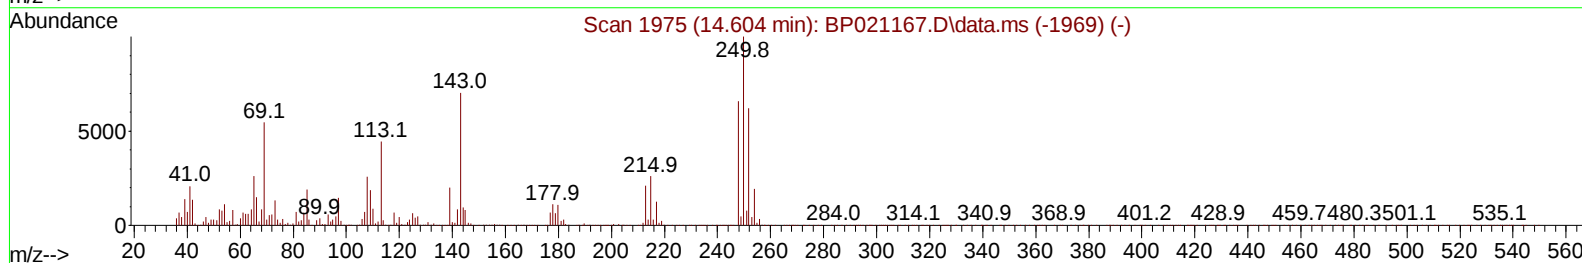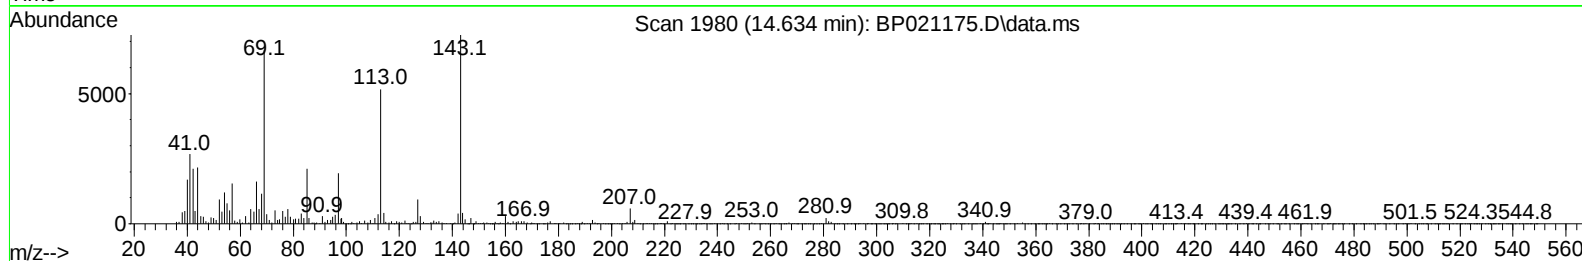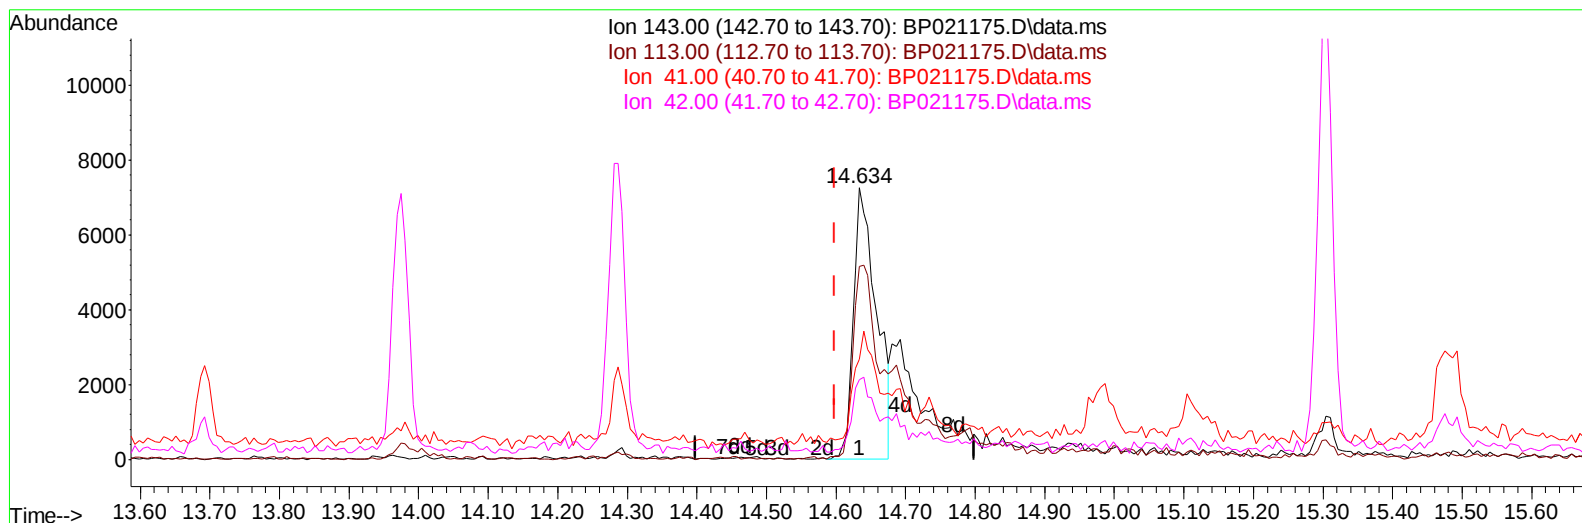

TIC: BP021175.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.634min (+ 0.035) 3.55 ng/u1

response 16600

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	71.20
41.00	37.90	36.89
42.00	27.10	29.31




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021175.D
Acq On : 26 Jul 2024 18:03
Operator : MA/JU
Sample : P3329-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E85

Manual IntegrationsAPPROVED

Quant Time: Jul 26 22:47:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

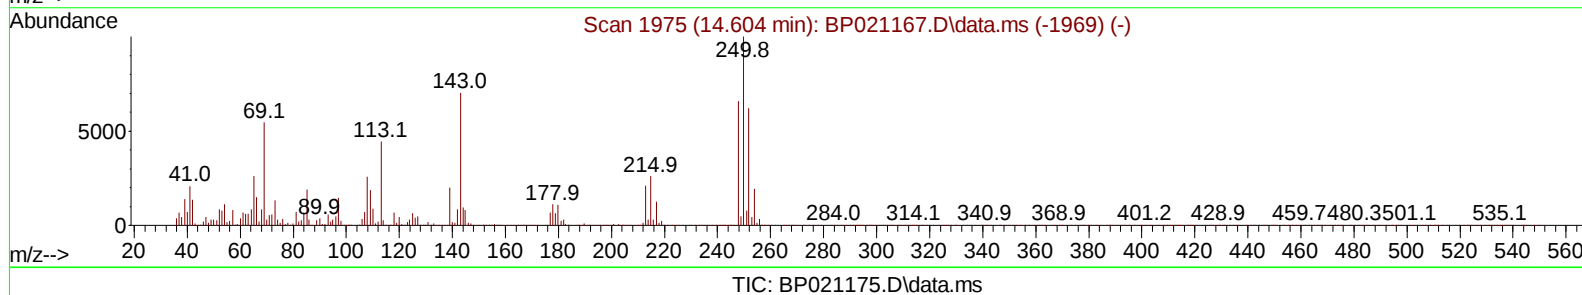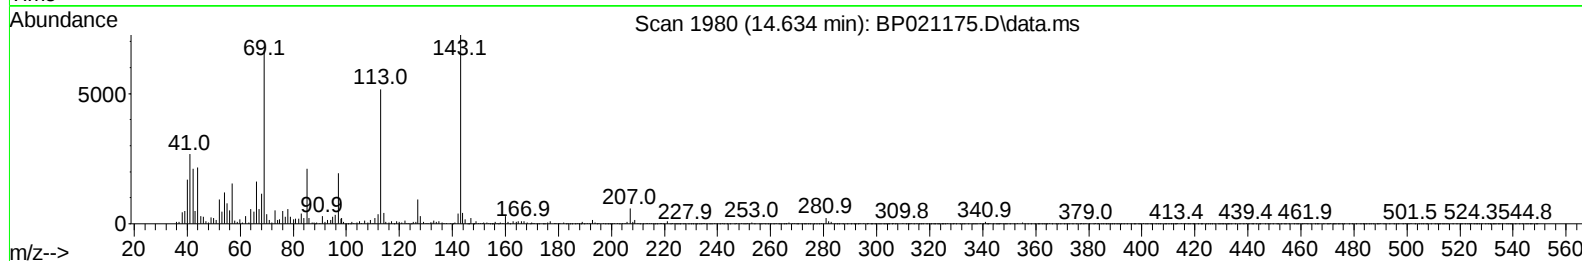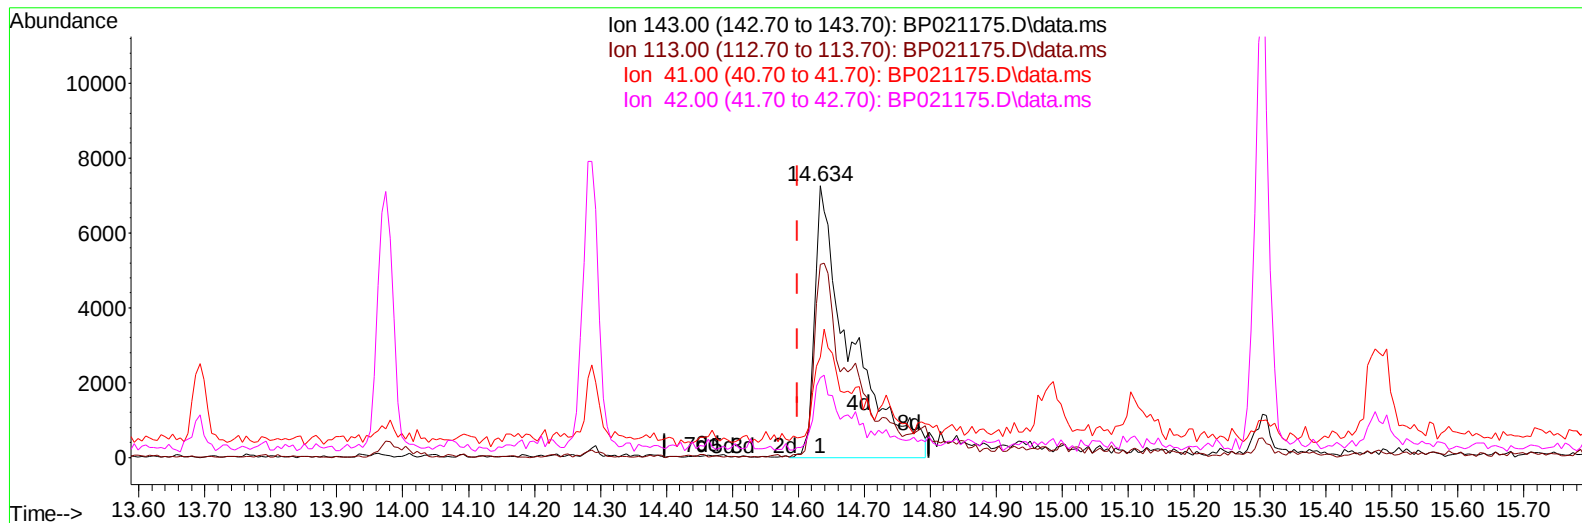

(54) 4-Nitrophenol-d4 (S)

14.634min (+ 0.035) 5.81 ng/ul m

response 27207

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	71.20
41.00	37.90	36.89
42.00	27.10	29.31

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021175.D
 Acq On : 26 Jul 2024 18:03
 Operator : MA/JU
 Sample : P3329-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E85

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/27/2024
 Supervised By :mohammad ahmed 07/29/2024

Quant Time: Jul 26 23:16:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	174933	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	681902	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.287	164	452483	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	981304	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	980110	20.000	ng/ul	0.00
88) Perylene-d12	24.880	264	1143122	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	8296	2.158	ng/uL	0.00
4) Pyridine-d5	3.605	84	84207	7.566	ng/ul	0.00
7) Phenol-d5	6.875	99	89042	6.243	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	220491	25.511	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132	266308	22.664	ng/ul	0.00
15) 4-Methylphenol-d8	8.381	113	171071	14.442	ng/ul	0.00
21) Nitrobenzene-d5	8.805	128	139118	26.266	ng/ul	0.00
24) 2-Nitrophenol-d4	9.516	143	154873	25.548	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.075	165	266161	24.281	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131	340676	23.460	ng/ul	0.00
46) Dimethylphthalate-d6	13.693	166	942233	28.645	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160	985575	26.684	ng/ul	0.00
54) 4-Nitrophenol-d4	14.634	143	27207m	5.813	ng/ul	0.04
60) Fluorene-d10	15.304	176	785541	29.110	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.487	200	72793	12.260	ng/ul	0.02
73) Anthracene-d10	17.210	188	1392046	31.939	ng/ul	0.00
81) Pyrene-d10	19.598	212	1720573	28.395	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.645	264	1878646	33.322	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021175.D
Acq On : 26 Jul 2024 18:03
Operator : MA/JU
Sample : P3329-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E85

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:16:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

