




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021176.D
Acq On : 26 Jul 2024 18:47
Operator : MA/JU
Sample : P3329-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E86

Manual IntegrationsAPPROVED

Quant Time: Jul 26 22:47:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

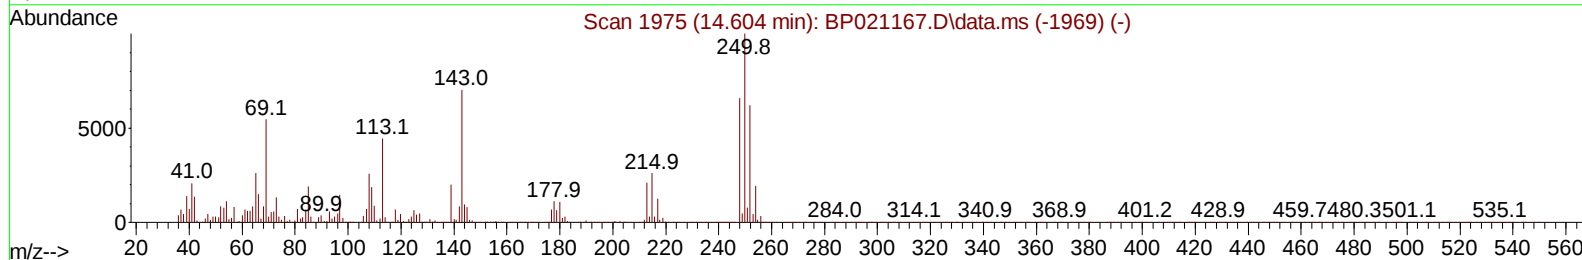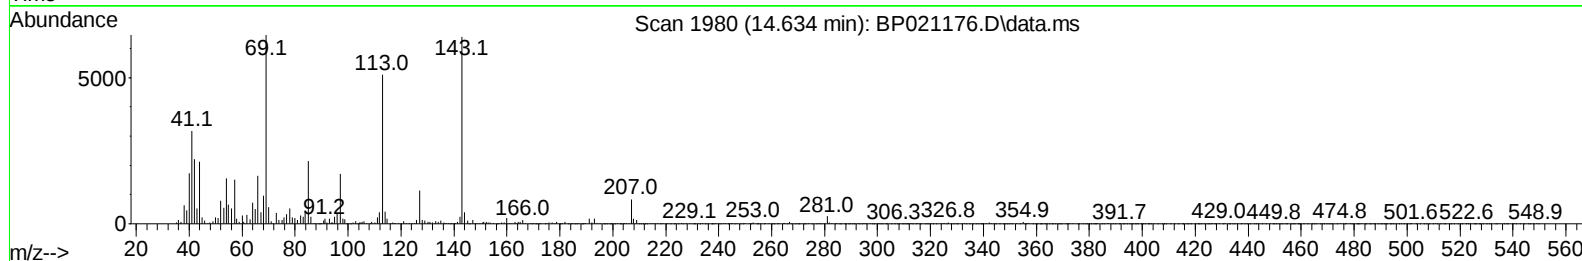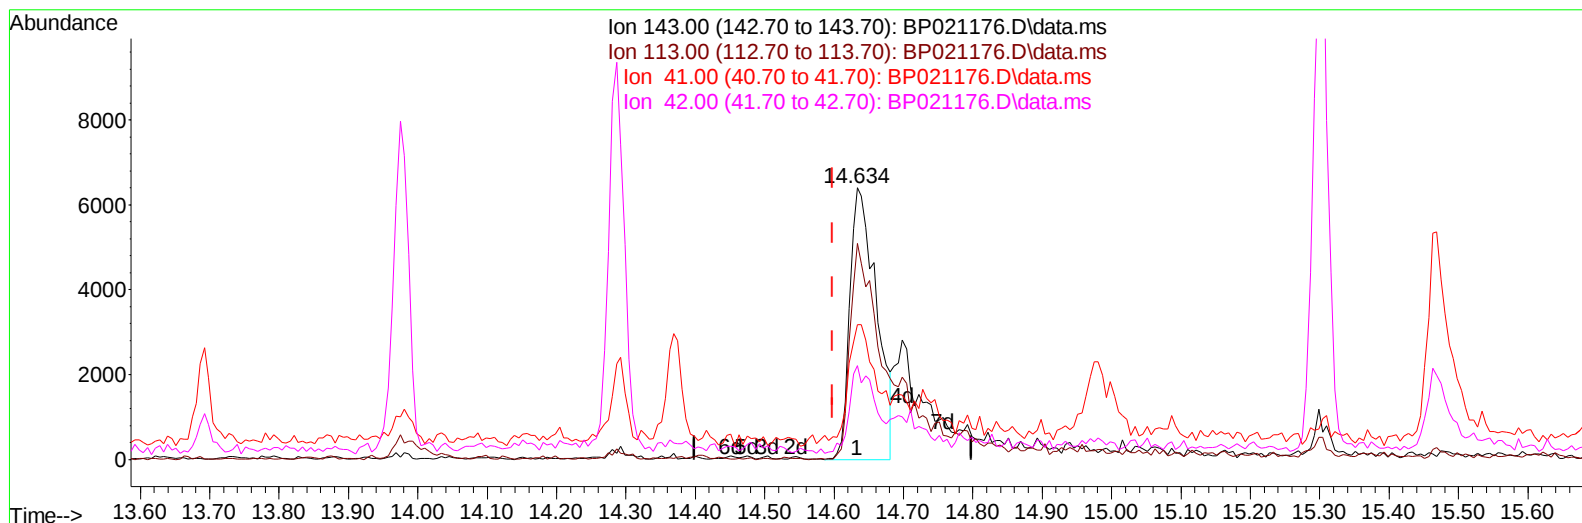

TIC: BP021176.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.634min (+ 0.035) 3.32 ng/u1

response 17062

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	79.65
41.00	37.90	49.68#
42.00	27.10	34.46#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021176.D
Acq On : 26 Jul 2024 18:47
Operator : MA/JU
Sample : P3329-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E86

Manual IntegrationsAPPROVED

Quant Time: Jul 26 22:47:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

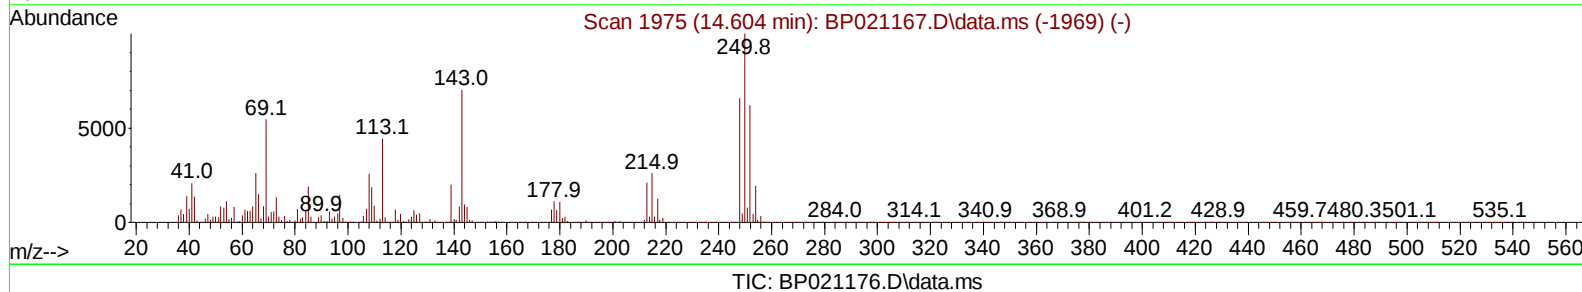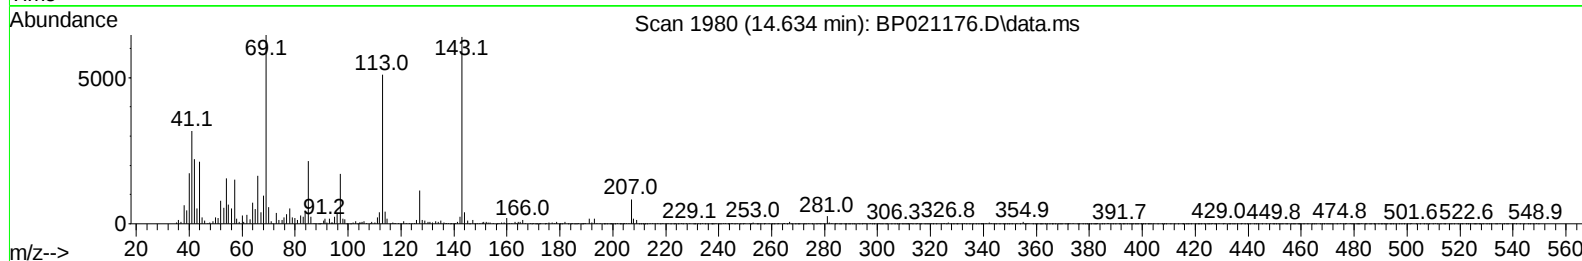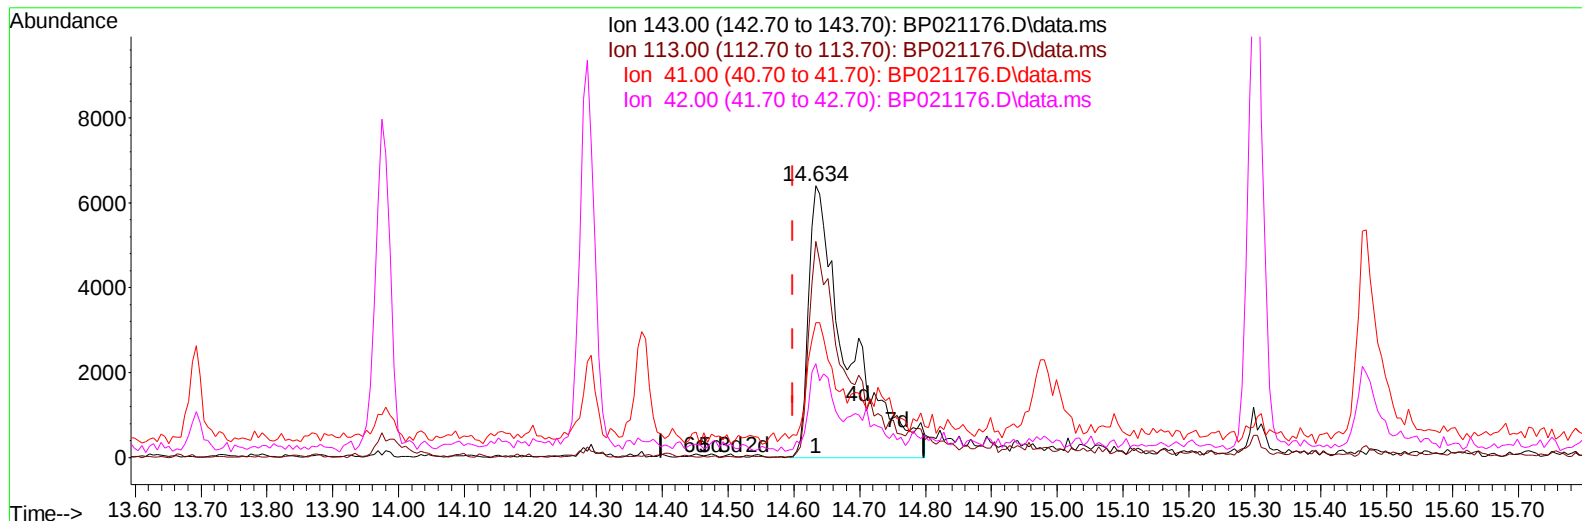

(54) 4-Nitrophenol-d4 (S)

14.634min (+ 0.035) 5.10 ng/ul m

response 26207

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	79.65
41.00	37.90	49.68#
42.00	27.10	34.46#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021176.D
 Acq On : 26 Jul 2024 18:47
 Operator : MA/JU
 Sample : P3329-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E86

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/27/2024
 Supervised By :mohammad ahmed 07/29/2024

Quant Time: Jul 26 23:17:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	216284	20.000	ng/ul	0.00
20) Naphthalene-d8	10.404	136	826131	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.287	164	496681	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.104	188	1006458	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	949813	20.000	ng/ul	0.00
88) Perylene-d12	24.863	264	1230417	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	20153	4.240	ng/uL	0.00
4) Pyridine-d5	3.599	84	115275	8.378	ng/ul	0.00
7) Phenol-d5	6.875	99	99022	5.616	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	243703	22.806	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132	302966	20.854	ng/ul	0.00
15) 4-Methylphenol-d8	8.381	113	188894	12.898	ng/ul	0.00
21) Nitrobenzene-d5	8.799	128	155624	24.253	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	180544	24.583	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	297362	22.392	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131	401500	22.821	ng/ul	0.00
46) Dimethylphthalate-d6	13.693	166	926982	25.674	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160	1017171	25.089	ng/ul	0.00
54) 4-Nitrophenol-d4	14.634	143	26207m	5.101	ng/ul	0.04
60) Fluorene-d10	15.304	176	808783	27.304	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	128344	21.076	ng/ul	0.00
73) Anthracene-d10	17.204	188	1305946	29.215	ng/ul	0.00
81) Pyrene-d10	19.592	212	1508085	25.682	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.639	264	1815071	29.910	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021176.D
Acq On : 26 Jul 2024 18:47
Operator : MA/JU
Sample : P3329-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E86

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:17:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

