




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021180.D
Acq On : 26 Jul 2024 22:28
Operator : MA/JU
Sample : PB162202BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK202

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:50:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

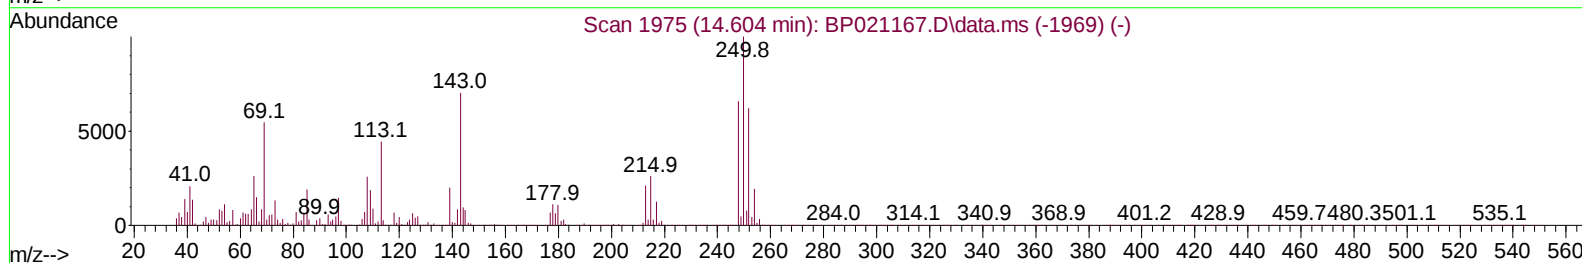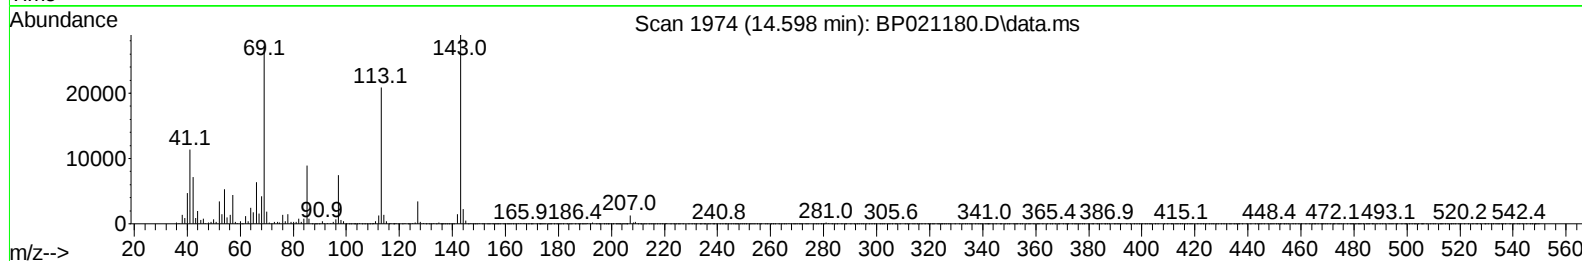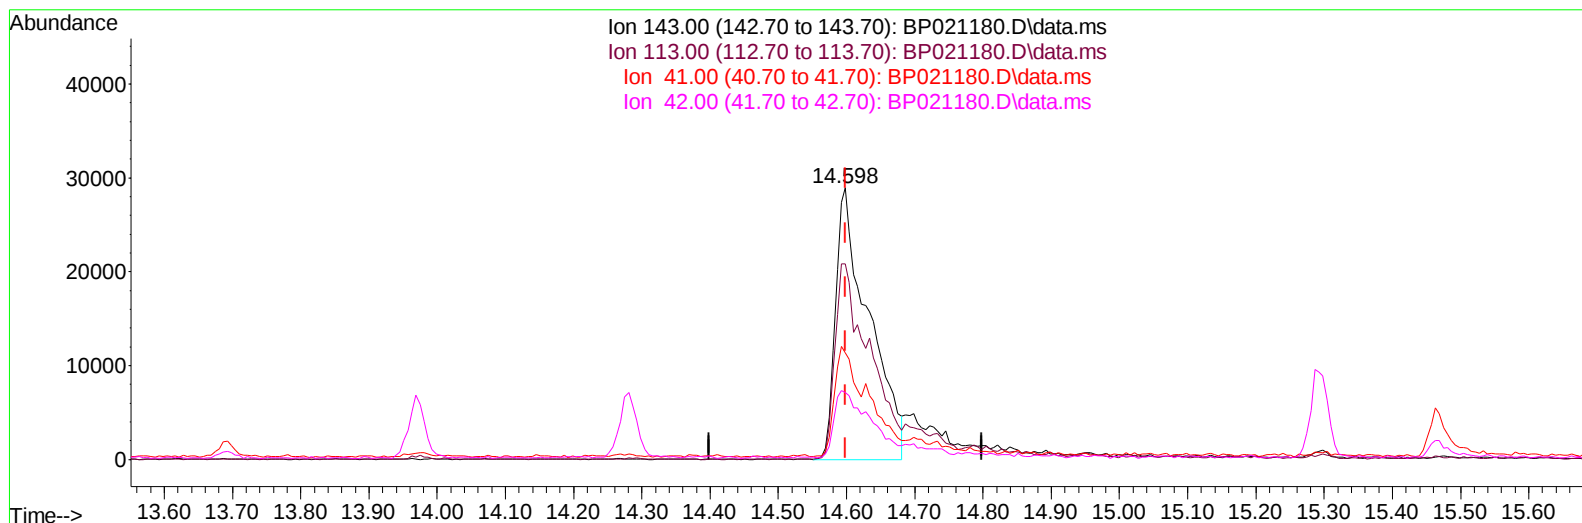

TIC: BP021180.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.598min (-0.000) 21.83 ng/u1

response 97522

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	72.07
41.00	37.90	39.20
42.00	27.10	24.76




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021180.D
Acq On : 26 Jul 2024 22:28
Operator : MA/JU
Sample : PB162202BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK202

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:50:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

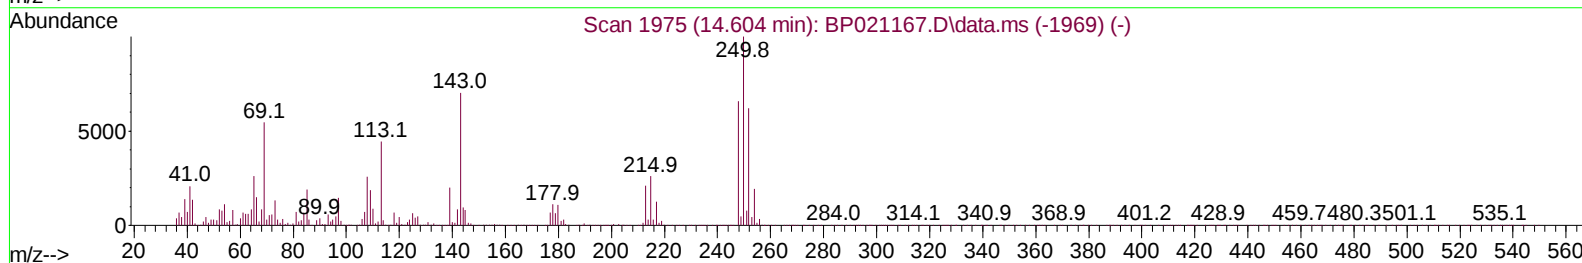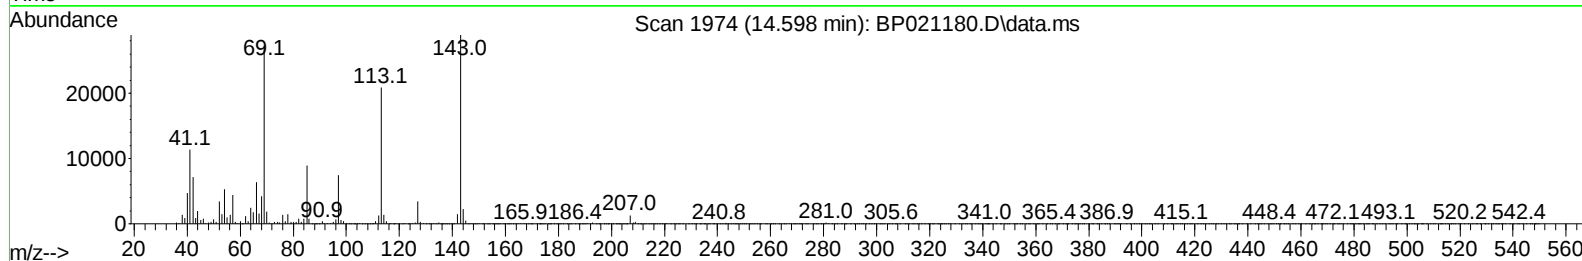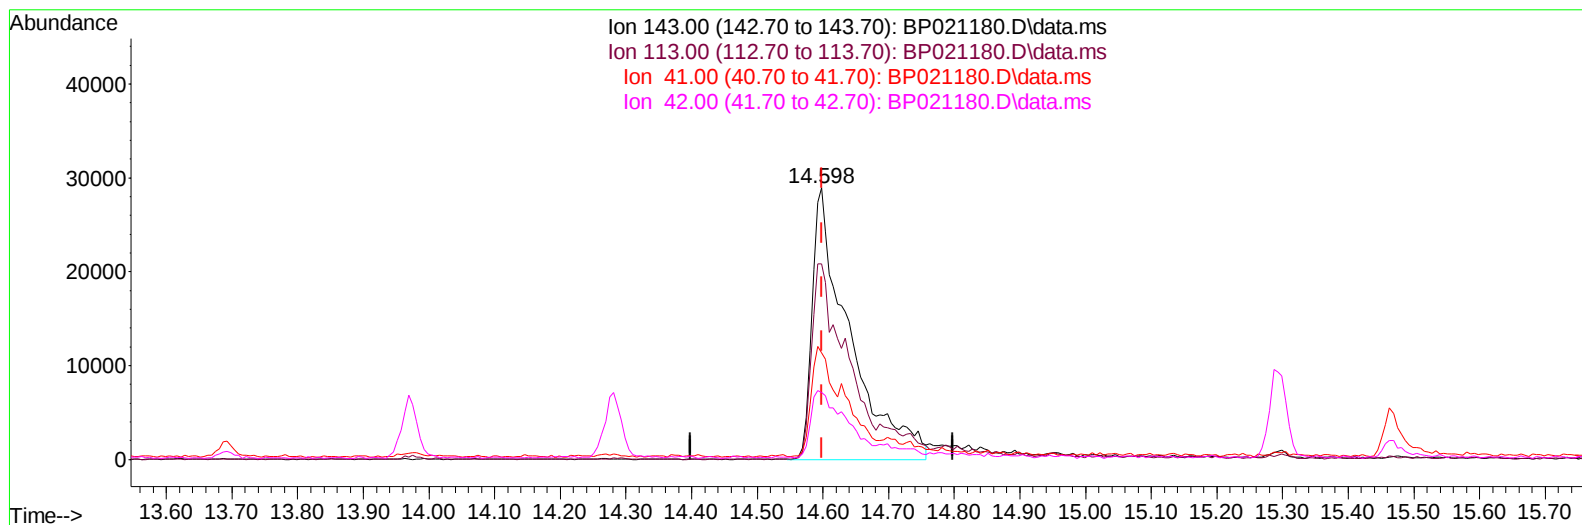

TIC: BP021180.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.598min (-0.000) 25.28 ng/ul m

response 112931

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	72.07
41.00	37.90	39.20
42.00	27.10	24.76

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021180.D
 Acq On : 26 Jul 2024 22:28
 Operator : MA/JU
 Sample : PB162202BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK202

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/27/2024
 Supervised By :mohammad ahmed 07/29/2024

Quant Time: Jul 26 23:51:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	172331	20.000	ng/ul	0.00
20) Naphthalene-d8	10.404	136	678585	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.281	164	431925	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	919985	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	927240	20.000	ng/ul	0.00
88) Perylene-d12	24.868	264	1125691	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	20911	5.522	ng/uL	0.00
4) Pyridine-d5	3.593	84	272894	24.891	ng/ul	0.00
7) Phenol-d5	6.857	99	347493	24.733	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	6.987	67	212490	24.956	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	290874	25.128	ng/ul	-0.01
15) 4-Methylphenol-d8	8.369	113	281047	24.085	ng/ul	-0.01
21) Nitrobenzene-d5	8.799	128	138715	26.318	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	160456	26.598	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	260191	23.853	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.575	131	378352	26.182	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	862043	27.455	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	947414	26.872	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.598	143	112931m	25.279	ng/ul	0.00
60) Fluorene-d10	15.292	176	717204	27.843	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.463	200	117521	21.113	ng/ul	0.00
73) Anthracene-d10	17.210	188	1137242	27.832	ng/ul	0.00
81) Pyrene-d10	19.592	212	1416183	24.704	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.639	264	1572522	28.324	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021180.D
Acq On : 26 Jul 2024 22:28
Operator : MA/JU
Sample : PB162202BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK202

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:51:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

