




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021181.D
Acq On : 26 Jul 2024 23:12
Operator : MA/JU
Sample : P3300-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:54:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

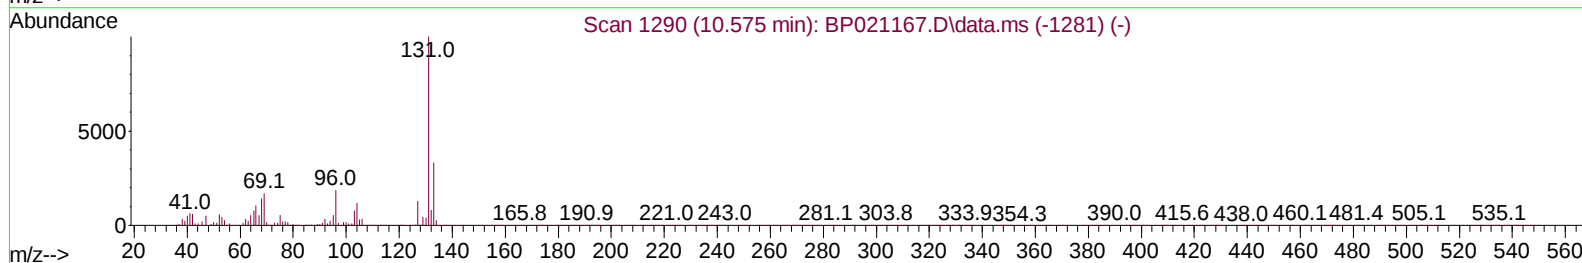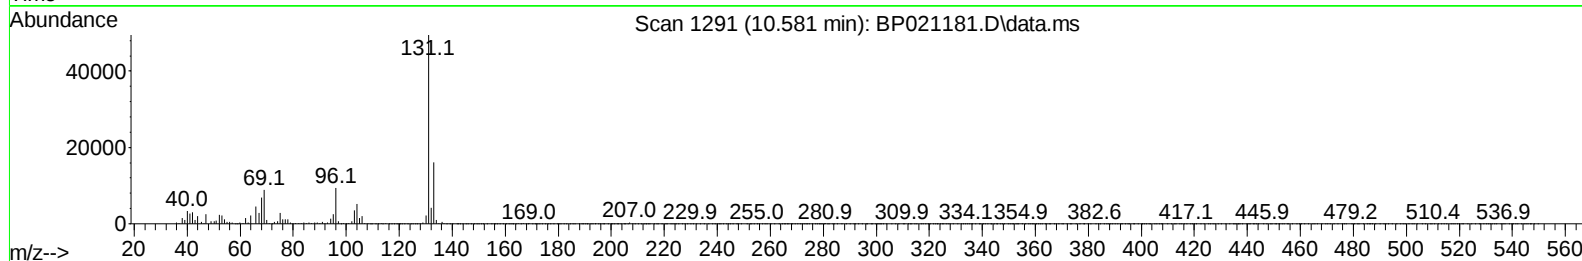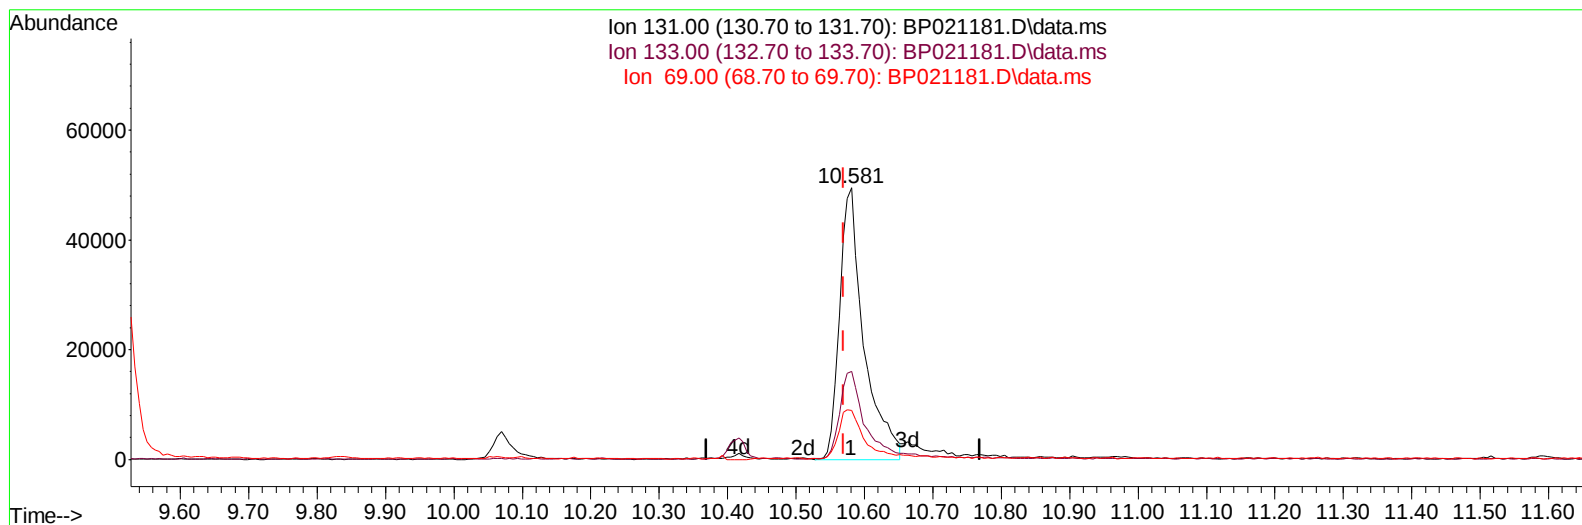

TIC: BP021181.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.581min (+ 0.012) 7.31 ng/ul

response 121178

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	32.53
69.00	17.40	18.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021181.D
Acq On : 26 Jul 2024 23:12
Operator : MA/JU
Sample : P3300-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:54:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

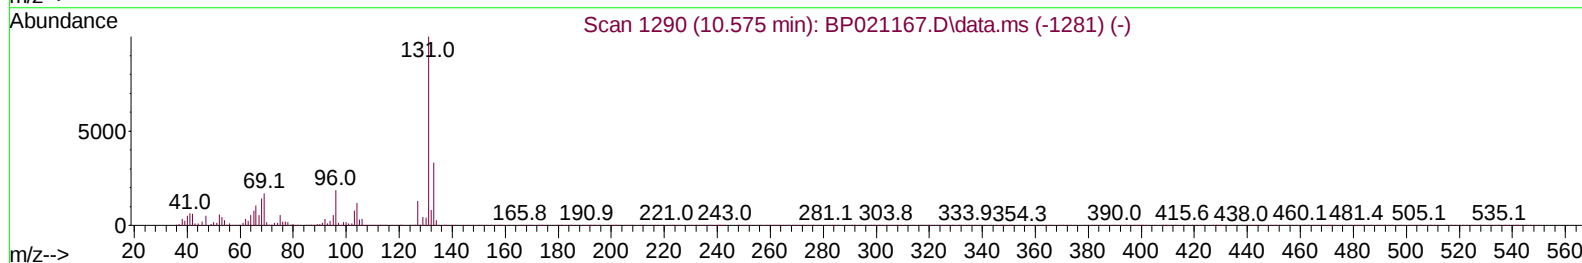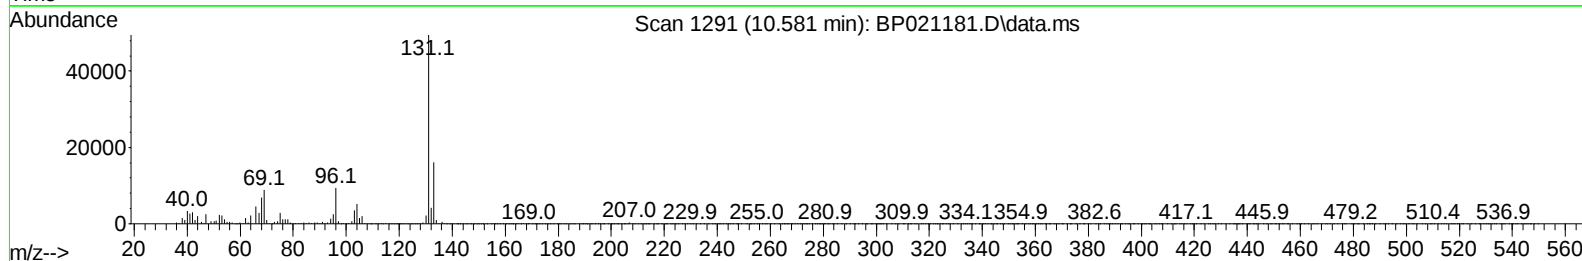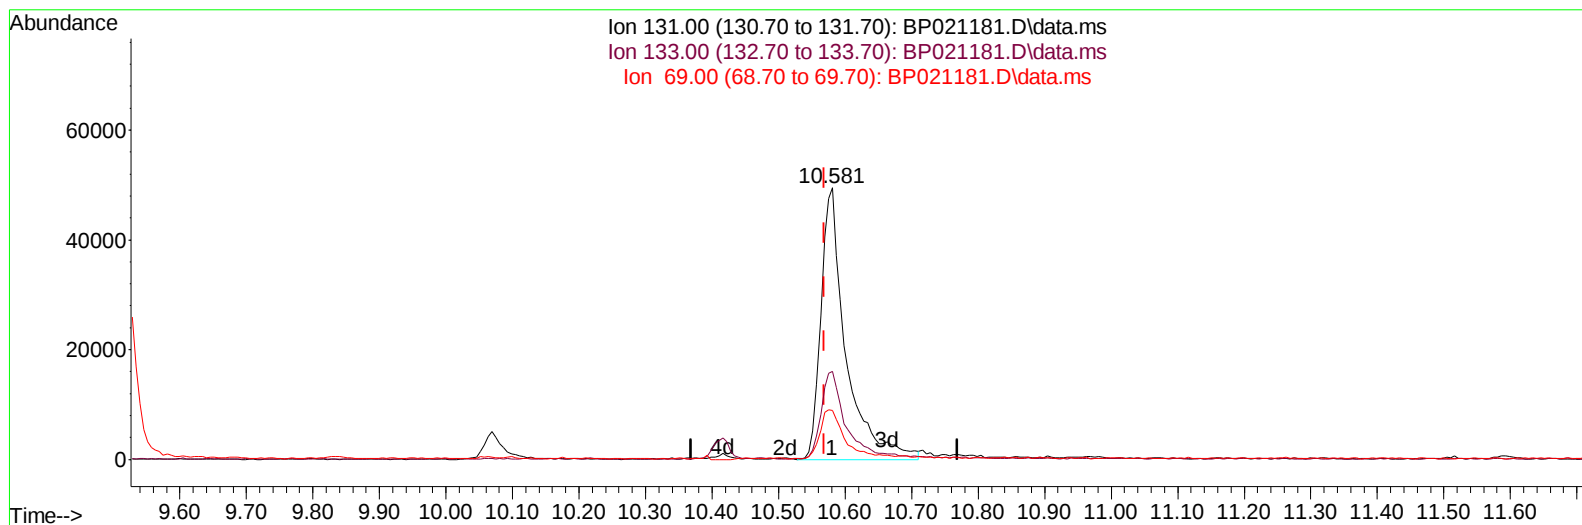

TIC: BP021181.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.581min (+ 0.012) 7.76 ng/ul m

response 128659

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	32.53
69.00	17.40	18.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021181.D
Acq On : 26 Jul 2024 23:12
Operator : MA/JU
Sample : P3300-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:54:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

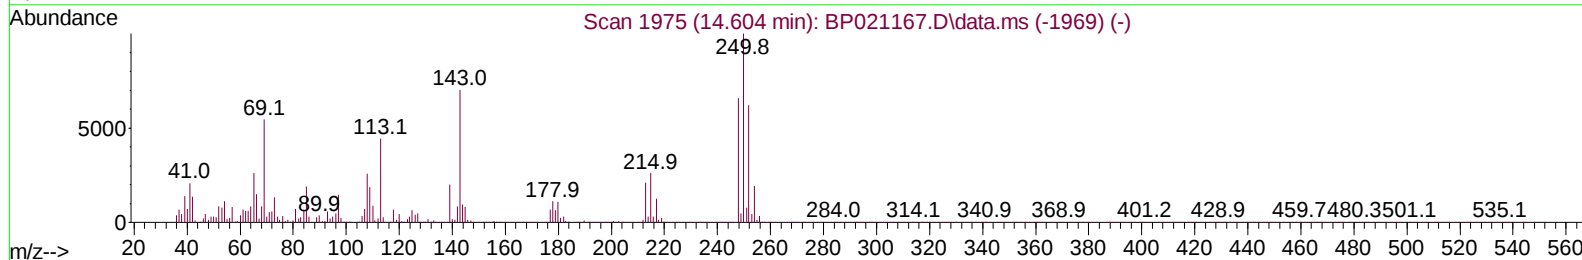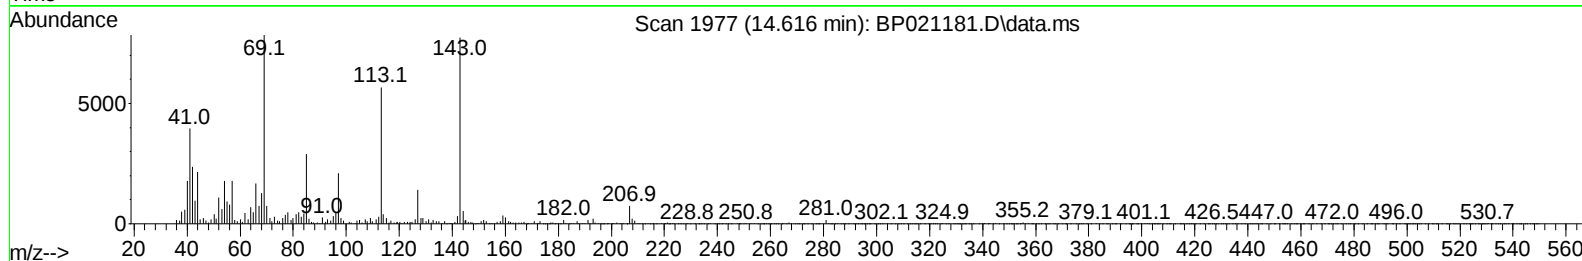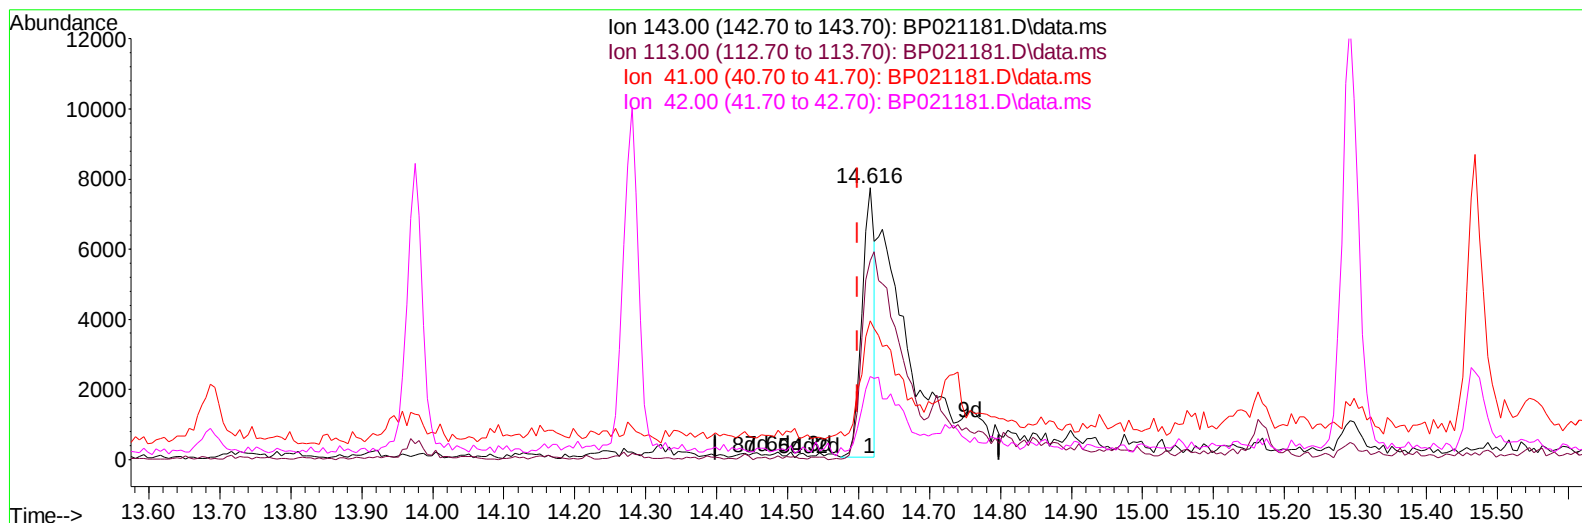

TIC: BP021181.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.616min (+ 0.018) 1.81 ng/ul

response 9546

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	73.28
41.00	37.90	51.04#
42.00	27.10	30.64




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021181.D
Acq On : 26 Jul 2024 23:12
Operator : MA/JU
Sample : P3300-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:54:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

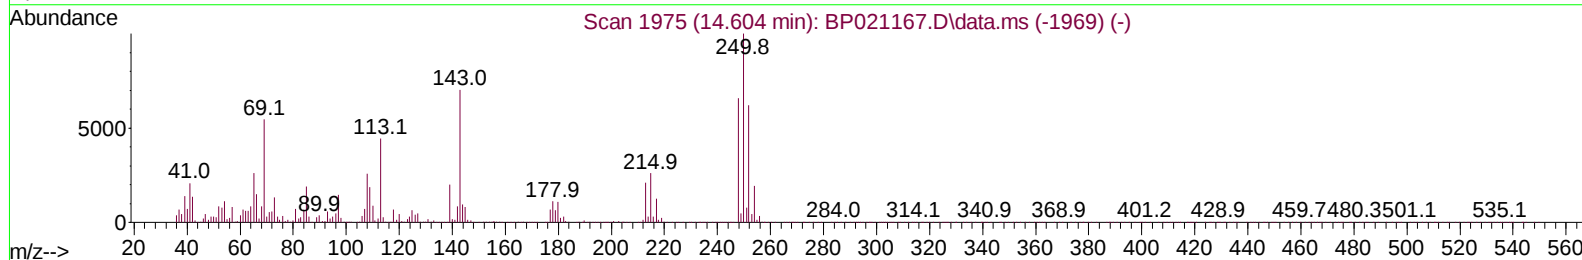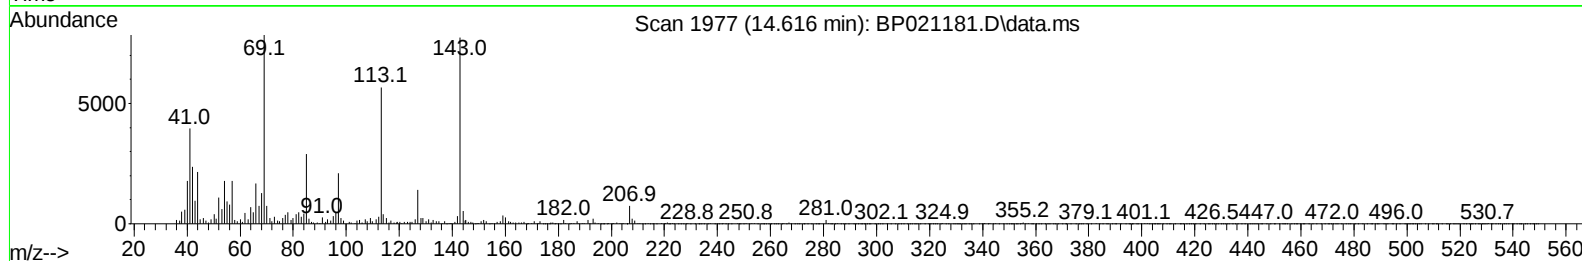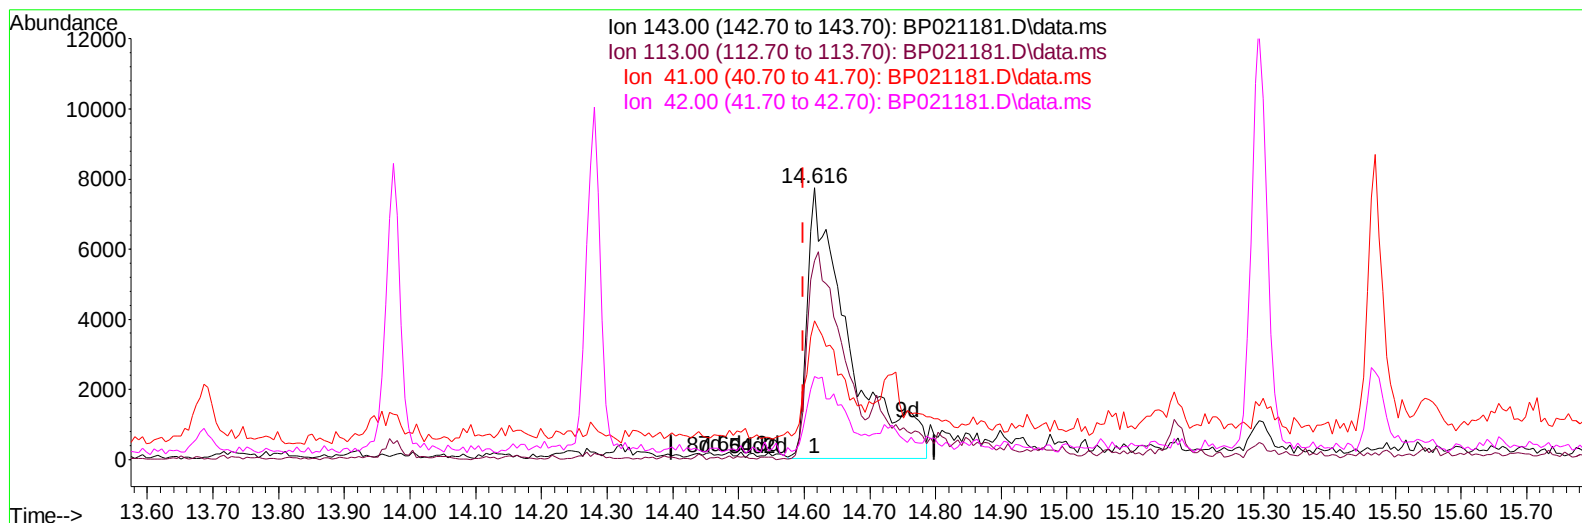

TIC: BP021181.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.616min (+ 0.018) 6.45 ng/ul m

response 33989

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	73.28
41.00	37.90	51.04#
42.00	27.10	30.64

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021181.D
 Acq On : 26 Jul 2024 23:12
 Operator : MA/JU
 Sample : P3300-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1G90

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/27/2024
 Supervised By :mohammad ahmed 07/29/2024

Quant Time: Jul 26 23:57:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	201471	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	778422	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.281	164	509631	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	1083735	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1073012	20.000	ng/ul	0.00
88) Perylene-d12	24.862	264	1293811	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	18303	4.134	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.869	99	94959	5.781	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	219393	22.040	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	269513	19.915	ng/ul	-0.01
15) 4-Methylphenol-d8	8.375	113	182740	13.395	ng/ul	0.00
21) Nitrobenzene-d5	8.805	128	144189	23.848	ng/ul	0.00
24) 2-Nitrophenol-d4	9.516	143	162584	23.494	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	274377	21.927	ng/ul	0.00
31) 4-Chloroaniline-d4	10.581	131	128659m	7.761	ng/ul	0.01
46) Dimethylphthalate-d6	13.687	166	963482	26.007	ng/ul	-0.01
49) Acenaphthylene-d8	13.975	160	1026766	24.682	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	33989m	6.448	ng/ul	0.02
60) Fluorene-d10	15.292	176	827664	27.232	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.469	200	150776	22.994	ng/ul	0.00
73) Anthracene-d10	17.198	188	1443576	29.991	ng/ul	0.00
81) Pyrene-d10	19.592	212	1739330	26.219	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.627	264	1970930	30.887	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021181.D
Acq On : 26 Jul 2024 23:12
Operator : MA/JU
Sample : P3300-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1G90

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:57:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 07/29/2024

