




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021196.D
Acq On : 27 Jul 2024 10:50
Operator : MA/JU
Sample : P3280-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZJ1

Manual IntegrationsAPPROVED

Quant Time: Jul 29 00:41:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 07/29/2024

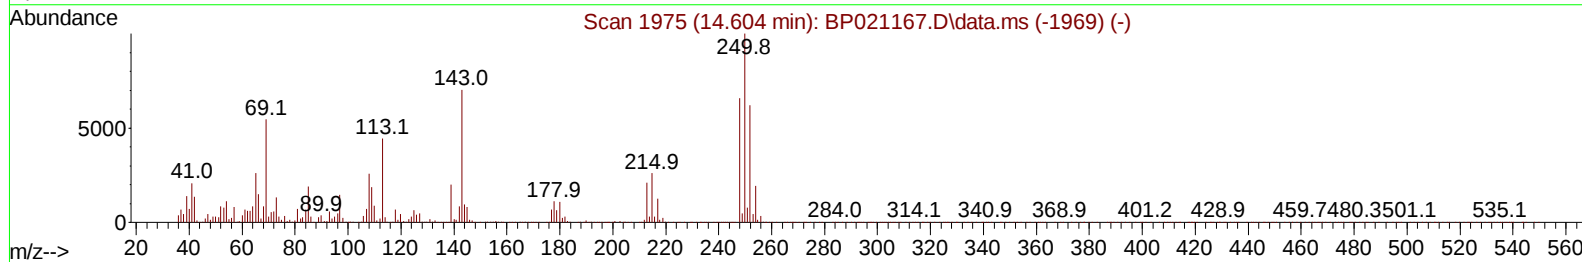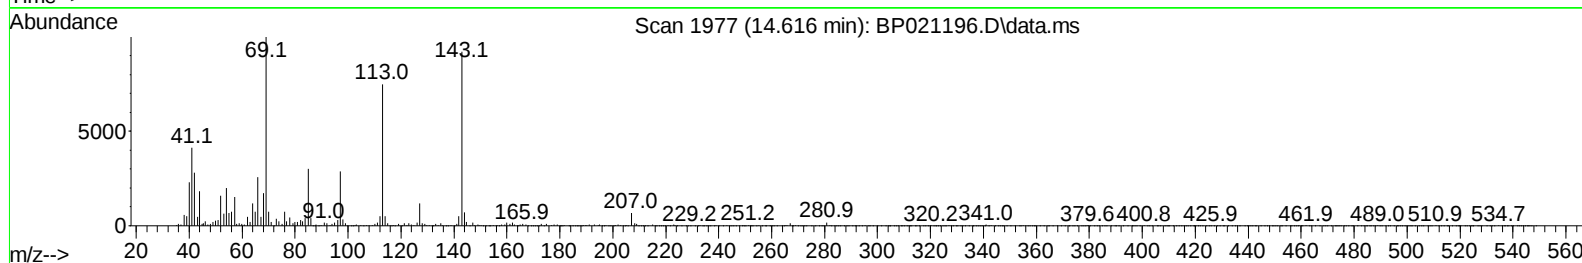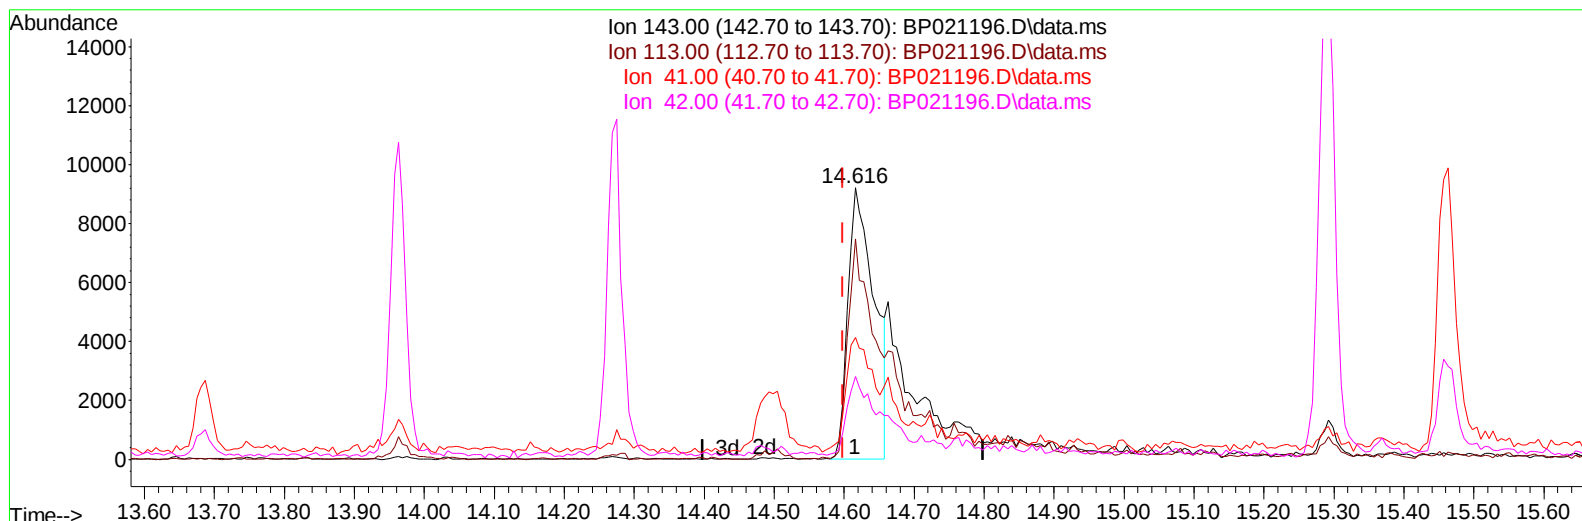

TIC: BP021196.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.616min (+ 0.018) 3.98 ng/u1

response 23777

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	81.28
41.00	37.90	44.97
42.00	27.10	30.43




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021196.D
Acq On : 27 Jul 2024 10:50
Operator : MA/JU
Sample : P3280-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZJ1

Manual IntegrationsAPPROVED

Quant Time: Jul 29 00:41:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 07/29/2024

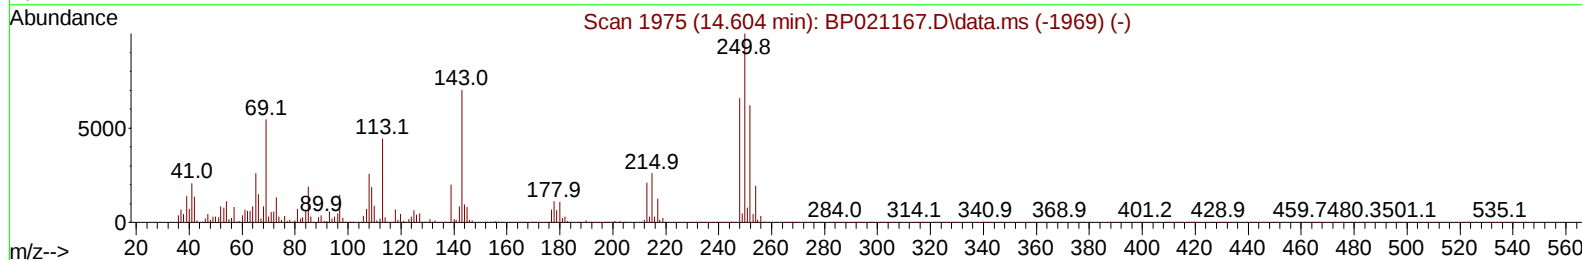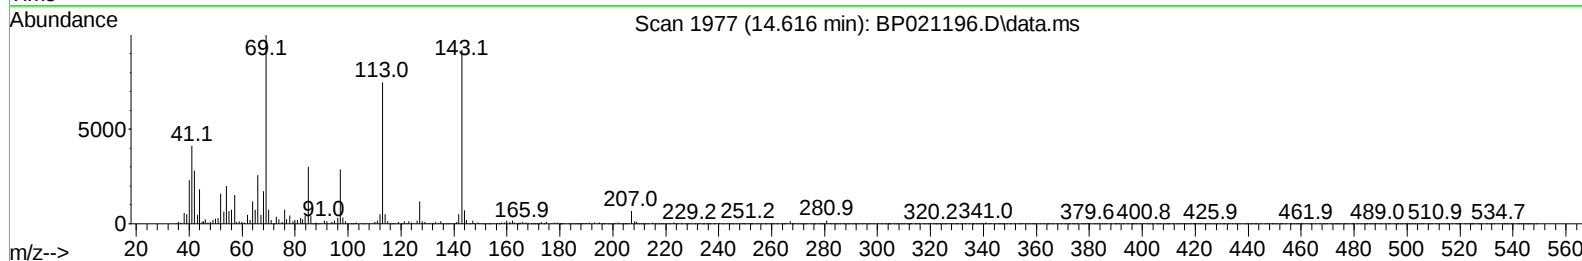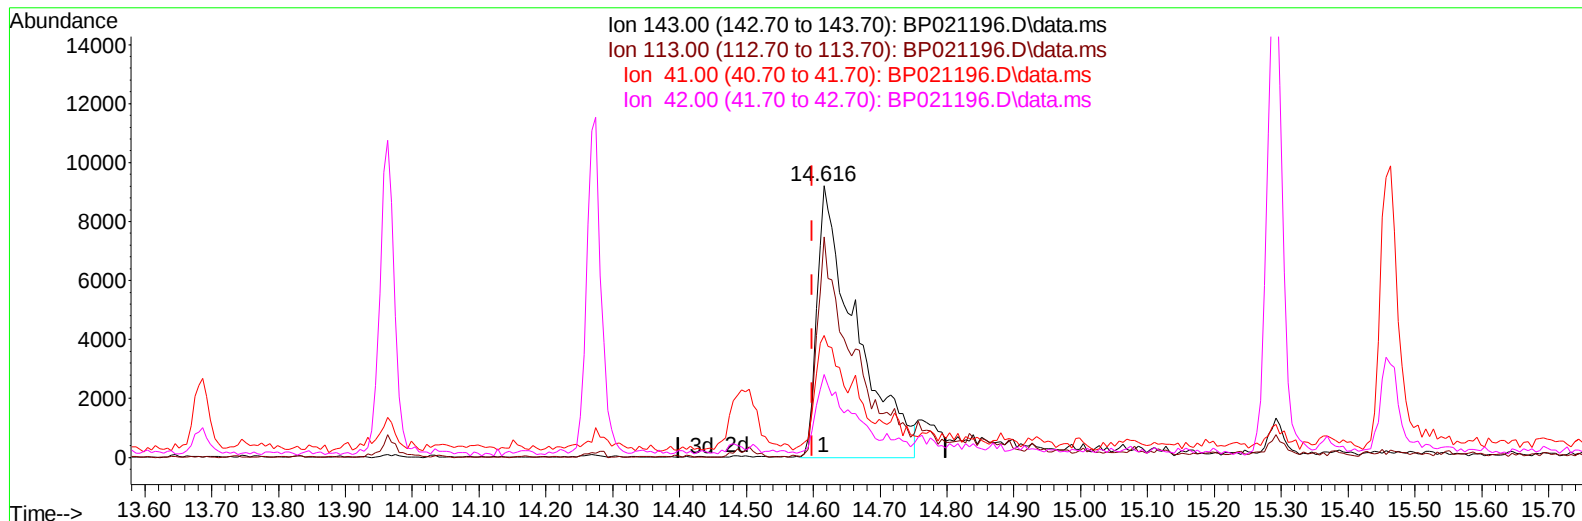

TIC: BP021196.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.616min (+ 0.018) 6.19 ng/ul m

response 36975

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	81.28
41.00	37.90	44.97
42.00	27.10	30.43

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021196.D
 Acq On : 27 Jul 2024 10:50
 Operator : MA/JU
 Sample : P3280-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZJ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/29/2024
 Supervised By :mohammad ahmed 07/29/2024

Quant Time: Jul 29 01:13:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	222624	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	883961	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.275	164	577379	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.092	188	1259588	20.000	ng/ul	-0.01
79) Chrysene-d12	21.545	240	1260493	20.000	ng/ul	-0.01
88) Perylene-d12	24.851	264	1478332	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	20469	4.184	ng/uL	0.00
4) Pyridine-d5	3.605	84	113915	8.043	ng/ul	0.00
7) Phenol-d5	6.869	99	117799	6.490	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	300969	27.363	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	353534	23.641	ng/ul	-0.01
15) 4-Methylphenol-d8	8.375	113	237636	15.764	ng/ul	0.00
21) Nitrobenzene-d5	8.805	128	195460	28.468	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	227006	28.887	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	375390	26.418	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131	417170	22.161	ng/ul	0.00
46) Dimethylphthalate-d6	13.687	166	1327246	31.622	ng/ul	-0.01
49) Acenaphthylene-d8	13.963	160	1418456	30.097	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.616	143	36975m	6.192	ng/ul	0.02
60) Fluorene-d10	15.292	176	1101867	32.000	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.463	200	228050	29.923	ng/ul	0.00
73) Anthracene-d10	17.192	188	1945756	34.780	ng/ul	-0.01
81) Pyrene-d10	19.580	212	2415030	30.990	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.627	264	2611795	35.822	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021196.D
Acq On : 27 Jul 2024 10:50
Operator : MA/JU
Sample : P3280-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZJ1

Manual IntegrationsAPPROVED

Quant Time: Jul 29 01:13:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 07/29/2024

