

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021175.D
 Acq On : 26 Jul 2024 18:03
 Operator : MA/JU
 Sample : P3329-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	38	rVB	16544	22438	0.50%	0.055%
2	3.605	103	105	119	rBV	134313	244249	5.41%	0.598%
3	3.899	150	155	160	rVB	23301	35097	0.78%	0.086%
4	4.258	212	216	221	rBV5	9949	14941	0.33%	0.037%
5	5.316	392	396	404	rBV3	6889	13853	0.31%	0.034%
6	5.534	429	433	437	rBV6	3406	5398	0.12%	0.013%
7	5.599	441	444	450	rBV3	5847	9759	0.22%	0.024%
8	5.681	454	458	460	rBV5	4668	5440	0.12%	0.013%
9	6.734	632	637	638	rBV5	4988	5521	0.12%	0.014%
10	6.828	650	653	655	rBV2	6206	8669	0.19%	0.021%
11	6.875	655	661	674	rVV	99907	247588	5.49%	0.606%
12	6.993	674	681	697	rVB	481195	782682	17.35%	1.915%
13	7.199	707	716	728	rBV	526448	941286	20.86%	2.304%
14	7.340	737	740	749	rVB	5129	11793	0.26%	0.029%
15	7.646	784	792	800	rBV	655504	1034547	22.93%	2.532%
16	7.710	800	803	814	rVB4	14711	38518	0.85%	0.094%
17	8.257	891	896	899	rBV7	4885	7438	0.16%	0.018%
18	8.381	909	917	931	rBV	369987	757440	16.79%	1.854%
19	8.734	972	977	982	rBV2	15509	28706	0.64%	0.070%
20	8.805	982	989	1006	rVV	579350	999489	22.15%	2.446%
21	8.952	1009	1014	1024	rVB	11244	24670	0.55%	0.060%
22	9.516	1100	1110	1123	rBV	445530	818114	18.13%	2.002%
23	10.075	1194	1205	1221	rBV	545743	1227766	27.21%	3.005%
24	10.340	1243	1250	1254	rBV	17957	35389	0.78%	0.087%
25	10.416	1255	1263	1280	rVB	711770	1427320	31.64%	3.493%
26	10.569	1283	1289	1309	rBV	565525	1111041	24.63%	2.719%
27	11.204	1392	1397	1401	rBV7	6524	10180	0.23%	0.025%
28	11.263	1403	1407	1411	rBV7	4119	5708	0.13%	0.014%
29	11.669	1472	1476	1480	rBV6	3241	5998	0.13%	0.015%
30	11.775	1486	1494	1509	rBV3	19645	58542	1.30%	0.143%
31	12.028	1530	1537	1544	rBV2	9571	21942	0.49%	0.054%
32	12.251	1569	1575	1582	rBV	18143	29311	0.65%	0.072%
33	13.069	1709	1714	1719	rBV9	2634	5137	0.11%	0.013%
34	13.128	1721	1724	1732	rVB9	3901	8881	0.20%	0.022%
35	13.251	1740	1745	1751	rVB8	7239	15409	0.34%	0.038%
36	13.498	1782	1787	1793	rBV10	6252	11377	0.25%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021175.D
 Acq On : 26 Jul 2024 18:03
 Operator : MA/JU
 Sample : P3329-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	13.693	1814	1820	1832	rBV	1505253	1966604	43.59%	4.813%
38	13.975	1861	1868	1880	rBV	1399313	2237487	49.59%	5.476%
39	14.287	1913	1921	1936	rVB	1268387	1999074	44.31%	4.892%
40	14.640	1972	1981	1988	rBV2	49073	125775	2.79%	0.308%
41	14.981	2033	2039	2046	rBV	13798	34073	0.76%	0.083%
42	15.051	2049	2051	2055	rVV4	9051	12516	0.28%	0.031%
43	15.110	2058	2061	2064	rVV3	14540	23566	0.52%	0.058%
44	15.134	2064	2065	2072	rVB5	12652	13415	0.30%	0.033%
45	15.304	2087	2094	2108	rBV	2099545	2930797	64.96%	7.172%
46	15.481	2114	2124	2140	rBV2	195744	524958	11.64%	1.285%
47	15.934	2197	2201	2206	rBV7	11151	16538	0.37%	0.040%
48	16.028	2212	2217	2224	rBV5	11551	21807	0.48%	0.053%
49	16.675	2324	2327	2334	rVB4	7687	10633	0.24%	0.026%
50	16.851	2353	2357	2361	rBV3	12345	18525	0.41%	0.045%
51	16.886	2361	2363	2369	rVB6	7635	11805	0.26%	0.029%
52	17.110	2394	2401	2409	rBV	1436808	2334699	51.75%	5.713%
53	17.210	2412	2418	2435	rVV	2427256	3511658	77.84%	8.594%
54	17.333	2437	2439	2446	rVB8	8164	11500	0.25%	0.028%
55	17.604	2483	2485	2492	rBV5	8226	11358	0.25%	0.028%
56	17.704	2499	2502	2511	rVB7	11082	15888	0.35%	0.039%
57	17.786	2511	2516	2524	rBV3	70262	93116	2.06%	0.228%
58	18.033	2554	2558	2568	rBV4	49634	111965	2.48%	0.274%
59	18.333	2607	2609	2614	rVB5	11384	13687	0.30%	0.033%
60	18.557	2645	2647	2652	rVB5	13166	13601	0.30%	0.033%
61	18.916	2705	2708	2715	rVB2	34523	49444	1.10%	0.121%
62	19.145	2743	2747	2753	rBV5	33500	60825	1.35%	0.149%
63	19.222	2757	2760	2765	rVV2	27062	41079	0.91%	0.101%
64	19.598	2818	2824	2842	rBV	2897781	4411427	97.78%	10.796%
65	21.563	3152	3158	3174	rVB	1697580	2732352	60.56%	6.687%
66	24.645	3673	3682	3698	rVB2	1612570	4511552	100.00%	11.041%
67	24.880	3714	3722	3736	rVB2	1007211	2959755	65.60%	7.243%




Sum of corrected areas: 40863116

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021175.D
Acq On : 26 Jul 2024 18:03
Operator : MA/JU
Sample : P3329-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

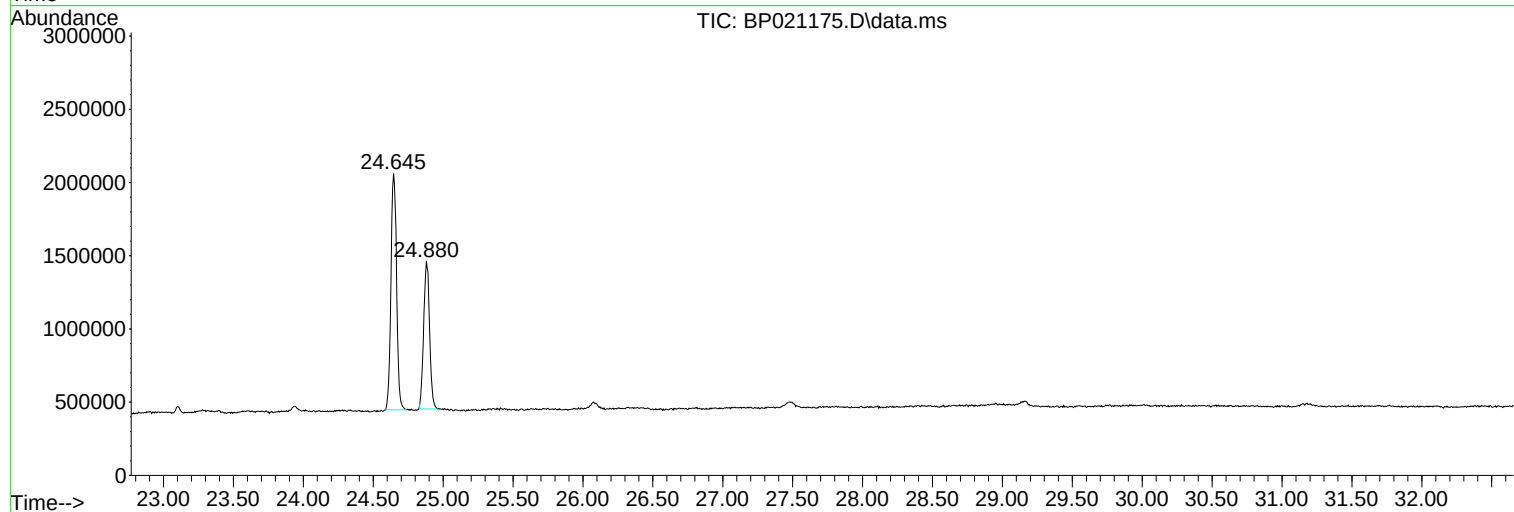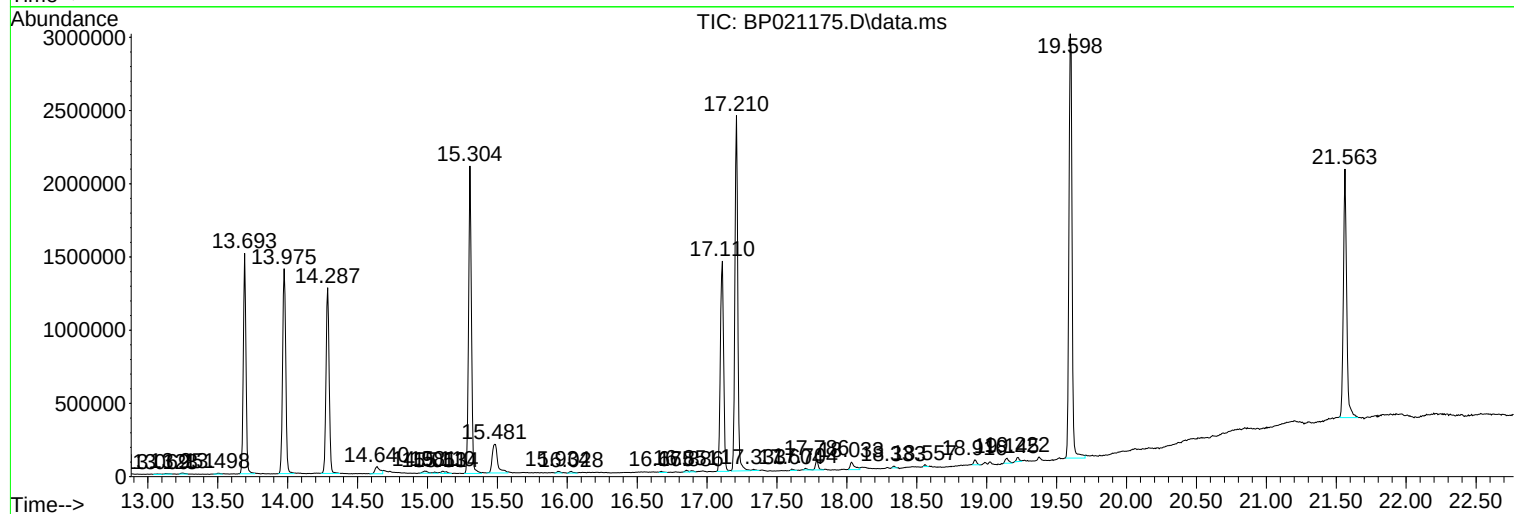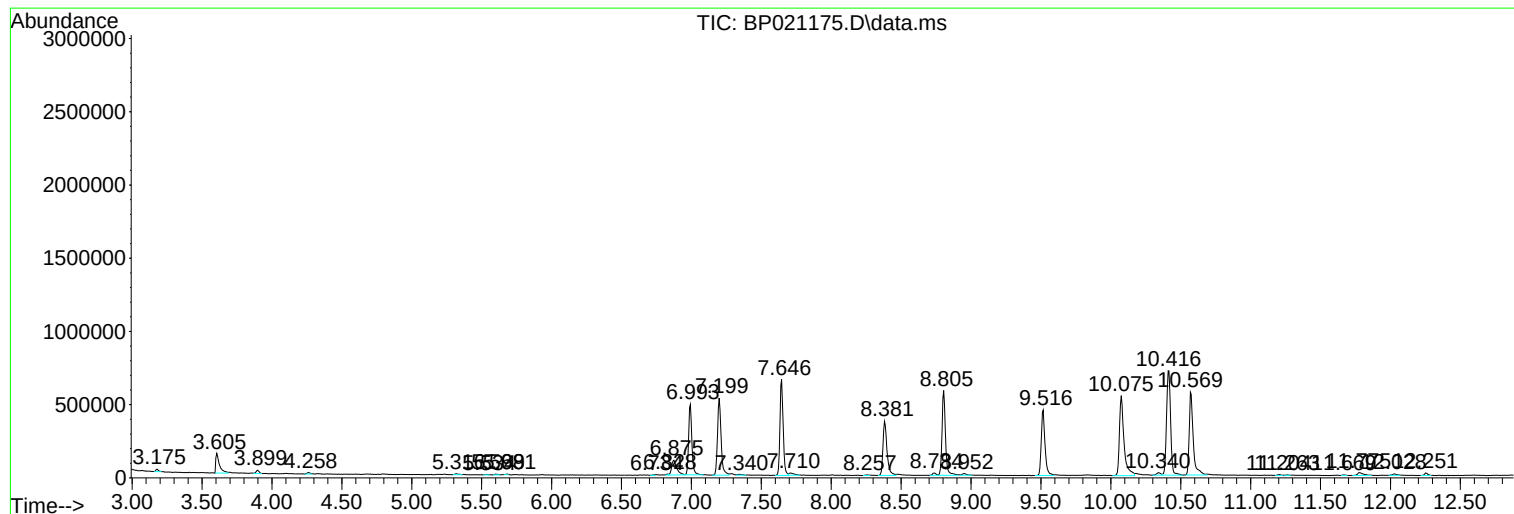

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021175.D
Acq On : 26 Jul 2024 18:03
Operator : MA/JU
Sample : P3329-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021175.D
Acq On : 26 Jul 2024 18:03
Operator : MA/JU
Sample : P3329-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc