

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021185.D
 Acq On : 27 Jul 2024 02:09
 Operator : MA/JU
 Sample : P3301-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	41	rVB	35607	51367	1.20%	0.139%
2	3.605	102	105	129	rBV	162888	294378	6.90%	0.798%
3	3.899	151	155	161	rVB	28790	44253	1.04%	0.120%
4	4.258	213	216	222	rBV7	6590	11184	0.26%	0.030%
5	4.311	222	225	230	rVB3	6987	9393	0.22%	0.025%
6	4.675	283	287	293	rVB9	3621	5815	0.14%	0.016%
7	4.793	302	307	316	rBV	13761	22454	0.53%	0.061%
8	5.193	371	375	377	rBV4	3820	5138	0.12%	0.014%
9	5.322	392	397	407	rVB3	8884	22121	0.52%	0.060%
10	5.605	441	445	449	rBV5	5092	6814	0.16%	0.018%
11	5.681	454	458	462	rVB3	7407	10475	0.25%	0.028%
12	6.740	632	638	642	rBV7	7506	14605	0.34%	0.040%
13	6.869	654	660	675	rVB	120850	272504	6.38%	0.739%
14	6.993	675	681	695	rBV	472094	771930	18.08%	2.093%
15	7.193	707	715	727	rBV	512805	959781	22.48%	2.602%
16	7.646	785	792	800	rBV	625554	1041028	24.39%	2.822%
17	7.705	800	802	806	rVB3	4078	7833	0.18%	0.021%
18	8.381	909	917	932	rBV	363870	800307	18.75%	2.170%
19	8.734	970	977	981	rBV3	11640	23547	0.55%	0.064%
20	8.799	982	988	1009	rVV	548034	969446	22.71%	2.628%
21	8.946	1009	1013	1020	rVB5	9100	16950	0.40%	0.046%
22	9.146	1042	1047	1051	rVB8	3365	5312	0.12%	0.014%
23	9.516	1103	1110	1128	rBV	504761	826173	19.35%	2.240%
24	10.063	1194	1203	1220	rBV	498976	1168032	27.36%	3.167%
25	10.340	1244	1250	1254	rBV2	11285	20073	0.47%	0.054%
26	10.404	1254	1261	1279	rVB	780309	1384571	32.43%	3.754%
27	10.575	1281	1290	1311	rBV	477214	1106841	25.93%	3.001%
28	11.199	1390	1396	1401	rBV7	6109	10447	0.24%	0.028%
29	11.257	1401	1406	1410	rBV8	2236	4298	0.10%	0.012%
30	11.787	1484	1496	1510	rBV3	17873	59316	1.39%	0.161%
31	12.028	1529	1537	1538	rBV3	7534	13529	0.32%	0.037%
32	12.257	1570	1576	1581	rVB	11292	19982	0.47%	0.054%
33	13.128	1720	1724	1728	rBV6	4438	7096	0.17%	0.019%
34	13.251	1740	1745	1746	rBV5	4326	6630	0.16%	0.018%
35	13.263	1746	1747	1752	rVB5	3736	4486	0.11%	0.012%
36	13.693	1811	1820	1833	rBV	1185412	1734305	40.63%	4.702%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021185.D
Acq On : 27 Jul 2024 02:09
Operator : MA/JU
Sample : P3301-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	13.969	1859	1867	1877	rBV	1149627	2010110	47.09%	5.450%
38	14.281	1907	1920	1933	rBV	1025796	1748805	40.97%	4.741%
39	14.640	1975	1981	1989	rBV2	42512	123007	2.88%	0.333%
40	14.734	1995	1997	2003	rVB7	8614	14087	0.33%	0.038%
41	14.969	2032	2037	2047	rBV2	15344	28224	0.66%	0.077%
42	15.110	2058	2061	2065	rVB	10556	10580	0.25%	0.029%
43	15.304	2086	2094	2114	rBV	1580094	2628350	61.57%	7.126%
44	15.463	2115	2121	2146	rBV	353174	810781	18.99%	2.198%
45	15.934	2197	2201	2207	rBV9	7811	13193	0.31%	0.036%
46	16.516	2298	2300	2306	rVB7	4127	4893	0.11%	0.013%
47	16.675	2323	2327	2331	rVB5	5056	6715	0.16%	0.018%
48	16.769	2340	2343	2347	rBV6	3478	5514	0.13%	0.015%
49	17.104	2393	2400	2411	rBV	1193714	1866115	43.72%	5.059%
50	17.210	2411	2418	2433	rVV	1994557	2975533	69.70%	8.067%
51	17.334	2437	2439	2444	rVB6	6965	9681	0.23%	0.026%
52	17.786	2511	2516	2523	rBV	104738	141023	3.30%	0.382%
53	18.033	2554	2558	2566	rBV4	45412	83770	1.96%	0.227%
54	18.551	2644	2646	2649	rBV4	8357	11410	0.27%	0.031%
55	19.139	2743	2746	2750	rBV3	29552	37570	0.88%	0.102%
56	19.375	2782	2786	2791	rBV7	32176	55690	1.30%	0.151%
57	19.592	2818	2823	2833	rBV	2586399	3531165	82.72%	9.573%
58	21.551	3151	3156	3170	rVB2	1242084	2142469	50.19%	5.809%
59	24.633	3671	3680	3698	rVB	1542508	4268762	100.00%	11.573%
60	24.857	3711	3718	3738	rVB2	784003	2625035	61.49%	7.117%


Sum of corrected areas: 36884896

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021185.D
Acq On : 27 Jul 2024 02:09
Operator : MA/JU
Sample : P3301-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

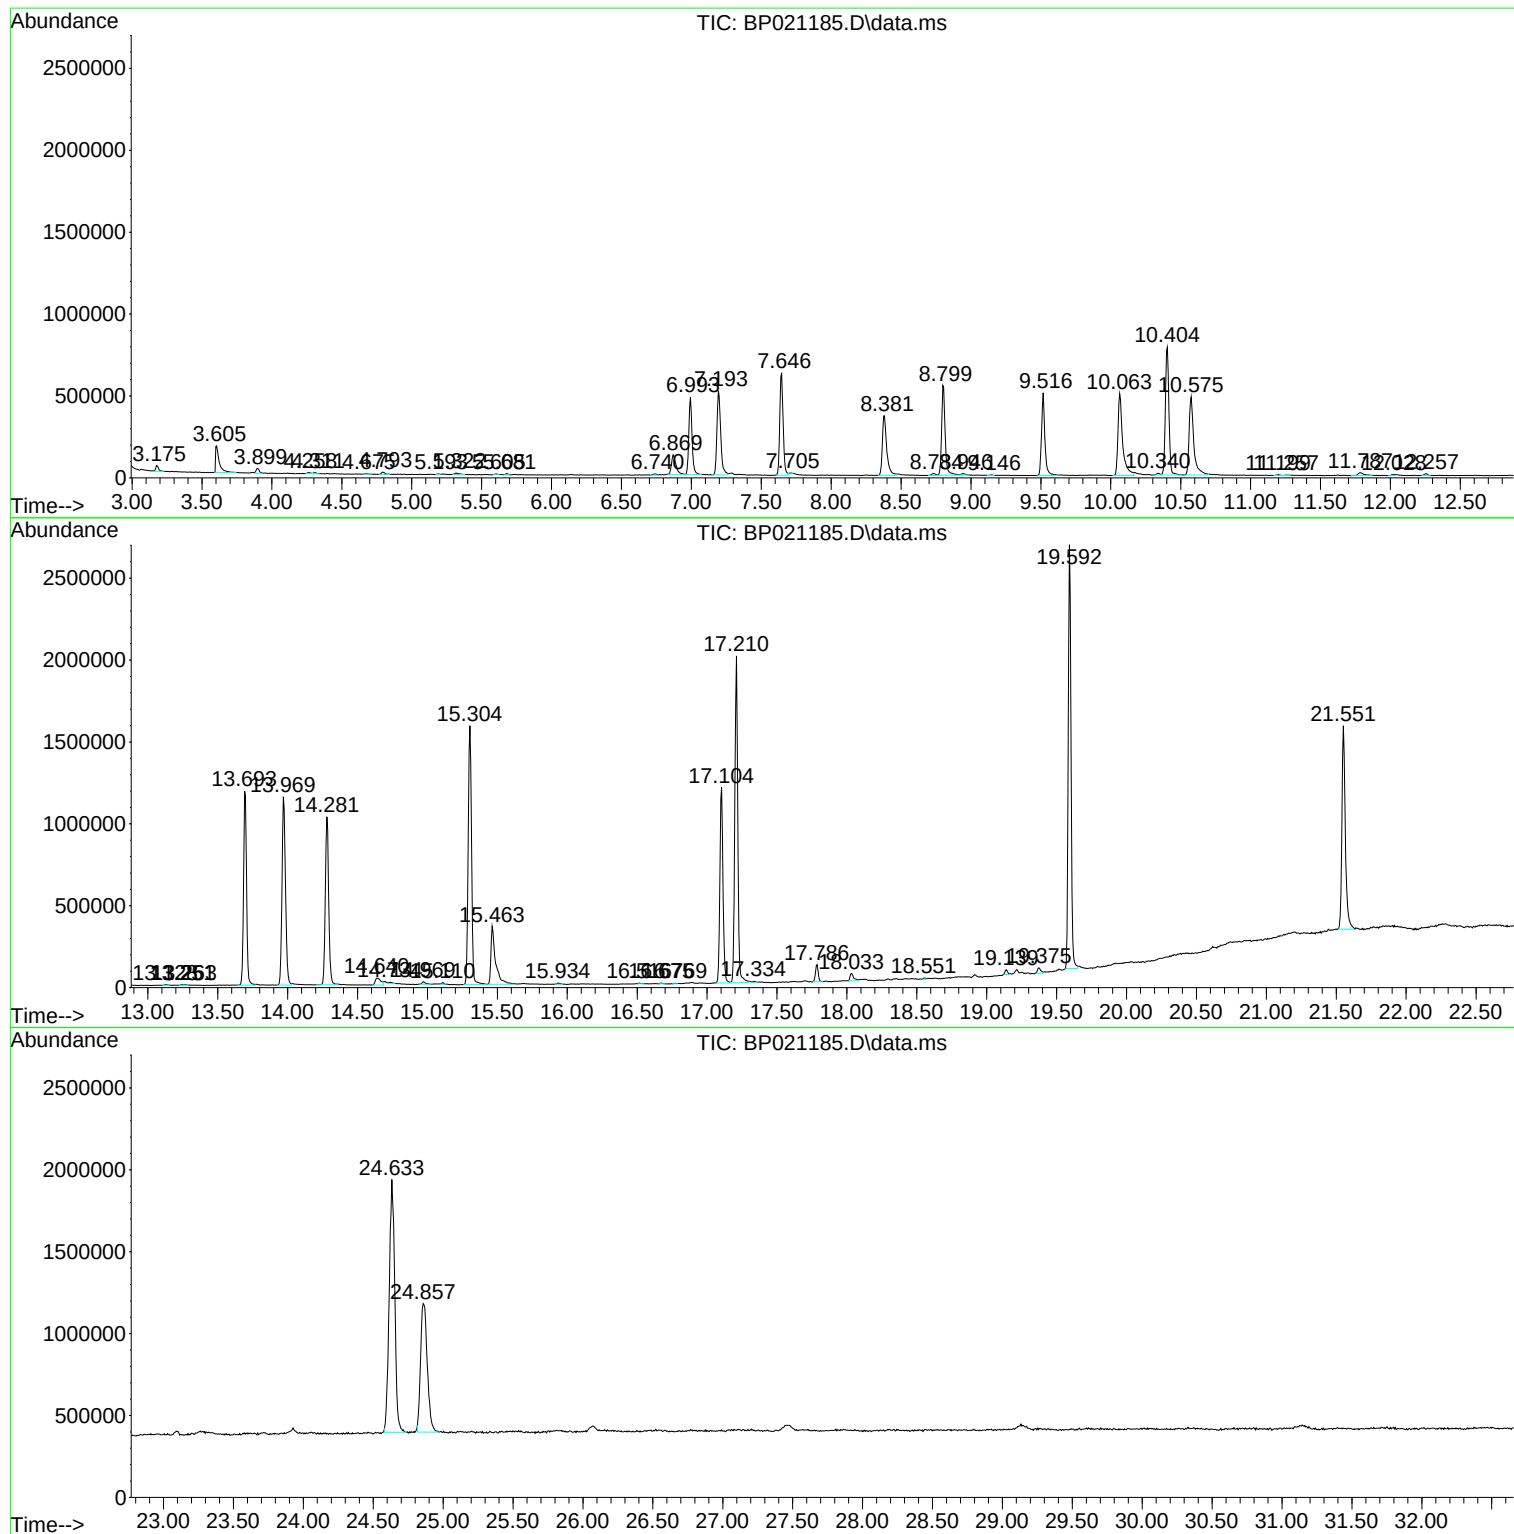

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021185.D
Acq On : 27 Jul 2024 02:09
Operator : MA/JU
Sample : P3301-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021185.D
Acq On : 27 Jul 2024 02:09
Operator : MA/JU
Sample : P3301-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc