

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021188.D
 Acq On : 27 Jul 2024 04:21
 Operator : MA/JU
 Sample : P3348-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08H7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	46	rVB	41106	73922	1.34%	0.143%
2	3.611	103	106	125	rBV	117215	228804	4.16%	0.443%
3	3.899	152	155	160	rVB2	11089	14851	0.27%	0.029%
4	4.264	214	217	222	rBV7	6776	9177	0.17%	0.018%
5	4.370	231	235	237	rBV4	5908	7141	0.13%	0.014%
6	4.405	237	241	250	rVB	75171	121981	2.22%	0.236%
7	4.675	283	287	293	rBV9	4713	8328	0.15%	0.016%
8	4.793	304	307	313	rVB3	5683	9518	0.17%	0.018%
9	5.681	455	458	462	rBV6	3462	5602	0.10%	0.011%
10	5.734	463	467	473	rVB5	7668	12141	0.22%	0.024%
11	5.934	495	501	504	rBV8	4245	6829	0.12%	0.013%
12	6.764	633	642	650	rBV5	10440	29064	0.53%	0.056%
13	6.870	653	660	675	rVV	257003	521784	9.48%	1.011%
14	6.993	675	681	694	rVB	644169	1048213	19.05%	2.031%
15	7.199	709	716	735	rBV	766377	1313352	23.86%	2.545%
16	7.334	735	739	751	rVB	10919	25440	0.46%	0.049%
17	7.640	783	791	800	rBV	702023	1169156	21.24%	2.265%
18	8.287	896	901	905	rBV5	7679	12858	0.23%	0.025%
19	8.369	909	915	930	rVV	694100	1279509	23.25%	2.479%
20	8.793	980	987	1004	rBV	712162	1325297	24.08%	2.568%
21	8.946	1009	1013	1020	rVB4	17610	31961	0.58%	0.062%
22	9.134	1038	1045	1051	rBV4	3117	7595	0.14%	0.015%
23	9.505	1100	1108	1121	rBV	608110	1165223	21.17%	2.258%
24	9.793	1149	1157	1167	rBV3	25612	73904	1.34%	0.143%
25	10.063	1196	1203	1218	rBV	740442	1682370	30.57%	3.260%
26	10.410	1254	1262	1276	rBV	978067	1623532	29.50%	3.146%
27	10.563	1281	1288	1305	rBV	616346	1266166	23.01%	2.453%
28	11.087	1370	1377	1378	rBV7	4440	5907	0.11%	0.011%
29	11.240	1396	1403	1413	rBV2	59365	155701	2.83%	0.302%
30	12.010	1527	1534	1540	rBV	16732	30722	0.56%	0.060%
31	12.857	1674	1678	1681	rVB6	4134	6530	0.12%	0.013%
32	13.116	1715	1722	1734	rVV	564215	853420	15.51%	1.654%
33	13.346	1754	1761	1765	rBV10	3496	6555	0.12%	0.013%
34	13.675	1811	1817	1833	rBV	1901147	2587387	47.01%	5.013%
35	13.963	1856	1866	1881	rBV	2021790	3044215	55.31%	5.898%
36	14.269	1912	1918	1929	rBV	1510481	2170090	39.43%	4.205%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021188.D
 Acq On : 27 Jul 2024 04:21
 Operator : MA/JU
 Sample : P3348-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08H7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	14.610	1971	1976	1982	rBV3	68213	164943	3.00%	0.320%
38	14.710	1990	1993	1998	rVB5	13158	17737	0.32%	0.034%
39	15.122	2059	2063	2071	rVB5	7287	10324	0.19%	0.020%
40	15.293	2085	2092	2110	rBV	2683017	3843677	69.84%	7.447%
41	15.463	2115	2121	2132	rBV	636129	1149852	20.89%	2.228%
42	15.922	2195	2199	2203	rVB	10692	13411	0.24%	0.026%
43	16.493	2292	2296	2304	rBV	5834	14019	0.25%	0.027%
44	17.104	2393	2400	2407	rBV	1781853	2644665	48.05%	5.124%
45	17.198	2410	2416	2428	rVV	3351075	4319334	78.48%	8.369%
46	17.787	2511	2516	2521	rVB9	10846	17408	0.32%	0.034%
47	18.022	2552	2556	2565	rBV	81588	148009	2.69%	0.287%
48	18.098	2567	2569	2575	rVB3	14632	17474	0.32%	0.034%
49	19.128	2741	2744	2750	rVB2	43226	61657	1.12%	0.119%
50	19.210	2754	2758	2761	rBV	39447	55865	1.02%	0.108%
51	19.369	2781	2785	2790	rBV3	67956	109897	2.00%	0.213%
52	19.586	2816	2822	2832	rBV	3950837	5237549	95.17%	10.148%
53	21.551	3150	3156	3170	rVB2	1789228	2987877	54.29%	5.789%
54	24.627	3670	3679	3693	rVB	1979421	5503616	100.00%	10.663%
55	24.857	3710	3718	3736	rVB	1169003	3360911	61.07%	6.512%




Sum of corrected areas: 51612470

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021188.D
Acq On : 27 Jul 2024 04:21
Operator : MA/JU
Sample : P3348-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08H7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

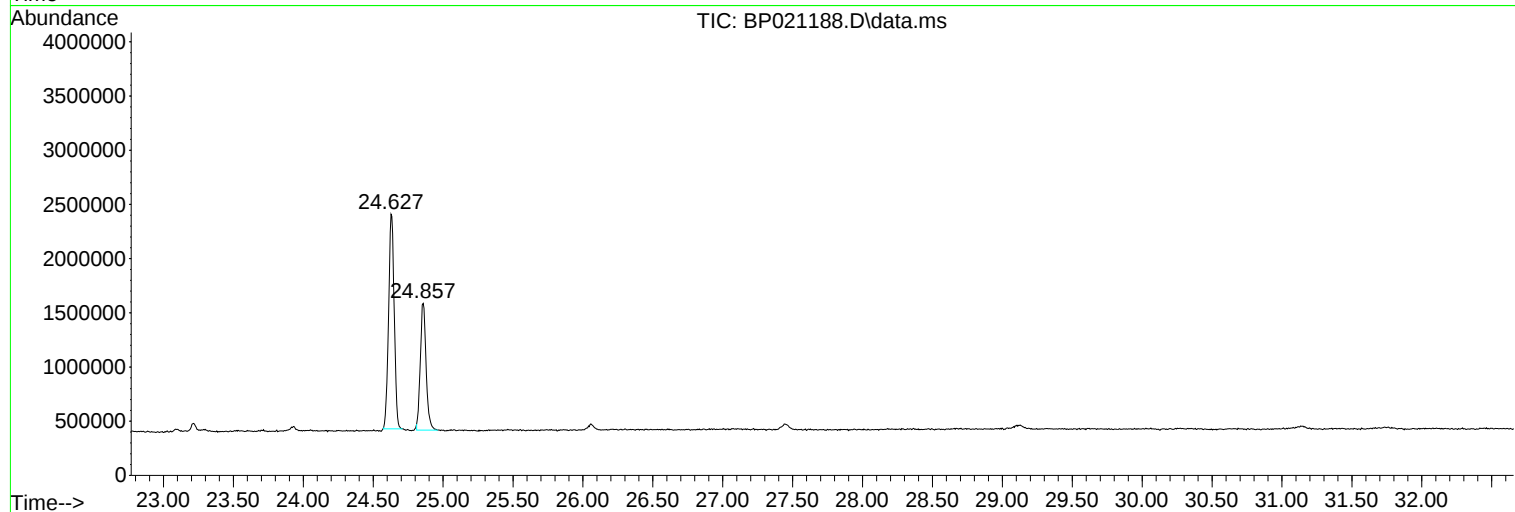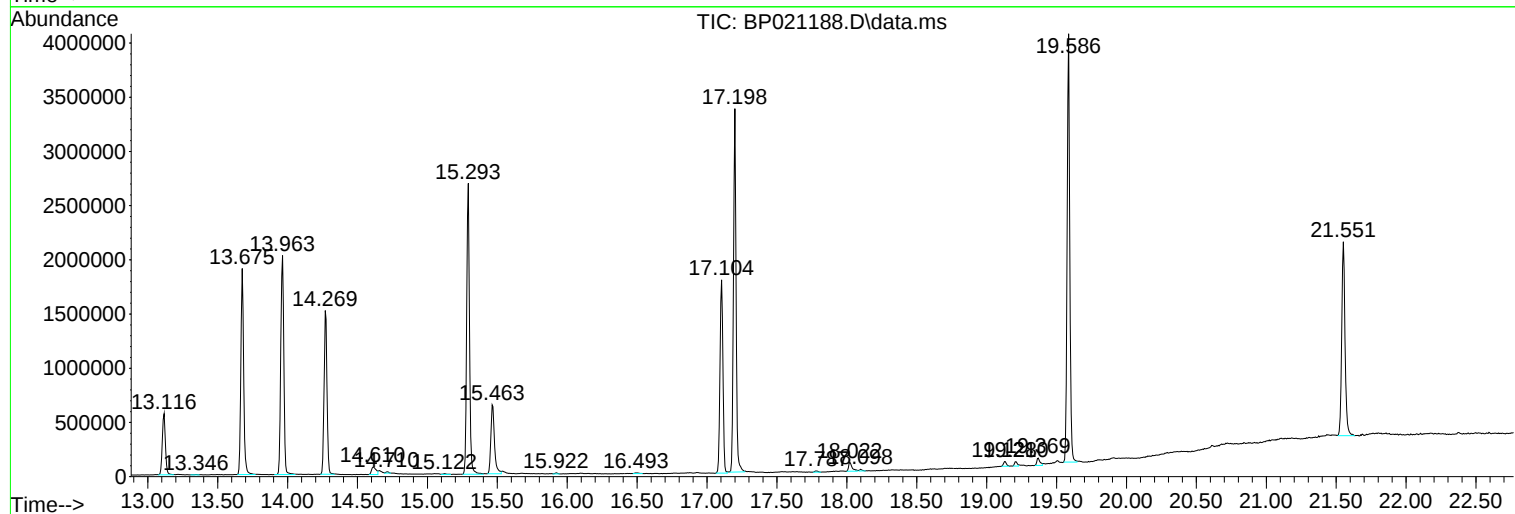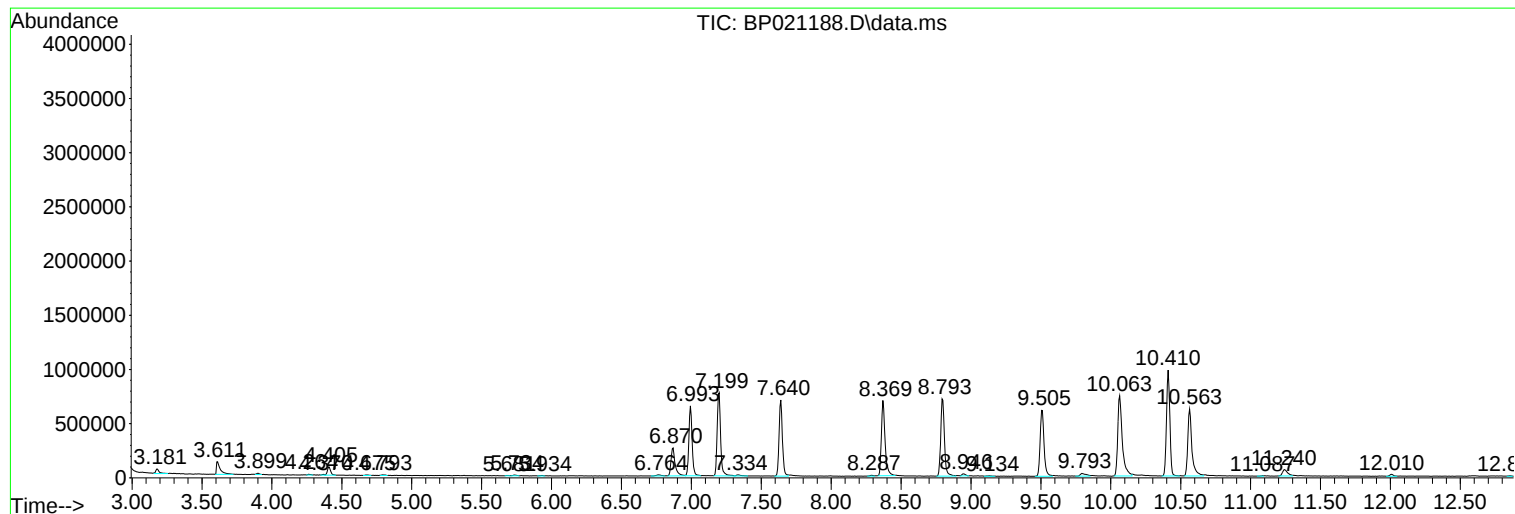

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021188.D
Acq On : 27 Jul 2024 04:21
Operator : MA/JU
Sample : P3348-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08H7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Phenol, 4-(1,1-dimethylprop... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.116	7.87 ng/ul	853420	Acenaphthene-d10	14.269

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, 4-(1,1-dimethylpropyl)-	164	C11H16O	000080-46-6	95
2			Phenol, 4-(1,1-dimethylpropyl)-	164	C11H16O	000080-46-6	94
3			Phenol, p-tert-butyl-	150	C10H14O	000098-54-4	90
4			Phenol, 4-(1,1-dimethylpropyl)-	164	C11H16O	000080-46-6	83
5			Hexestrol	270	C18H22O2	000084-16-2	80

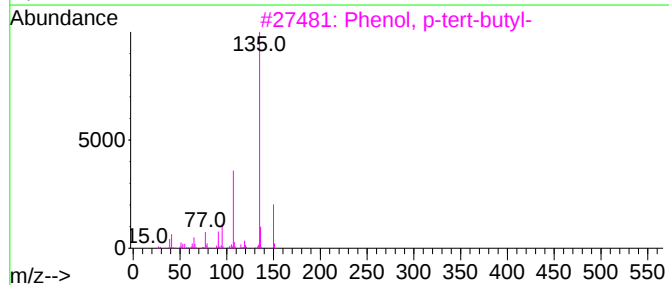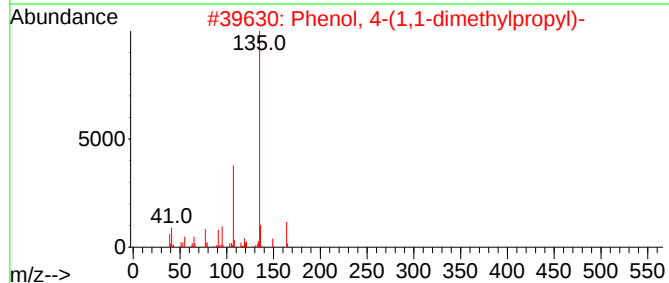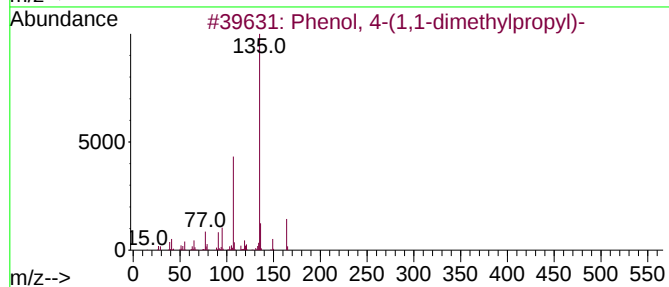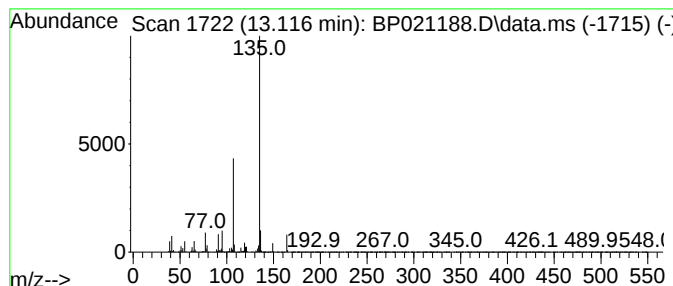

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021188.D
Acq On : 27 Jul 2024 04:21
Operator : MA/JU
Sample : P3348-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08H7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, 4-(1,1-...	13.116	7.9	ng/ul	853420	3	14.269	2170090	20.0