

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021190.D
 Acq On : 27 Jul 2024 05:49
 Operator : MA/JU
 Sample : P3348-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08J2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	40	rVB	35664	53502	1.00%	0.105%
2	3.610	103	106	117	rBV	76446	146305	2.73%	0.288%
3	3.893	151	154	164	rVB	14642	24124	0.45%	0.048%
4	4.269	214	218	221	rBV5	6333	8085	0.15%	0.016%
5	4.363	232	234	236	rBV2	7584	7766	0.15%	0.015%
6	4.410	236	242	251	rVB	455494	715079	13.36%	1.409%
7	4.681	282	288	290	rBV7	5800	7023	0.13%	0.014%
8	5.328	391	398	402	rBV9	3105	6808	0.13%	0.013%
9	5.728	463	466	475	rVB8	5793	12341	0.23%	0.024%
10	5.928	495	500	506	rVB9	4046	7661	0.14%	0.015%
11	6.757	634	641	650	rBV10	4997	16335	0.31%	0.032%
12	6.869	653	660	674	rBV	131571	306193	5.72%	0.603%
13	6.992	674	681	693	rVB	583318	938487	17.53%	1.849%
14	7.198	708	716	736	rBV	621033	1168600	21.83%	2.303%
15	7.334	736	739	748	rVB9	8743	17613	0.33%	0.035%
16	7.640	782	791	801	rBV	763332	1228894	22.96%	2.422%
17	8.304	896	904	908	rBV9	5158	12635	0.24%	0.025%
18	8.375	908	916	933	rVV	504726	910582	17.01%	1.794%
19	8.798	981	988	1007	rBV	669539	1195188	22.33%	2.355%
20	8.951	1009	1014	1020	rVV4	14311	23402	0.44%	0.046%
21	9.510	1099	1109	1124	rBV	557614	1048737	19.59%	2.067%
22	9.804	1153	1159	1171	rBV2	26677	74307	1.39%	0.146%
23	10.069	1195	1204	1224	rBV	739324	1552689	29.01%	3.060%
24	10.416	1255	1263	1276	rBV	965002	1714592	32.04%	3.379%
25	10.569	1281	1289	1307	rBV	528812	1191129	22.26%	2.347%
26	11.116	1371	1382	1383	rBV	3945	7503	0.14%	0.015%
27	11.192	1390	1395	1398	rBV6	5886	11498	0.21%	0.023%
28	11.245	1398	1404	1414	rVV3	57284	144266	2.70%	0.284%
29	11.951	1516	1524	1531	rBV2	14655	28577	0.53%	0.056%
30	12.016	1531	1535	1542	rVB2	12752	25408	0.47%	0.050%
31	12.586	1628	1632	1633	rBV4	5543	5802	0.11%	0.011%
32	13.122	1717	1723	1735	rBV	72571	126747	2.37%	0.250%
33	13.239	1739	1743	1749	rVB8	3265	5748	0.11%	0.011%
34	13.692	1814	1820	1840	rBV	1853868	2476873	46.28%	4.881%
35	13.980	1857	1869	1876	rBV2	1719912	2860901	53.45%	5.638%
36	14.286	1912	1921	1929	rBV	1476196	2348888	43.89%	4.629%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021190.D
 Acq On : 27 Jul 2024 05:49
 Operator : MA/JU
 Sample : P3348-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08J2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	14.616	1971	1977	1994	rBV2	62078	222520	4.16%	0.439%
38	14.727	1994	1996	2001	rVB6	9183	14876	0.28%	0.029%
39	15.057	2045	2052	2055	rBV7	6046	11246	0.21%	0.022%
40	15.139	2061	2066	2068	rBV6	4891	7707	0.14%	0.015%
41	15.298	2085	2093	2109	rBV	2350412	3740520	69.89%	7.371%
42	15.474	2116	2123	2133	rBV	706870	1227161	22.93%	2.418%
43	16.092	2226	2228	2235	rVB8	3468	5770	0.11%	0.011%
44	16.504	2293	2298	2299	rBV5	4361	6349	0.12%	0.013%
45	17.104	2394	2400	2410	rBV	2088753	2848632	53.22%	5.614%
46	17.204	2410	2417	2434	rVV	2673883	4322237	80.76%	8.518%
47	17.792	2513	2517	2522	rBV7	12108	17955	0.34%	0.035%
48	18.039	2553	2559	2568	rBV4	81243	181386	3.39%	0.357%
49	19.133	2741	2745	2751	rBV2	39322	58258	1.09%	0.115%
50	19.221	2756	2760	2763	rBV	38527	54713	1.02%	0.108%
51	19.368	2781	2785	2793	rBV4	51367	95655	1.79%	0.189%
52	19.592	2816	2823	2836	rBV	3347836	5300970	99.04%	10.446%
53	21.551	3150	3156	3165	rBV	1839148	3195867	59.71%	6.298%
54	24.627	3670	3679	3695	rVB	1941109	5352093	100.00%	10.547%
55	24.850	3709	3717	3736	rVB	1170090	3650995	68.22%	7.195%




Sum of corrected areas: 50745198

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021190.D
Acq On : 27 Jul 2024 05:49
Operator : MA/JU
Sample : P3348-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08J2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

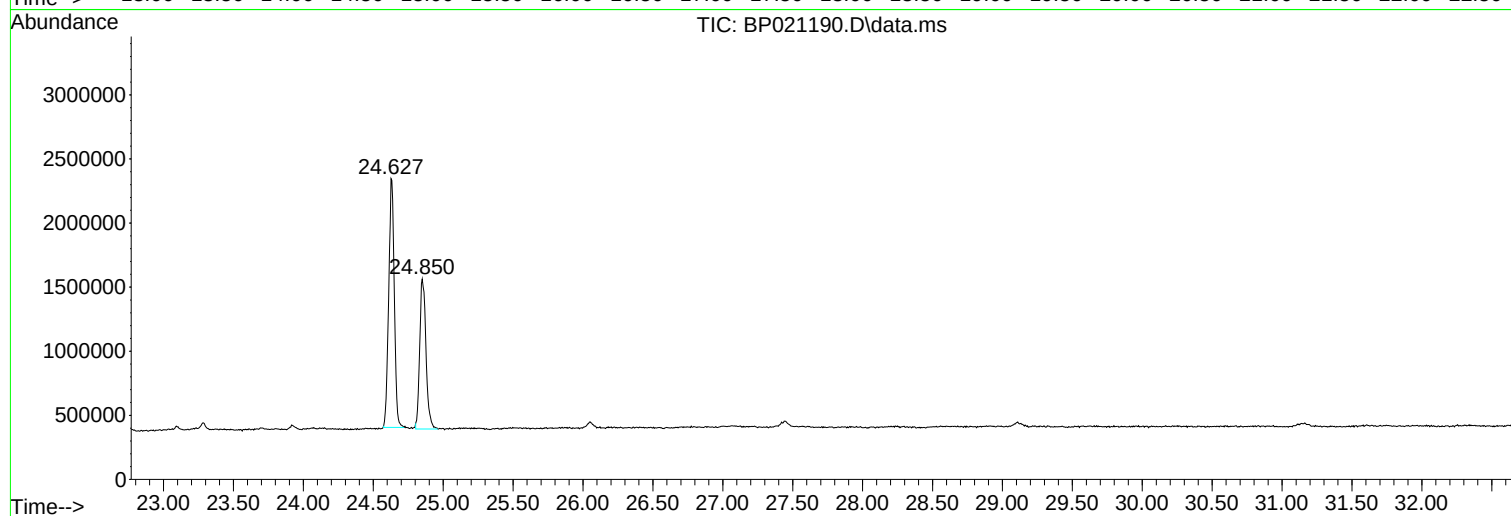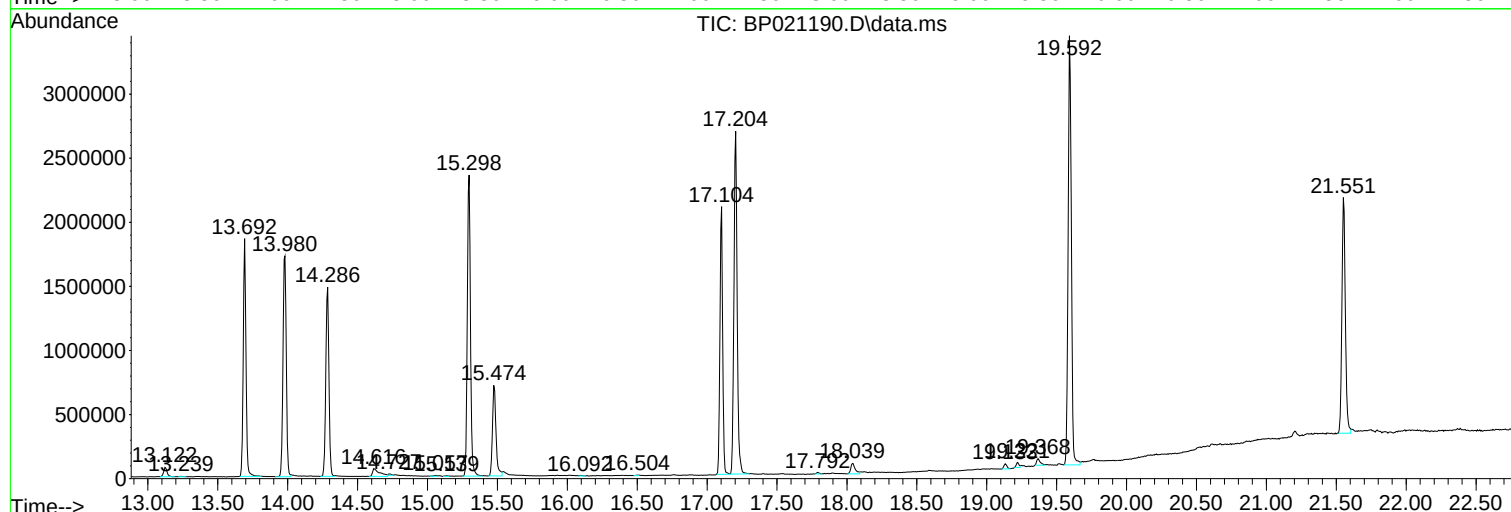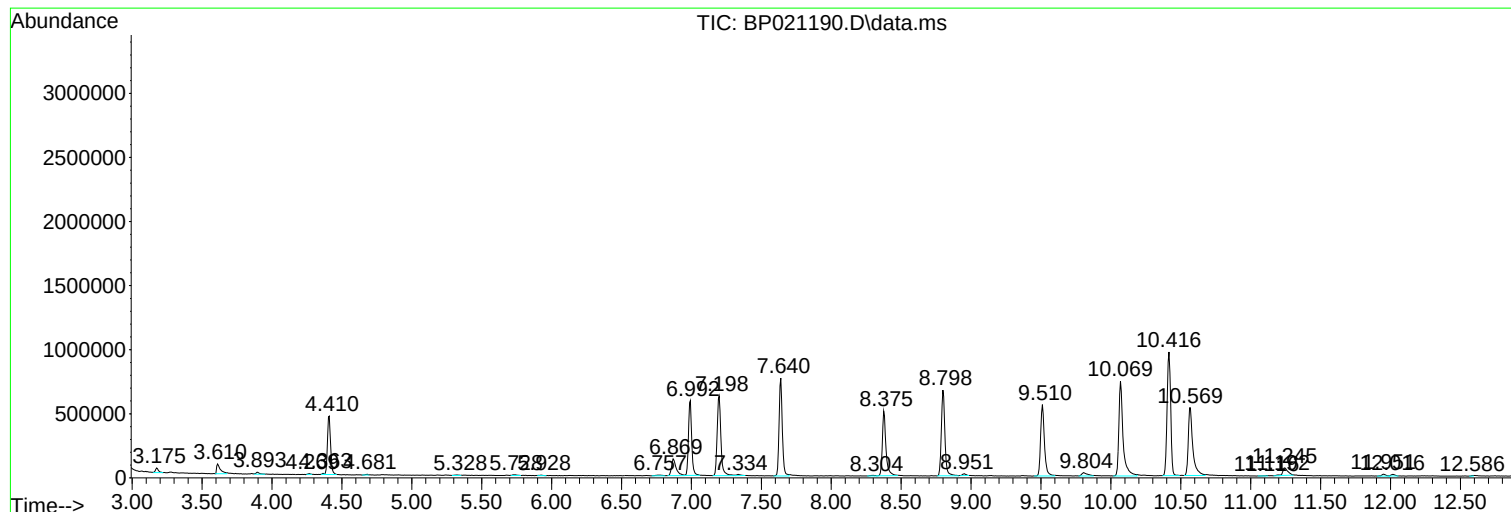

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021190.D
Acq On : 27 Jul 2024 05:49
Operator : MA/JU
Sample : P3348-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08J2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021190.D
Acq On : 27 Jul 2024 05:49
Operator : MA/JU
Sample : P3348-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08J2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------