

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
 Data File : BP021201.D
 Acq On : 27 Jul 2024 14:28
 Operator : MA/JU
 Sample : P3280-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	29	rBV3	13680	18074	0.30%	0.033%
2	3.181	30	33	36	rVV	18452	21902	0.36%	0.040%
3	3.605	102	105	121	rBV	158925	292321	4.82%	0.529%
4	3.893	151	154	163	rVB	28846	46720	0.77%	0.085%
5	4.305	222	224	229	rVB2	6856	8173	0.13%	0.015%
6	4.411	236	242	248	rBV2	29439	52689	0.87%	0.095%
7	4.799	303	308	314	rBV	14904	26147	0.43%	0.047%
8	5.005	339	343	348	rVB3	8578	12848	0.21%	0.023%
9	5.252	381	385	390	rVB7	4252	6913	0.11%	0.013%
10	6.740	631	638	644	rVB2	6873	10833	0.18%	0.020%
11	6.864	652	659	675	rBV	185878	414706	6.84%	0.751%
12	6.993	675	681	700	rVB	638386	1116119	18.41%	2.021%
13	7.187	707	714	735	rBV	755627	1359262	22.42%	2.462%
14	7.640	784	791	806	rBV	739254	1317212	21.73%	2.385%
15	7.987	845	850	858	rBV2	13594	26778	0.44%	0.048%
16	8.369	907	915	937	rBV	563156	1210831	19.97%	2.193%
17	8.799	978	988	1008	rBV	764275	1441536	23.78%	2.611%
18	9.128	1041	1044	1049	rVB6	4651	6872	0.11%	0.012%
19	9.511	1101	1109	1129	rBV	646326	1248195	20.59%	2.260%
20	10.058	1195	1202	1227	rBV	852222	1843439	30.41%	3.338%
21	10.399	1253	1260	1275	rVB	1164158	1802383	29.73%	3.264%
22	10.569	1278	1289	1316	rBV	581492	1541266	25.42%	2.791%
23	11.963	1517	1526	1530	rBV10	4483	10037	0.17%	0.018%
24	12.028	1530	1537	1547	rVB4	9024	27240	0.45%	0.049%
25	13.687	1807	1819	1833	rBV	1653003	2844130	46.91%	5.151%
26	13.781	1833	1835	1840	rVB4	5975	9140	0.15%	0.017%
27	13.963	1858	1866	1882	rBV	2129990	3278035	54.07%	5.936%
28	14.269	1911	1918	1934	rBV	1603677	2454033	40.48%	4.444%
29	14.446	1943	1948	1953	rBV8	4941	10877	0.18%	0.020%
30	14.610	1969	1976	1988	rBV4	58261	224514	3.70%	0.407%
31	15.075	2053	2055	2060	rVB5	5641	6343	0.10%	0.011%
32	15.287	2084	2091	2105	rBV	2480007	4127123	68.08%	7.474%
33	15.381	2105	2107	2114	rVB8	11315	18249	0.30%	0.033%
34	15.463	2114	2121	2143	rBV	815362	1458820	24.06%	2.642%
35	15.775	2170	2174	2179	rVB2	7299	10291	0.17%	0.019%
36	17.092	2392	2398	2409	rBV	2014491	2990300	49.32%	5.415%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021201.D
Acq On : 27 Jul 2024 14:28
Operator : MA/JU
Sample : P3280-11
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZH8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	17.198	2409	2416	2432	rVV	2690651	4640309	76.54%	8.403%
38	17.781	2513	2515	2519	rBV5	7938	10177	0.17%	0.018%
39	18.034	2553	2558	2564	rBV	94046	146038	2.41%	0.264%
40	19.134	2741	2745	2750	rVB2	43940	60354	1.00%	0.109%
41	19.216	2755	2759	2762	rBV	41436	59363	0.98%	0.108%
42	19.357	2780	2783	2795	rBV5	71816	142363	2.35%	0.258%
43	19.586	2816	2822	2835	rBV	3768528	5705020	94.10%	10.331%
44	21.551	3150	3156	3165	rBV2	1918589	3305546	54.52%	5.986%
45	24.621	3669	3678	3694	rVB	2156367	6062566	100.00%	10.979%
46	24.857	3709	3718	3735	rVB	1238442	3794331	62.59%	6.871%




Sum of corrected areas: 55220418

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021201.D
Acq On : 27 Jul 2024 14:28
Operator : MA/JU
Sample : P3280-11
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

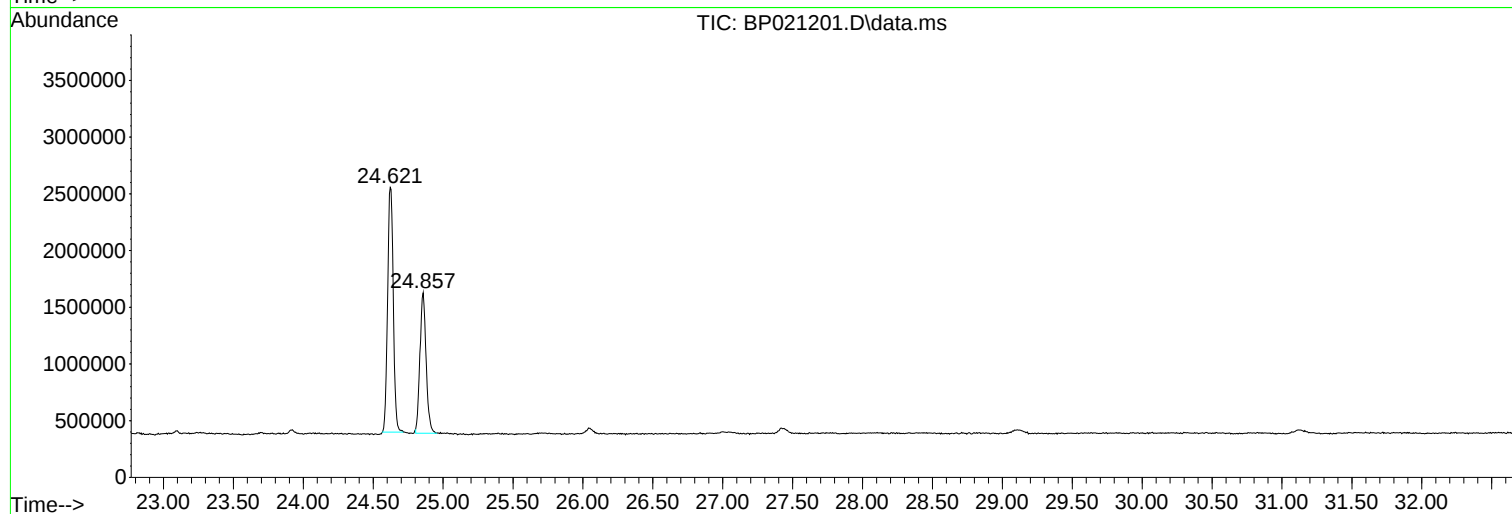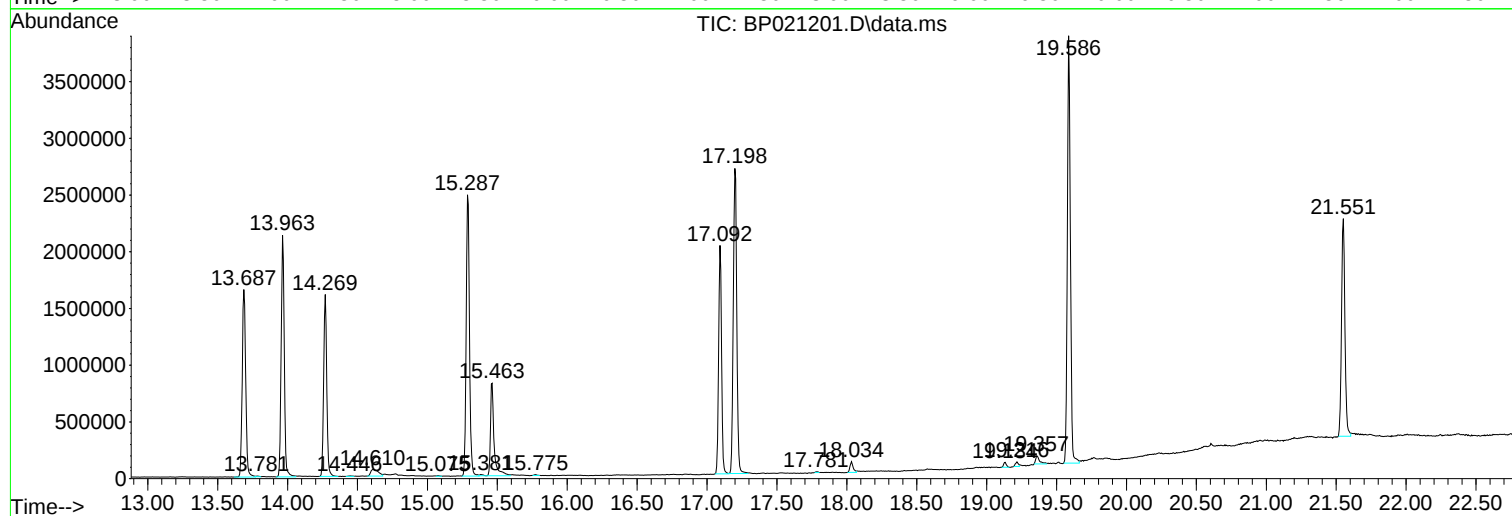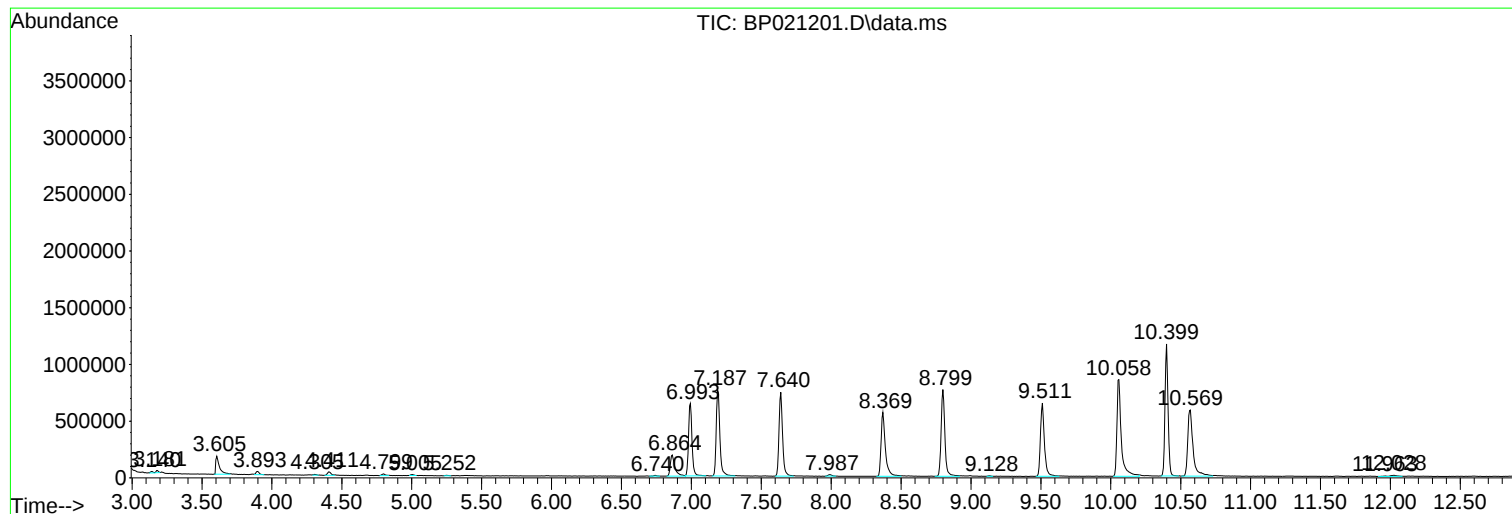

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021201.D
Acq On : 27 Jul 2024 14:28
Operator : MA/JU
Sample : P3280-11
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072624\
Data File : BP021201.D
Acq On : 27 Jul 2024 14:28
Operator : MA/JU
Sample : P3280-11
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------