


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP072721\
Data File : BP006361.D
Acq On : 27 Jul 2021 12:36
Operator : CG/JU
Sample : M3063-02DL 25X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Manual Integrations
APPROVED

mohammad
7/28/2021 11:33:46 AM

Quant Time: Jul 27 13:39:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 04:29:12 2021
Response via : Initial Calibration

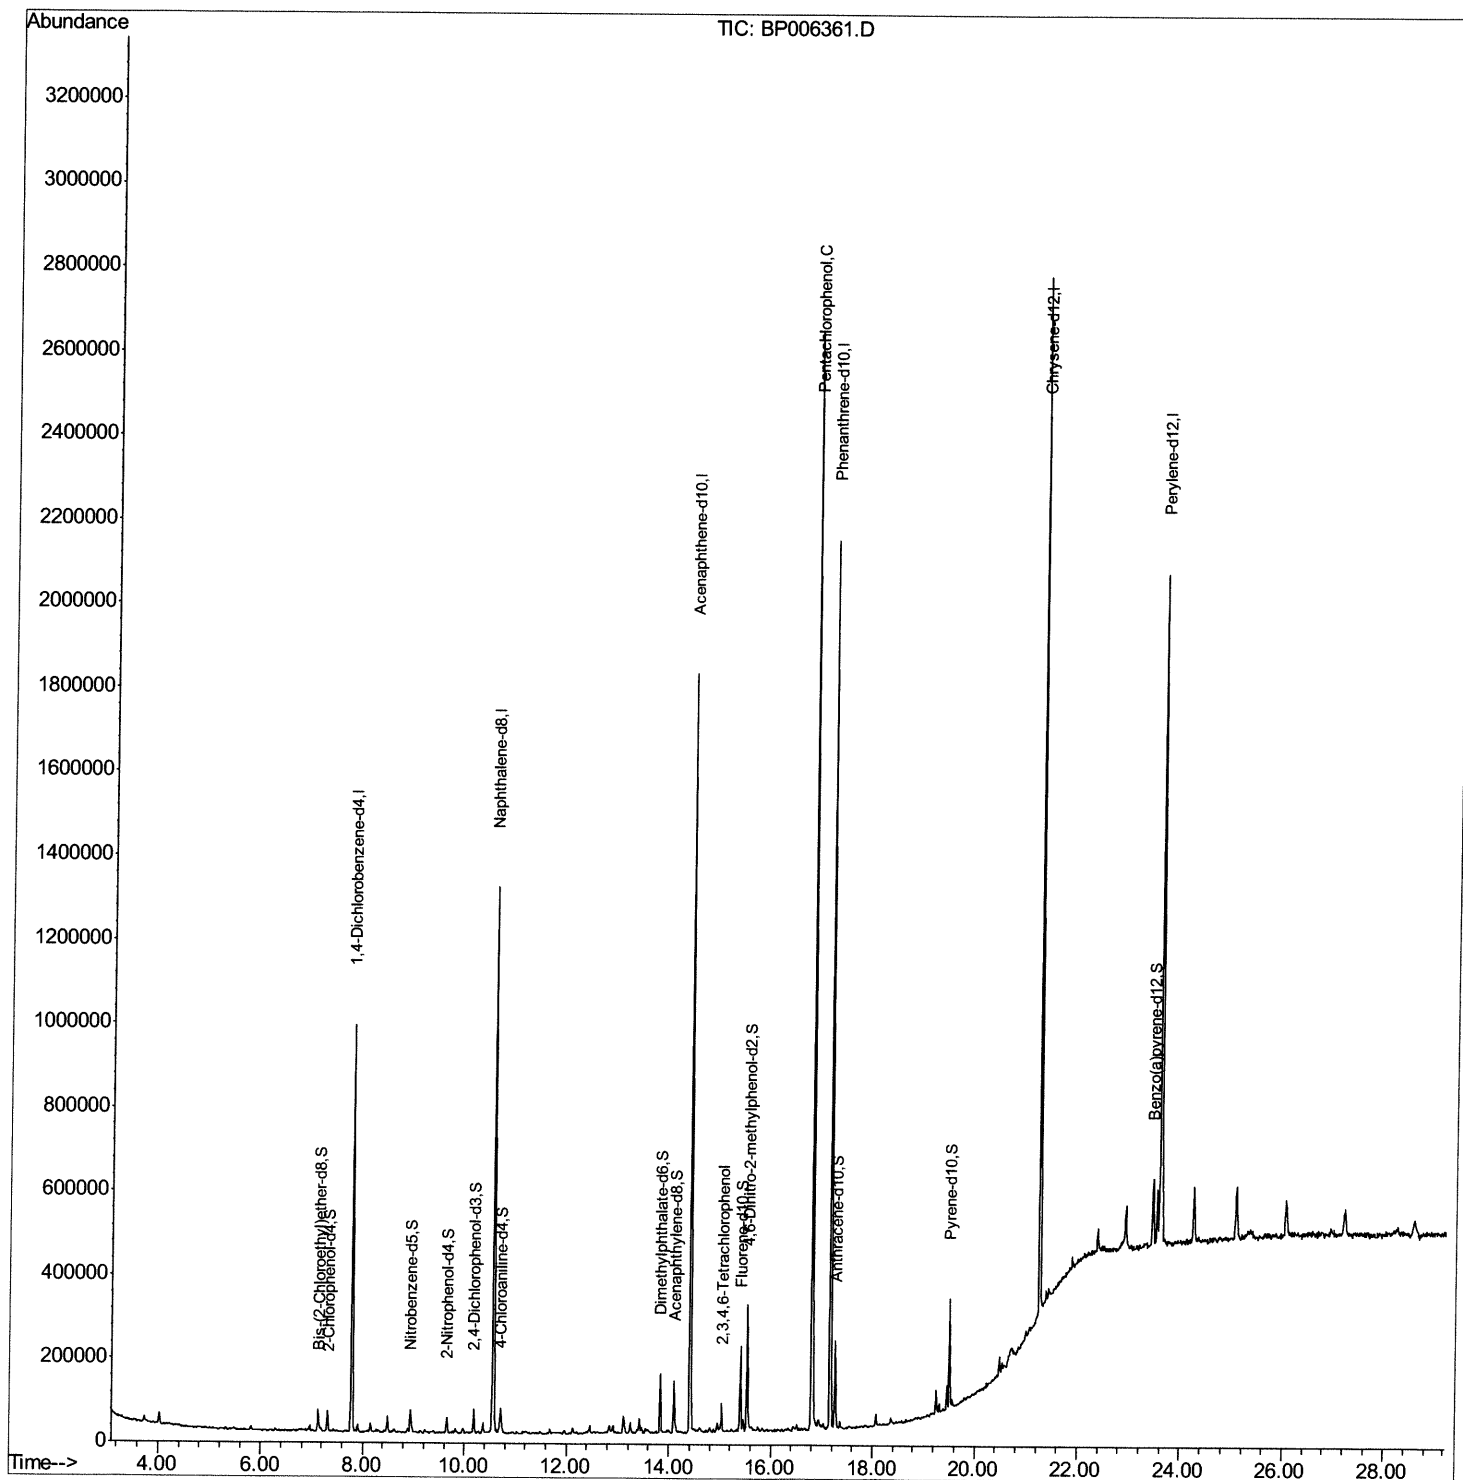

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP072721\
 Data File : BP006361.D
 Acq On : 27 Jul 2021 12:36
 Operator : CG/JU
 Sample : M3063-02DL 25X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 C0AT9DL

Manual Integrations
APPROVED

mohammad
 7/28/2021 11:33:46 AM

Quant Time: Jul 27 13:34:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration

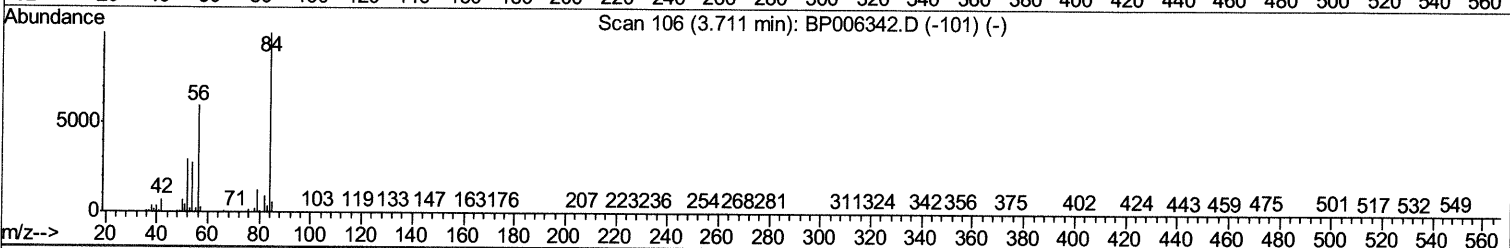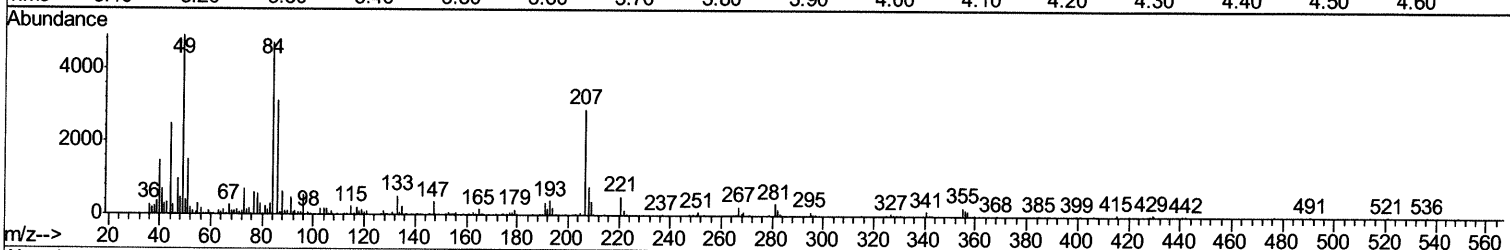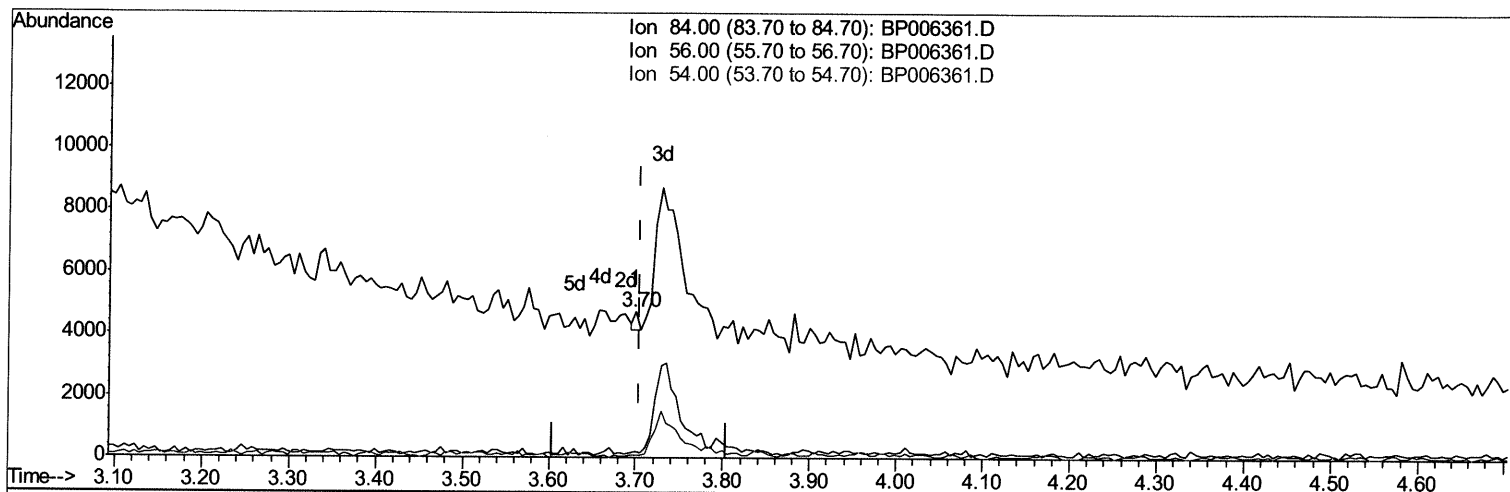

TIC: BP006361.D

(4) Pyridine-d5 (S)

3.699min (-0.006) 0.01ng/ul

response 209

Ion	Exp%	Act%
84.00	100	100
56.00	58.30	3.93#
54.00	26.70	1.53#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP072721\
 Data File : BP006361.D
 Acq On : 27 Jul 2021 12:36
 Operator : CG/JU
 Sample : M3063-02DL 25X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:33:46 AM

Quant Time: Jul 27 13:34:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration

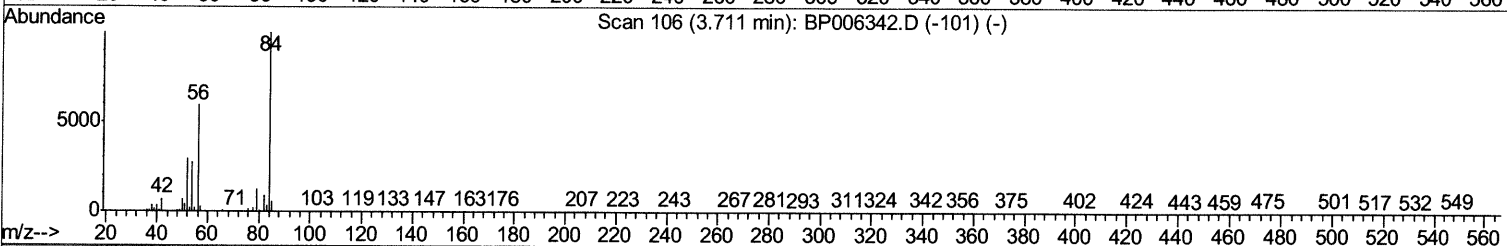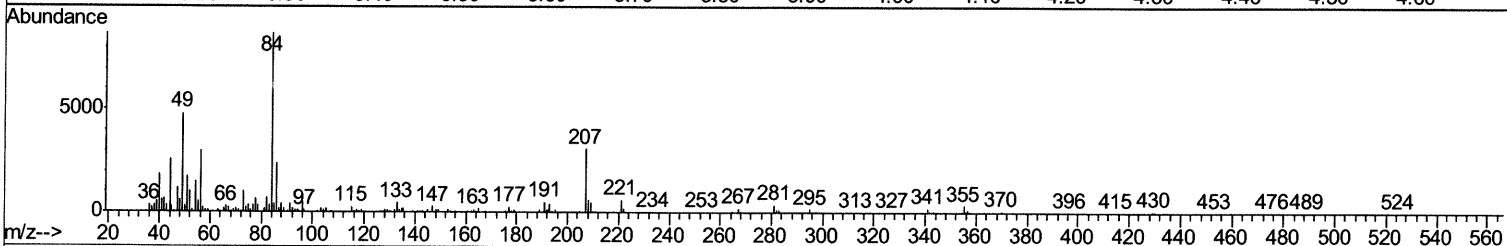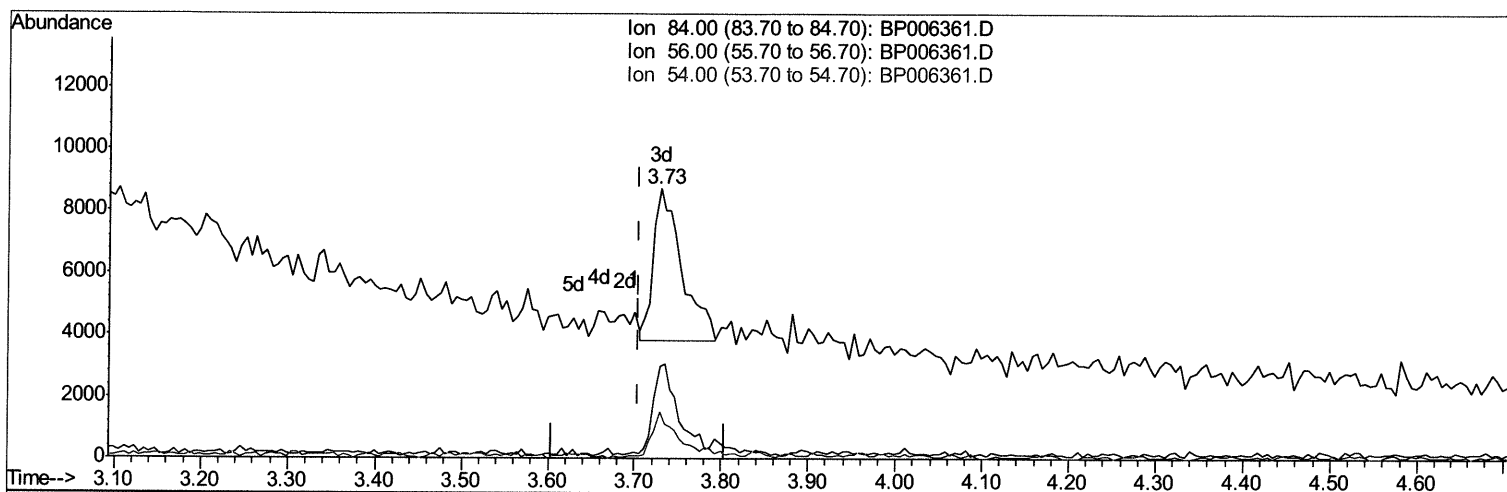

TIC: BP006361.D

(4) Pyridine-d5 (S)

3.728min (+0.024) 0.59ng/ul m 07/29/21 JU

response 11253

Ion	Exp%	Act%
84.00	100	100
56.00	58.30	34.03#
54.00	26.70	17.39#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
 Data File : BP006361.D
 Acq On : 27 Jul 2021 12:36
 Operator : CG/JU
 Sample : M3063-02DL 25X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Manual Integrations
 APPROVED

mohammad
 7/28/2021 11:33:46 AM

Quant Time: Jul 27 13:39:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	240206	20.00	ng/ul	0.00
20) Naphthalene-d8	10.57	136	1002866	20.00	ng/ul	-0.01
38) Acenaphthene-d10	14.41	164	565562	20.00	ng/ul	-0.01
64) Phenanthrene-d10	17.16	188	1121218	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	1041778	20.00	ng/ul	0.00
88) Perylene-d12	23.61	264	1072556	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	1805	0.28	ng/uL	0.01
4) Pyridine-d5	3.73	84	11253m	0.59	ng/ul	> 0.02
7) Phenol-d5	6.96	99	7468	0.33	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.13	67	23648	1.68	ng/ul	0.00
11) 2-Chlorophenol-d4	7.32	132	20833	1.24	ng/ul	-0.01
15) 4-Methylphenol-d8	8.49	113	14335	0.81	ng/ul	-0.01
21) Nitrobenzene-d5	8.95	128	11971	1.60	ng/ul	0.00
24) 2-Nitrophenol-d4	9.66	143	10676	1.50	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.19	165	19684	1.41	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.71	131	33064	1.44	ng/ul	0.00
46) Dimethylphthalate-d6	13.83	166	84777	2.11	ng/ul	-0.01
49) Acenaphthylene-d8	14.10	160	84409	1.71	ng/ul	0.00
54) 4-Nitrophenol-d4	14.61	143	2211	0.28	ng/ul	0.00
60) Fluorene-d10	15.40	176	69783	2.06	ng/ul	-0.01
65) 4,6-Dinitro-2-methylphenol	15.54	200	24980	4.00	ng/ul	0.00
73) Anthracene-d10	17.26	188	108374	2.14	ng/ul	0.00
81) Pyrene-d10	19.50	212	121097	2.26	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.46	264	106047	1.95	ng/ul	0.00

Target Compounds

						Ovalue
58) 2,3,4,6-Tetrachlorophenol	15.04	232	10594	1.315	ng/ul	93
71) Pentachlorophenol	16.81	266	355588	46.971	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed