

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
 Data File : BP006361.D
 Acq On : 27 Jul 2021 12:36
 Operator : CG/JU
 Sample : M3063-02DL 25X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006361.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.728	107	109	117	rBV3	12517	17542	0.49%	0.075%
2	4.028	155	160	164	rVB	26272	39074	1.09%	0.167%
3	5.816	459	464	467	rBV2	8533	12647	0.35%	0.054%
4	6.287	539	544	553	rBV10	5431	11267	0.32%	0.048%
5	6.963	652	659	662	rVV2	13183	24746	0.69%	0.106%
6	7.128	682	687	693	rBV	53057	89982	2.52%	0.385%
7	7.181	693	696	703	rVB4	9709	16291	0.46%	0.070%
8	7.281	709	713	714	rBV4	4622	5382	0.15%	0.023%
9	7.316	714	719	726	rVB	49175	78469	2.20%	0.336%
10	7.434	735	739	743	rBV5	4795	7092	0.20%	0.030%
11	7.693	781	783	788	rVB6	4283	5131	0.14%	0.022%
12	7.787	791	799	806	rVV	972819	1511623	42.35%	6.471%
13	7.863	809	812	814	rVV3	4261	5157	0.14%	0.022%
14	7.899	814	818	823	rVB	18574	27530	0.77%	0.118%
15	8.093	847	851	856	rVV8	3798	6854	0.19%	0.029%
16	8.158	856	862	868	rVB2	23111	37472	1.05%	0.160%
17	8.281	878	883	885	rBV5	6194	9487	0.27%	0.041%
18	8.322	888	890	895	rVB6	3878	5516	0.15%	0.024%
19	8.428	903	908	911	rBV7	5741	10315	0.29%	0.044%
20	8.487	913	918	927	rVB	39664	65915	1.85%	0.282%
21	8.581	931	934	937	rBV5	5137	7030	0.20%	0.030%
22	8.628	937	942	945	rVB5	6926	12023	0.34%	0.051%
23	8.887	980	986	990	rVV5	9544	16991	0.48%	0.073%
24	8.940	990	995	1007	rVB2	54814	115234	3.23%	0.493%
25	9.228	1038	1044	1048	rBV9	6833	12056	0.34%	0.052%
26	9.405	1070	1074	1078	rVB5	4349	6244	0.17%	0.027%
27	9.657	1109	1117	1125	rBV2	37974	68610	1.92%	0.294%
28	9.769	1132	1136	1139	rBV5	5139	7745	0.22%	0.033%
29	9.822	1141	1145	1150	rVB4	8528	13911	0.39%	0.060%
30	9.969	1163	1170	1176	rBV5	13046	27836	0.78%	0.119%
31	10.187	1202	1207	1217	rVB	56576	98713	2.77%	0.423%
32	10.369	1231	1238	1246	rBV	27364	50132	1.40%	0.215%
33	10.499	1255	1260	1262	rVV6	4505	7562	0.21%	0.032%
34	10.569	1264	1272	1279	rVV	1302075	2132138	59.73%	9.127%
35	10.634	1279	1283	1288	rVV7	6573	11906	0.33%	0.051%
36	10.710	1288	1296	1307	rVB2	60710	141735	3.97%	0.607%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
 Data File : BP006361.D
 Acq On : 27 Jul 2021 12:36
 Operator : CG/JU
 Sample : M3063-02DL 25X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	11.034	1348	1351	1358	rVB9	5088	11069	0.31%	0.047%
38	11.151	1368	1371	1373	rBV3	5254	5571	0.16%	0.024%
39	11.228	1380	1384	1389	rVB8	5620	9084	0.25%	0.039%
40	11.487	1423	1428	1430	rBV6	3598	5928	0.17%	0.025%
41	11.681	1455	1461	1467	rVB5	11380	20353	0.57%	0.087%
42	11.969	1503	1510	1516	rVB5	8394	19883	0.56%	0.085%
43	12.128	1530	1537	1541	rBV2	14526	26086	0.73%	0.112%
44	12.204	1546	1550	1555	rVB8	4732	7957	0.22%	0.034%
45	12.451	1584	1592	1597	rVB4	17975	33474	0.94%	0.143%
46	12.598	1614	1617	1623	rVB8	4256	6783	0.19%	0.029%
47	12.840	1652	1658	1664	rVV6	19422	38689	1.08%	0.166%
48	12.910	1666	1670	1675	rVV4	18003	28119	0.79%	0.120%
49	12.951	1675	1677	1680	rVB4	4231	5077	0.14%	0.022%
50	13.116	1699	1705	1712	rBV3	40732	83540	2.34%	0.358%
51	13.245	1720	1727	1735	rBV	26485	42121	1.18%	0.180%
52	13.381	1745	1750	1753	rBV7	8527	15778	0.44%	0.068%
53	13.422	1753	1757	1762	rVV	34106	54110	1.52%	0.232%
54	13.469	1762	1765	1771	rVB2	16204	24486	0.69%	0.105%
55	13.545	1774	1778	1782	rBV5	12606	20008	0.56%	0.086%
56	13.587	1782	1785	1788	rVB5	5917	7122	0.20%	0.030%
57	13.745	1806	1812	1813	rVV6	3845	5692	0.16%	0.024%
58	13.828	1821	1826	1833	rVV	139310	200390	5.61%	0.858%
59	13.963	1847	1849	1852	rVB4	6057	5130	0.14%	0.022%
60	14.004	1852	1856	1863	rVB10	7511	14898	0.42%	0.064%
61	14.104	1863	1873	1878	rBV	126041	208852	5.85%	0.894%
62	14.181	1884	1886	1893	rBV7	4678	6363	0.18%	0.027%
63	14.410	1913	1925	1933	rBV	1810280	2668091	74.74%	11.421%
64	14.587	1951	1955	1956	rVV4	6921	8451	0.24%	0.036%
65	14.604	1956	1958	1971	rVB10	12870	27256	0.76%	0.117%
66	14.740	1975	1981	1984	rBV8	4830	8918	0.25%	0.038%
67	14.810	1989	1993	1996	rBV4	8772	12291	0.34%	0.053%
68	14.881	2001	2005	2010	rVB7	7969	11646	0.33%	0.050%
69	14.951	2010	2017	2021	rBV6	23333	40849	1.14%	0.175%
70	14.992	2021	2024	2027	rVV4	9017	12912	0.36%	0.055%
71	15.034	2027	2031	2037	rVB	67112	96854	2.71%	0.415%
72	15.234	2061	2065	2073	rBV	5996	14663	0.41%	0.063%
73	15.404	2088	2094	2099	rBV	203176	288208	8.07%	1.234%
74	15.457	2099	2103	2109	rVB	29095	45331	1.27%	0.194%
75	15.539	2109	2117	2124	rBV	302750	487101	13.65%	2.085%
76	15.622	2128	2131	2137	rVB6	9153	14524	0.41%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
 Data File : BP006361.D
 Acq On : 27 Jul 2021 12:36
 Operator : CG/JU
 Sample : M3063-02DL 25X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

77	15.757	2150	2154	2160	rVB9	9732	18096	0.51%	0.077%
78	15.834	2160	2167	2169	rBV8	7088	12560	0.35%	0.054%
79	16.087	2208	2210	2214	rBV5	4059	5943	0.17%	0.025%
80	16.151	2216	2221	2223	rVV6	4685	6784	0.19%	0.029%
81	16.228	2231	2234	2237	rVB5	4409	5530	0.15%	0.024%
82	16.445	2267	2271	2277	rBV7	10478	22459	0.63%	0.096%
83	16.516	2279	2283	2288	rVB4	12747	18702	0.52%	0.080%
84	16.616	2298	2300	2304	rVB5	7280	9334	0.26%	0.040%
85	16.675	2307	2310	2315	rVB7	4621	7260	0.20%	0.031%
86	16.810	2326	2333	2347	rBV	2615469	3569704	100.00%	15.280%
87	16.934	2350	2354	2359	rVV3	14668	33123	0.93%	0.142%
88	17.034	2369	2371	2376	rVB6	13329	17366	0.49%	0.074%
89	17.163	2387	2393	2404	rVV	2114754	3010519	84.34%	12.887%
90	17.263	2404	2410	2419	rVV	207537	314826	8.82%	1.348%
91	17.363	2423	2427	2431	rBV6	15079	21321	0.60%	0.091%
92	18.069	2543	2547	2553	rBV6	25776	35660	1.00%	0.153%
93	18.369	2594	2598	2602	rBV3	15847	23840	0.67%	0.102%
94	19.251	2745	2748	2754	rBV	53457	62888	1.76%	0.269%
95	19.310	2755	2758	2763	rVB4	20413	25312	0.71%	0.108%
96	19.457	2780	2783	2786	rBV	54527	53327	1.49%	0.228%
97	19.504	2786	2791	2798	rVV	258057	344875	9.66%	1.476%
98	20.480	2954	2957	2962	rBV4	42872	56493	1.58%	0.242%
99	21.263	3085	3090	3095	rBV	2461804	3122125	87.46%	13.364%
100	23.610	3482	3489	3498	rVB2	1588462	3202309	89.71%	13.708%




Sum of corrected areas: 23361372

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
Data File : BP006361.D
Acq On : 27 Jul 2021 12:36
Operator : CG/JU
Sample : M3063-02DL 25X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

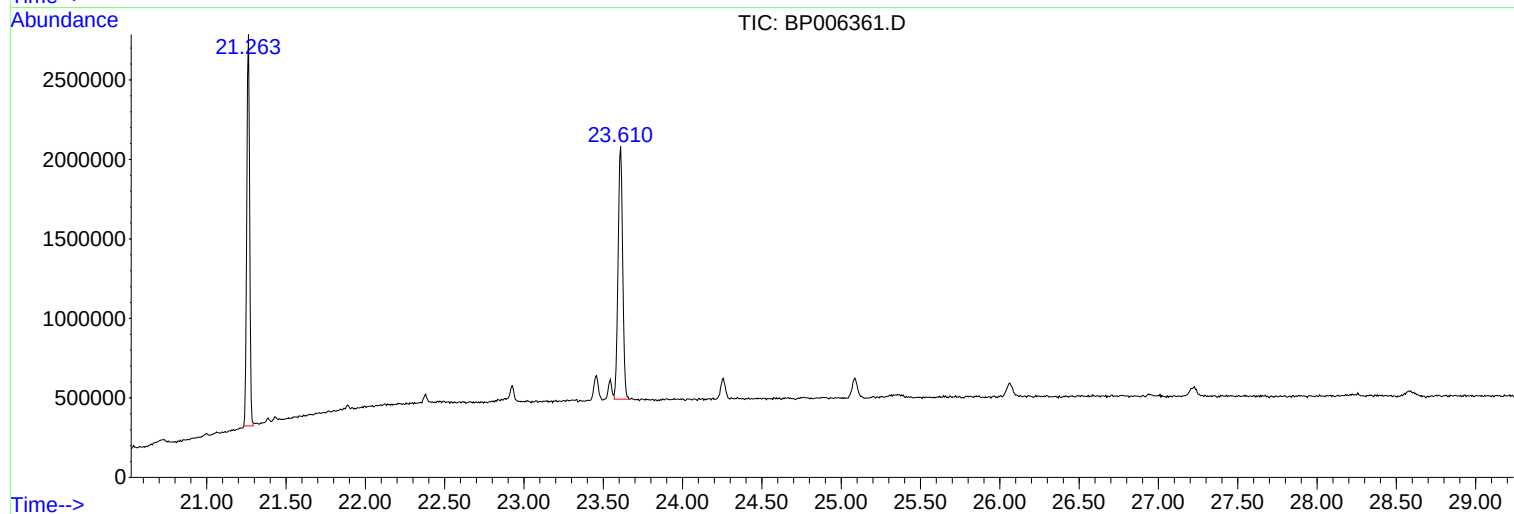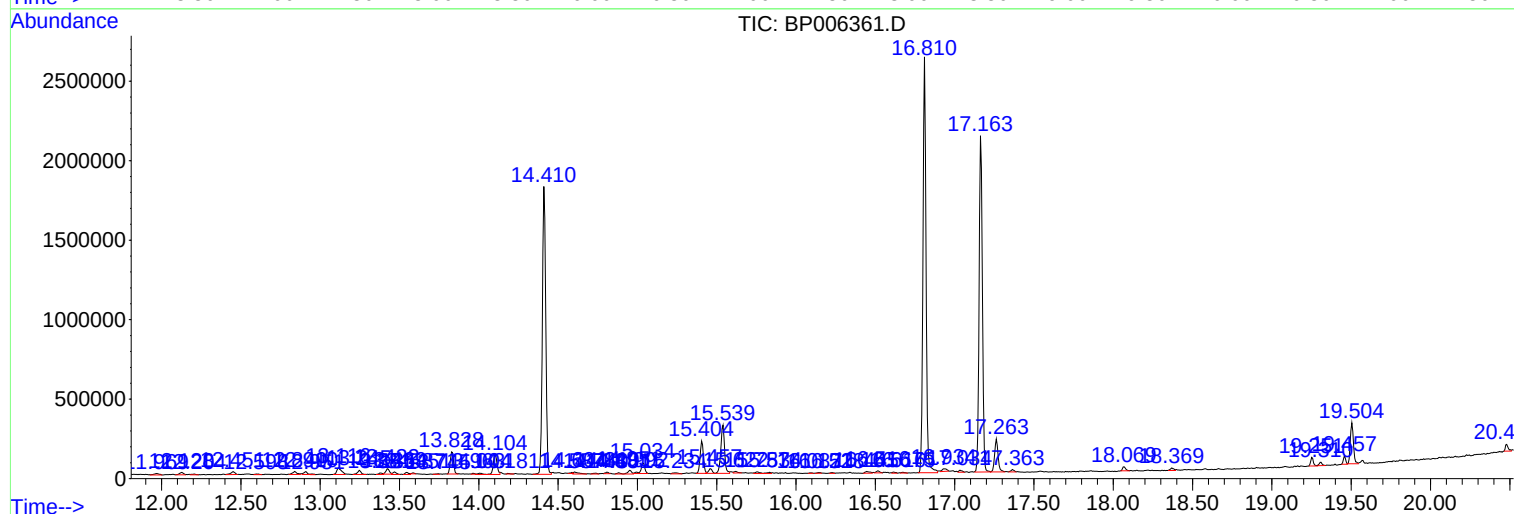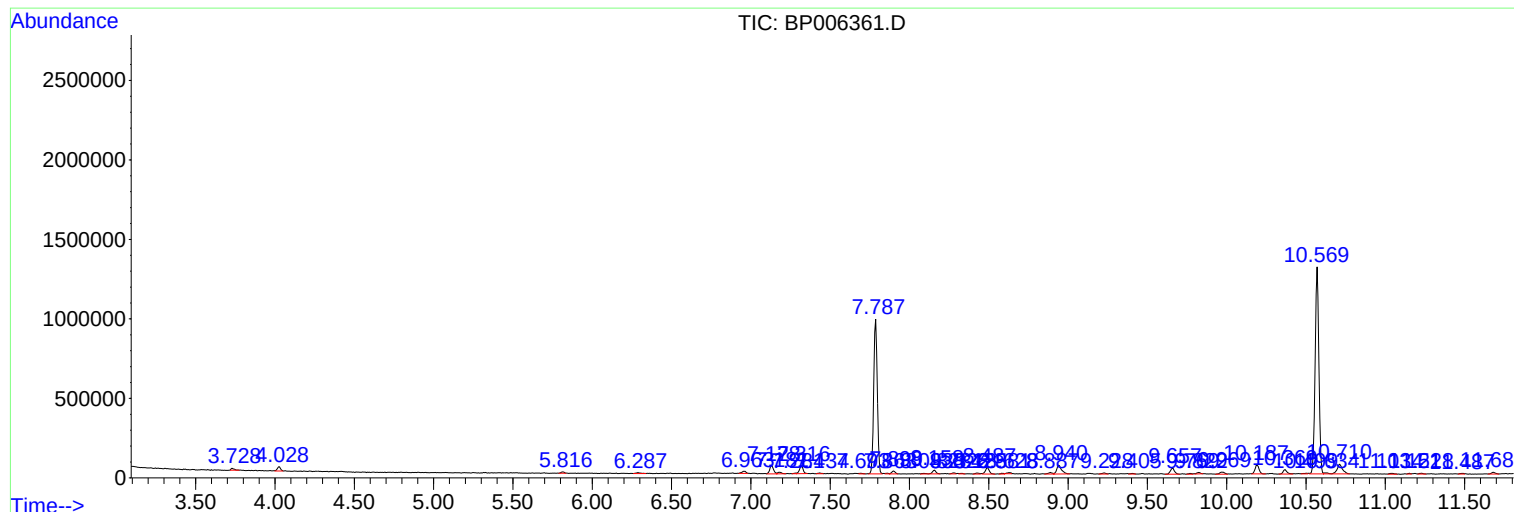

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
Data File : BP006361.D
Acq On : 27 Jul 2021 12:36
Operator : CG/JU
Sample : M3063-02DL 25X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
Data File : BP006361.D
Acq On : 27 Jul 2021 12:36
Operator : CG/JU
Sample : M3063-02DL 25X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
