

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
 Data File : BP006363.D
 Acq On : 27 Jul 2021 14:06
 Operator : CG/JU
 Sample : M3084-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0031

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006363.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	49	rVB	40826	66340	1.78%	0.148%
2	3.711	102	106	116	rBV	113227	183159	4.90%	0.409%
3	3.928	139	143	148	rVB3	11504	17902	0.48%	0.040%
4	4.016	155	158	167	rVB	17470	28399	0.76%	0.063%
5	4.240	191	196	200	rBV5	8482	14016	0.38%	0.031%
6	5.569	417	422	432	rBV	93245	152705	4.09%	0.341%
7	5.899	474	478	484	rVB5	5505	10208	0.27%	0.023%
8	6.475	573	576	581	rVB7	5917	9596	0.26%	0.021%
9	6.740	616	621	624	rBV6	8362	14102	0.38%	0.032%
10	6.775	624	627	632	rVB6	8722	13417	0.36%	0.030%
11	6.952	651	657	671	rVB	559991	906987	24.29%	2.027%
12	7.128	677	687	698	rVB	474152	756169	20.25%	1.690%
13	7.316	712	719	726	rBV	600351	925307	24.78%	2.068%
14	7.416	732	736	739	rBV4	9749	13829	0.37%	0.031%
15	7.687	776	782	789	rVB4	16497	27584	0.74%	0.062%
16	7.787	790	799	806	rVV	1020524	1634289	43.76%	3.652%
17	7.916	819	821	828	rVB6	5570	9153	0.25%	0.020%
18	8.010	830	837	842	rBV6	7430	13019	0.35%	0.029%
19	8.487	912	918	926	rBV	700921	1091450	29.22%	2.439%
20	8.610	932	939	945	rVB4	9239	19984	0.54%	0.045%
21	8.940	987	995	1002	rBV	536762	872521	23.36%	1.950%
22	9.010	1002	1007	1011	rVV8	4164	8760	0.23%	0.020%
23	9.369	1064	1068	1072	rVB6	5964	10014	0.27%	0.022%
24	9.657	1110	1117	1128	rBV	390746	652252	17.46%	1.458%
25	9.881	1150	1155	1161	rVB10	6676	12446	0.33%	0.028%
26	10.187	1201	1207	1219	rBV	636215	1059284	28.36%	2.367%
27	10.363	1228	1237	1247	rBV	138948	240587	6.44%	0.538%
28	10.569	1264	1272	1279	rBV	1472584	2459742	65.86%	5.497%
29	10.622	1279	1281	1287	rVB	12719	14643	0.39%	0.033%
30	10.710	1287	1296	1313	rBV	612191	1035766	27.73%	2.315%
31	11.363	1400	1407	1412	rBV9	8217	15880	0.43%	0.035%
32	12.010	1511	1517	1521	rVB8	5807	8454	0.23%	0.019%
33	12.075	1524	1528	1532	rBV5	5777	9047	0.24%	0.020%
34	12.157	1535	1542	1548	rVB3	13753	23328	0.62%	0.052%
35	12.234	1548	1555	1560	rBV2	8452	14014	0.38%	0.031%
36	12.451	1587	1592	1598	rVB4	7851	14043	0.38%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
 Data File : BP006363.D
 Acq On : 27 Jul 2021 14:06
 Operator : CG/JU
 Sample : M3084-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0031

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	12.781	1640	1648	1653	rVV7	10834	18159	0.49%	0.041%
38	13.028	1685	1690	1695	rVB3	11663	19051	0.51%	0.043%
39	13.151	1707	1711	1715	rBV6	9984	15270	0.41%	0.034%
40	13.251	1721	1728	1732	rBV7	11694	15750	0.42%	0.035%

41	13.322	1732	1740	1747	rVV	66023	122569	3.28%	0.274%
42	13.386	1747	1751	1756	rVB8	4901	9463	0.25%	0.021%
43	13.575	1779	1783	1785	rVV4	5745	8589	0.23%	0.019%
44	13.628	1789	1792	1797	rVB7	6542	11037	0.30%	0.025%
45	13.739	1806	1811	1814	rVB6	8881	13545	0.36%	0.030%

46	13.834	1820	1827	1836	rVV	1210206	1671883	44.77%	3.736%
47	13.904	1837	1839	1845	rVV7	5540	10274	0.28%	0.023%
48	13.969	1845	1850	1854	rVB8	5868	11753	0.31%	0.026%
49	14.104	1863	1873	1885	rBV	1318156	1915650	51.29%	4.281%
50	14.322	1907	1910	1915	rBV4	11978	16582	0.44%	0.037%

51	14.410	1917	1925	1933	rBV	2170726	3132744	83.88%	7.001%
52	14.475	1933	1936	1945	rVB9	12503	27153	0.73%	0.061%
53	14.610	1951	1959	1972	rBV	458028	700732	18.76%	1.566%
54	14.775	1983	1987	1989	rVV5	6205	10863	0.29%	0.024%
55	14.810	1989	1993	1996	rVV2	20214	33096	0.89%	0.074%

56	14.839	1996	1998	2003	rVB5	14865	17947	0.48%	0.040%
57	14.886	2003	2006	2011	rBV7	5770	8622	0.23%	0.019%
58	15.228	2062	2064	2070	rVB5	6685	11438	0.31%	0.026%
59	15.281	2070	2073	2080	rVB4	12522	18004	0.48%	0.040%
60	15.404	2088	2094	2101	rBV	1682971	2449506	65.59%	5.474%

61	15.457	2101	2103	2108	rVB3	15538	20876	0.56%	0.047%
62	15.522	2108	2114	2123	rBV	392057	548823	14.70%	1.227%
63	15.645	2131	2135	2141	rBV3	20294	31436	0.84%	0.070%
64	15.751	2150	2153	2159	rBV4	7949	10504	0.28%	0.023%
65	15.904	2176	2179	2187	rVB6	10673	20943	0.56%	0.047%

66	15.969	2187	2190	2193	rBV5	8245	11139	0.30%	0.025%
67	16.145	2216	2220	2226	rBV6	14695	20347	0.54%	0.045%
68	16.204	2226	2230	2235	rVB6	14130	17763	0.48%	0.040%
69	16.316	2245	2249	2254	rVB8	10189	17987	0.48%	0.040%
70	16.410	2259	2265	2266	rBV5	6276	10125	0.27%	0.023%

71	16.575	2290	2293	2297	rVB6	7414	10862	0.29%	0.024%
72	16.822	2330	2335	2337	rBV3	13041	18891	0.51%	0.042%
73	16.904	2344	2349	2352	rBV7	12817	22397	0.60%	0.050%
74	16.945	2353	2356	2360	rVV4	29090	44345	1.19%	0.099%
75	16.980	2360	2362	2369	rVB7	13369	23454	0.63%	0.052%

76	17.075	2375	2378	2381	rBV5	8586	11818	0.32%	0.026%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
 Data File : BP006363.D
 Acq On : 27 Jul 2021 14:06
 Operator : CG/JU
 Sample : M3084-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0031

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

77	17.163	2386	2393	2398	rBV	2493275	3567363	95.52%	7.972%
78	17.204	2398	2400	2404	rVV	154255	198017	5.30%	0.443%
79	17.263	2404	2410	2424	rVB	1846731	2602936	69.70%	5.817%
80	17.569	2458	2462	2468	rVB	19867	30055	0.80%	0.067%
81	17.686	2480	2482	2485	rVB4	10752	9443	0.25%	0.021%
82	17.857	2507	2511	2516	rVB	63046	80851	2.16%	0.181%
83	18.016	2535	2538	2539	rBV3	14300	15956	0.43%	0.036%
84	18.069	2543	2547	2555	rVB2	182364	259826	6.96%	0.581%
85	18.222	2570	2573	2577	rBV4	22981	31164	0.83%	0.070%
86	18.257	2577	2579	2583	rVB4	15418	18398	0.49%	0.041%
87	18.339	2590	2593	2603	rBV9	34041	78623	2.11%	0.176%
88	18.527	2622	2625	2627	rBV	16866	16854	0.45%	0.038%
89	18.921	2690	2692	2697	rVB4	27907	31179	0.83%	0.070%
90	18.992	2697	2704	2713	rVB2	181651	274551	7.35%	0.614%
91	19.127	2724	2727	2729	rBV	55429	67481	1.81%	0.151%
92	19.180	2732	2736	2741	rVB	180544	256210	6.86%	0.573%
93	19.310	2755	2758	2763	rBV2	83893	95351	2.55%	0.213%
94	19.504	2786	2791	2800	rBV	2179338	3183904	85.25%	7.115%
95	20.021	2877	2879	2882	rBV3	37220	29474	0.79%	0.066%
96	20.057	2883	2885	2889	rVV2	42684	42454	1.14%	0.095%
97	20.992	3041	3044	3049	rBV2	346047	437479	11.71%	0.978%
98	21.263	3085	3090	3095	rBV	2853998	3734677	100.00%	8.346%
99	23.457	3458	3463	3472	rVB2	1365645	2620217	70.16%	5.856%
100	23.609	3483	3489	3500	rVB2	1765120	3594308	96.24%	8.033%


Sum of corrected areas: 44746557

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
Data File : BP006363.D
Acq On : 27 Jul 2021 14:06
Operator : CG/JU
Sample : M3084-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0031

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

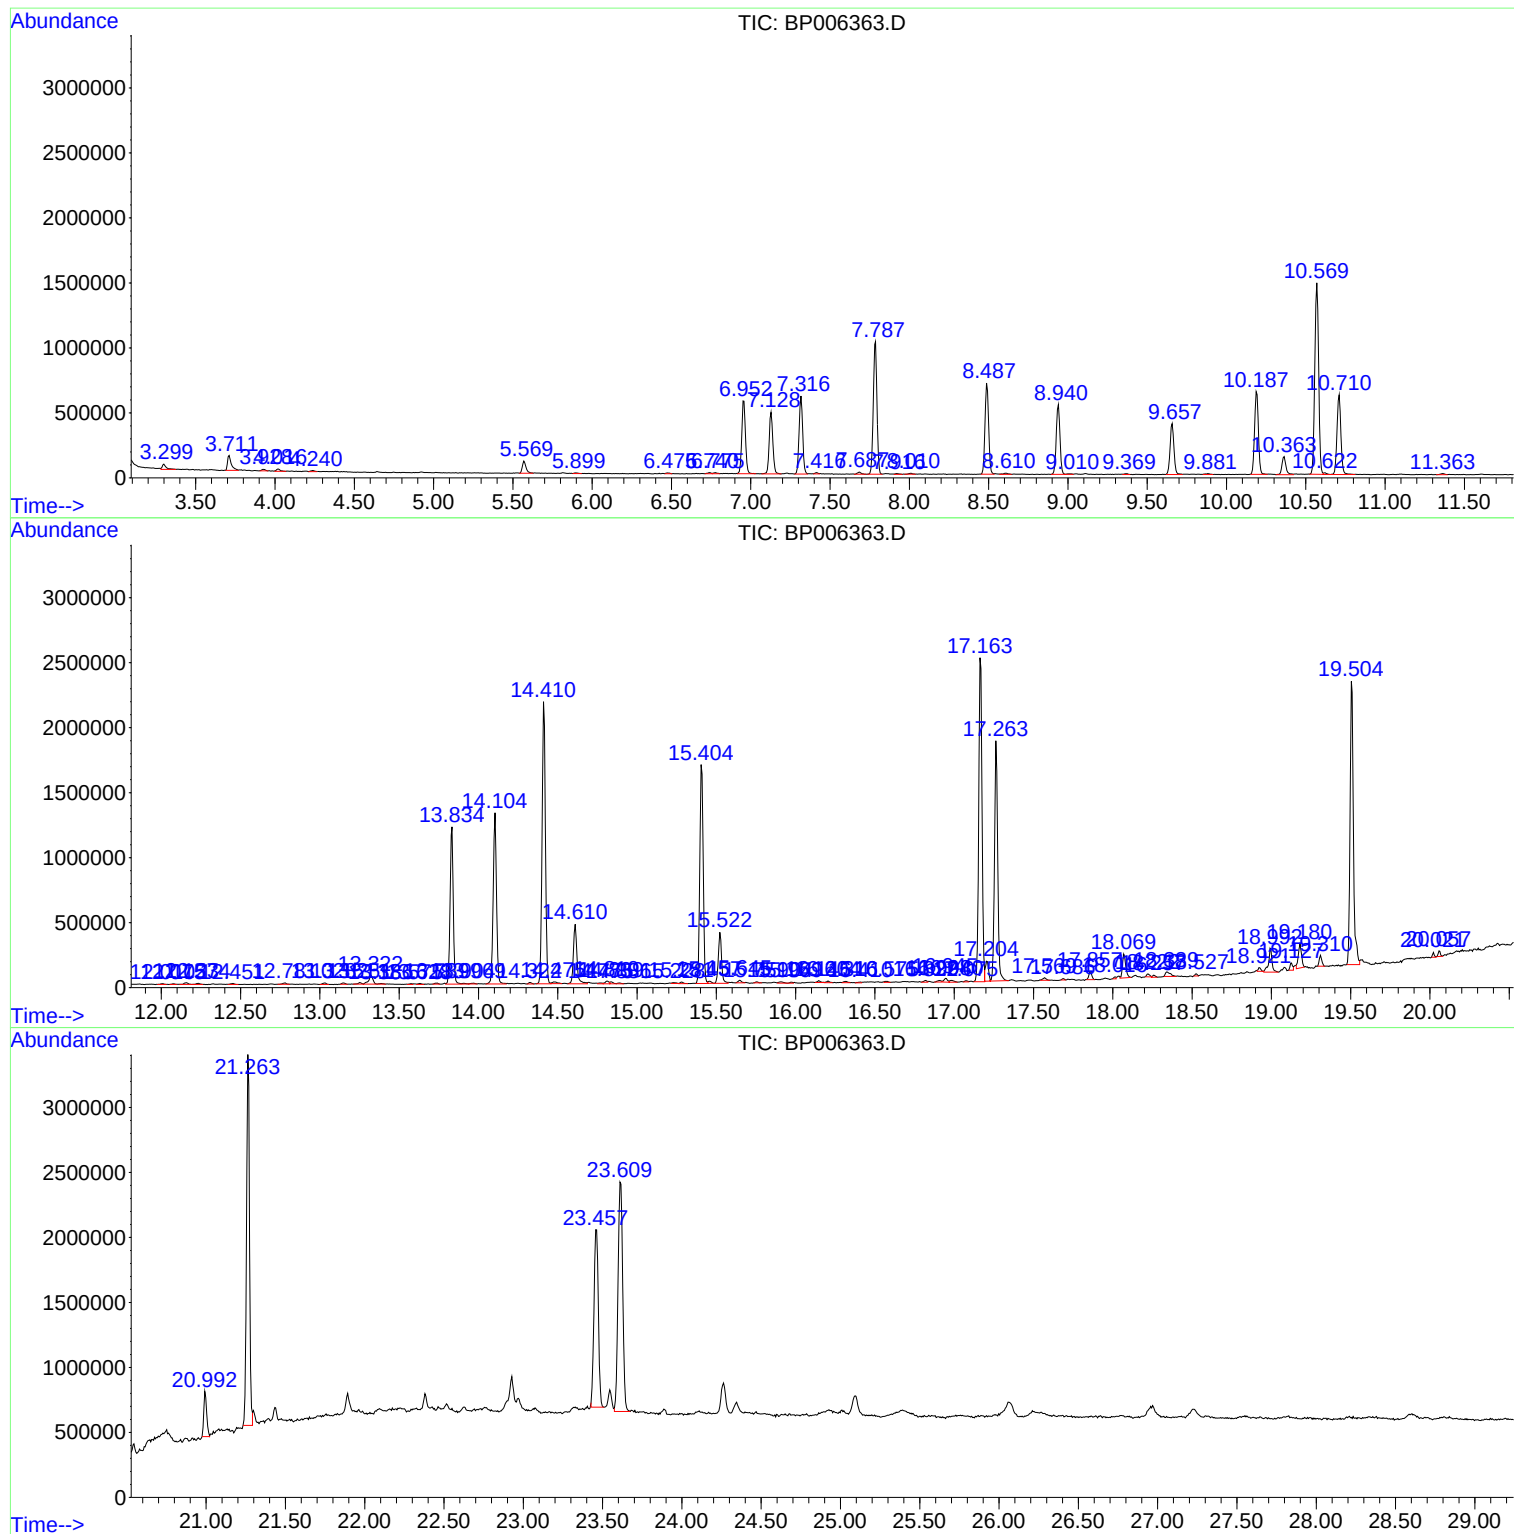

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
Data File : BP006363.D
Acq On : 27 Jul 2021 14:06
Operator : CG/JU
Sample : M3084-13
Misc :
ALS Vial : 9 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0031

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
20.990	2.34 ng/ul	437479	Chrysene-d12		21.262	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	9-Tricosene, (Z)-		322	C23H46	027519-02-4	97
2	17-Pentatriacontene		491	C35H70	006971-40-0	94
3	Pentadecafluorooctanoic acid, oc...		666	C26H37F15O2	1000406-04-8	93
4	Dichloroacetic acid, heptadecyl ...		366	C19H36Cl2O2	1000282-98-2	91
5	17-Pentatriacontene		491	C35H70	006971-40-0	91

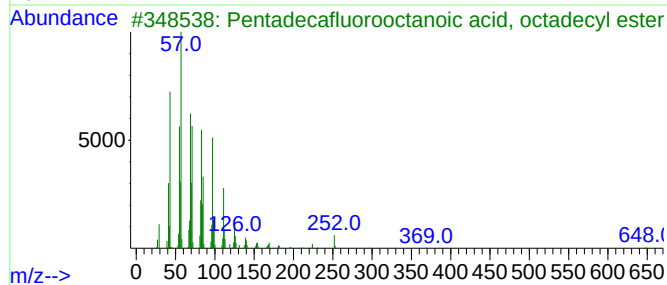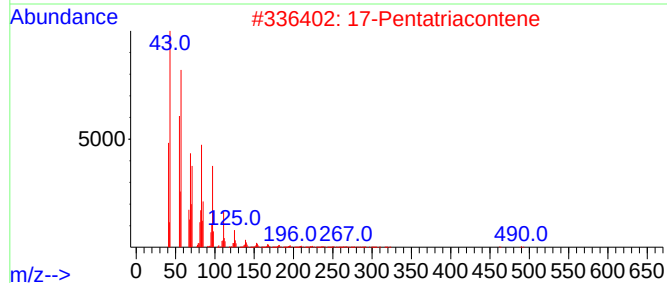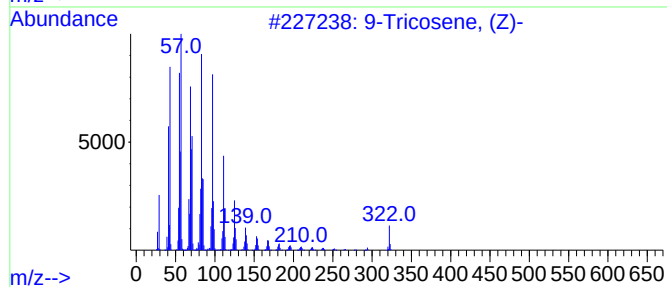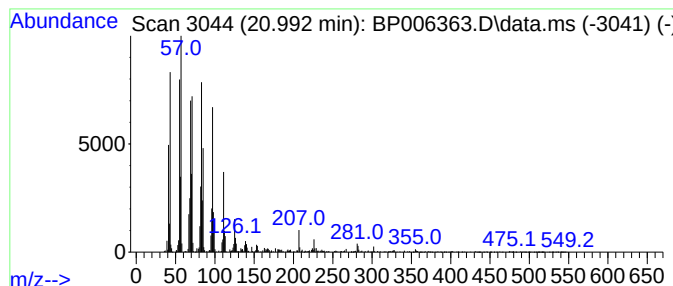

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072721\
Data File : BP006363.D
Acq On : 27 Jul 2021 14:06
Operator : CG/JU
Sample : M3084-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0031

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.990	2.3	ng/u1	437479	5	21.262	3734680	20.0