




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011129.D
Acq On : 27 Jul 2022 14:47
Operator : CG/JU
Sample : N3871-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ06

Manual IntegrationsAPPROVED

Quant Time: Jul 28 00:02:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 14:31:36 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/28/2022
Supervised By :mohammad ahmed 07/28/2022

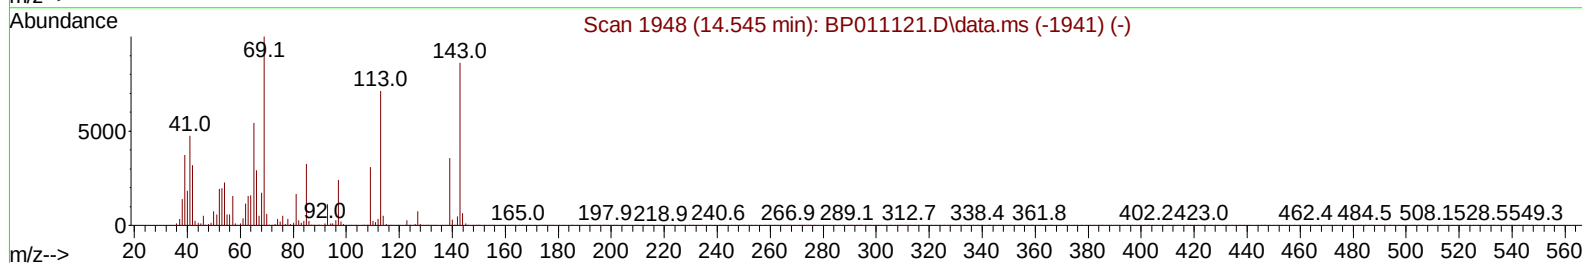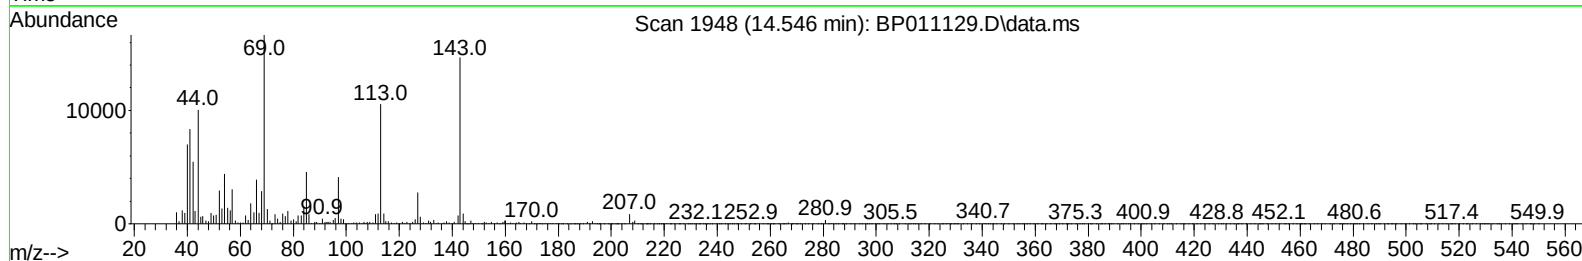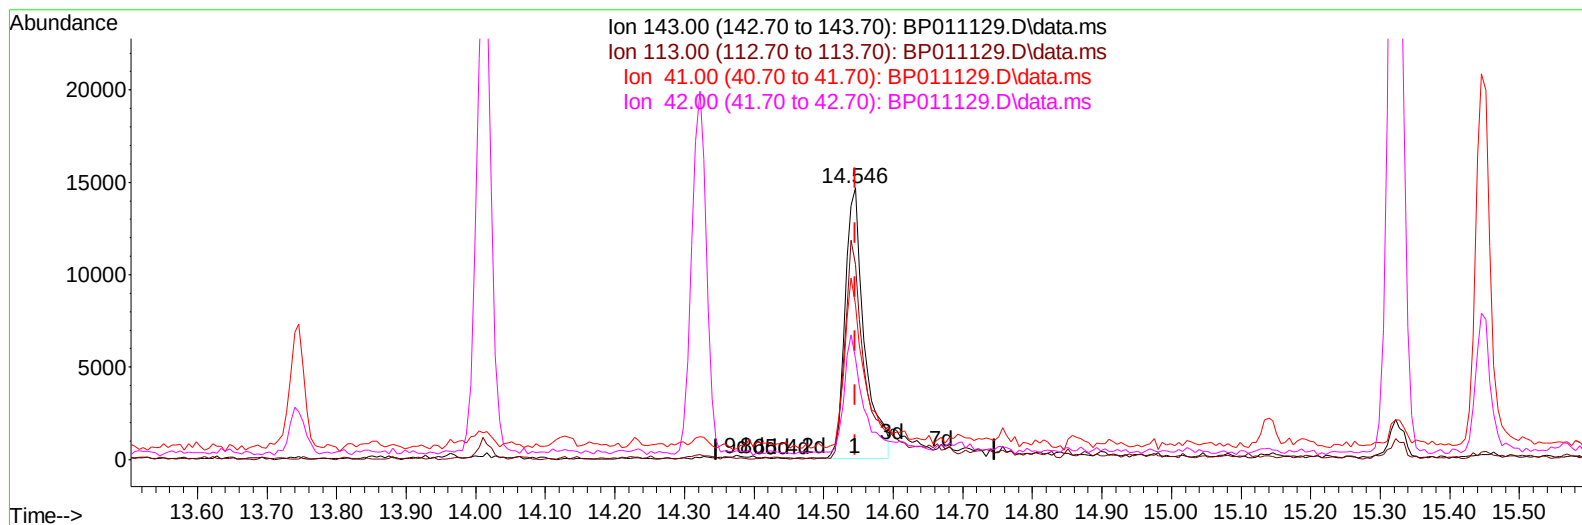

TIC: BP011129.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.546min (+ 0.000) 3.10 ng/ul

response 28233

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	71.75#
41.00	59.00	56.97
42.00	41.10	37.24




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011129.D
 Acq On : 27 Jul 2022 14:47
 Operator : CG/JU
 Sample : N3871-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ06

Manual IntegrationsAPPROVED

Quant Time: Jul 28 00:02:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 14:31:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/28/2022
 Supervised By :mohammad ahmed 07/28/2022

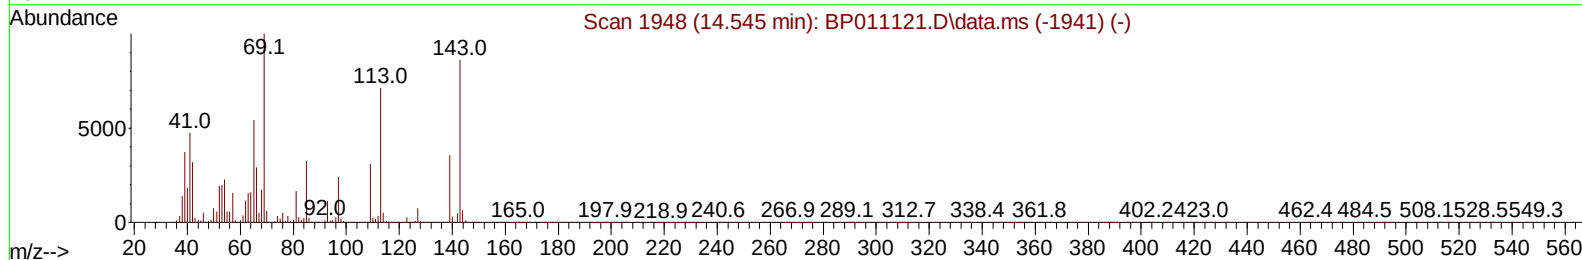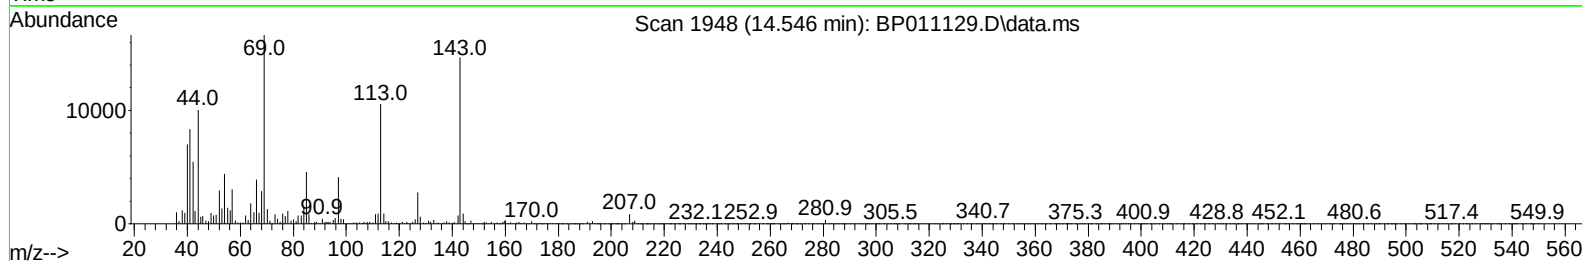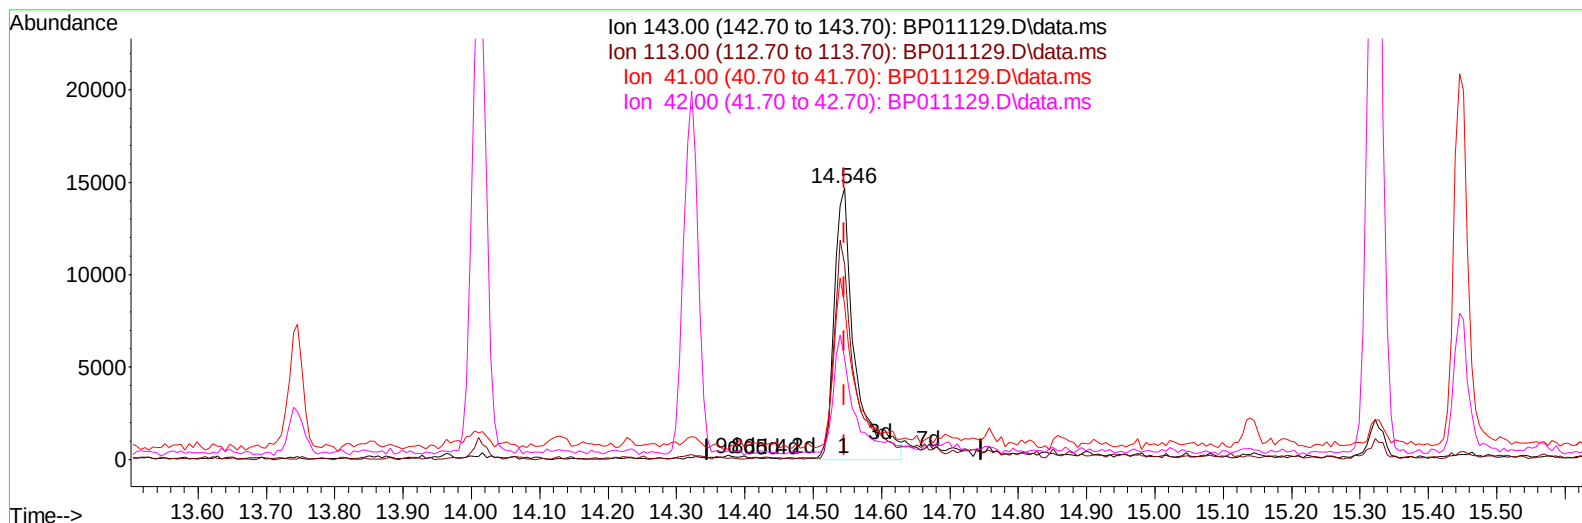

TIC: BP011129.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.546min (+ 0.000) 3.44 ng/ul m

response 31301

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	71.75#
41.00	59.00	56.97
42.00	41.10	37.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011129.D
 Acq On : 27 Jul 2022 14:47
 Operator : CG/JU
 Sample : N3871-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ06

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/28/2022
 Supervised By :mohammad ahmed 07/28/2022

Quant Time: Jul 28 00:02:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 14:31:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	312186	20.000	ng/ul	0.00
20) Naphthalene-d8	10.452	136	1271995	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.322	164	657426	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.087	188	1206798	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.210	240	1113611	20.000	ng/ul	# 0.00
88) Perylene-d12	23.551	264	1235227	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	45372	5.240	ng/uL	0.00
4) Pyridine-d5	3.576	84	224610	10.035	ng/ul	0.00
7) Phenol-d5	6.840	99	179166	6.991	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	679872	41.258	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	572500	27.648	ng/ul	0.00
15) 4-Methylphenol-d8	8.375	113	345442	16.838	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	383582	41.380	ng/ul	0.00
24) 2-Nitrophenol-d4	9.540	143	353672	38.558	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.075	165	544578	32.465	ng/ul	0.00
31) 4-Chloroaniline-d4	10.599	131	666859	24.115	ng/ul	0.00
46) Dimethylphthalate-d6	13.746	166	1900894	42.305	ng/ul	0.00
49) Acenaphthylene-d8	14.010	160	2314439	43.656	ng/ul	0.00
54) 4-Nitrophenol-d4	14.546	143	31301m	3.442	ng/ul	0.00
60) Fluorene-d10	15.322	176	1547741	40.524	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	203019	33.997	ng/ul	0.00
73) Anthracene-d10	17.187	188	2246330	43.785	ng/ul	0.00
81) Pyrene-d10	19.445	212	2531726	43.287	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	2598574	43.801	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011129.D
Acq On : 27 Jul 2022 14:47
Operator : CG/JU
Sample : N3871-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ06

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/28/2022
Supervised By :mohammad ahmed 07/28/2022

Quant Time: Jul 28 00:02:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 14:31:36 2022
Response via : Initial Calibration

