




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011132.D
 Acq On : 27 Jul 2022 16:31
 Operator : CG/JU
 Sample : N3871-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ03

Manual IntegrationsAPPROVED

Quant Time: Jul 28 00:02:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 14:31:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/28/2022
 Supervised By :mohammad ahmed 07/28/2022

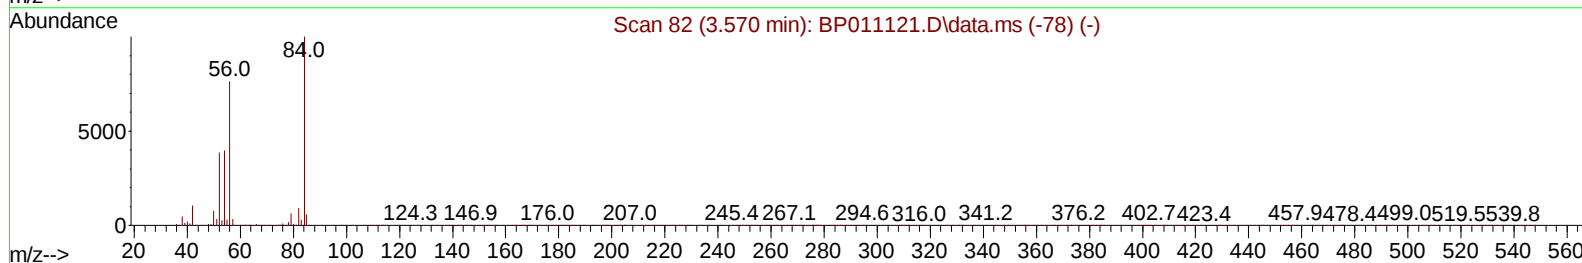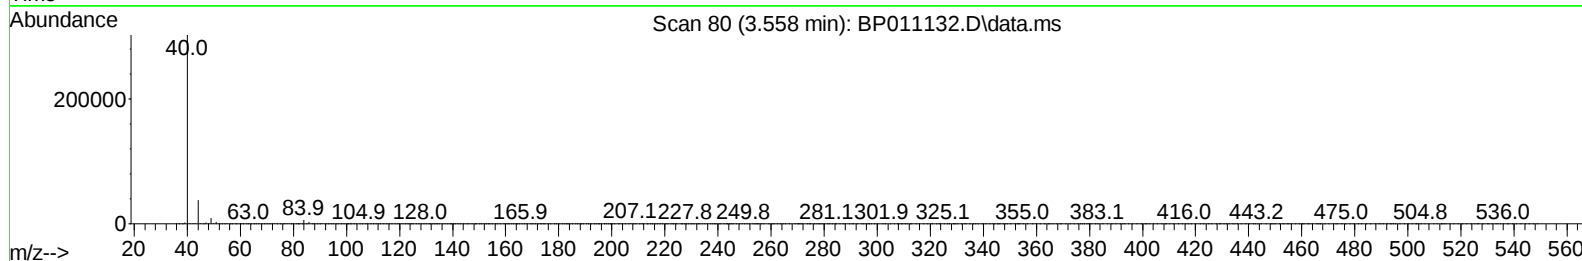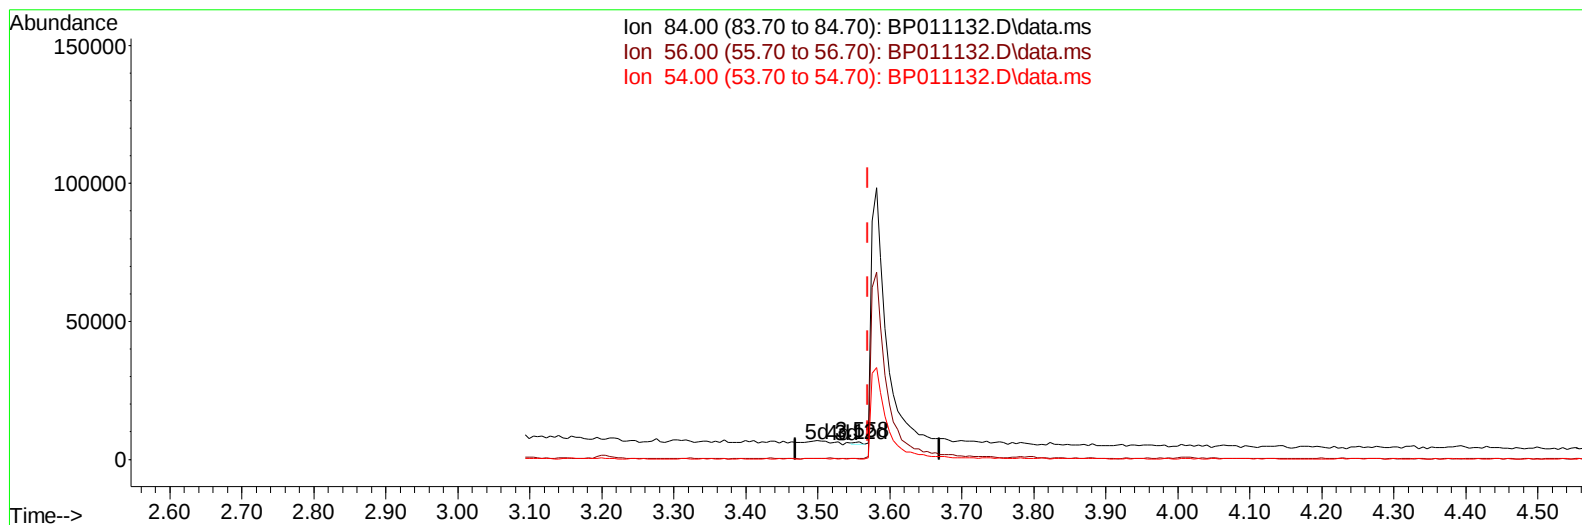

TIC: BP011132.D\data.ms

(4) Pyridine-d5 (S)

3.558min (-0.012) 0.02 ng/u1

response 485

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	84.50	5.90#
54.00	44.80	2.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011132.D
 Acq On : 27 Jul 2022 16:31
 Operator : CG/JU
 Sample : N3871-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ03

Manual IntegrationsAPPROVED

Quant Time: Jul 28 00:02:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 14:31:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/28/2022
 Supervised By :mohammad ahmed 07/28/2022

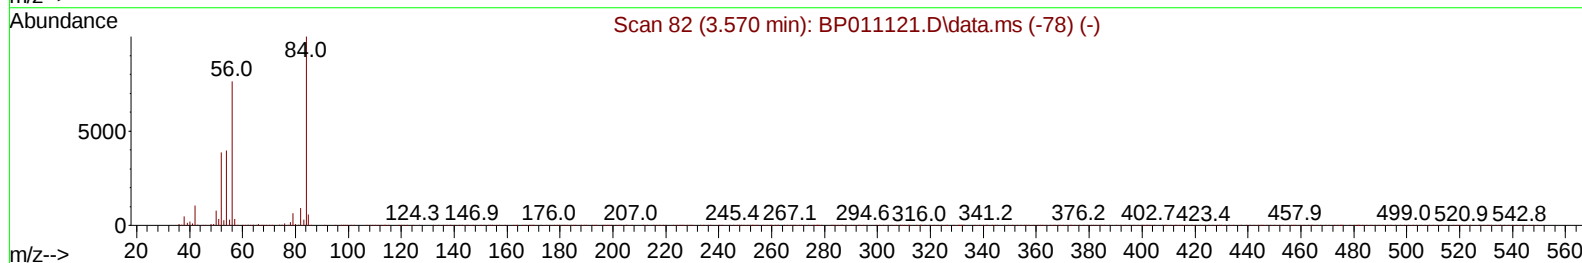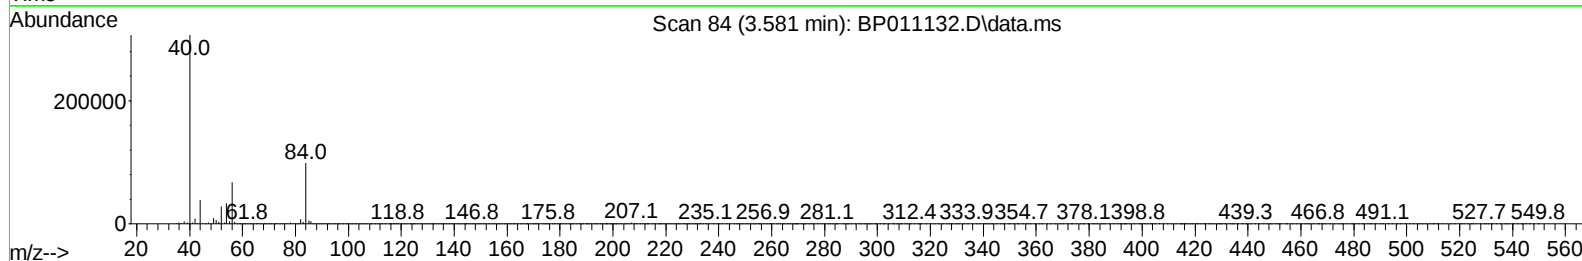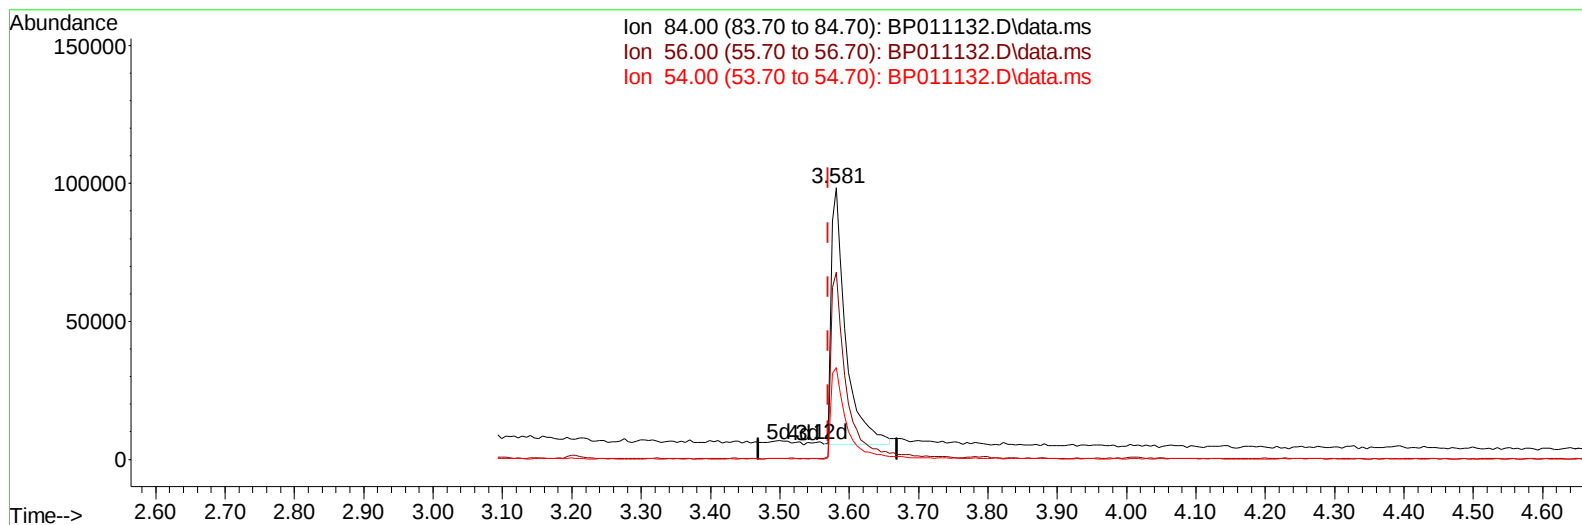

TIC: BP011132.D\data.ms

(4) Pyridine-d5 (S)

3.581min (+ 0.012) 6.25 ng/ul m

response 134146

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	84.50	68.97
54.00	44.80	33.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011132.D
Acq On : 27 Jul 2022 16:31
Operator : CG/JU
Sample : N3871-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ03

Manual IntegrationsAPPROVED

Quant Time: Jul 28 00:02:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 14:31:36 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/28/2022
Supervised By :mohammad ahmed 07/28/2022

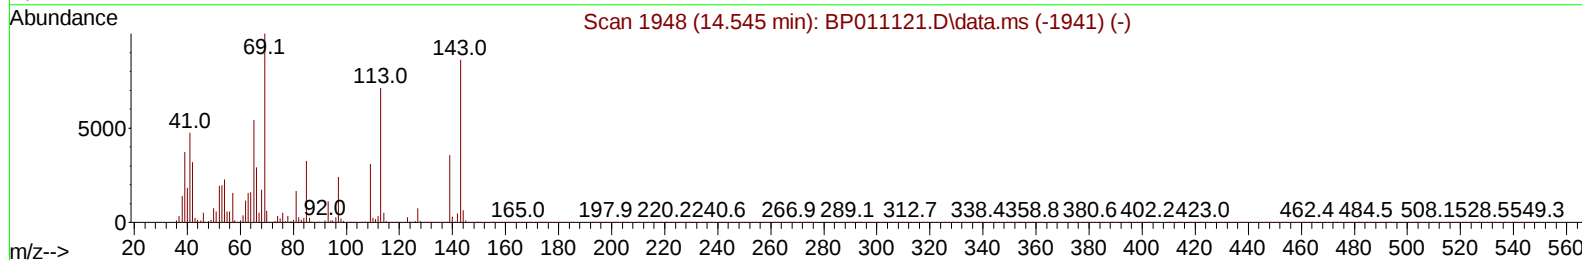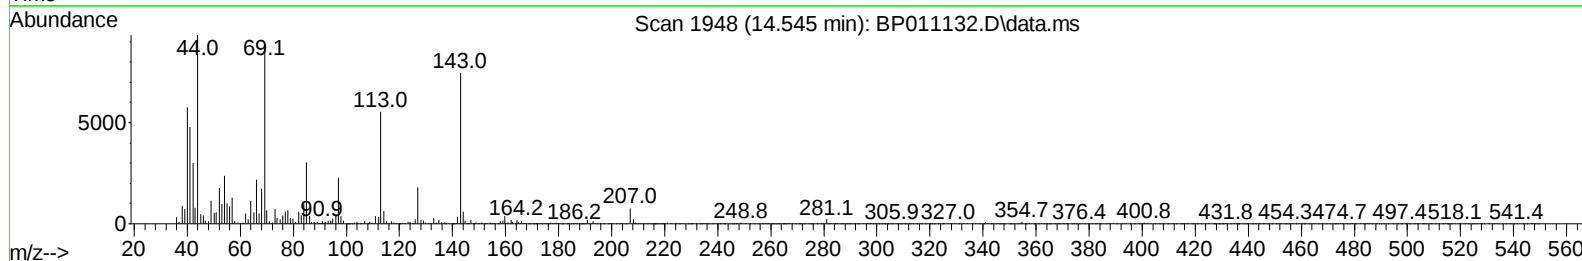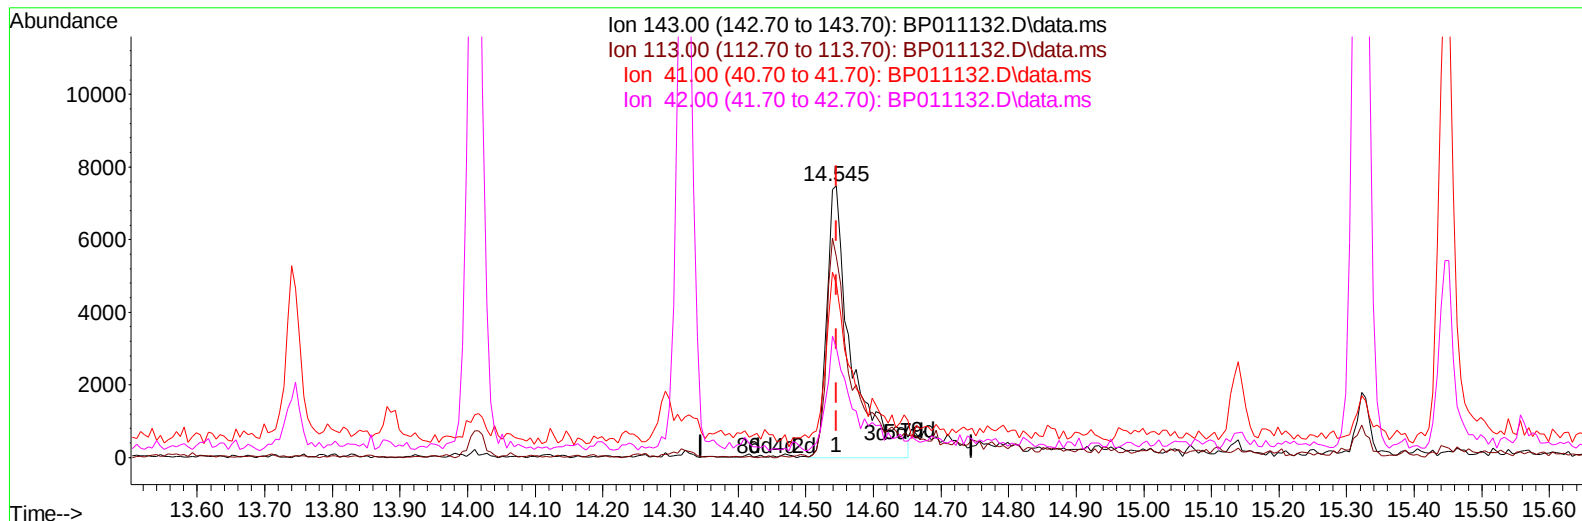

TIC: BP011132.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.545min (+ 0.000) 2.34 ng/ul m

response 19350

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	73.90#
41.00	59.00	64.08
42.00	41.10	40.37

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011132.D
 Acq On : 27 Jul 2022 16:31
 Operator : CG/JU
 Sample : N3871-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ03

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/28/2022
 Supervised By :mohammad ahmed 07/28/2022

Quant Time: Jul 28 00:02:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 14:31:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	299191	20.000	ng/ul	0.00
20) Naphthalene-d8	10.452	136	1219501	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.322	164	598979	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.087	188	1044736	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.210	240	1050000	20.000	ng/ul	# 0.00
88) Perylene-d12	23.545	264	1161447	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	37238	4.487	ng/uL	0.00
4) Pyridine-d5	3.581	84	134146m	6.254	ng/ul	0.01
7) Phenol-d5	6.840	99	146195	5.953	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	544268	34.464	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	461351	23.248	ng/ul	0.00
15) 4-Methylphenol-d8	8.375	113	273766	13.924	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	301870	33.967	ng/ul	0.00
24) 2-Nitrophenol-d4	9.540	143	269235	30.616	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.075	165	417030	25.931	ng/ul	0.00
31) 4-Chloroaniline-d4	10.599	131	637875	24.059	ng/ul	0.00
46) Dimethylphthalate-d6	13.746	166	1342529	32.794	ng/ul	0.00
49) Acenaphthylene-d8	14.010	160	1707967	35.360	ng/ul	0.00
54) 4-Nitrophenol-d4	14.545	143	19350m	2.335	ng/ul	0.00
60) Fluorene-d10	15.322	176	1114924	32.040	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	134318	25.982	ng/ul	-0.01
73) Anthracene-d10	17.187	188	1777106	40.012	ng/ul	0.00
81) Pyrene-d10	19.445	212	1994080	36.160	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	2243506	40.218	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011132.D
Acq On : 27 Jul 2022 16:31
Operator : CG/JU
Sample : N3871-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ03

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/28/2022
Supervised By :mohammad ahmed 07/28/2022

Quant Time: Jul 28 00:02:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 14:31:36 2022
Response via : Initial Calibration

