




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011153.D
Acq On : 28 Jul 2022 05:12
Operator : CG/JU
Sample : N3871-21
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ18

Manual IntegrationsAPPROVED

Quant Time: Jul 28 05:45:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 00:46:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/28/2022
Supervised By :mohammad ahmed 07/28/2022

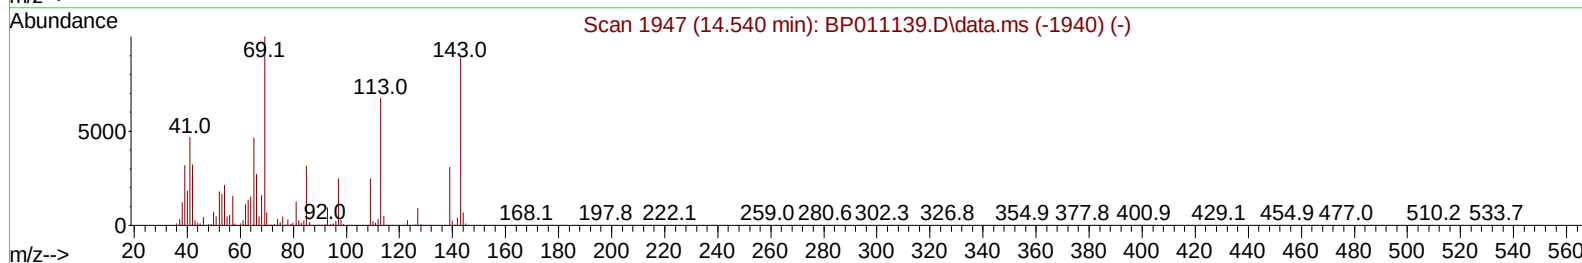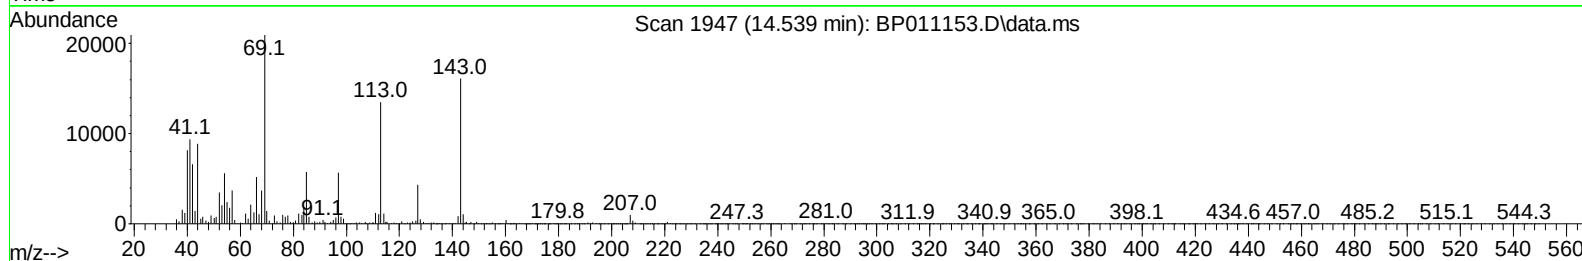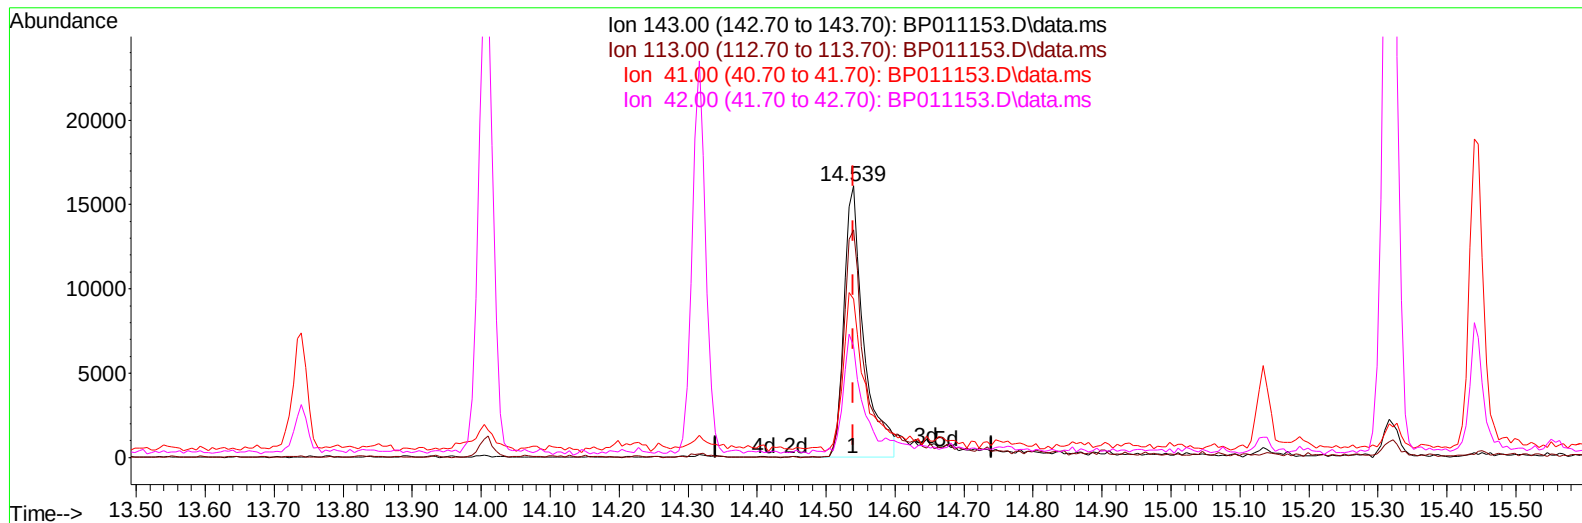

TIC: BP011153.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.539min (-0.000) 3.35 ng/u1

response 32155

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	83.79
41.00	59.00	58.35
42.00	41.10	40.89




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011153.D
Acq On : 28 Jul 2022 05:12
Operator : CG/JU
Sample : N3871-21
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ18

Manual IntegrationsAPPROVED

Quant Time: Jul 28 05:45:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 00:46:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/28/2022
Supervised By :mohammad ahmed 07/28/2022

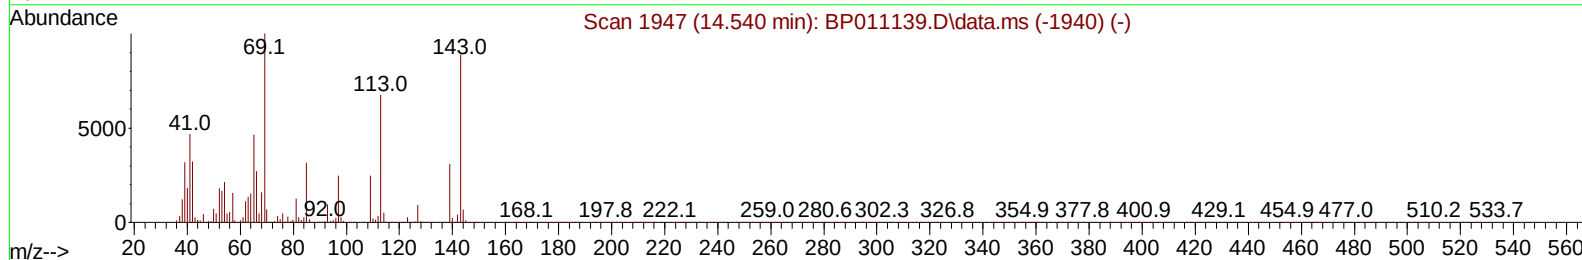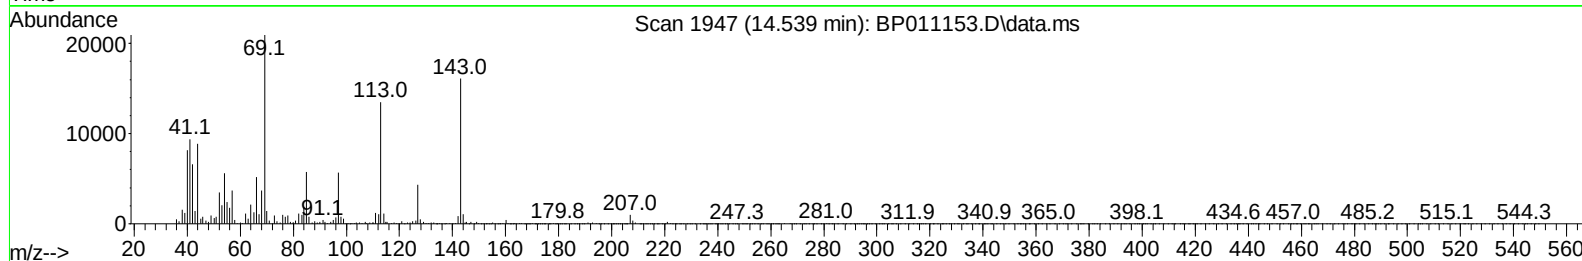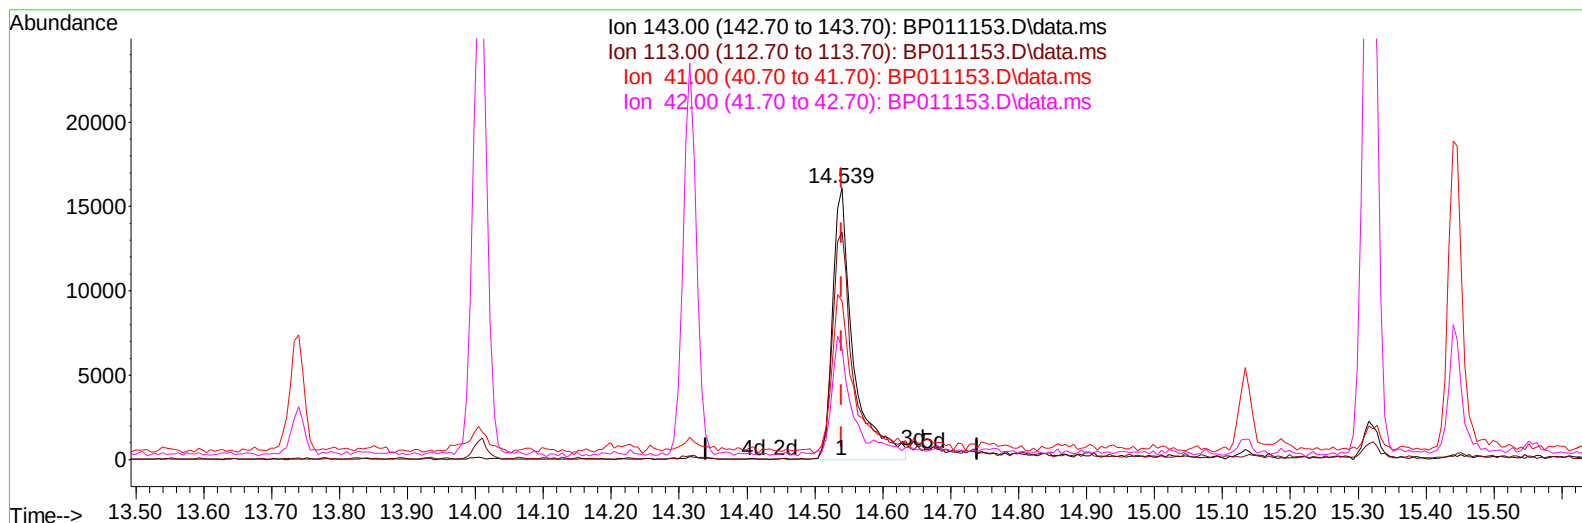

TIC: BP011153.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.539min (-0.000) 3.57 ng/ul m

response 34322

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	83.79
41.00	59.00	58.35
42.00	41.10	40.89

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011153.D
 Acq On : 28 Jul 2022 05:12
 Operator : CG/JU
 Sample : N3871-21
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ18

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/28/2022
 Supervised By :mohammad ahmed 07/28/2022

Quant Time: Jul 28 05:45:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 00:46:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.657	152	334447	20.000	ng/ul	0.00
20) Naphthalene-d8	10.446	136	1379196	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.316	164	694215	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.086	188	1254636	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.204	240	1214651	20.000	ng/ul	# 0.00
88) Perylene-d12	23.539	264	1352904	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	41008	4.420	ng/uL	0.00
4) Pyridine-d5	3.581	84	87761	3.660	ng/ul	0.01
7) Phenol-d5	6.834	99	235785	8.588	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.999	67	741632	42.010	ng/ul	0.00
11) 2-Chlorophenol-d4	7.187	132	668971	30.156	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	414919	18.879	ng/ul	0.00
21) Nitrobenzene-d5	8.816	128	416116	41.401	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	386613	38.874	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	598605	32.912	ng/ul	0.00
31) 4-Chloroaniline-d4	10.593	131	761812	25.407	ng/ul	0.00
46) Dimethylphthalate-d6	13.740	166	1937623	40.838	ng/ul	0.00
49) Acenaphthylene-d8	14.010	160	2461343	43.967	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	34322m	3.574	ng/ul	0.00
60) Fluorene-d10	15.322	176	1604590	39.786	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	187546	30.209	ng/ul	0.00
73) Anthracene-d10	17.181	188	2327599	43.639	ng/ul	0.00
81) Pyrene-d10	19.439	212	2629070	41.212	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.392	264	2841600	43.731	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011153.D
Acq On : 28 Jul 2022 05:12
Operator : CG/JU
Sample : N3871-21
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ18

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/28/2022
Supervised By :mohammad ahmed 07/28/2022

Quant Time: Jul 28 05:45:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 00:46:32 2022
Response via : Initial Calibration

