

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011122.D
 Acq On : 27 Jul 2022 10:45
 Operator : CG/JU
 Sample : PB146439BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK439

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	10	13	17	rVB	126769	140029	2.69%	0.209%
2	3.569	79	82	101	rVB	1449518	2046691	39.25%	3.048%
3	6.840	632	638	655	rVB	1467832	2297190	44.05%	3.421%
4	7.005	660	666	680	rVB	1302159	1956434	37.52%	2.913%
5	7.193	692	698	713	rVB	1555427	2385207	45.74%	3.552%
6	7.663	771	778	788	rVB	1194460	1877058	35.99%	2.795%
7	8.375	892	899	914	rBV	1713221	2735176	52.45%	4.073%
8	8.822	968	975	987	rBV	1488619	2379864	45.64%	3.544%
9	9.540	1090	1097	1110	rBV	1062862	1780668	34.15%	2.652%
10	10.075	1181	1188	1205	rBV	1475785	2525646	48.43%	3.761%
11	10.451	1245	1252	1260	rBV	1599921	2604160	49.94%	3.878%
12	10.598	1270	1277	1296	rBV	1513335	2723196	52.22%	4.055%
13	12.063	1520	1526	1534	rBV3	19907	46346	0.89%	0.069%
14	13.045	1689	1693	1699	rVB9	6256	11733	0.22%	0.017%
15	13.292	1733	1735	1741	rVB7	4241	5440	0.10%	0.008%
16	13.745	1805	1812	1825	rBV	2478189	3341997	64.09%	4.976%
17	13.839	1827	1828	1834	rVB5	5132	6851	0.13%	0.010%
18	14.016	1851	1858	1874	rBV	2848793	4154526	79.67%	6.186%
19	14.322	1902	1910	1920	rBV	2023592	2906521	55.74%	4.328%
20	14.539	1941	1947	1964	rBV	770545	1317463	25.26%	1.962%
21	15.328	2074	2081	2092	rBV	3310081	4743531	90.96%	7.063%
22	15.451	2096	2102	2114	rVV	891919	1259180	24.15%	1.875%
23	15.563	2117	2121	2131	rVB	40167	66167	1.27%	0.099%
24	15.898	2174	2178	2182	rBV7	4310	5612	0.11%	0.008%
25	16.045	2198	2203	2206	rBV6	7911	11546	0.22%	0.017%
26	16.116	2209	2215	2220	rBV5	13253	19665	0.38%	0.029%
27	16.439	2265	2270	2273	rVV5	8756	12880	0.25%	0.019%
28	16.486	2275	2278	2283	rVB6	7516	11111	0.21%	0.017%
29	16.769	2322	2326	2332	rBV9	6731	9608	0.18%	0.014%
30	16.875	2339	2344	2349	rBV5	6793	12465	0.24%	0.019%
31	17.092	2374	2381	2390	rBV	2032355	2841642	54.49%	4.231%
32	17.192	2391	2398	2414	rVV	3294408	4608163	88.37%	6.862%
33	19.022	2706	2709	2716	rVB4	35297	47133	0.90%	0.070%
34	19.092	2717	2721	2725	rVV	28132	39491	0.76%	0.059%
35	19.445	2775	2781	2789	rBV	3822073	4976905	95.44%	7.411%
36	21.210	3076	3081	3091	rBV	2344877	2945180	56.48%	4.386%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011122.D
Acq On : 27 Jul 2022 10:45
Operator : CG/JU
Sample : PB146439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK439

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

37	23.398	3447	3453	3461	rBV2	2751547	5214836	100.00%	7.765%
38	23.551	3473	3479	3489	rVB2	1573759	3089395	59.24%	4.600%




Sum of corrected areas: 67156706

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011122.D
Acq On : 27 Jul 2022 10:45
Operator : CG/JU
Sample : PB146439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

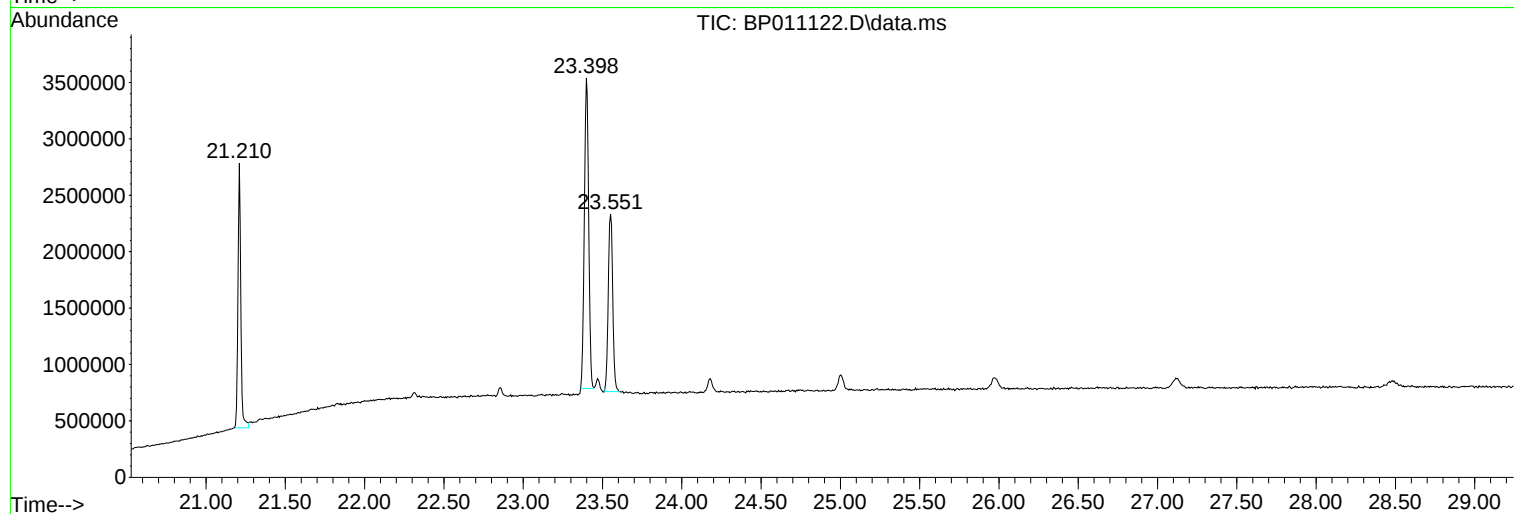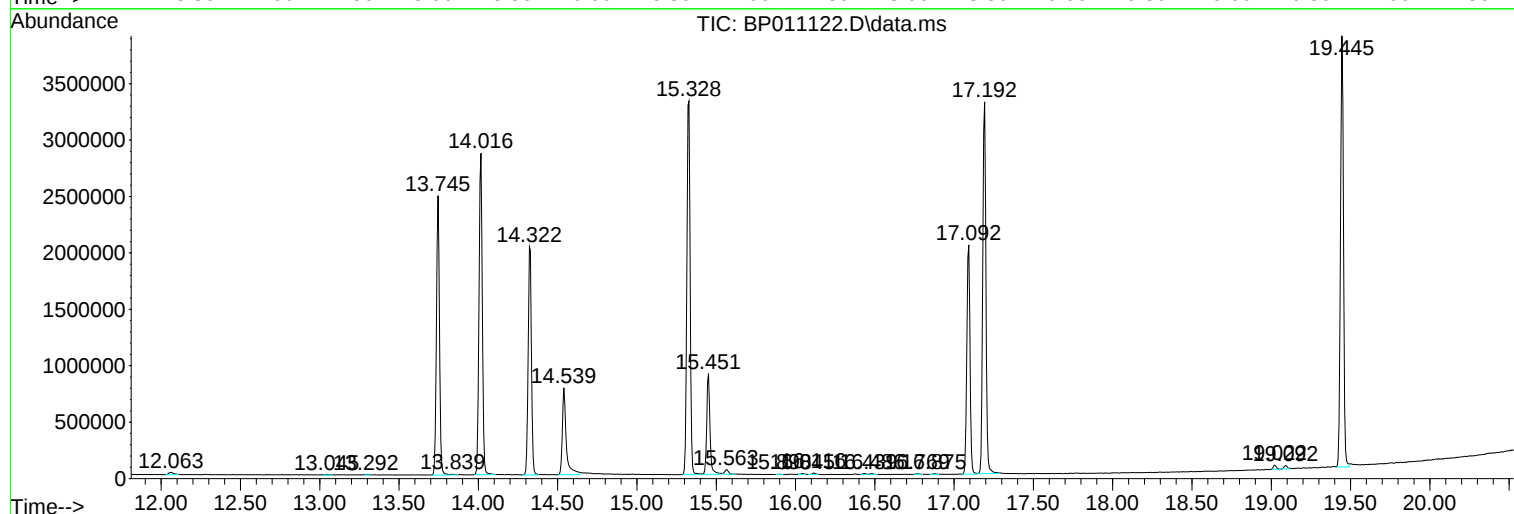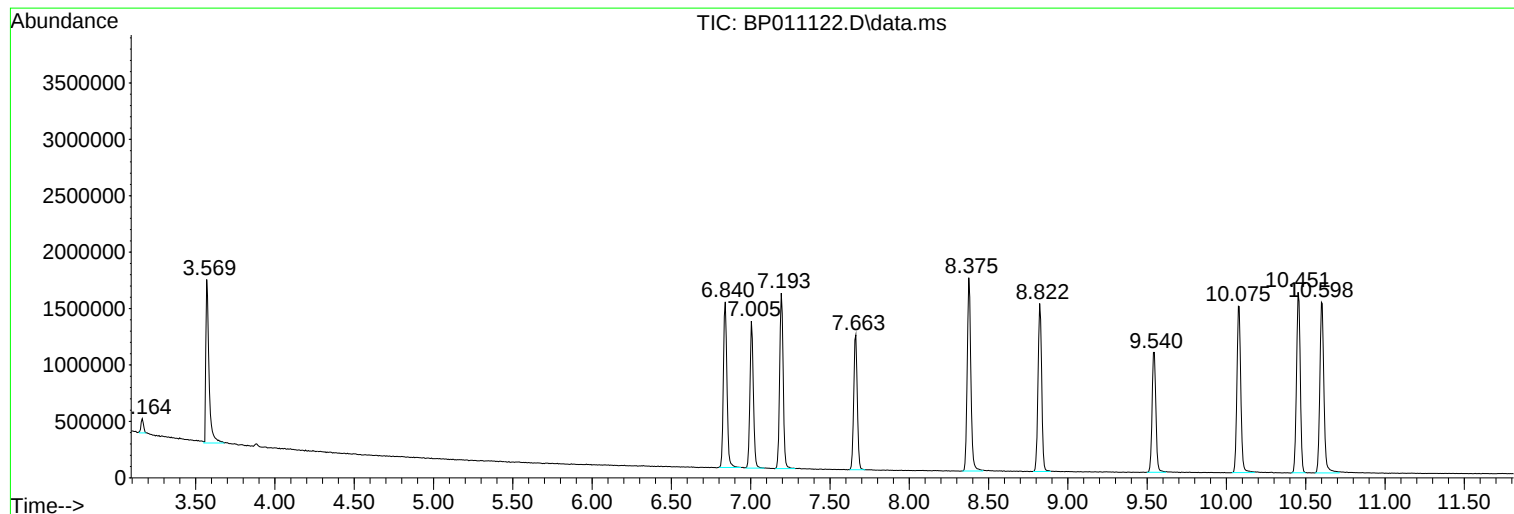

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011122.D
Acq On : 27 Jul 2022 10:45
Operator : CG/JU
Sample : PB146439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011122.D
Acq On : 27 Jul 2022 10:45
Operator : CG/JU
Sample : PB146439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc