

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011123.D
 Acq On : 27 Jul 2022 11:20
 Operator : CG/JU
 Sample : PB146441BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK441

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	10	13	20	rVB2	120891	152054	2.76%	0.238%
2	3.570	79	82	95	rBV	1360765	1779164	32.25%	2.784%
3	6.840	632	638	648	rBV	1341198	2059778	37.34%	3.223%
4	7.005	660	666	679	rVB	1175719	1788191	32.41%	2.798%
5	7.193	692	698	708	rBV	1421308	2155368	39.07%	3.372%
6	7.658	771	777	786	rBV	958512	1532972	27.79%	2.399%
7	8.375	892	899	923	rBV	1542929	2520391	45.69%	3.943%
8	8.822	968	975	983	rBV	1366599	2182593	39.56%	3.415%
9	9.540	1090	1097	1110	rBV	997438	1656357	30.02%	2.592%
10	10.075	1181	1188	1206	rBV	1406584	2348172	42.57%	3.674%
11	10.452	1245	1252	1262	rVB	1312381	2146809	38.92%	3.359%
12	10.599	1270	1277	1300	rBV	1443650	2527797	45.82%	3.955%
13	12.063	1520	1526	1531	rBV3	17017	31226	0.57%	0.049%
14	13.040	1689	1692	1696	rBV5	3103	6164	0.11%	0.010%
15	13.293	1731	1735	1739	rVB6	4635	5949	0.11%	0.009%
16	13.745	1805	1812	1824	rBV	2332042	3240389	58.74%	5.070%
17	14.016	1849	1858	1872	rBV	2741507	3919125	71.04%	6.132%
18	14.322	1904	1910	1922	rBV	1701588	2431759	44.08%	3.805%
19	14.540	1940	1947	1967	rBV	786596	1374643	24.92%	2.151%
20	15.322	2074	2080	2095	rBV	3268586	4594349	83.28%	7.188%
21	15.451	2096	2102	2116	rVV	894108	1306971	23.69%	2.045%
22	15.563	2116	2121	2131	rVB2	41131	71206	1.29%	0.111%
23	15.975	2186	2191	2196	rVV2	41269	59993	1.09%	0.094%
24	16.045	2196	2203	2209	rVV	54013	80392	1.46%	0.126%
25	16.110	2209	2214	2223	rVB8	16092	31854	0.58%	0.050%
26	16.375	2254	2259	2263	rBV	45572	55628	1.01%	0.087%
27	16.434	2263	2269	2273	rVV	92548	130585	2.37%	0.204%
28	16.481	2273	2277	2284	rVB	83031	112129	2.03%	0.175%
29	16.769	2320	2326	2331	rBV10	6352	12333	0.22%	0.019%
30	16.869	2339	2343	2348	rBV7	5733	11419	0.21%	0.018%
31	17.092	2374	2381	2389	rBV	1760363	2552055	46.26%	3.993%
32	17.192	2391	2398	2412	rVV2	3232865	4656084	84.40%	7.285%
33	19.022	2705	2709	2714	rBV3	34553	48910	0.89%	0.077%
34	19.086	2717	2720	2724	rVV	29946	41760	0.76%	0.065%
35	19.445	2775	2781	2789	rBV	4126934	5217679	94.58%	8.164%
36	21.210	3076	3081	3092	rBV	2064481	2707548	49.08%	4.236%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011123.D
Acq On : 27 Jul 2022 11:20
Operator : CG/JU
Sample : PB146441BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

37	23.398	3446	3453	3461	rBV	2961847	5516646	100.00%	8.631%
38	23.545	3472	3478	3488	rVB2	1469277	2846880	51.61%	4.454%




Sum of corrected areas: 63913322

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011123.D
Acq On : 27 Jul 2022 11:20
Operator : CG/JU
Sample : PB146441BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

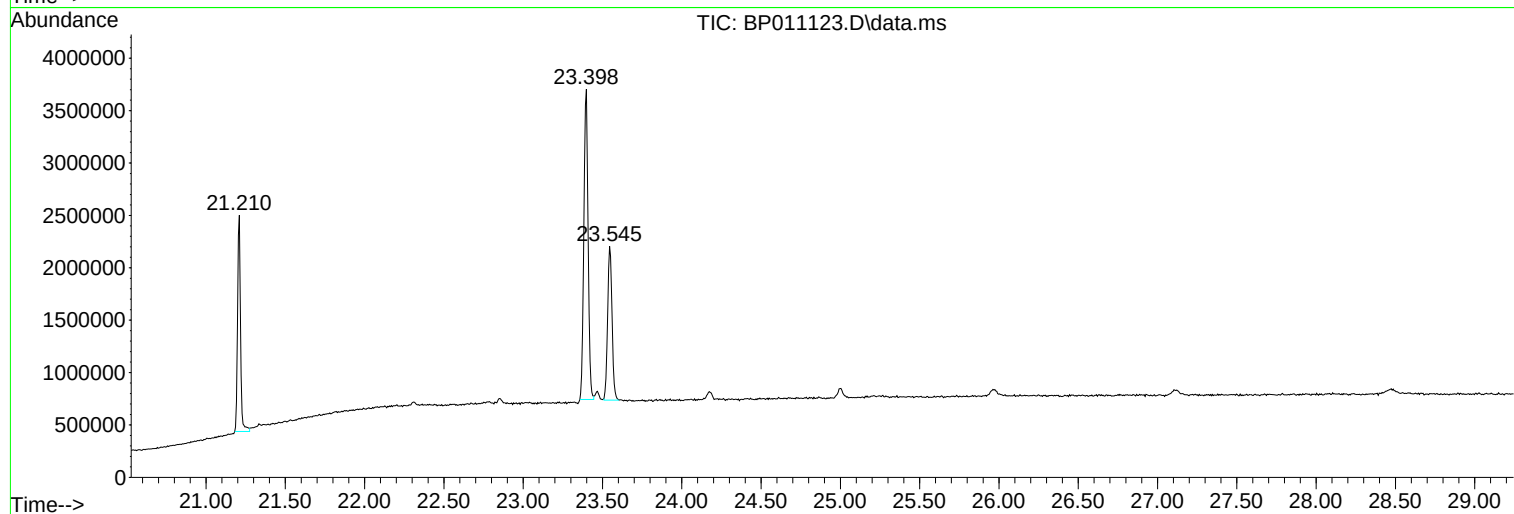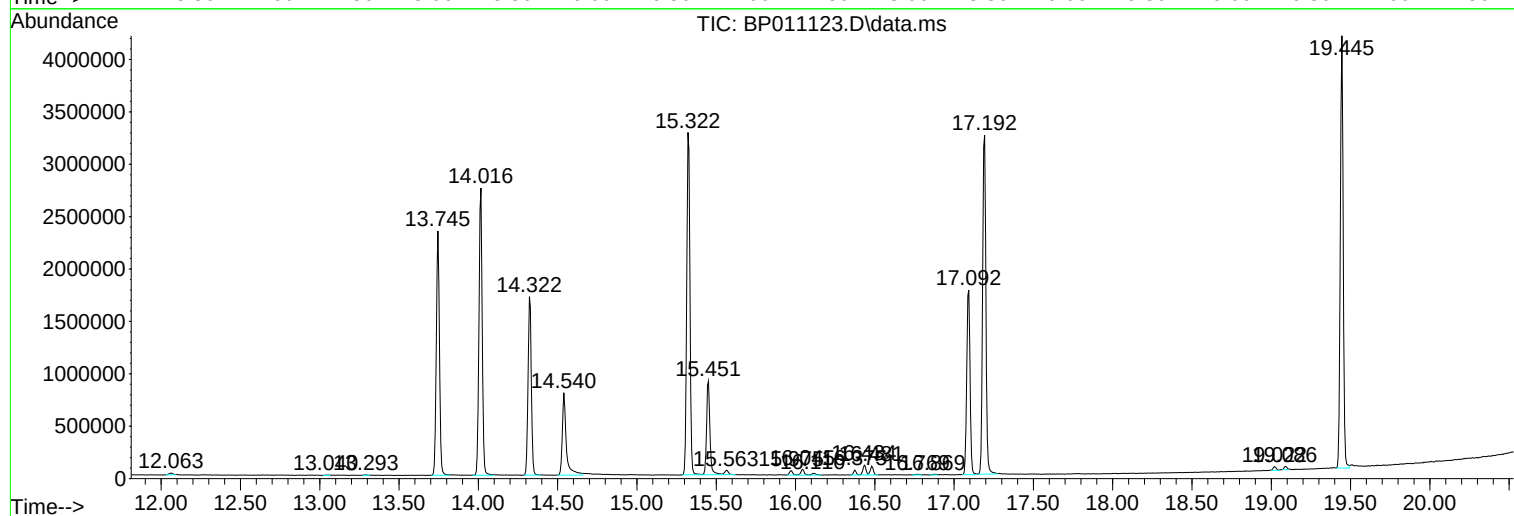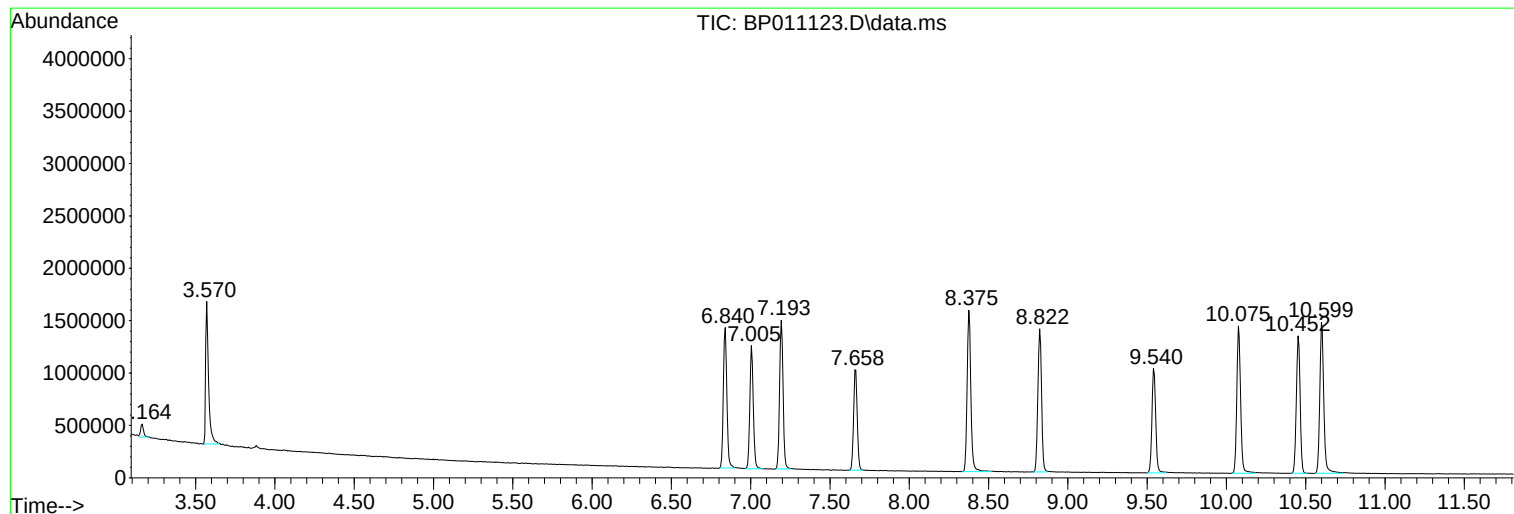

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011123.D
Acq On : 27 Jul 2022 11:20
Operator : CG/JU
Sample : PB146441BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011123.D
Acq On : 27 Jul 2022 11:20
Operator : CG/JU
Sample : PB146441BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc