

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011126.D
 Acq On : 27 Jul 2022 13:03
 Operator : CG/JU
 Sample : N3871-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	11	rBV	720472	949219	12.35%	1.325%
2	3.575	81	83	98	rVB	400948	589470	7.67%	0.823%
3	6.840	632	638	646	rVB	304719	475148	6.18%	0.663%
4	7.005	660	666	677	rVB	1374212	2061561	26.83%	2.877%
5	7.193	692	698	709	rBV	1252525	1878503	24.45%	2.622%
6	7.658	771	777	787	rVB	1267238	1973419	25.68%	2.754%
7	8.375	893	899	910	rBV	891025	1416681	18.44%	1.977%
8	8.822	967	975	990	rBV	1626745	2632170	34.26%	3.674%
9	9.540	1090	1097	1112	rVB	1124998	1816352	23.64%	2.535%
10	10.075	1181	1188	1199	rBV	1505730	2446363	31.84%	3.414%
11	10.452	1245	1252	1260	rBV	1675676	2727290	35.50%	3.806%
12	10.599	1270	1277	1295	rBV	1381226	2392445	31.14%	3.339%
13	11.016	1344	1348	1354	rVB5	6601	10693	0.14%	0.015%
14	11.081	1354	1359	1362	rBV6	5511	11110	0.14%	0.016%
15	11.269	1386	1391	1394	rBV5	12586	24556	0.32%	0.034%
16	12.057	1518	1525	1531	rBV3	26623	50884	0.66%	0.071%
17	12.257	1554	1559	1564	rBV8	4773	8935	0.12%	0.012%
18	12.681	1625	1631	1633	rBV4	7305	11755	0.15%	0.016%
19	12.934	1669	1674	1679	rBV4	13996	19938	0.26%	0.028%
20	13.228	1720	1724	1729	rVB3	8896	12405	0.16%	0.017%
21	13.328	1737	1741	1745	rVB6	6059	9494	0.12%	0.013%
22	13.746	1805	1812	1824	rBV	2957390	4019041	52.31%	5.609%
23	14.016	1850	1858	1869	rVV	3198637	4634807	60.32%	6.469%
24	14.134	1872	1878	1880	rVV6	5644	12614	0.16%	0.018%
25	14.322	1903	1910	1917	rBV	2022156	2944540	38.32%	4.110%
26	14.545	1942	1948	1963	rBV2	106057	246854	3.21%	0.345%
27	14.734	1976	1980	1983	rBV3	23918	33732	0.44%	0.047%
28	14.857	1996	2001	2007	rVB10	4168	7937	0.10%	0.011%
29	15.140	2045	2049	2058	rBV3	32344	58209	0.76%	0.081%
30	15.322	2072	2080	2087	rBV	3926497	5666036	73.74%	7.908%
31	15.375	2087	2089	2096	rVV4	34619	53199	0.69%	0.074%
32	15.451	2096	2102	2115	rVV	1236334	1702839	22.16%	2.377%
33	15.563	2115	2121	2130	rVB3	49491	100027	1.30%	0.140%
34	15.892	2171	2177	2184	rBV3	5715	11670	0.15%	0.016%
35	16.122	2211	2216	2221	rVB6	14011	21237	0.28%	0.030%
36	16.569	2289	2292	2298	rVB8	6024	9741	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011126.D
 Acq On : 27 Jul 2022 13:03
 Operator : CG/JU
 Sample : N3871-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.769	2322	2326	2332	rBV8	15637	22514	0.29%	0.031%
38	16.869	2337	2343	2348	rBV7	13264	25181	0.33%	0.035%
39	17.034	2366	2371	2374	rBV7	5368	8978	0.12%	0.013%
40	17.092	2374	2381	2389	rBV	2080758	2929389	38.13%	4.088%
41	17.192	2391	2398	2408	rBV	4361084	6021638	78.37%	8.404%
42	17.398	2429	2433	2437	rVB2	14260	18261	0.24%	0.025%
43	17.781	2493	2498	2502	rBV7	8727	12935	0.17%	0.018%
44	18.004	2532	2536	2541	rBV8	13548	20954	0.27%	0.029%
45	18.069	2544	2547	2552	rVB	33299	42996	0.56%	0.060%
46	19.022	2705	2709	2713	rBV2	50593	65587	0.85%	0.092%
47	19.092	2717	2721	2725	rBV	46003	58045	0.76%	0.081%
48	19.392	2770	2772	2775	rBV4	15868	16611	0.22%	0.023%
49	19.445	2775	2781	2789	rBV	5292946	6821397	88.78%	9.520%
50	21.210	3076	3081	3091	rBV	2570372	3299028	42.94%	4.604%
51	23.398	3446	3453	3461	rBV2	4124796	7683336	100.00%	10.723%
52	23.551	3473	3479	3492	rVB	1876542	3564084	46.39%	4.974%




Sum of corrected areas: 71651808

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011126.D
Acq On : 27 Jul 2022 13:03
Operator : CG/JU
Sample : N3871-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

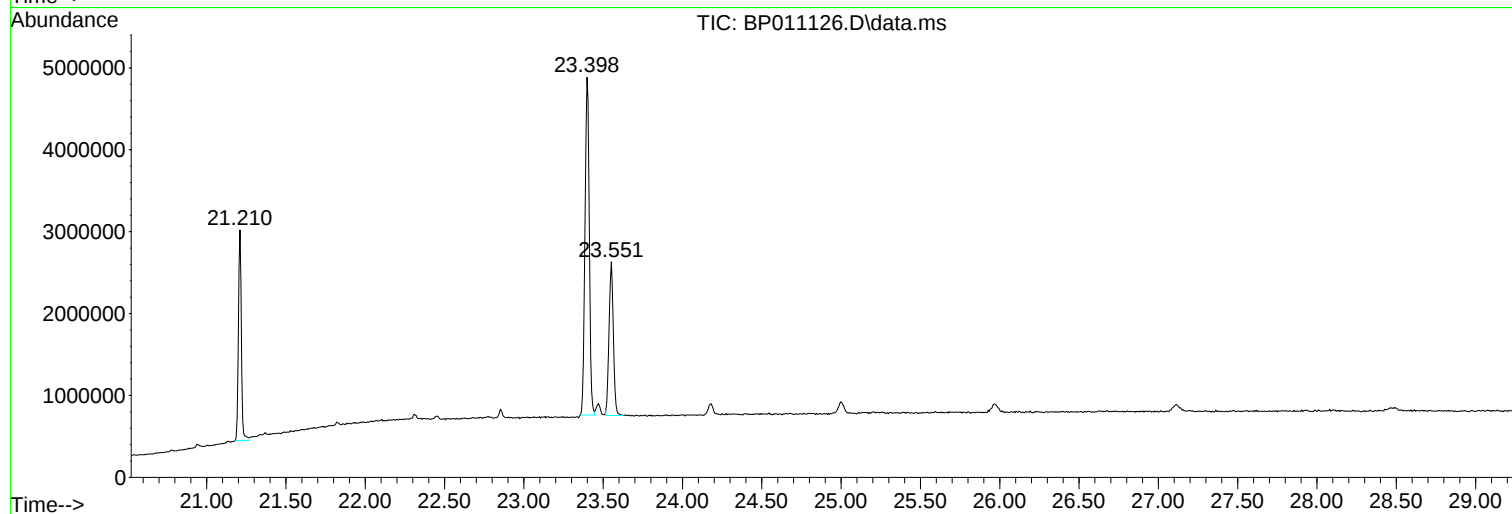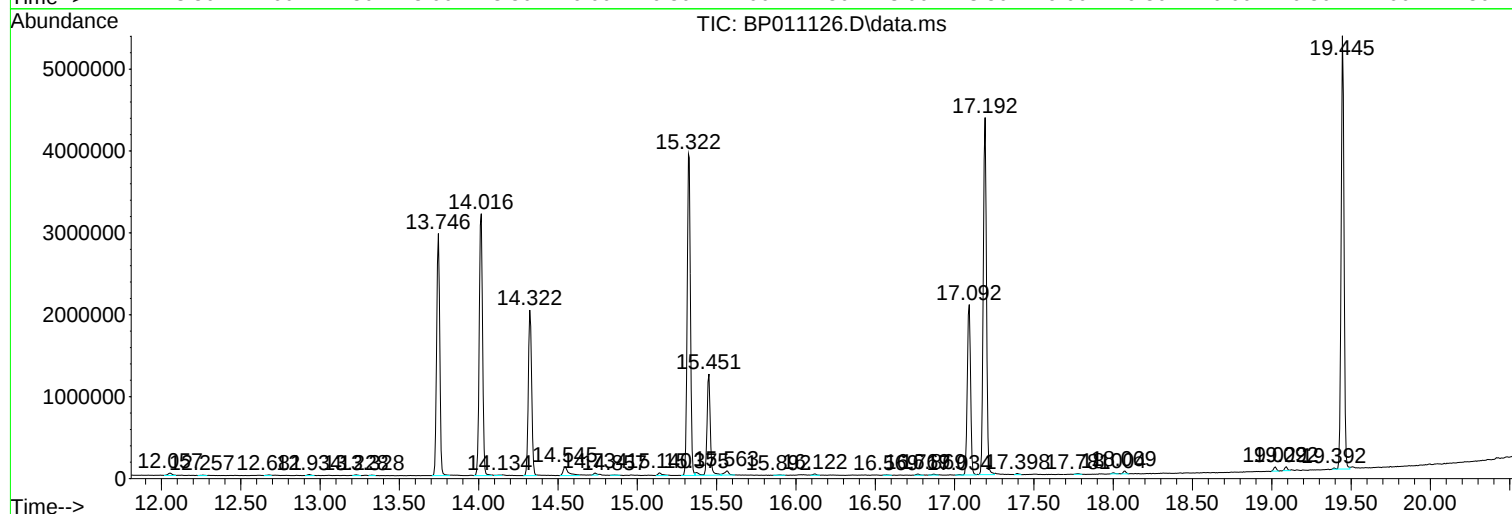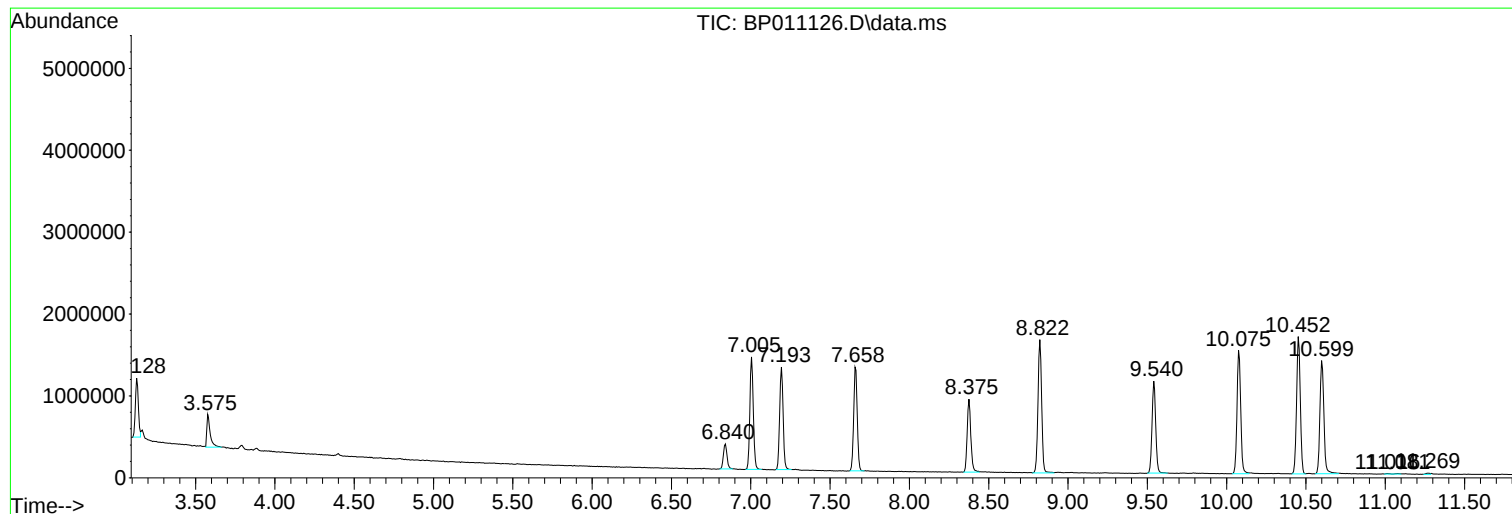

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011126.D
Acq On : 27 Jul 2022 13:03
Operator : CG/JU
Sample : N3871-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011126.D
Acq On : 27 Jul 2022 13:03
Operator : CG/JU
Sample : N3871-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--		
					#	RT	Resp Conc
