

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011127.D
 Acq On : 27 Jul 2022 13:38
 Operator : CG/JU
 Sample : N3871-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.575	81	83	97	rVB	313275	459628	6.96%	0.661%
2	6.840	633	638	647	rVB	273829	447725	6.78%	0.644%
3	7.005	660	666	683	rVB	1367351	2104073	31.88%	3.026%
4	7.193	692	698	709	rBV	1204661	1835335	27.81%	2.639%
5	7.658	771	777	787	rVB	1187702	1829442	27.72%	2.631%
6	8.375	893	899	914	rBV	832509	1330589	20.16%	1.913%
7	8.822	968	975	988	rBV	1645885	2647529	40.11%	3.807%
8	9.540	1090	1097	1110	rBV	1184287	1916066	29.03%	2.755%
9	10.075	1181	1188	1203	rBV	1548217	2501961	37.91%	3.598%
10	10.452	1245	1252	1261	rBV	1643920	2642715	40.04%	3.800%
11	10.599	1270	1277	1296	rBV	1412880	2473733	37.48%	3.557%
12	11.734	1468	1470	1477	rVB5	7453	12009	0.18%	0.017%
13	12.057	1519	1525	1530	rBV2	25664	45807	0.69%	0.066%
14	12.269	1555	1561	1571	rVB2	3707	9978	0.15%	0.014%
15	12.675	1626	1630	1638	rBV9	6046	11159	0.17%	0.016%
16	12.934	1670	1674	1679	rBV6	10761	16407	0.25%	0.024%
17	13.234	1719	1725	1727	rBV6	6355	8993	0.14%	0.013%
18	13.746	1805	1812	1824	rBV	2972197	4134540	62.64%	5.946%
19	14.010	1849	1857	1872	rBV	3322221	4916693	74.49%	7.071%
20	14.322	1902	1910	1918	rBV	2196039	3089934	46.82%	4.444%
21	14.545	1942	1948	1963	rBV3	71314	185991	2.82%	0.267%
22	14.769	1978	1986	1989	rVV10	5998	12234	0.19%	0.018%
23	15.140	2044	2049	2058	rBV	68028	93475	1.42%	0.134%
24	15.322	2073	2080	2095	rBV	4211159	5905341	89.47%	8.492%
25	15.445	2095	2101	2116	rVV	1218186	1701110	25.77%	2.446%
26	15.563	2116	2121	2128	rVB3	51370	83821	1.27%	0.121%
27	16.034	2193	2201	2203	rBV9	5728	12219	0.19%	0.018%
28	16.116	2211	2215	2220	rVB4	14692	24332	0.37%	0.035%
29	16.775	2320	2327	2329	rBV7	8523	14500	0.22%	0.021%
30	16.869	2337	2343	2348	rBV7	10361	19605	0.30%	0.028%
31	17.087	2374	2380	2391	rBV	2200869	3148438	47.70%	4.528%
32	17.187	2391	2397	2409	rBV2	4227073	6132135	92.91%	8.818%
33	17.392	2430	2432	2437	rVB4	8656	10508	0.16%	0.015%
34	17.775	2494	2497	2502	rVB7	10786	12823	0.19%	0.018%
35	17.998	2531	2535	2540	rBV8	13321	20806	0.32%	0.030%
36	18.075	2545	2548	2555	rVB	11334	17489	0.26%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011127.D
 Acq On : 27 Jul 2022 13:38
 Operator : CG/JU
 Sample : N3871-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ04

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	19.022	2704	2709	2715	rBV3	49838	74930	1.14%	0.108%
38	19.086	2716	2720	2729	rVV	47607	79045	1.20%	0.114%
39	19.157	2730	2732	2736	rVB5	13731	15021	0.23%	0.022%
40	19.392	2769	2772	2775	rBV3	20709	25637	0.39%	0.037%
41	19.445	2775	2781	2788	rBV	5194538	6549839	99.24%	9.419%
42	21.210	3076	3081	3088	rBV	2429538	3089241	46.80%	4.443%
43	23.398	3446	3453	3460	rBV2	3485664	6600250	100.00%	9.492%
44	23.545	3472	3478	3489	rVB2	1656558	3274517	49.61%	4.709%




Sum of corrected areas: 69537623

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011127.D
Acq On : 27 Jul 2022 13:38
Operator : CG/JU
Sample : N3871-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

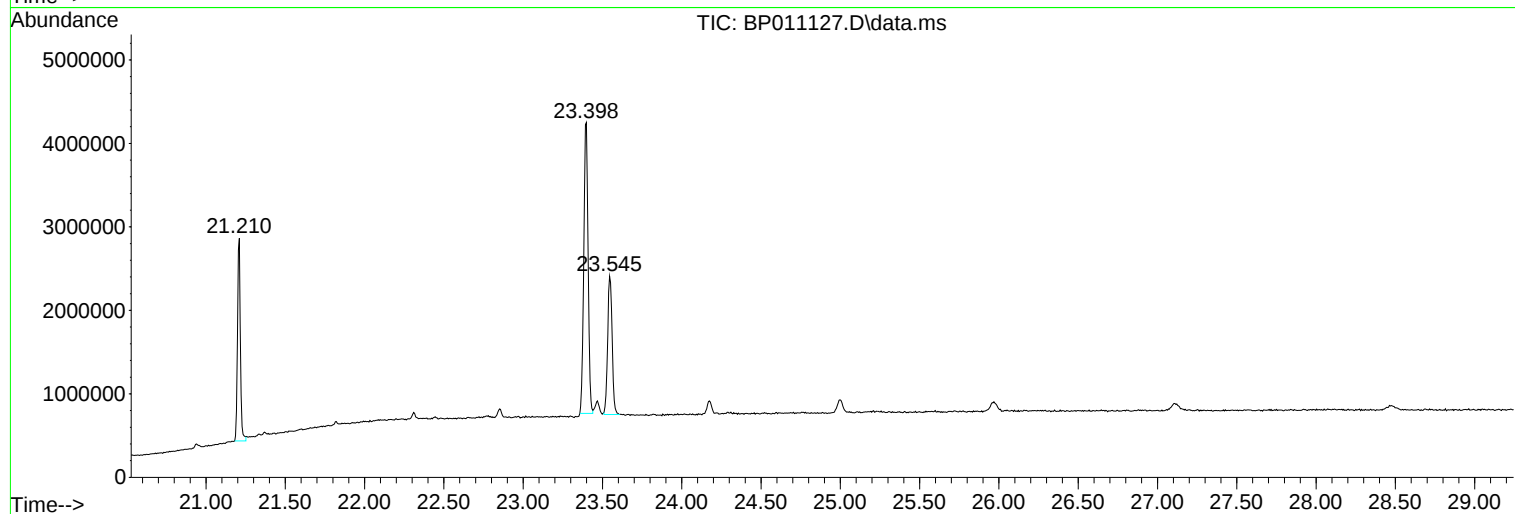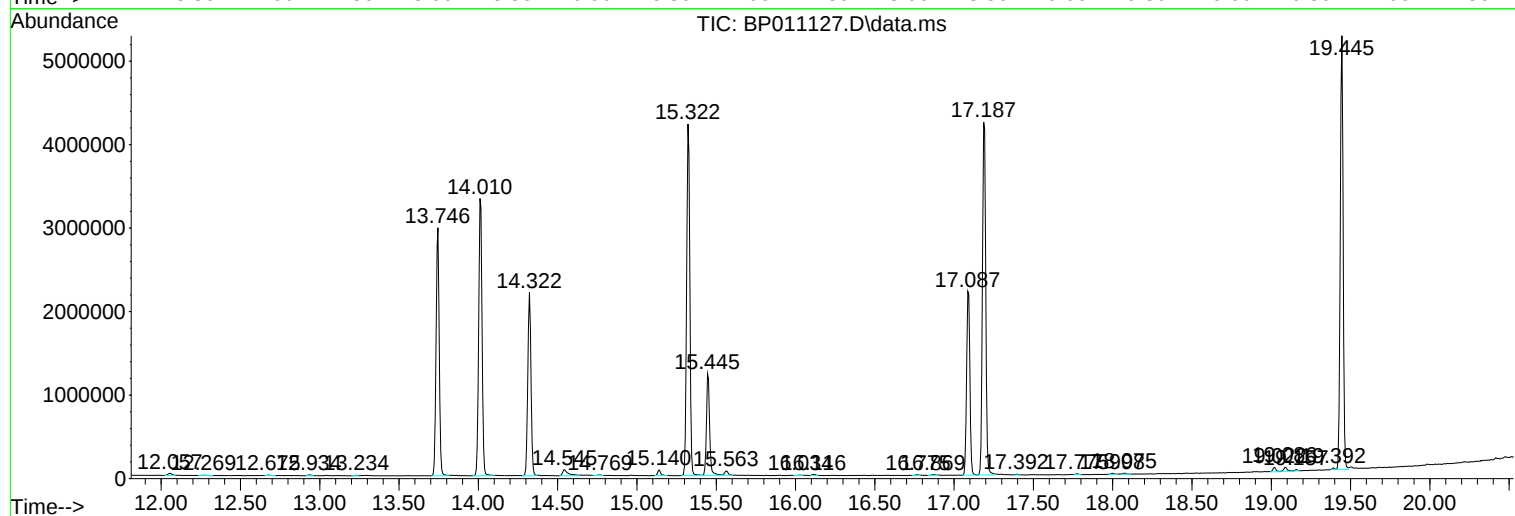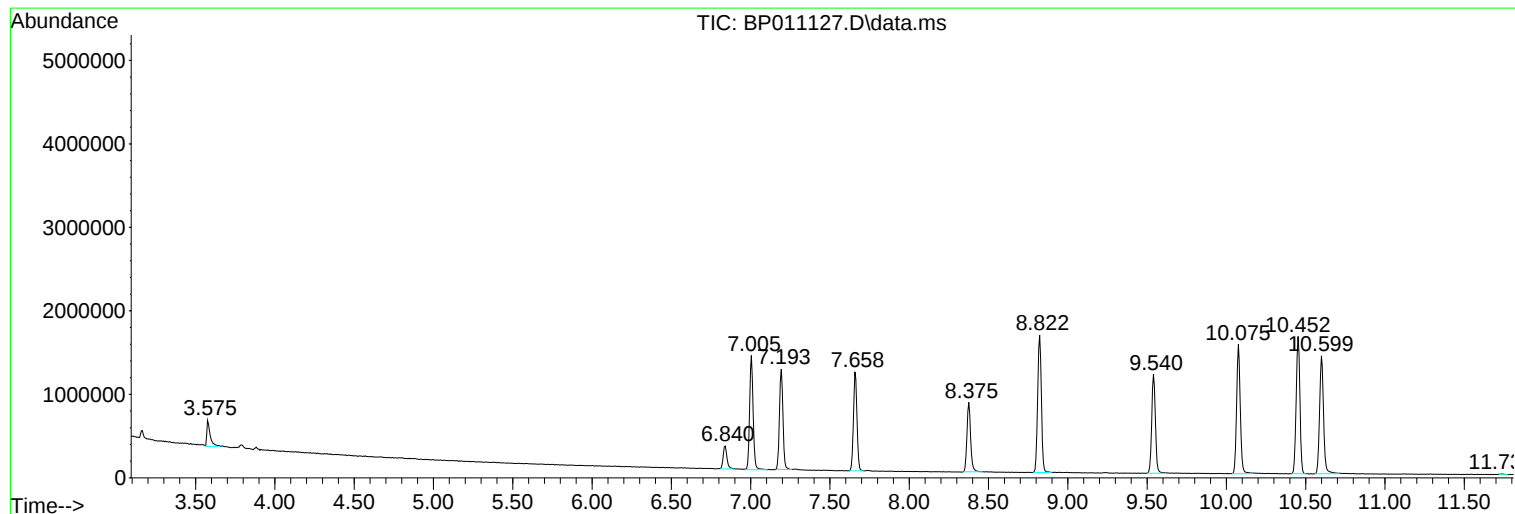

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011127.D
Acq On : 27 Jul 2022 13:38
Operator : CG/JU
Sample : N3871-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011127.D
Acq On : 27 Jul 2022 13:38
Operator : CG/JU
Sample : N3871-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc