

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011128.D
 Acq On : 27 Jul 2022 14:12
 Operator : CG/JU
 Sample : N3871-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.129	3	7	24	rVB	1864210	2786296	33.72%	3.458%
2	3.576	81	83	96	rVB	432924	624843	7.56%	0.775%
3	6.840	633	638	647	rVB	291606	473297	5.73%	0.587%
4	7.005	660	666	677	rVB	1216861	1843858	22.31%	2.288%
5	7.193	692	698	710	rVB	1125913	1721723	20.84%	2.137%
6	7.658	771	777	785	rBV	1246178	1916000	23.19%	2.378%
7	8.375	893	899	910	rBV	849902	1351330	16.35%	1.677%
8	8.822	968	975	986	rBV	1471617	2371411	28.70%	2.943%
9	9.234	1043	1045	1051	rVB4	11244	13705	0.17%	0.017%
10	9.540	1090	1097	1112	rBV	1084942	1736670	21.02%	2.155%
11	10.075	1180	1188	1197	rBV	1469460	2384846	28.86%	2.960%
12	10.452	1244	1252	1262	rBV	1722172	2770366	33.53%	3.438%
13	10.599	1269	1277	1295	rBV	1180039	2076985	25.13%	2.578%
14	11.275	1387	1392	1401	rVB9	11303	23672	0.29%	0.029%
15	11.740	1465	1471	1475	rVB6	6963	12384	0.15%	0.015%
16	12.052	1516	1524	1530	rVB4	25169	46779	0.57%	0.058%
17	12.675	1626	1630	1636	rBV6	12164	21783	0.26%	0.027%
18	12.928	1669	1673	1679	rVB2	22322	35575	0.43%	0.044%
19	13.228	1720	1724	1730	rBV7	7738	14059	0.17%	0.017%
20	13.746	1805	1812	1821	rBV	3021669	4204190	50.88%	5.217%
21	14.016	1849	1858	1876	rBV	3279110	4794128	58.02%	5.949%
22	14.322	1903	1910	1919	rBV	2374252	3423890	41.43%	4.249%
23	14.404	1922	1924	1929	rVB6	6677	10189	0.12%	0.013%
24	14.540	1941	1947	1961	rBV	162960	346629	4.19%	0.430%
25	14.763	1978	1985	1989	rVB8	10056	20763	0.25%	0.026%
26	15.140	2043	2049	2052	rBV	54365	76139	0.92%	0.094%
27	15.322	2073	2080	2086	rBV	4184579	6079991	73.58%	7.545%
28	15.375	2086	2089	2096	rVV	182733	266626	3.23%	0.331%
29	15.451	2096	2102	2115	rVV	1502137	2097800	25.39%	2.603%
30	15.563	2115	2121	2126	rVB3	52197	83328	1.01%	0.103%
31	15.704	2143	2145	2150	rVB5	7014	8644	0.10%	0.011%
32	15.898	2175	2178	2180	rBV4	6528	8529	0.10%	0.011%
33	15.963	2185	2189	2193	rBV7	4396	9229	0.11%	0.011%
34	16.028	2194	2200	2202	rVV7	8789	14922	0.18%	0.019%
35	16.057	2204	2205	2212	rVV5	8942	14951	0.18%	0.019%
36	16.116	2212	2215	2219	rVB4	18389	24059	0.29%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011128.D
 Acq On : 27 Jul 2022 14:12
 Operator : CG/JU
 Sample : N3871-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.240	2231	2236	2238	rBV6	5823	9801	0.12%	0.012%
38	16.498	2277	2280	2285	rBV7	5854	8686	0.11%	0.011%
39	16.763	2321	2325	2329	rVB6	7902	12944	0.16%	0.016%
40	16.869	2339	2343	2346	rBV5	14976	20554	0.25%	0.026%
41	17.028	2367	2370	2373	rBV5	10835	12751	0.15%	0.016%
42	17.092	2374	2381	2391	rVV	2842647	3900721	47.20%	4.841%
43	17.192	2391	2398	2411	rBV2	4927991	6967115	84.31%	8.646%
44	17.398	2428	2433	2441	rBV3	18483	35208	0.43%	0.044%
45	17.610	2466	2469	2473	rBV6	8767	11336	0.14%	0.014%
46	17.787	2494	2499	2504	rVB	73740	97229	1.18%	0.121%
47	17.998	2532	2535	2540	rBV2	54521	80360	0.97%	0.100%
48	18.075	2544	2548	2551	rVB	33231	41513	0.50%	0.052%
49	19.022	2705	2709	2713	rVB2	65996	84986	1.03%	0.105%
50	19.086	2717	2720	2724	rBV	55588	70078	0.85%	0.087%
51	19.157	2730	2732	2736	rBV5	14800	14844	0.18%	0.018%
52	19.392	2770	2772	2775	rBV2	25103	24934	0.30%	0.031%
53	19.445	2775	2781	2789	rBV	6082848	8047294	97.38%	9.987%
54	20.945	3032	3036	3044	rBV3	156633	322231	3.90%	0.400%
55	21.210	3076	3081	3091	rBV	3402947	4353450	52.68%	5.403%
56	23.398	3446	3453	3461	rBV2	4221609	8263518	100.00%	10.255%
57	23.551	3472	3479	3492	rVB2	2245346	4491952	54.36%	5.574%




Sum of corrected areas: 80581094

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011128.D
Acq On : 27 Jul 2022 14:12
Operator : CG/JU
Sample : N3871-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

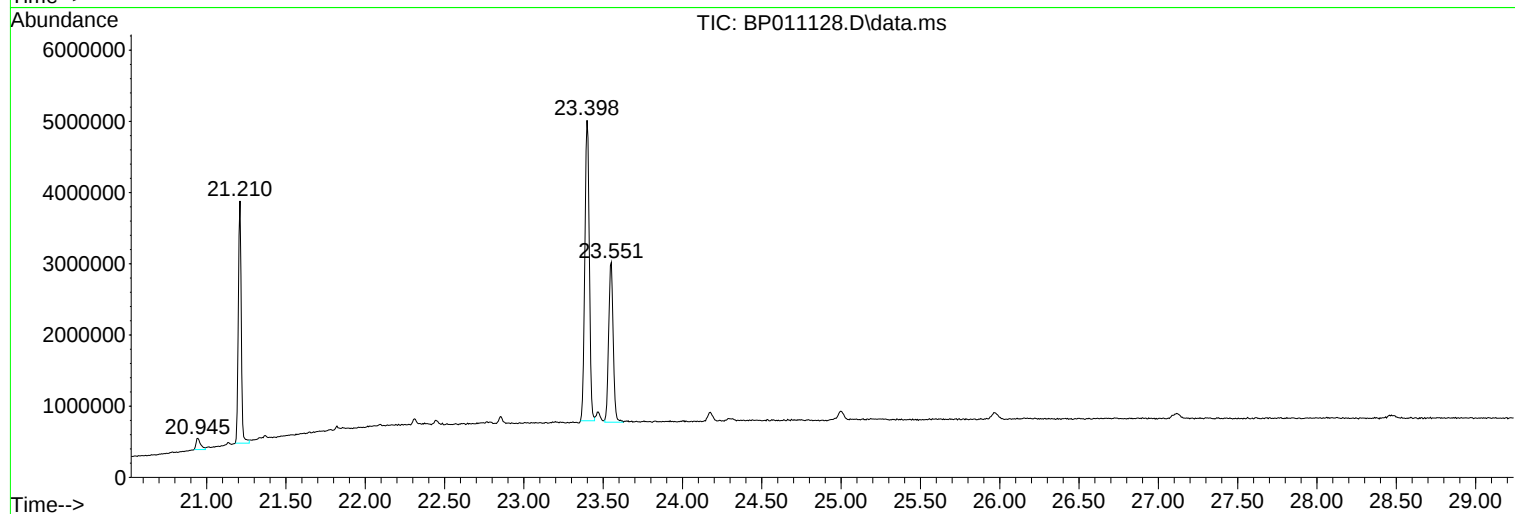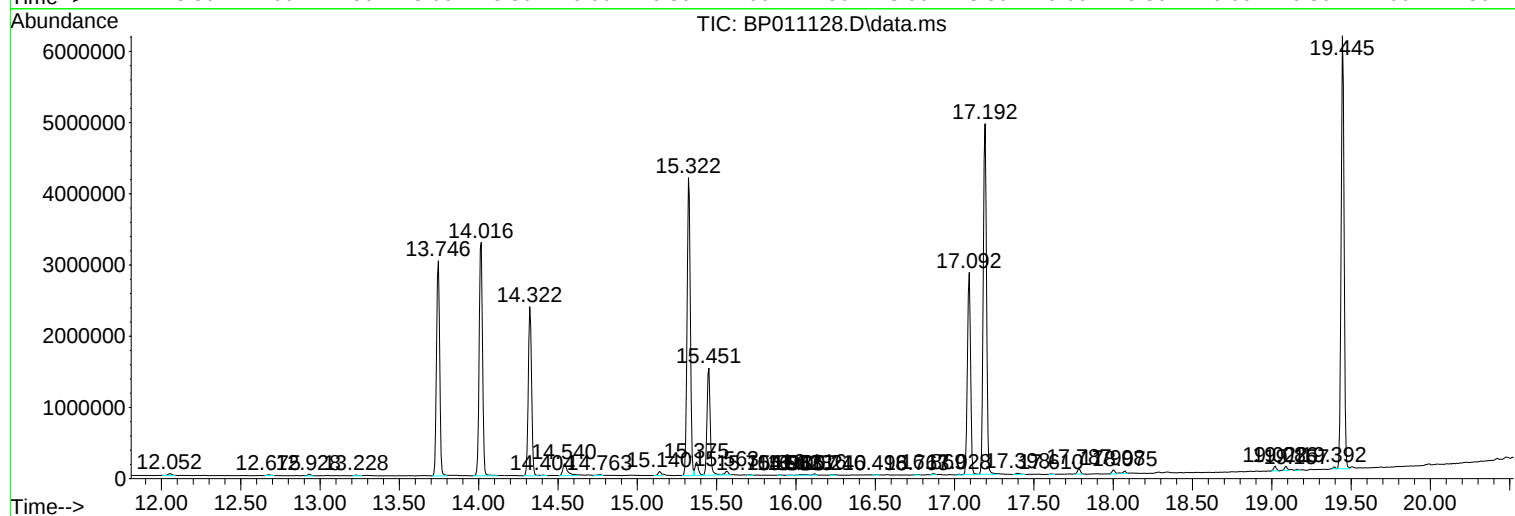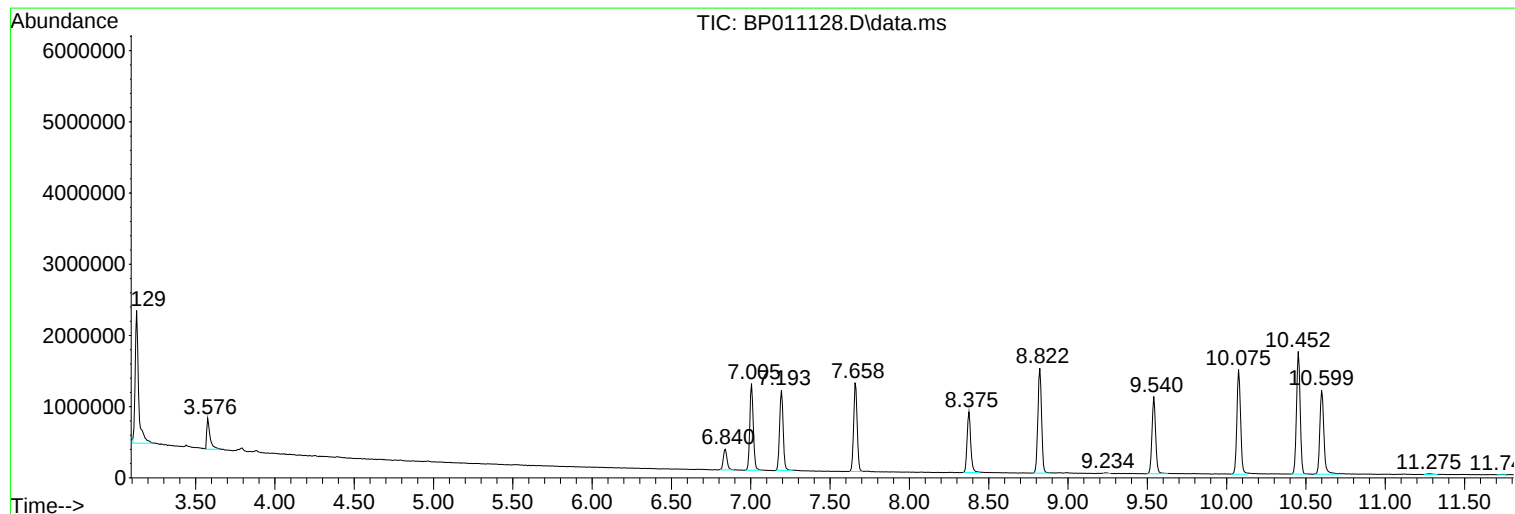

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011128.D
Acq On : 27 Jul 2022 14:12
Operator : CG/JU
Sample : N3871-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011128.D
Acq On : 27 Jul 2022 14:12
Operator : CG/JU
Sample : N3871-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc