

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011130.D
 Acq On : 27 Jul 2022 15:21
 Operator : CG/JU
 Sample : N3871-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ02

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	10	rBV	344233	425776	6.98%	0.592%
2	3.575	81	83	90	rBV	327215	434270	7.12%	0.604%
3	4.399	218	223	234	rVB	367018	530038	8.69%	0.737%
4	6.840	632	638	656	rVB	304602	511534	8.39%	0.711%
5	7.005	660	666	677	rVB	1348158	2049478	33.60%	2.850%
6	7.193	692	698	708	rBV	1237672	1865761	30.59%	2.595%
7	7.657	771	777	787	rVB	1427614	2176012	35.67%	3.026%
8	8.375	893	899	915	rBV	885159	1419339	23.27%	1.974%
9	8.822	968	975	984	rBV	1646337	2634046	43.18%	3.663%
10	9.540	1090	1097	1114	rBV	1198968	1922854	31.52%	2.674%
11	10.075	1181	1188	1203	rBV	1533891	2497942	40.95%	3.474%
12	10.451	1244	1252	1260	rBV	1964729	3182033	52.17%	4.425%
13	10.598	1270	1277	1294	rBV	1518677	2585386	42.38%	3.596%
14	11.581	1442	1444	1450	rVB6	6703	8510	0.14%	0.012%
15	11.740	1469	1471	1476	rVB3	6203	6804	0.11%	0.009%
16	12.051	1518	1524	1533	rBV4	27195	54399	0.89%	0.076%
17	12.675	1625	1630	1636	rBV10	6162	10035	0.16%	0.014%
18	12.928	1669	1673	1679	rVB7	9460	15539	0.25%	0.022%
19	13.040	1687	1692	1696	rVB8	3854	7838	0.13%	0.011%
20	13.222	1720	1723	1727	rVB6	6686	9269	0.15%	0.013%
21	13.287	1729	1734	1738	rVV5	4506	6580	0.11%	0.009%
22	13.745	1805	1812	1824	rBV	3076004	4232580	69.39%	5.886%
23	14.010	1850	1857	1873	rBV	3409994	4869514	79.83%	6.772%
24	14.322	1903	1910	1917	rBV	2645964	3711048	60.84%	5.161%
25	14.539	1941	1947	1965	rBV	83404	220787	3.62%	0.307%
26	14.757	1981	1984	1990	rVB8	6198	11021	0.18%	0.015%
27	15.139	2043	2049	2061	rBV2	38398	61867	1.01%	0.086%
28	15.322	2073	2080	2095	rBV	4255976	5893627	96.62%	8.196%
29	15.445	2095	2101	2115	rVV	1192569	1680739	27.55%	2.337%
30	15.563	2117	2121	2126	rVV2	51414	85445	1.40%	0.119%
31	15.616	2128	2130	2134	rVB5	6012	6295	0.10%	0.009%
32	15.822	2158	2165	2166	rBV6	4510	6672	0.11%	0.009%
33	16.028	2194	2200	2201	rVB6	5490	7520	0.12%	0.010%
34	16.110	2211	2214	2219	rVB5	14667	23714	0.39%	0.033%
35	16.428	2267	2268	2273	rVB5	5623	6336	0.10%	0.009%
36	16.475	2273	2276	2279	rBV5	4428	7017	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011130.D
 Acq On : 27 Jul 2022 15:21
 Operator : CG/JU
 Sample : N3871-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.575	2289	2293	2298	rBV8	5592	8172	0.13%	0.011%
38	16.769	2320	2326	2331	rBV10	6617	11210	0.18%	0.016%
39	16.869	2338	2343	2349	rBV6	12488	26552	0.44%	0.037%
40	16.975	2357	2361	2364	rBV6	6413	6679	0.11%	0.009%
41	17.086	2373	2380	2391	rBV	2494077	3605659	59.11%	5.014%
42	17.186	2391	2397	2413	rVV2	4049659	5973714	97.93%	8.308%
43	17.398	2428	2433	2436	rBV2	7811	13596	0.22%	0.019%
44	17.610	2465	2469	2473	rBV7	7323	11732	0.19%	0.016%
45	17.775	2495	2497	2503	rVB6	5188	6281	0.10%	0.009%
46	17.998	2532	2535	2541	rBV8	7864	12480	0.20%	0.017%
47	18.075	2545	2548	2553	rVB2	11549	13676	0.22%	0.019%
48	19.016	2705	2708	2714	rBV2	45176	58225	0.95%	0.081%
49	19.086	2717	2720	2725	rVV	43094	51980	0.85%	0.072%
50	19.392	2769	2772	2775	rBV5	22368	26327	0.43%	0.037%
51	19.445	2775	2781	2789	rVV	4842235	6099789	100.00%	8.483%
52	21.210	3076	3081	3089	rBV	2532318	3277160	53.73%	4.558%
53	23.398	3446	3453	3460	rBV2	3207046	6087686	99.80%	8.466%
54	23.545	3472	3478	3488	rVB2	1758983	3437345	56.35%	4.780%




Sum of corrected areas: 71905888

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011130.D
Acq On : 27 Jul 2022 15:21
Operator : CG/JU
Sample : N3871-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

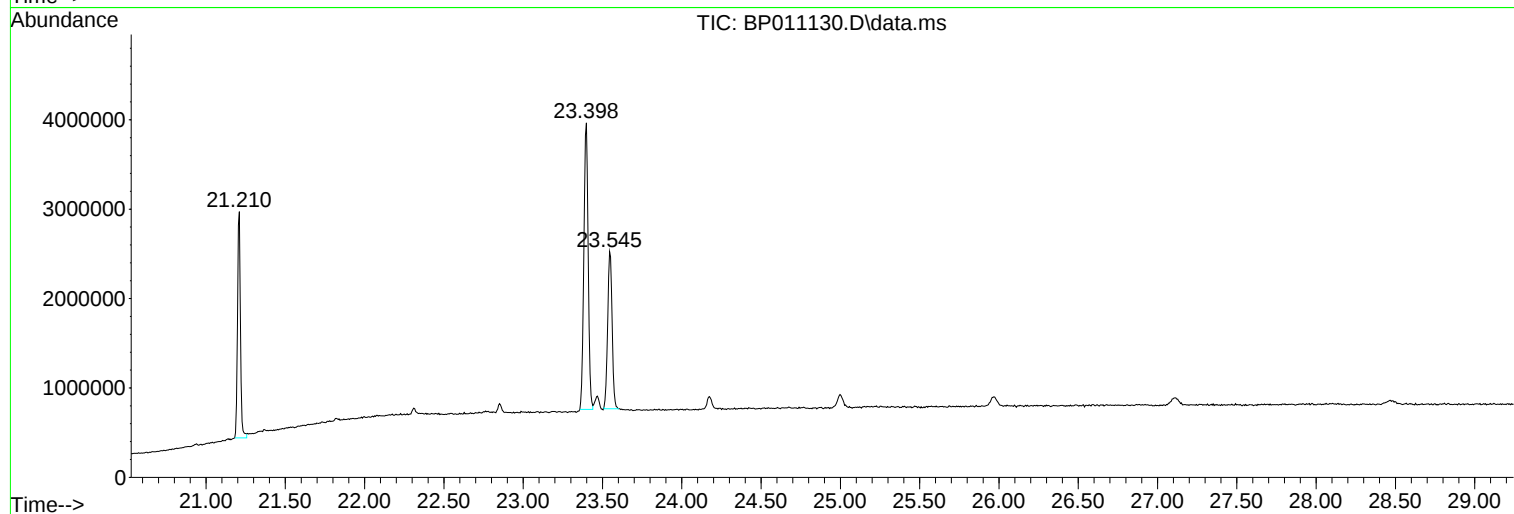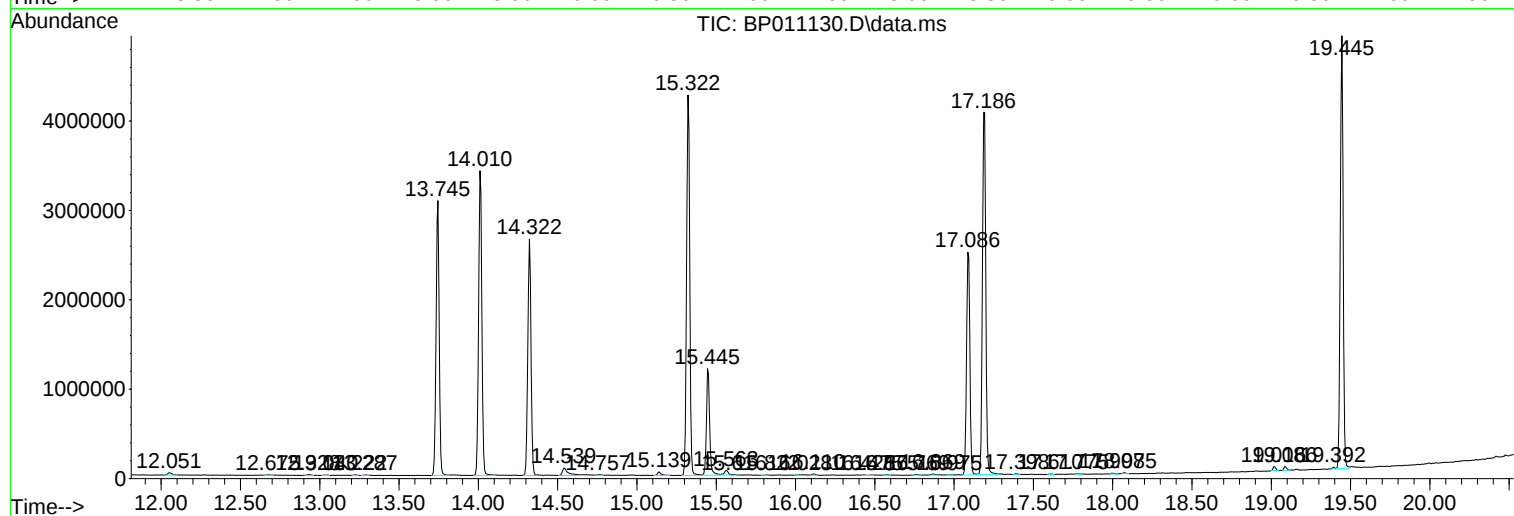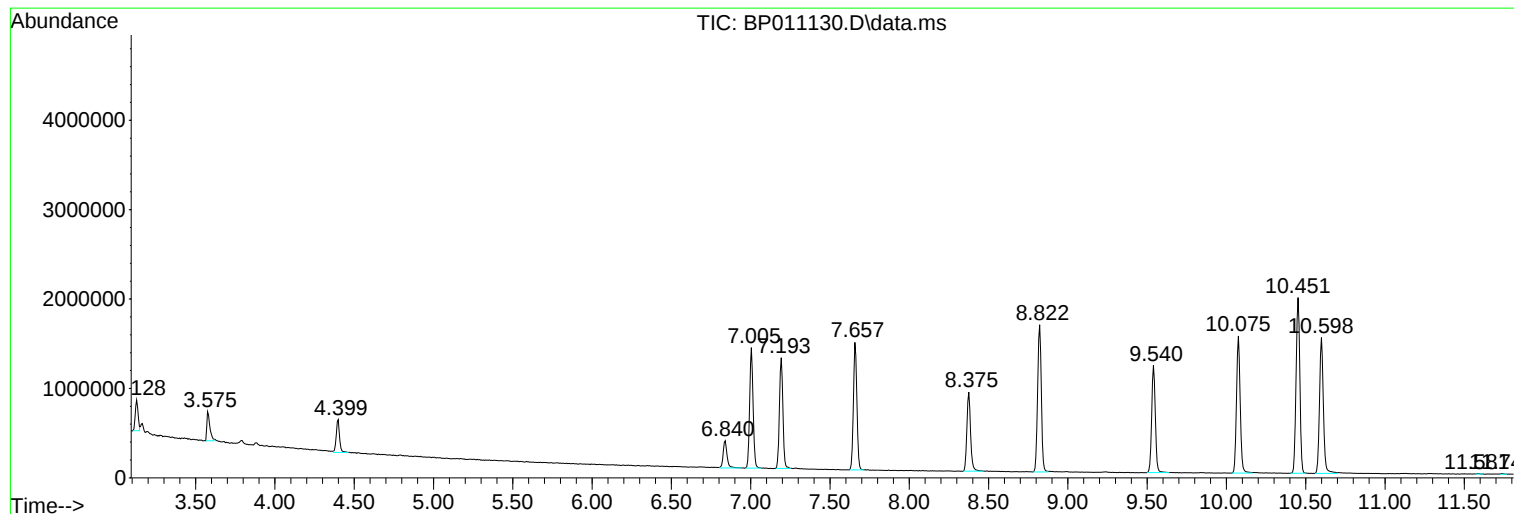

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011130.D
Acq On : 27 Jul 2022 15:21
Operator : CG/JU
Sample : N3871-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011130.D
Acq On : 27 Jul 2022 15:21
Operator : CG/JU
Sample : N3871-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc