

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011132.D
 Acq On : 27 Jul 2022 16:31
 Operator : CG/JU
 Sample : N3871-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.581	81	84	94	rVB	268726	374688	5.74%	0.601%
2	6.840	633	638	652	rVB	275629	469551	7.20%	0.753%
3	7.005	660	666	676	rVB	1247155	1888815	28.95%	3.028%
4	7.193	692	698	709	rVB	1149590	1752593	26.87%	2.810%
5	7.658	771	777	786	rVB	1265005	1938149	29.71%	3.107%
6	8.375	893	899	914	rBV	768978	1263578	19.37%	2.026%
7	8.822	968	975	984	rVB	1454448	2308665	35.39%	3.701%
8	9.052	1010	1014	1018	rVB4	9920	14195	0.22%	0.023%
9	9.234	1042	1045	1050	rVB2	15876	24320	0.37%	0.039%
10	9.540	1090	1097	1110	rBV	1028387	1660435	25.45%	2.662%
11	10.075	1180	1188	1199	rBV	1355257	2192329	33.61%	3.515%
12	10.452	1244	1252	1260	rBV	1667796	2648957	40.61%	4.247%
13	10.599	1269	1277	1293	rBV	1293199	2224385	34.10%	3.566%
14	10.810	1311	1313	1321	rVB6	4016	7615	0.12%	0.012%
15	11.016	1344	1348	1353	rBV8	5952	9174	0.14%	0.015%
16	11.116	1361	1365	1369	rVB4	8318	14855	0.23%	0.024%
17	11.734	1462	1470	1476	rBV	136093	211873	3.25%	0.340%
18	11.793	1476	1480	1489	rVB3	17980	30085	0.46%	0.048%
19	11.928	1500	1503	1507	rVB5	5105	6925	0.11%	0.011%
20	11.975	1507	1511	1514	rBV6	5133	7765	0.12%	0.012%
21	12.052	1520	1524	1530	rVB3	22127	39156	0.60%	0.063%
22	12.263	1557	1560	1568	rVB9	6821	12745	0.20%	0.020%
23	12.616	1615	1620	1626	rBV5	41001	61151	0.94%	0.098%
24	12.687	1626	1632	1637	rVB8	5238	11178	0.17%	0.018%
25	12.863	1655	1662	1670	rBV	94615	149675	2.29%	0.240%
26	12.928	1670	1673	1682	rVB7	9990	19261	0.30%	0.031%
27	13.228	1718	1724	1730	rBV5	10627	18402	0.28%	0.030%
28	13.746	1802	1812	1825	rBV	2299742	3208252	49.18%	5.143%
29	13.887	1832	1836	1841	rVB7	14079	19654	0.30%	0.032%
30	14.010	1849	1857	1866	rBV	2754441	3926251	60.19%	6.294%
31	14.322	1899	1910	1919	rBV	1981941	2848618	43.67%	4.567%
32	14.404	1922	1924	1928	rVV4	6193	8946	0.14%	0.014%
33	14.545	1943	1948	1961	rBV	61014	158982	2.44%	0.255%
34	15.140	2044	2049	2059	rVB2	36836	61859	0.95%	0.099%
35	15.322	2073	2080	2088	rBV	3231189	4524559	69.36%	7.253%
36	15.445	2095	2101	2116	rBV	905288	1284776	19.69%	2.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011132.D
 Acq On : 27 Jul 2022 16:31
 Operator : CG/JU
 Sample : N3871-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.563	2116	2121	2126	rVV3	42963	69830	1.07%	0.112%
38	15.604	2126	2128	2132	rVB5	5432	7698	0.12%	0.012%
39	16.028	2196	2200	2202	rBV5	5881	9211	0.14%	0.015%
40	16.116	2210	2215	2220	rVB6	12262	20540	0.31%	0.033%
41	16.692	2308	2313	2320	rBV	34944	47457	0.73%	0.076%
42	16.769	2320	2326	2330	rVB9	5307	12040	0.18%	0.019%
43	17.087	2372	2380	2391	rBV	1962424	2785961	42.71%	4.466%
44	17.187	2391	2397	2409	rBV2	3469447	5003039	76.69%	8.021%
45	17.392	2428	2432	2436	rVB5	6444	10782	0.17%	0.017%
46	17.769	2494	2496	2501	rVB5	6624	9675	0.15%	0.016%
47	17.957	2525	2528	2530	rBV4	5767	7648	0.12%	0.012%
48	18.010	2533	2537	2541	rVV5	15257	21723	0.33%	0.035%
49	18.075	2544	2548	2553	rVV	10886	16064	0.25%	0.026%
50	18.492	2617	2619	2622	rBV3	7974	7362	0.11%	0.012%
51	18.563	2627	2631	2634	rBV4	14031	17956	0.28%	0.029%
52	19.016	2705	2708	2713	rVB4	40611	53210	0.82%	0.085%
53	19.086	2717	2720	2726	rVB2	36197	51250	0.79%	0.082%
54	19.392	2769	2772	2775	rBV5	16628	18298	0.28%	0.029%
55	19.445	2775	2781	2789	rBV	4380559	5602501	85.88%	8.982%
56	21.210	3076	3081	3092	rBV	2390652	3201262	49.07%	5.132%
57	23.398	3446	3453	3460	rBV2	3444020	6523512	100.00%	10.458%
58	23.545	3472	3478	3487	rVB2	1788291	3478327	53.32%	5.576%




Sum of corrected areas: 62377763

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011132.D
Acq On : 27 Jul 2022 16:31
Operator : CG/JU
Sample : N3871-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

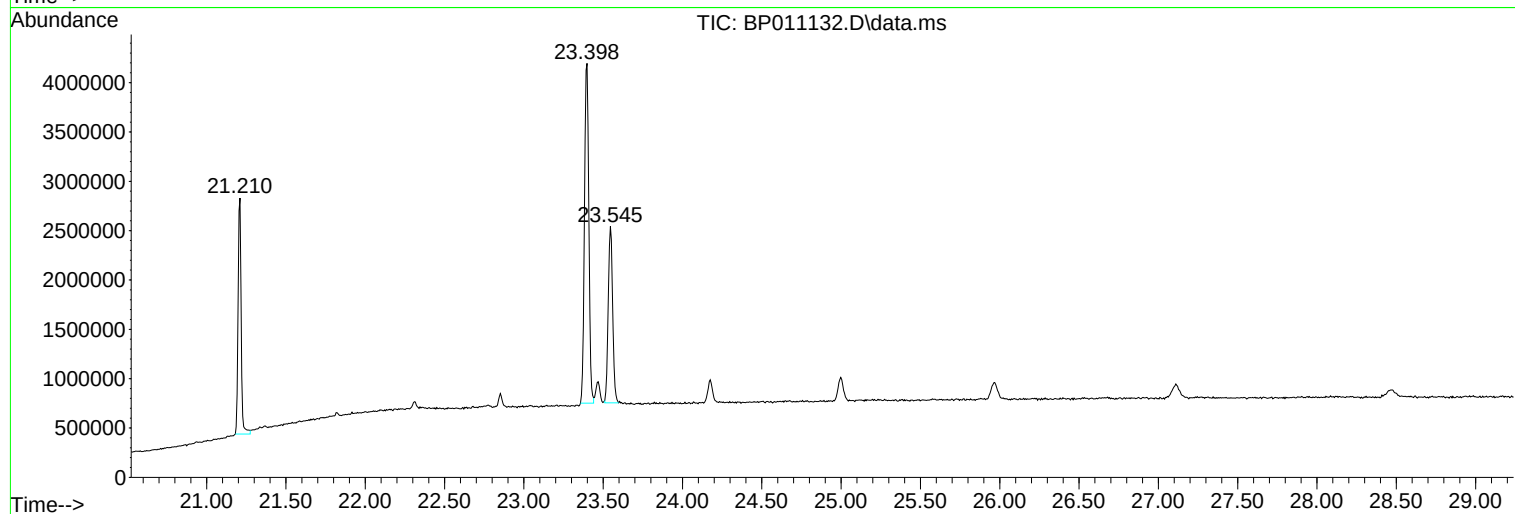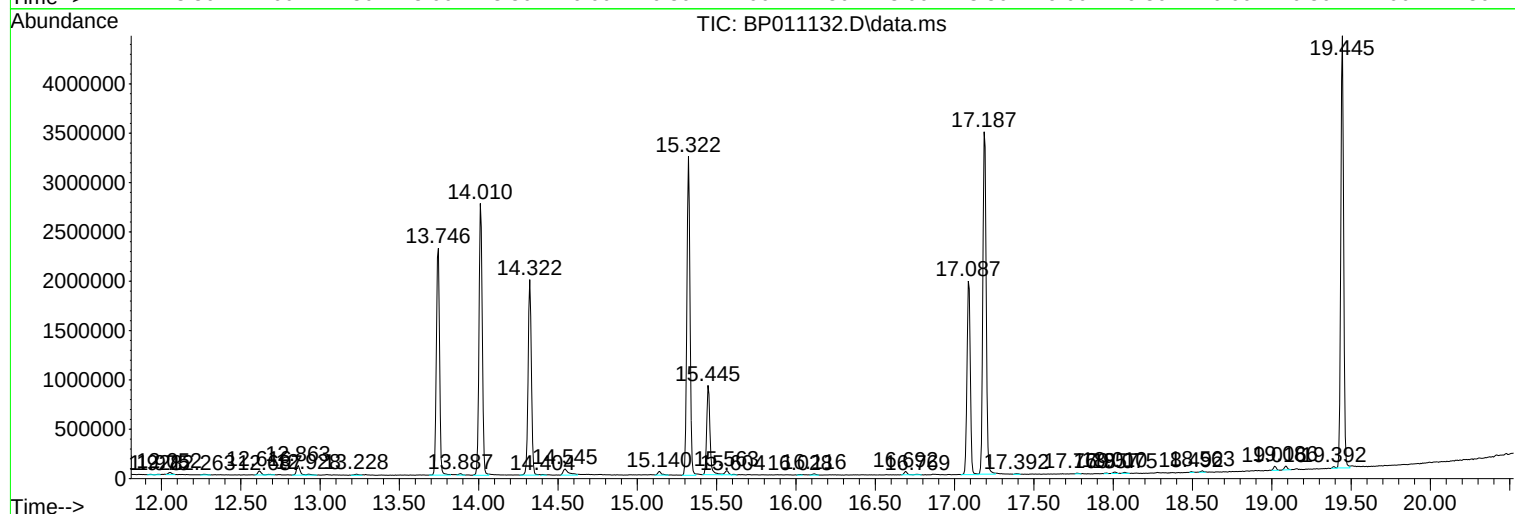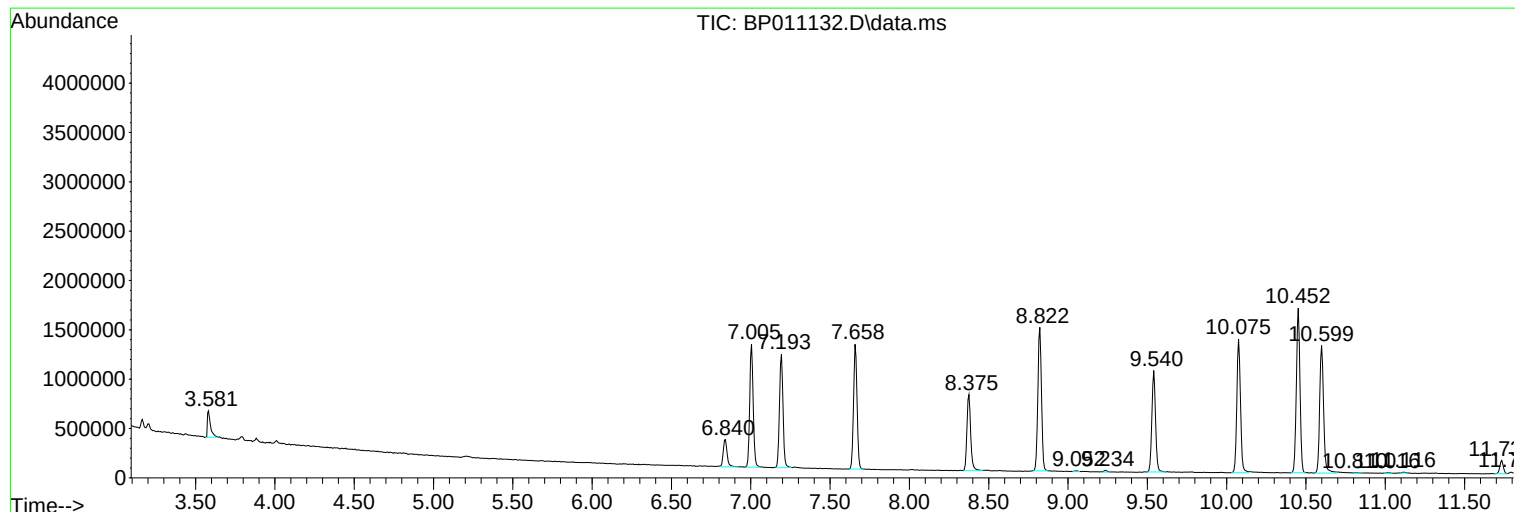

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011132.D
Acq On : 27 Jul 2022 16:31
Operator : CG/JU
Sample : N3871-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011132.D
Acq On : 27 Jul 2022 16:31
Operator : CG/JU
Sample : N3871-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc