

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011133.D
 Acq On : 27 Jul 2022 17:05
 Operator : CG/JU
 Sample : N3871-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	25	rVB	1871297	2586080	40.73%	3.570%
2	3.575	80	83	99	rVB	353215	534724	8.42%	0.738%
3	4.399	219	223	231	rVB	138507	205462	3.24%	0.284%
4	6.840	633	638	653	rVB	283397	488950	7.70%	0.675%
5	7.004	660	666	682	rVB	1311680	2044809	32.21%	2.823%
6	7.193	692	698	710	rBV	1194307	1810165	28.51%	2.499%
7	7.657	771	777	787	rBV	1441277	2195074	34.57%	3.030%
8	8.375	893	899	912	rBV	850816	1355653	21.35%	1.871%
9	8.822	968	975	990	rVB	1588505	2530940	39.86%	3.494%
10	9.234	1041	1045	1051	rVB	28257	45000	0.71%	0.062%
11	9.540	1089	1097	1108	rBV	1149648	1861797	29.33%	2.570%
12	10.075	1181	1188	1203	rBV	1501916	2454764	38.66%	3.389%
13	10.269	1217	1221	1226	rBV6	7814	16660	0.26%	0.023%
14	10.451	1245	1252	1260	rBV	1956313	3148533	49.59%	4.347%
15	10.598	1270	1277	1297	rBV	1284556	2218760	34.95%	3.063%
16	11.116	1360	1365	1373	rVB3	14913	26896	0.42%	0.037%
17	11.245	1383	1387	1392	rBV2	22680	34349	0.54%	0.047%
18	11.734	1467	1470	1476	rVB3	17792	26202	0.41%	0.036%
19	12.051	1518	1524	1530	rVB3	25524	45722	0.72%	0.063%
20	12.269	1558	1561	1566	rVB7	6483	9877	0.16%	0.014%
21	12.675	1622	1630	1637	rBV9	9065	19395	0.31%	0.027%
22	12.928	1670	1673	1676	rBV3	10457	11768	0.19%	0.016%
23	13.039	1687	1692	1696	rBV6	4363	8287	0.13%	0.011%
24	13.228	1721	1724	1729	rVB7	5030	7410	0.12%	0.010%
25	13.639	1790	1794	1798	rBV7	4623	7472	0.12%	0.010%
26	13.745	1805	1812	1823	rBV	2789466	3923352	61.80%	5.416%
27	13.845	1823	1829	1840	rVB5	20600	54767	0.86%	0.076%
28	14.010	1848	1857	1873	rBV	3096315	4594064	72.36%	6.342%
29	14.122	1873	1876	1884	rVB9	7047	14895	0.23%	0.021%
30	14.322	1901	1910	1919	rBV	2603556	3602285	56.74%	4.973%
31	14.539	1942	1947	1962	rBV3	78280	197433	3.11%	0.273%
32	14.763	1982	1985	1990	rVB6	7116	8060	0.13%	0.011%
33	15.139	2042	2049	2058	rBV	60213	89869	1.42%	0.124%
34	15.322	2073	2080	2095	rBV	4025190	5496591	86.58%	7.588%
35	15.445	2095	2101	2115	rVV	1163004	1553015	24.46%	2.144%
36	15.563	2116	2121	2128	rVB	47055	78943	1.24%	0.109%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011133.D
 Acq On : 27 Jul 2022 17:05
 Operator : CG/JU
 Sample : N3871-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.692	2142	2143	2148	rVB5	4509	7214	0.11%	0.010%
38	15.892	2173	2177	2180	rBV5	4239	6766	0.11%	0.009%
39	16.033	2194	2201	2208	rBV5	11380	32343	0.51%	0.045%
40	16.110	2210	2214	2219	rVB5	14828	23689	0.37%	0.033%
41	16.292	2240	2245	2248	rBV7	4127	6817	0.11%	0.009%
42	16.375	2255	2259	2262	rBV6	4620	6624	0.10%	0.009%
43	16.569	2288	2292	2299	rVB10	6841	12935	0.20%	0.018%
44	16.763	2320	2325	2331	rBV10	8736	16297	0.26%	0.022%
45	16.869	2339	2343	2347	rBV6	7497	12925	0.20%	0.018%
46	17.086	2374	2380	2391	rBV	2494823	3510583	55.30%	4.846%
47	17.186	2391	2397	2412	rVV2	4018876	5719056	90.08%	7.895%
48	17.392	2430	2432	2439	rVB4	9428	14696	0.23%	0.020%
49	17.492	2445	2449	2452	rBV6	5061	6801	0.11%	0.009%
50	17.998	2532	2535	2538	rBV5	7345	8342	0.13%	0.012%
51	18.075	2545	2548	2551	rVB3	11267	13879	0.22%	0.019%
52	19.022	2704	2709	2713	rBV2	46720	66718	1.05%	0.092%
53	19.086	2715	2720	2725	rBV2	47789	73824	1.16%	0.102%
54	19.157	2727	2732	2735	rVV5	18202	31796	0.50%	0.044%
55	19.392	2769	2772	2775	rBV2	20027	21318	0.34%	0.029%
56	19.445	2775	2781	2789	rBV	4532431	5976815	94.14%	8.251%
57	21.204	3076	3080	3089	rBV	2723725	3499832	55.13%	4.831%
58	23.398	3446	3453	3460	rBV	3356003	6348807	100.00%	8.764%
59	23.545	3472	3478	3487	rVB2	1935368	3711780	58.46%	5.124%




Sum of corrected areas: 72437880

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011133.D
Acq On : 27 Jul 2022 17:05
Operator : CG/JU
Sample : N3871-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

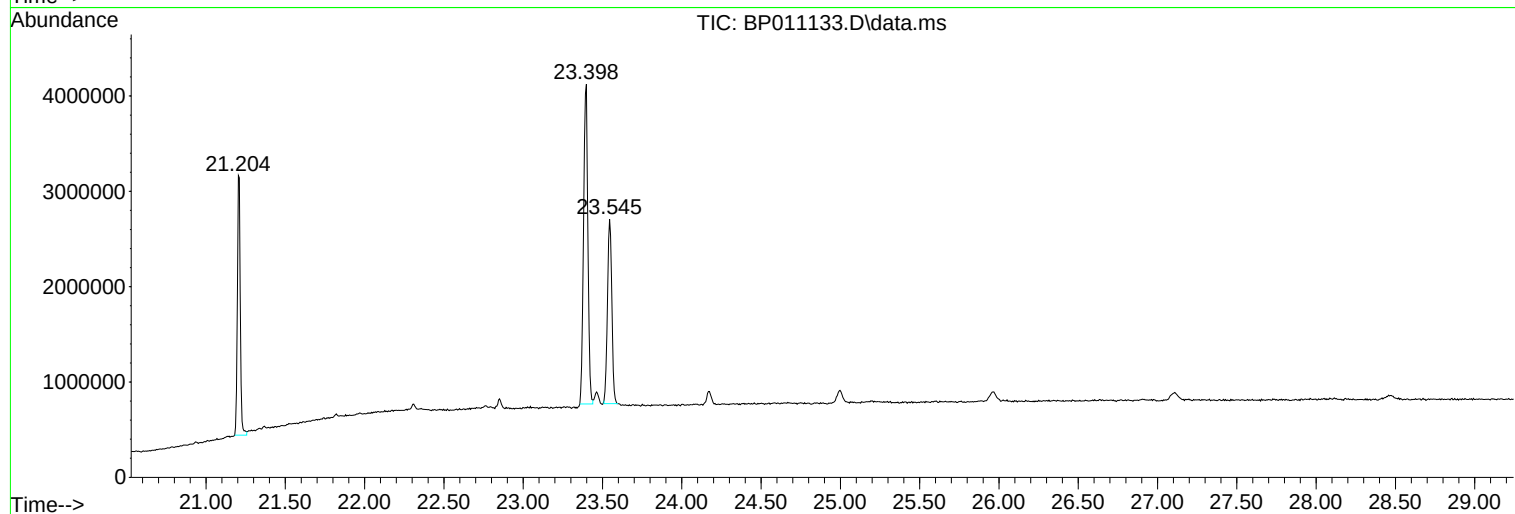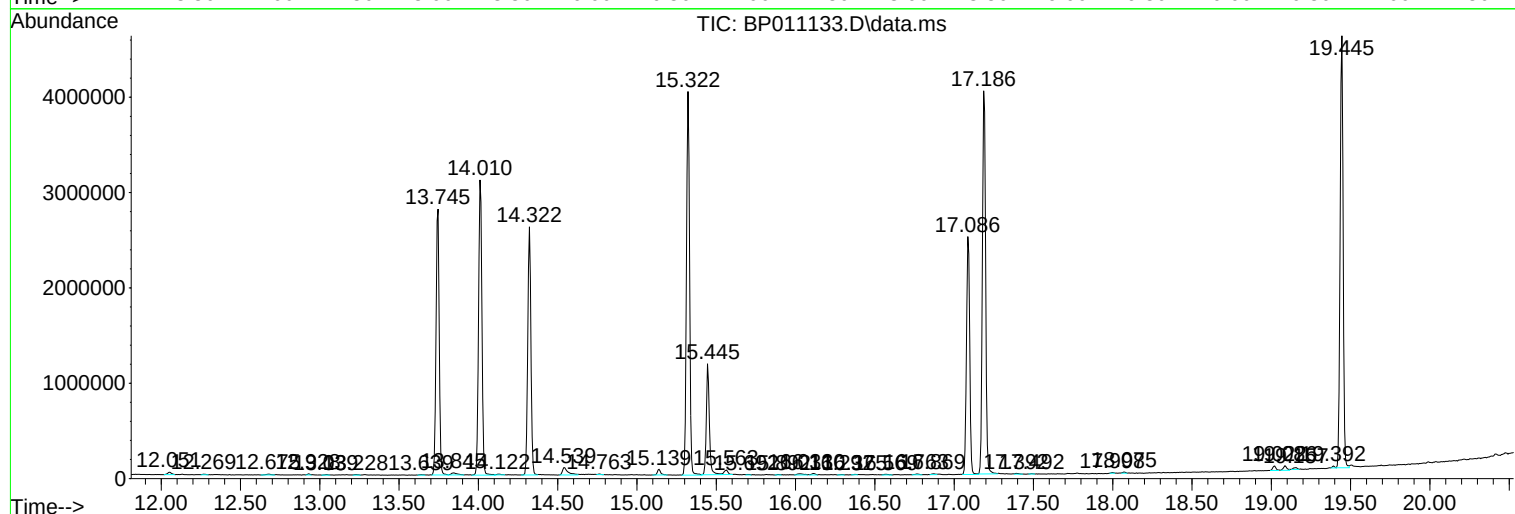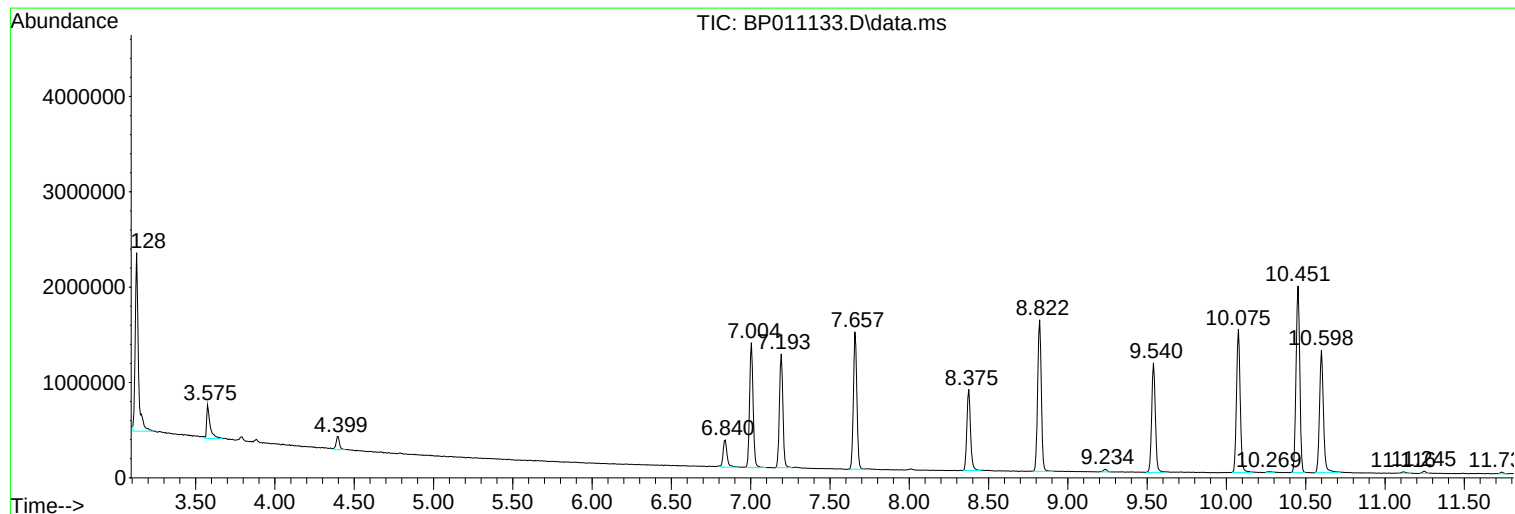

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011133.D
Acq On : 27 Jul 2022 17:05
Operator : CG/JU
Sample : N3871-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011133.D
Acq On : 27 Jul 2022 17:05
Operator : CG/JU
Sample : N3871-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc