

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011135.D
 Acq On : 27 Jul 2022 18:15
 Operator : CG/JU
 Sample : N3871-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	25	rVB	2192209	2989512	40.19%	3.796%
2	3.575	80	83	93	rBV	409144	534732	7.19%	0.679%
3	4.399	220	223	226	rVB2	106070	128720	1.73%	0.163%
4	6.834	632	637	652	rVB	309501	535639	7.20%	0.680%
5	7.005	660	666	675	rVB	1448758	2197603	29.55%	2.790%
6	7.193	692	698	709	rVB	1285252	1981208	26.64%	2.516%
7	7.657	771	777	787	rVB	1430864	2215434	29.79%	2.813%
8	8.375	892	899	912	rBV	916106	1471327	19.78%	1.868%
9	8.822	968	975	989	rVB	1740618	2803314	37.69%	3.560%
10	8.946	992	996	1001	rVB2	30792	45095	0.61%	0.057%
11	9.540	1089	1097	1113	rBV	1251932	2023504	27.21%	2.569%
12	10.075	1181	1188	1205	rBV	1631617	2647638	35.60%	3.362%
13	10.451	1245	1252	1261	rVB	1933340	3132295	42.11%	3.977%
14	10.598	1269	1277	1294	rBV	1599190	2711030	36.45%	3.442%
15	11.263	1385	1390	1394	rBV5	21404	41010	0.55%	0.052%
16	12.051	1518	1524	1529	rBV2	31350	50390	0.68%	0.064%
17	12.669	1626	1629	1633	rBV5	6708	10793	0.15%	0.014%
18	12.934	1665	1674	1680	rBV9	16518	34043	0.46%	0.043%
19	13.040	1688	1692	1697	rVB7	6819	10562	0.14%	0.013%
20	13.228	1719	1724	1729	rBV4	9887	16960	0.23%	0.022%
21	13.287	1729	1734	1739	rVV5	5504	10425	0.14%	0.013%
22	13.745	1804	1812	1823	rBV	2975820	4287445	57.64%	5.444%
23	14.010	1846	1857	1875	rBV	3409739	5074065	68.22%	6.443%
24	14.322	1903	1910	1919	rBV	2493603	3530011	47.46%	4.482%
25	14.539	1941	1947	1959	rBV	95820	216367	2.91%	0.275%
26	14.757	1981	1984	1992	rVB10	7532	12851	0.17%	0.016%
27	15.139	2044	2049	2056	rBV2	37351	57009	0.77%	0.072%
28	15.322	2073	2080	2087	rBV	4496883	6118850	82.27%	7.769%
29	15.445	2095	2101	2114	rBV	1254796	1710442	23.00%	2.172%
30	15.563	2115	2121	2134	rVB	56244	101866	1.37%	0.129%
31	15.704	2142	2145	2149	rVB5	5564	8238	0.11%	0.010%
32	15.898	2173	2178	2181	rBV7	6819	8326	0.11%	0.011%
33	16.016	2193	2198	2200	rBV6	5567	9047	0.12%	0.011%
34	16.116	2210	2215	2221	rVB5	15574	24528	0.33%	0.031%
35	16.763	2320	2325	2331	rVB7	7371	12974	0.17%	0.016%
36	16.869	2339	2343	2347	rBV6	10894	18322	0.25%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011135.D
 Acq On : 27 Jul 2022 18:15
 Operator : CG/JU
 Sample : N3871-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	17.028	2367	2370	2373	rBV4	5819	7804	0.10%	0.010%
38	17.086	2374	2380	2390	rVV	2546082	3545860	47.67%	4.502%
39	17.186	2391	2397	2413	rVV2	4547435	6295292	84.64%	7.994%
40	17.392	2429	2432	2438	rVB2	13390	17036	0.23%	0.022%
41	17.769	2494	2496	2503	rVB7	8984	12723	0.17%	0.016%
42	17.998	2531	2535	2539	rBV6	16628	22552	0.30%	0.029%
43	18.069	2544	2547	2551	rVV	26328	33037	0.44%	0.042%
44	19.016	2704	2708	2713	rBV3	54016	71933	0.97%	0.091%
45	19.086	2716	2720	2724	rVV	49378	62455	0.84%	0.079%
46	19.392	2769	2772	2774	rBV4	17942	19177	0.26%	0.024%
47	19.445	2775	2781	2789	rVV	5227614	6865231	92.30%	8.717%
48	21.204	3076	3080	3090	rBV	2863477	3649095	49.06%	4.633%
49	23.398	3446	3453	3461	rBV2	3951375	7437794	100.00%	9.444%
50	23.545	3472	3478	3487	rVB	2048803	3933278	52.88%	4.994%




Sum of corrected areas: 78754842

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011135.D
Acq On : 27 Jul 2022 18:15
Operator : CG/JU
Sample : N3871-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

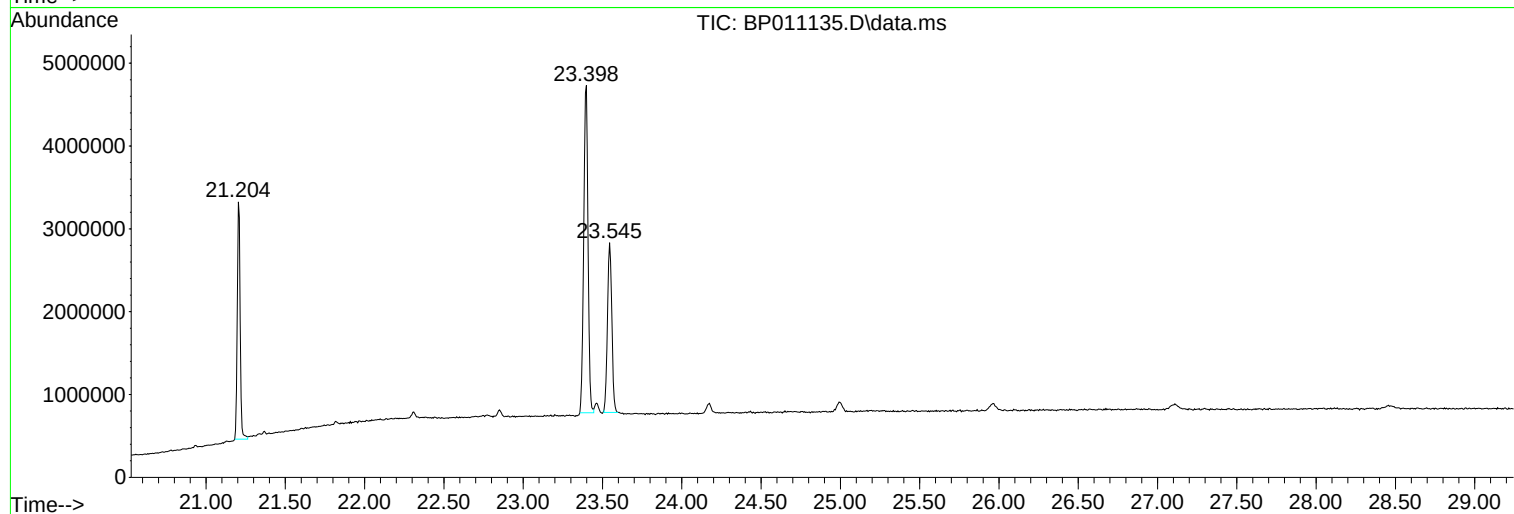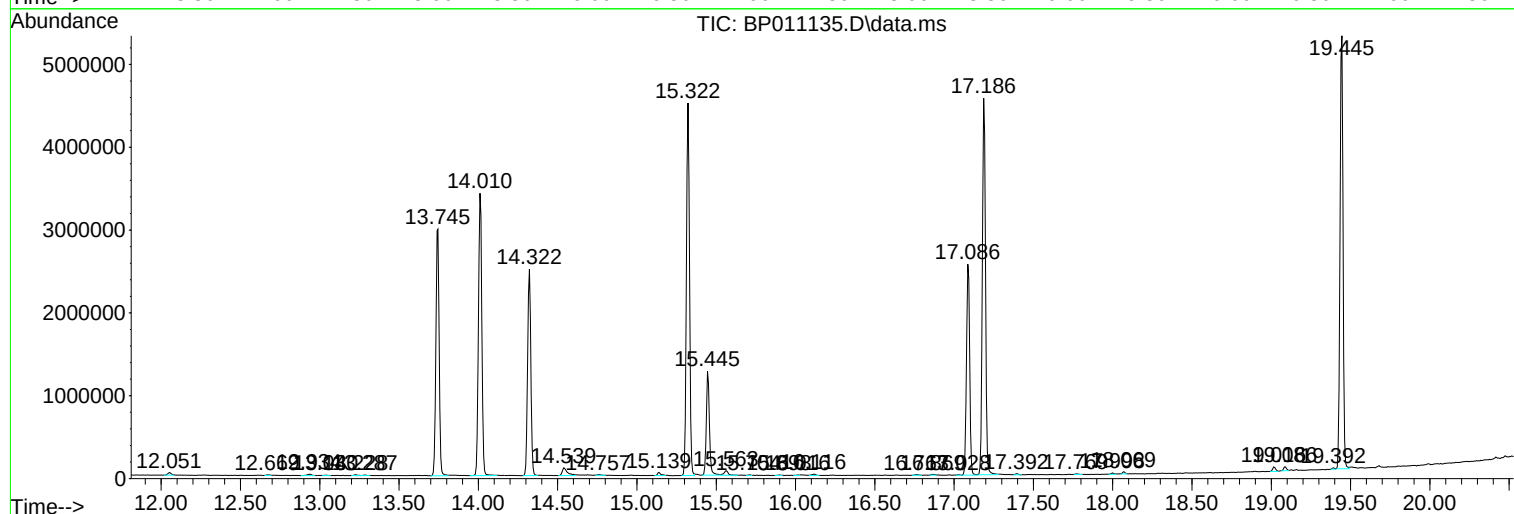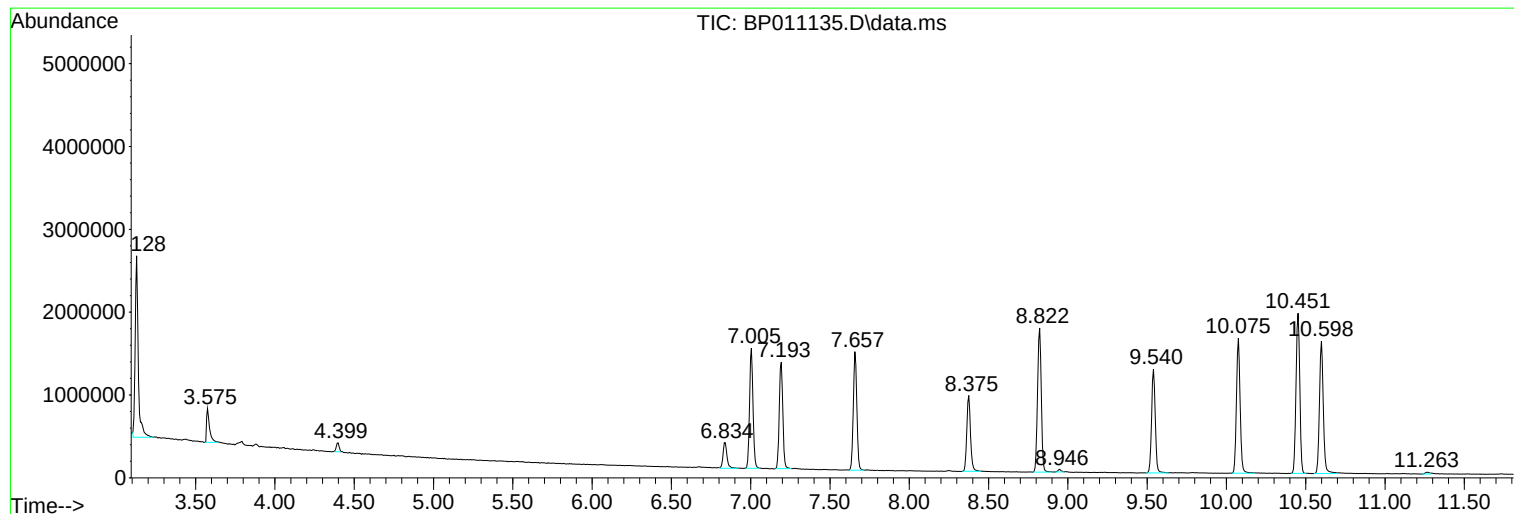

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011135.D
Acq On : 27 Jul 2022 18:15
Operator : CG/JU
Sample : N3871-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011135.D
Acq On : 27 Jul 2022 18:15
Operator : CG/JU
Sample : N3871-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc