

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011136.D
 Acq On : 27 Jul 2022 18:50
 Operator : CG/JU
 Sample : N3871-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	11	rBV	847694	1153629	15.14%	1.606%
2	3.575	81	83	94	rBV	332476	472318	6.20%	0.658%
3	6.840	632	638	644	rBV	309985	467402	6.13%	0.651%
4	7.004	660	666	676	rVB	1342193	2035161	26.71%	2.833%
5	7.193	692	698	710	rVB	1277451	1947138	25.56%	2.711%
6	7.657	771	777	787	rBV	1357083	2098835	27.55%	2.922%
7	8.375	893	899	914	rVB	896018	1441933	18.93%	2.007%
8	8.822	968	975	988	rVB	1611536	2553800	33.52%	3.555%
9	9.234	1041	1045	1052	rVB2	34889	53228	0.70%	0.074%
10	9.539	1090	1097	1112	rBV	1154247	1869653	24.54%	2.603%
11	10.075	1181	1188	1206	rBV	1591867	2636345	34.60%	3.670%
12	10.257	1213	1219	1224	rBV5	23175	52712	0.69%	0.073%
13	10.451	1245	1252	1259	rBV	1740722	2824663	37.07%	3.933%
14	10.598	1270	1277	1294	rBV	653529	1334274	17.51%	1.858%
15	11.110	1362	1364	1372	rVB6	8559	17731	0.23%	0.025%
16	11.245	1383	1387	1392	rBV4	9438	18821	0.25%	0.026%
17	11.733	1466	1470	1476	rVB2	21630	34709	0.46%	0.048%
18	12.051	1519	1524	1533	rVB	29941	52204	0.69%	0.073%
19	12.675	1626	1630	1636	rVB8	7696	12840	0.17%	0.018%
20	12.928	1668	1673	1677	rVB5	8238	11844	0.16%	0.016%
21	13.739	1805	1811	1823	rBV	2817937	3980809	52.25%	5.542%
22	13.851	1825	1830	1839	rVB	7416	22737	0.30%	0.032%
23	14.010	1850	1857	1871	rBV	3241038	4688116	61.53%	6.527%
24	14.122	1872	1876	1882	rVV7	9621	17283	0.23%	0.024%
25	14.227	1891	1894	1899	rVB6	5754	9715	0.13%	0.014%
26	14.322	1903	1910	1918	rBV	2152081	3034234	39.82%	4.224%
27	14.539	1941	1947	1959	rBV	102159	223932	2.94%	0.312%
28	14.698	1969	1974	1980	rBV2	29229	53556	0.70%	0.075%
29	14.757	1982	1984	1989	rVB6	7879	10420	0.14%	0.015%
30	15.139	2043	2049	2055	rBV2	25563	38847	0.51%	0.054%
31	15.322	2073	2080	2092	rBV	4126209	5576700	73.20%	7.764%
32	15.445	2095	2101	2115	rVV	1192953	1649303	21.65%	2.296%
33	15.563	2115	2121	2127	rVV3	51014	91531	1.20%	0.127%
34	16.116	2211	2215	2218	rVV3	17361	19693	0.26%	0.027%
35	16.369	2255	2258	2264	rBV8	7047	12799	0.17%	0.018%
36	16.569	2286	2292	2294	rBV7	7157	11419	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011136.D
 Acq On : 27 Jul 2022 18:50
 Operator : CG/JU
 Sample : N3871-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.768	2321	2326	2330	rVB8	7899	9287	0.12%	0.013%
38	17.021	2366	2369	2374	rBV7	8397	10605	0.14%	0.015%
39	17.086	2374	2380	2387	rBV	2291448	3126758	41.04%	4.353%
40	17.186	2391	2397	2411	rVV2	4313082	5989060	78.61%	8.338%
41	17.298	2414	2416	2422	rVB7	8320	12818	0.17%	0.018%
42	17.392	2428	2432	2435	rBV2	9648	13781	0.18%	0.019%
43	17.492	2444	2449	2454	rBV8	10968	19579	0.26%	0.027%
44	17.716	2483	2487	2491	rBV6	18124	26448	0.35%	0.037%
45	17.780	2493	2498	2504	rVV3	45530	68578	0.90%	0.095%
46	17.998	2530	2535	2541	rBV5	32695	58215	0.76%	0.081%
47	18.074	2544	2548	2553	rVB2	20065	30749	0.40%	0.043%
48	19.015	2705	2708	2713	rBV2	51085	67481	0.89%	0.094%
49	19.086	2716	2720	2724	rBV	51658	69270	0.91%	0.096%
50	19.445	2775	2781	2788	rBV	5484664	6861569	90.06%	9.553%
51	21.209	3076	3081	3086	rBV	2722925	3492364	45.84%	4.862%
52	23.398	3446	3453	3460	rBV2	4031596	7618950	100.00%	10.607%
53	23.545	3472	3478	3488	rVB2	1990811	3822563	50.17%	5.322%




Sum of corrected areas: 71828409

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011136.D
Acq On : 27 Jul 2022 18:50
Operator : CG/JU
Sample : N3871-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

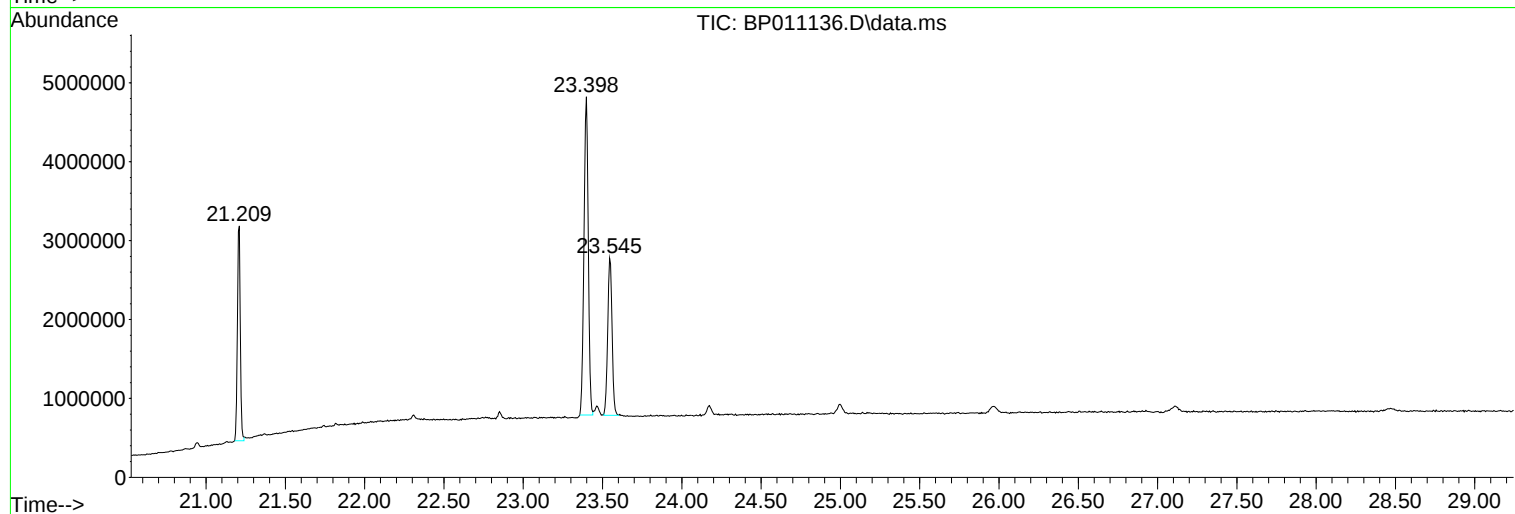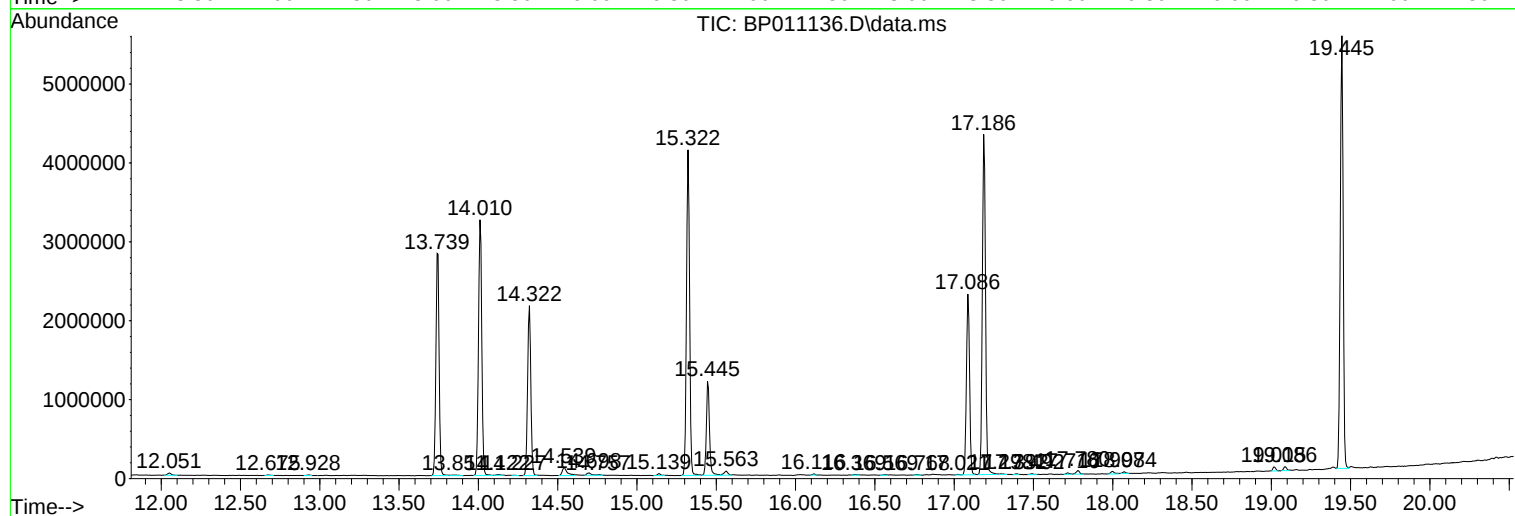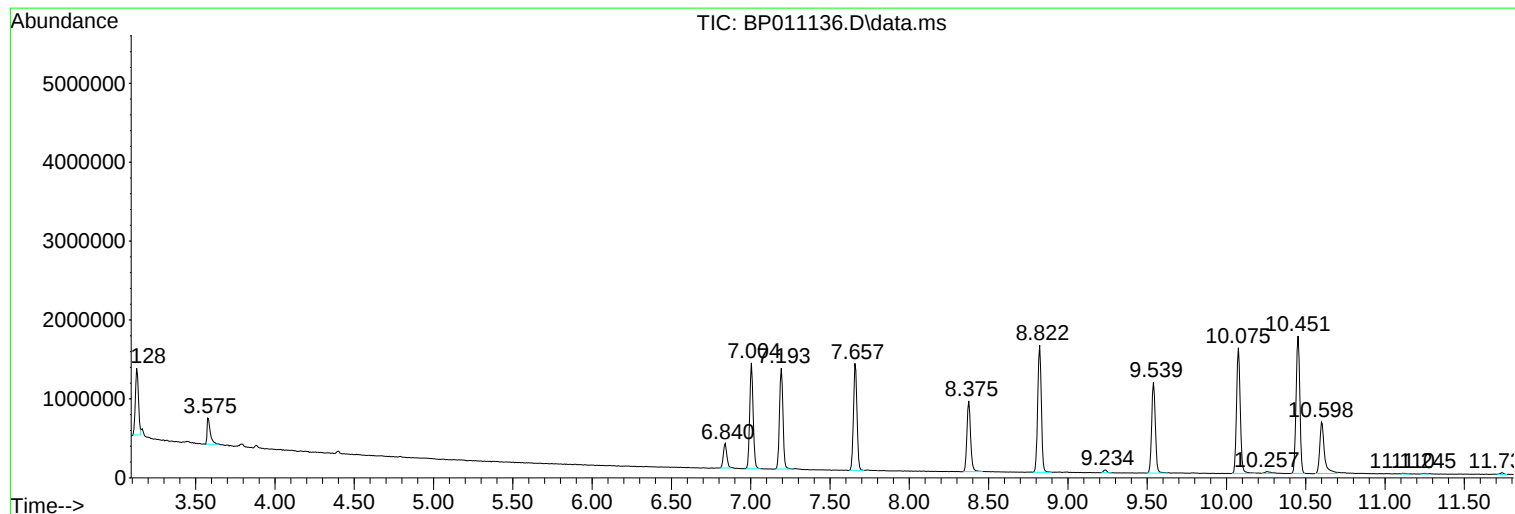

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011136.D
Acq On : 27 Jul 2022 18:50
Operator : CG/JU
Sample : N3871-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011136.D
Acq On : 27 Jul 2022 18:50
Operator : CG/JU
Sample : N3871-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc