

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011137.D
 Acq On : 27 Jul 2022 19:24
 Operator : CG/JU
 Sample : N3871-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	11	rBV	743662	929311	12.37%	1.362%
2	3.575	81	83	95	rVB	372573	521390	6.94%	0.764%
3	6.840	633	638	649	rVB	282774	460820	6.13%	0.675%
4	7.005	660	666	677	rVB	1288344	1985000	26.42%	2.910%
5	7.193	692	698	709	rVB	1155416	1799889	23.95%	2.638%
6	7.658	771	777	789	rVB	1177822	1822544	24.25%	2.671%
7	8.375	892	899	917	rBV	794892	1299498	17.29%	1.905%
8	8.822	968	975	984	rBV	1501833	2415632	32.15%	3.541%
9	8.946	992	996	1002	rBV2	32567	50816	0.68%	0.074%
10	9.540	1090	1097	1106	rBV	1058376	1726801	22.98%	2.531%
11	10.075	1180	1188	1203	rBV	1424933	2314975	30.81%	3.393%
12	10.452	1244	1252	1262	rBV	1496046	2472848	32.91%	3.625%
13	10.599	1270	1277	1295	rBV	1391559	2393162	31.85%	3.508%
14	11.122	1362	1366	1371	rVB7	5624	10260	0.14%	0.015%
15	11.269	1387	1391	1397	rBV9	7389	17699	0.24%	0.026%
16	12.051	1518	1524	1529	rBV2	27123	45494	0.61%	0.067%
17	12.675	1623	1630	1636	rVB9	8301	15914	0.21%	0.023%
18	12.934	1670	1674	1682	rVB9	12706	24393	0.32%	0.036%
19	13.228	1719	1724	1729	rVB6	7834	12477	0.17%	0.018%
20	13.287	1729	1734	1737	rBV7	4904	9487	0.13%	0.014%
21	13.740	1805	1811	1820	rBV	2478375	3535338	47.05%	5.182%
22	14.010	1846	1857	1872	rBV	2985992	4301524	57.24%	6.305%
23	14.322	1903	1910	1923	rBV	1921337	2717098	36.16%	3.983%
24	14.540	1942	1947	1963	rBV	84858	210126	2.80%	0.308%
25	14.763	1981	1985	1992	rVB7	8498	16653	0.22%	0.024%
26	15.140	2044	2049	2057	rBV2	28124	40579	0.54%	0.059%
27	15.322	2070	2080	2095	rBV	3804226	5243067	69.77%	7.685%
28	15.445	2095	2101	2113	rVV	1162123	1544540	20.55%	2.264%
29	15.563	2113	2121	2126	rVB4	47440	110689	1.47%	0.162%
30	16.028	2195	2200	2202	rBV6	5022	8095	0.11%	0.012%
31	16.116	2210	2215	2222	rVB5	15391	25290	0.34%	0.037%
32	16.769	2320	2326	2330	rBV9	9263	17121	0.23%	0.025%
33	16.863	2338	2342	2346	rVB6	10171	13767	0.18%	0.020%
34	17.028	2366	2370	2374	rBV7	5490	9017	0.12%	0.013%
35	17.086	2374	2380	2388	rVV	2157632	2917806	38.83%	4.277%
36	17.186	2390	2397	2412	rVV2	4112123	5780723	76.93%	8.473%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011137.D
 Acq On : 27 Jul 2022 19:24
 Operator : CG/JU
 Sample : N3871-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	17.392	2429	2432	2436	rBV2	11386	11242	0.15%	0.016%
38	17.998	2531	2535	2542	rBV10	10459	15530	0.21%	0.023%
39	18.069	2543	2547	2551	rVV	28679	34615	0.46%	0.051%
40	19.016	2705	2708	2714	rVB2	48103	58689	0.78%	0.086%
41	19.086	2716	2720	2724	rBV	50689	65254	0.87%	0.096%
42	19.392	2769	2772	2775	rBV4	20962	23746	0.32%	0.035%
43	19.445	2775	2781	2788	rBV	5205980	6846390	91.11%	10.035%
44	21.204	3076	3080	3090	rBV	2653098	3317828	44.15%	4.863%
45	23.392	3445	3452	3460	rBV2	3859302	7514369	100.00%	11.014%
46	23.545	3471	3478	3487	rVB2	1783529	3515767	46.79%	5.153%




Sum of corrected areas: 68223273

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011137.D
Acq On : 27 Jul 2022 19:24
Operator : CG/JU
Sample : N3871-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

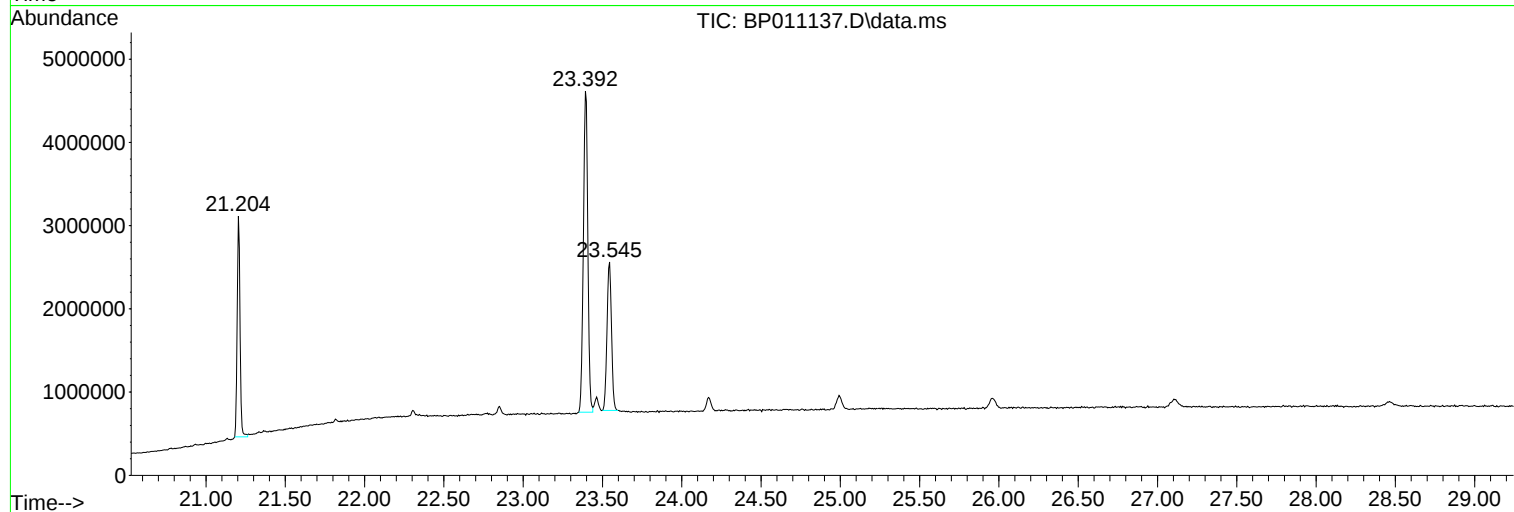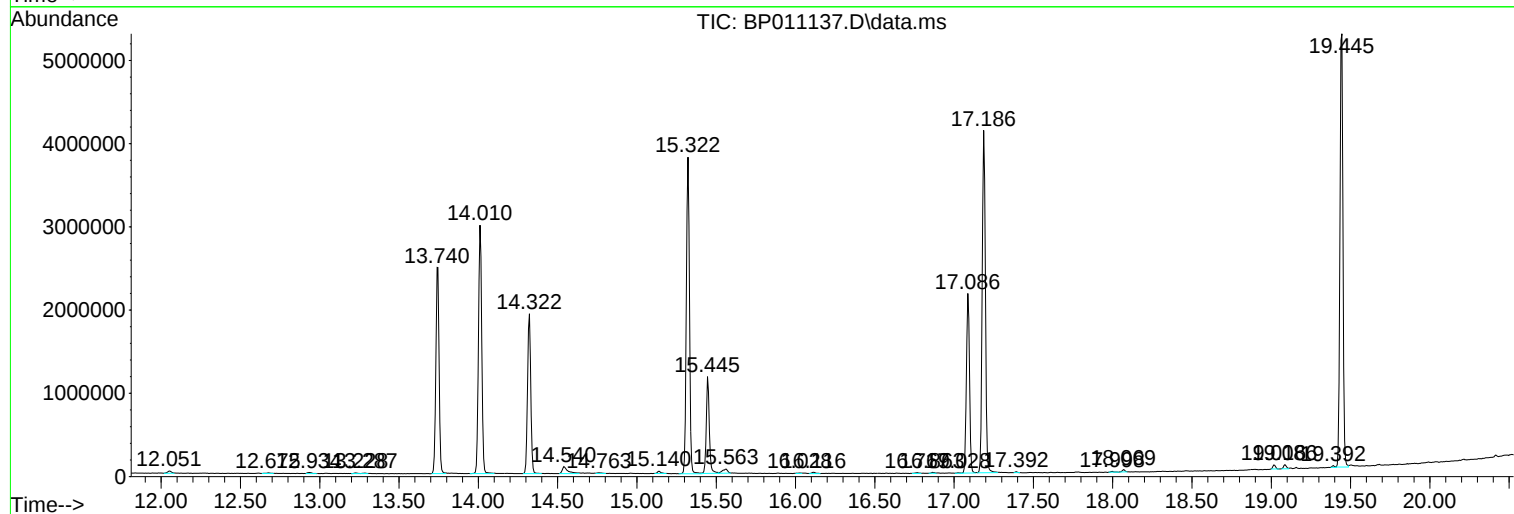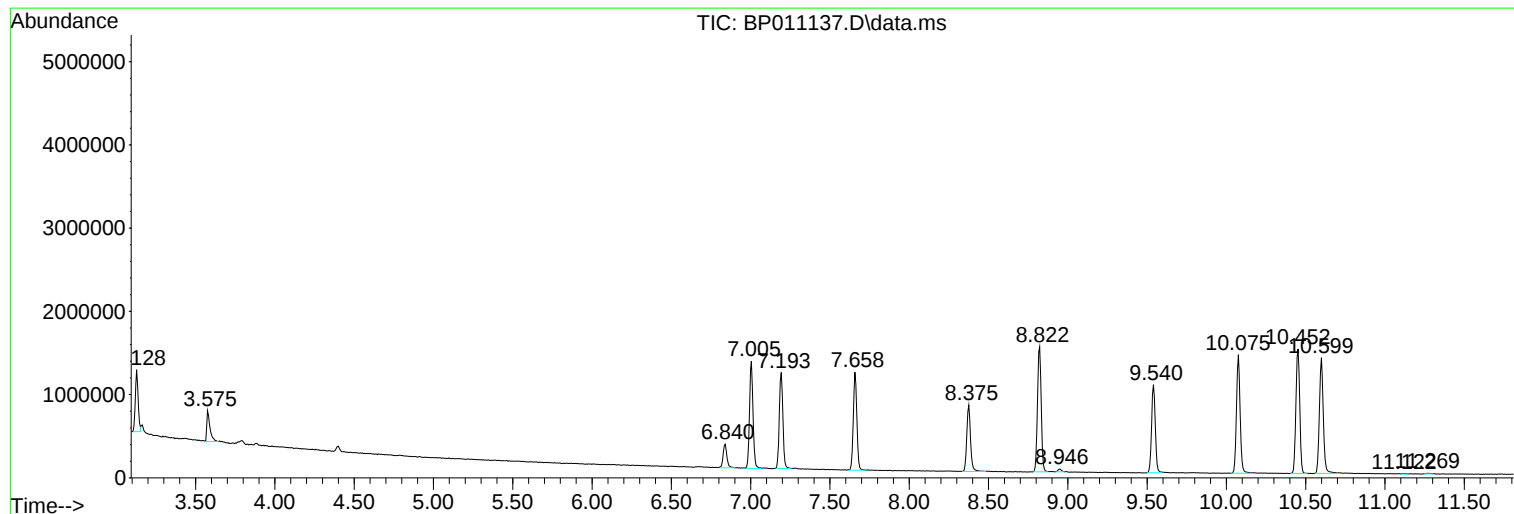

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011137.D
Acq On : 27 Jul 2022 19:24
Operator : CG/JU
Sample : N3871-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011137.D
Acq On : 27 Jul 2022 19:24
Operator : CG/JU
Sample : N3871-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc