

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011140.D
 Acq On : 27 Jul 2022 21:43
 Operator : CG/JU
 Sample : PB146443BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK443

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	10	12	20	rVB	134851	167807	2.52%	0.208%
2	3.570	79	82	99	rVB	1544803	2129955	32.03%	2.635%
3	6.834	631	637	650	rBV	1740132	2727673	41.02%	3.374%
4	7.005	660	666	680	rVB	1480558	2315094	34.82%	2.864%
5	7.193	691	698	710	rVB	1803810	2818691	42.39%	3.487%
6	7.658	771	777	786	rVB	1354930	2062588	31.02%	2.552%
7	8.375	892	899	909	rBV	2011137	3258885	49.01%	4.032%
8	8.822	968	975	985	rBV	1712856	2822275	42.45%	3.492%
9	9.540	1090	1097	1106	rBV	1329471	2151782	32.36%	2.662%
10	10.075	1181	1188	1210	rBV	1812738	3086066	46.41%	3.818%
11	10.452	1244	1252	1260	rBV	1741166	2903946	43.67%	3.593%
12	10.599	1269	1277	1293	rBV	1879479	3270453	49.19%	4.046%
13	12.057	1518	1525	1535	rVB2	25472	52707	0.79%	0.065%
14	13.287	1730	1734	1739	rVB3	6496	8783	0.13%	0.011%
15	13.740	1803	1811	1823	rBV	3055208	4065113	61.14%	5.029%
16	14.010	1850	1857	1872	rBV	3493094	5007577	75.31%	6.195%
17	14.322	1901	1910	1918	rBV	2252218	3275933	49.27%	4.053%
18	14.534	1939	1946	1969	rBV	1025401	1783266	26.82%	2.206%
19	15.322	2073	2080	2095	rBV	4156869	5761440	86.65%	7.128%
20	15.445	2095	2101	2115	rVV	1136105	1561762	23.49%	1.932%
21	15.563	2116	2121	2127	rVB	49159	77104	1.16%	0.095%
22	16.110	2207	2214	2219	rBV6	14244	22655	0.34%	0.028%
23	16.769	2321	2326	2329	rVB7	5960	8882	0.13%	0.011%
24	16.875	2337	2344	2347	rBV7	5438	11792	0.18%	0.015%
25	17.086	2372	2380	2390	rBV	2409525	3356061	50.47%	4.152%
26	17.186	2390	2397	2415	rVV	4000908	5681271	85.44%	7.028%
27	19.016	2704	2708	2713	rBV3	45749	63514	0.96%	0.079%
28	19.086	2716	2720	2725	rBV	42347	60627	0.91%	0.075%
29	19.439	2774	2780	2789	rBV	4869589	6290634	94.61%	7.782%
30	21.204	3075	3080	3089	rBV	2912949	3636552	54.69%	4.499%
31	23.392	3445	3452	3460	rBV2	3633519	6649155	100.00%	8.226%
32	23.539	3471	3477	3487	rVB2	1931595	3742300	56.28%	4.630%




Sum of corrected areas: 80832343

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011140.D
Acq On : 27 Jul 2022 21:43
Operator : CG/JU
Sample : PB146443BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

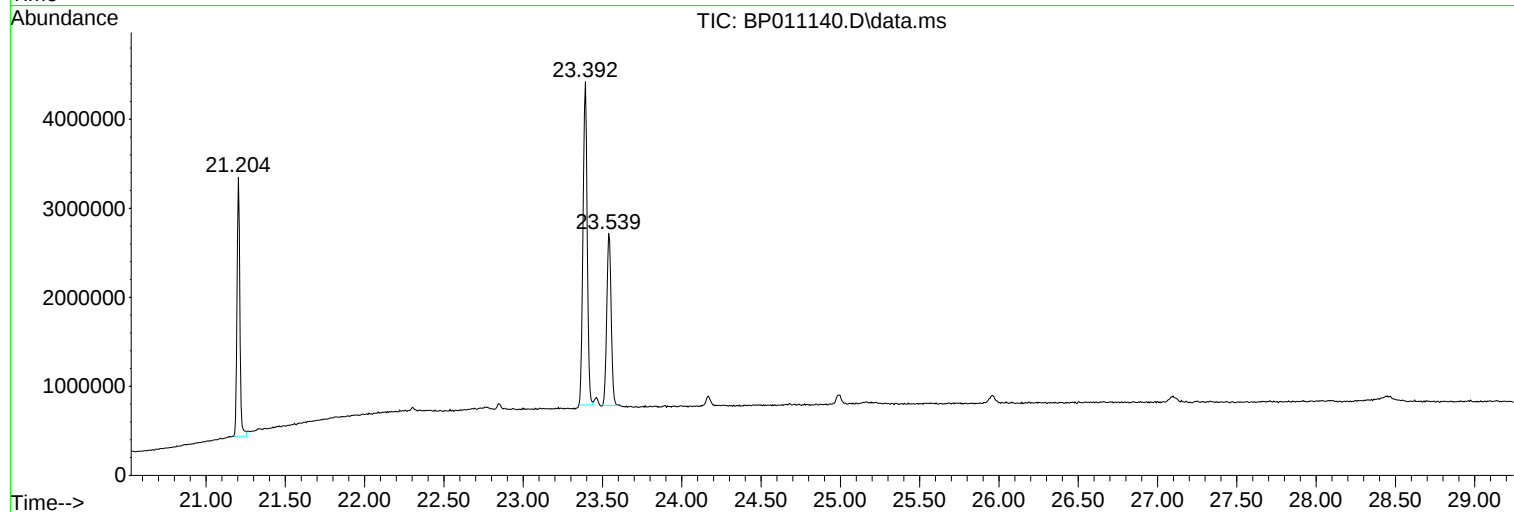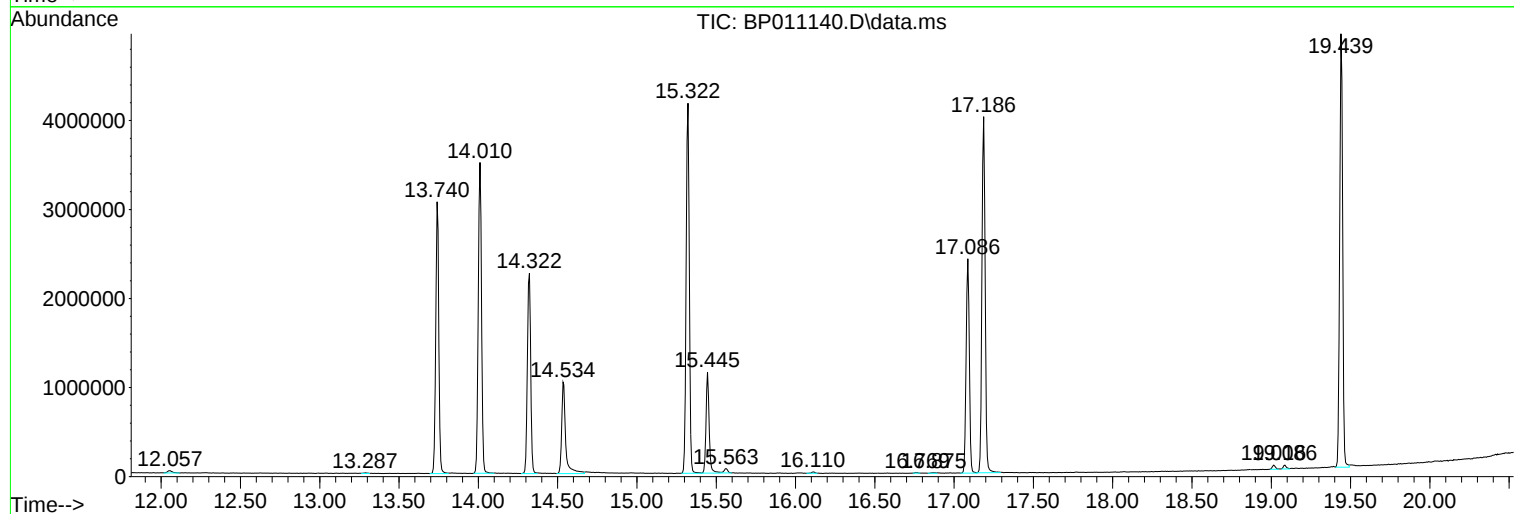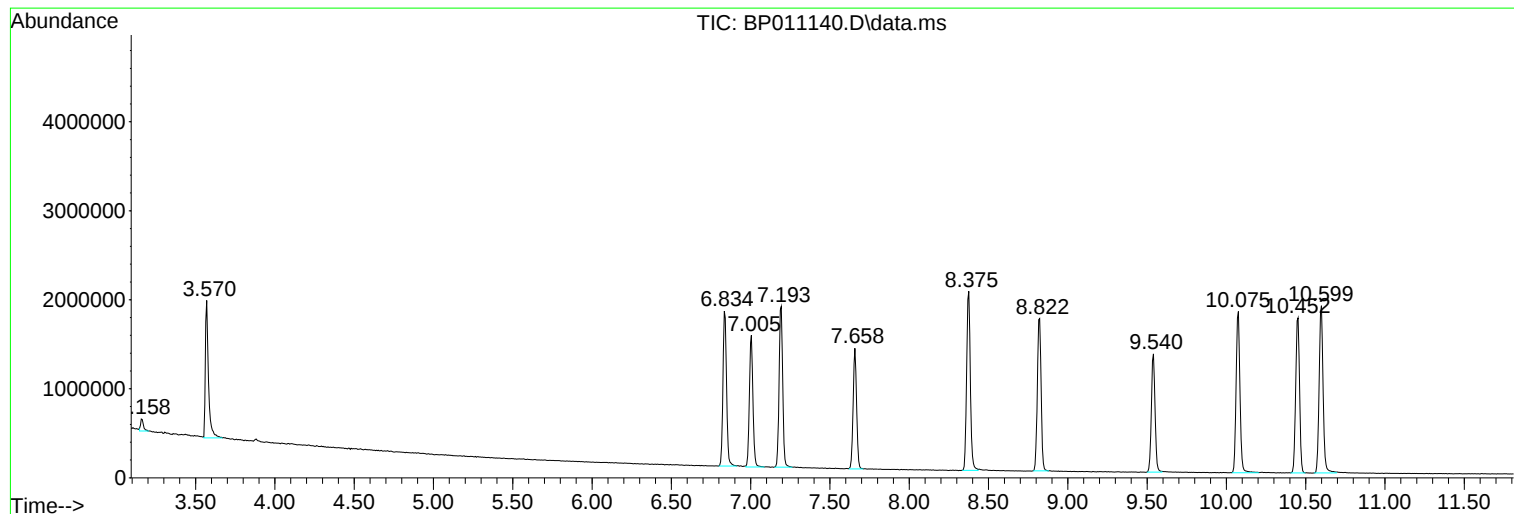

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011140.D
Acq On : 27 Jul 2022 21:43
Operator : CG/JU
Sample : PB146443BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011140.D
Acq On : 27 Jul 2022 21:43
Operator : CG/JU
Sample : PB146443BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc