

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011151.D
 Acq On : 28 Jul 2022 04:03
 Operator : CG/JU
 Sample : N3871-22
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	80	83	95	rVB	428168	591583	7.14%	0.755%
2	6.834	632	637	652	rVB	348323	585092	7.06%	0.747%
3	6.999	659	665	677	rVB	1536934	2344770	28.29%	2.994%
4	7.187	691	697	706	rBV	1416996	2173949	26.23%	2.776%
5	7.658	770	777	784	rVB	1445879	2288967	27.62%	2.922%
6	8.369	892	898	911	rBV	1001253	1606327	19.38%	2.051%
7	8.816	967	974	985	rBV	1831483	2954669	35.65%	3.772%
8	9.234	1042	1045	1050	rVB2	14418	18341	0.22%	0.023%
9	9.534	1089	1096	1106	rBV	1327325	2143282	25.86%	2.736%
10	10.069	1180	1187	1200	rBV	1730810	2865349	34.58%	3.658%
11	10.446	1244	1251	1262	rVB	1916870	3163487	38.17%	4.039%
12	10.593	1269	1276	1293	rBV	1504385	2652421	32.01%	3.386%
13	11.269	1388	1391	1396	rVB5	6572	12099	0.15%	0.015%
14	11.734	1465	1470	1475	rVB2	10911	19351	0.23%	0.025%
15	12.046	1515	1523	1532	rVV3	34553	64161	0.77%	0.082%
16	12.669	1623	1629	1633	rBV6	11099	20766	0.25%	0.027%
17	12.922	1666	1672	1679	rBV4	17520	27529	0.33%	0.035%
18	13.222	1719	1723	1727	rBV6	8542	12842	0.15%	0.016%
19	13.740	1804	1811	1823	rBV	3317559	4436235	53.53%	5.664%
20	13.851	1827	1830	1833	rVB5	5740	8889	0.11%	0.011%
21	14.010	1847	1857	1865	rBV	3608178	5275138	63.65%	6.735%
22	14.316	1901	1909	1920	rBV	2318174	3333705	40.23%	4.256%
23	14.404	1920	1924	1929	rVB6	7157	13009	0.16%	0.017%
24	14.540	1940	1947	1959	rBV	101521	233581	2.82%	0.298%
25	14.757	1981	1984	1991	rVB9	8926	13382	0.16%	0.017%
26	15.134	2043	2048	2052	rBV	50294	69860	0.84%	0.089%
27	15.316	2072	2079	2086	rBV	4331398	6201701	74.83%	7.918%
28	15.369	2086	2088	2095	rVV7	28703	48037	0.58%	0.061%
29	15.445	2095	2101	2111	rVV	1216652	1687357	20.36%	2.154%
30	15.557	2115	2120	2125	rVV	56447	92296	1.11%	0.118%
31	15.604	2125	2128	2136	rVB10	8178	19381	0.23%	0.025%
32	15.887	2172	2176	2182	rBV8	7581	15595	0.19%	0.020%
33	16.022	2193	2199	2201	rVV7	8040	15584	0.19%	0.020%
34	16.051	2201	2204	2210	rVV8	11951	25635	0.31%	0.033%
35	16.110	2210	2214	2222	rVB4	18116	29572	0.36%	0.038%
36	16.757	2321	2324	2331	rVB8	7962	12596	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011151.D
 Acq On : 28 Jul 2022 04:03
 Operator : CG/JU
 Sample : N3871-22
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.863	2338	2342	2345	rBV5	13596	20877	0.25%	0.027%
38	17.087	2373	2380	2390	rBV	2306092	3229732	38.97%	4.123%
39	17.187	2390	2397	2411	rVV2	4311991	6292642	75.93%	8.034%
40	17.392	2426	2432	2440	rBV5	12311	23742	0.29%	0.030%
41	17.781	2494	2498	2502	rVB2	24125	34411	0.42%	0.044%
42	17.992	2530	2534	2538	rBV3	38072	50629	0.61%	0.065%
43	18.069	2543	2547	2551	rVB	19610	26393	0.32%	0.034%
44	19.010	2703	2707	2713	rBV	55509	83958	1.01%	0.107%
45	19.081	2716	2719	2723	rVV	49916	61893	0.75%	0.079%
46	19.439	2774	2780	2788	rBV	5570645	7129640	86.03%	9.102%
47	20.933	3031	3034	3045	rBV5	160852	341236	4.12%	0.436%
48	21.204	3075	3080	3085	rBV	2821088	3590797	43.33%	4.584%
49	23.386	3444	3451	3459	rBV2	4440114	8287268	100.00%	10.580%
50	23.539	3470	3477	3488	rVB2	2059852	4076587	49.19%	5.205%




Sum of corrected areas: 78326343

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011151.D
Acq On : 28 Jul 2022 04:03
Operator : CG/JU
Sample : N3871-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

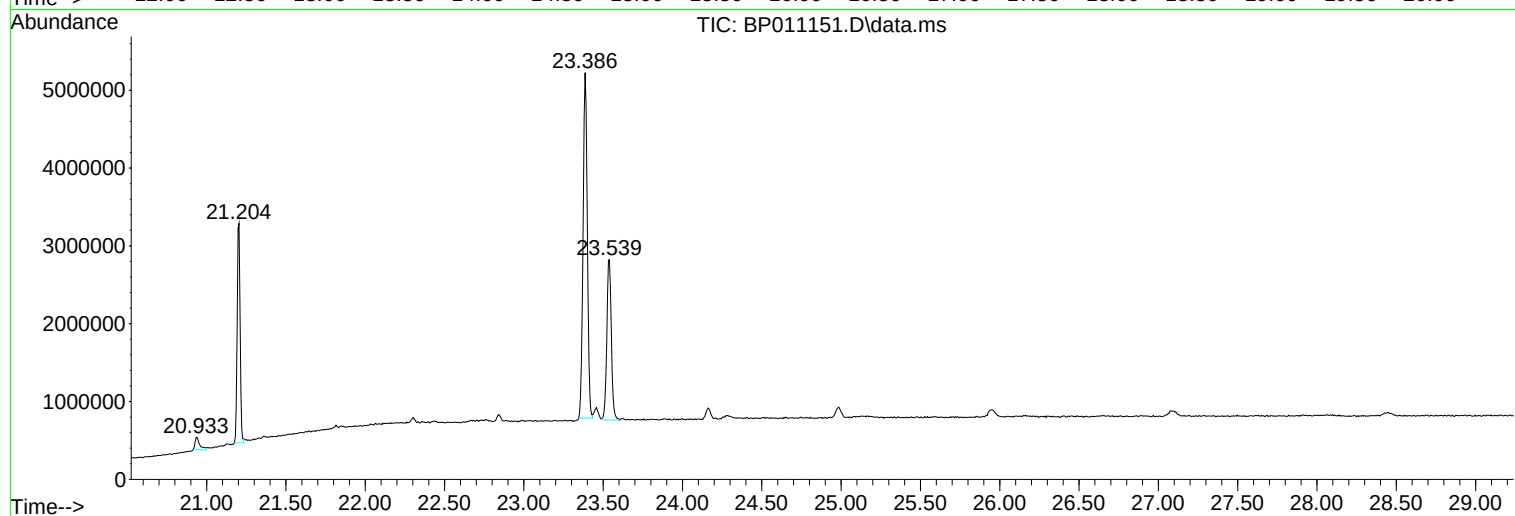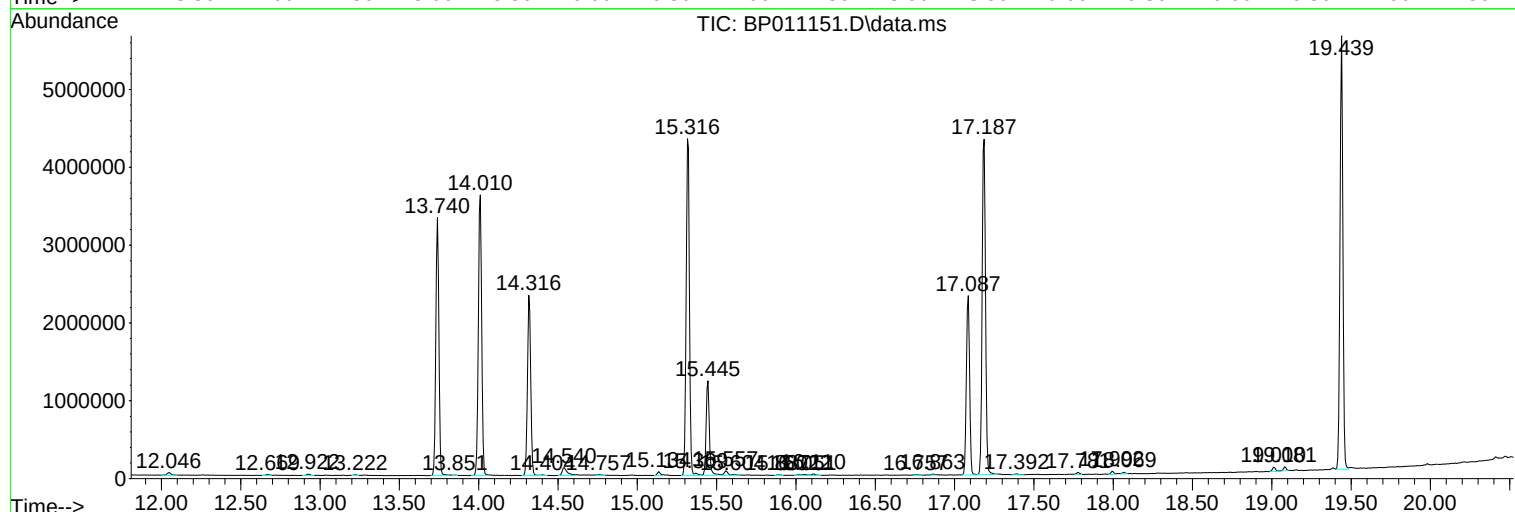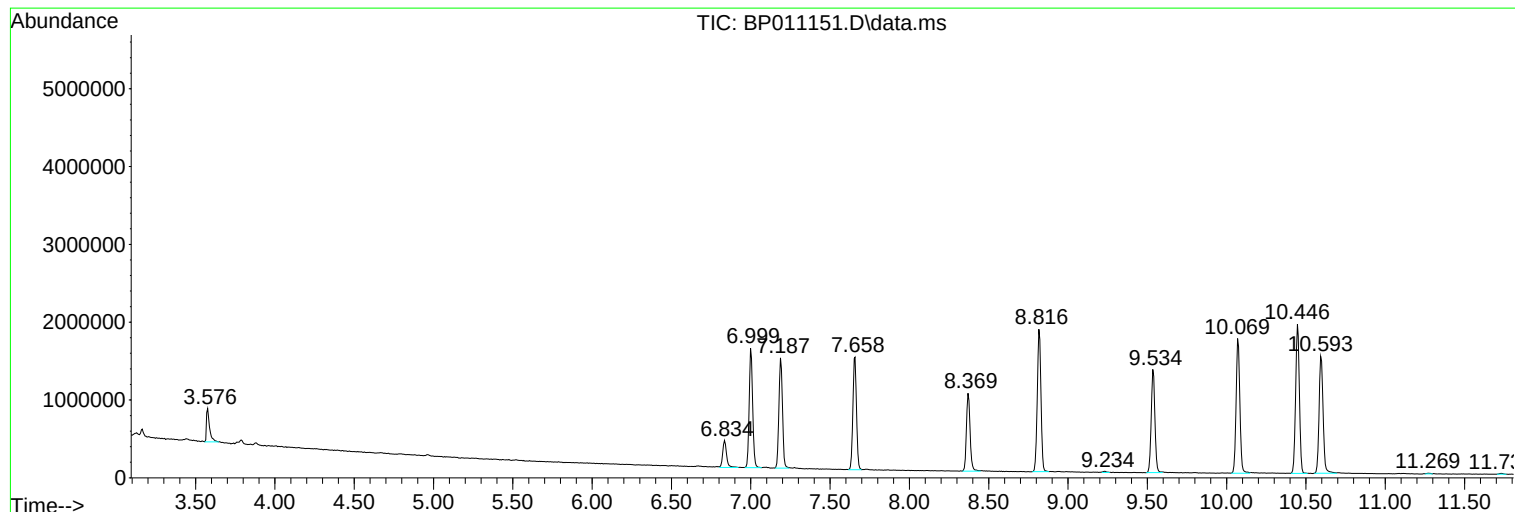

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011151.D
Acq On : 28 Jul 2022 04:03
Operator : CG/JU
Sample : N3871-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011151.D
Acq On : 28 Jul 2022 04:03
Operator : CG/JU
Sample : N3871-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc