

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011153.D
 Acq On : 28 Jul 2022 05:12
 Operator : CG/JU
 Sample : N3871-21
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	10	rBV2	206573	229510	2.75%	0.282%
2	3.581	82	84	96	rVB	179615	264706	3.18%	0.325%
3	6.834	632	637	651	rVB	463124	724149	8.69%	0.890%
4	6.999	659	665	676	rVB	1679939	2584168	31.00%	3.177%
5	7.187	691	697	708	rBV	1644221	2515595	30.18%	3.093%
6	7.657	770	777	785	rBV	1379490	2161439	25.93%	2.657%
7	8.369	892	898	911	rBV	1192740	1908762	22.90%	2.347%
8	8.816	967	974	990	rVB	2019596	3240092	38.87%	3.983%
9	9.228	1042	1044	1049	rVB2	13732	16393	0.20%	0.020%
10	9.534	1089	1096	1109	rBV	1460490	2349447	28.19%	2.888%
11	10.069	1180	1187	1207	rBV	1947208	3180178	38.15%	3.910%
12	10.251	1214	1218	1226	rBV5	11421	25205	0.30%	0.031%
13	10.446	1244	1251	1260	rBV	1854157	2986250	35.82%	3.671%
14	10.593	1269	1276	1288	rBV	1537199	2636636	31.63%	3.241%
15	11.110	1361	1364	1372	rVB3	13235	22946	0.28%	0.028%
16	11.240	1380	1386	1392	rBV3	18792	43468	0.52%	0.053%
17	11.728	1465	1469	1474	rVB5	8927	17559	0.21%	0.022%
18	12.045	1517	1523	1529	rVV	34767	58529	0.70%	0.072%
19	12.669	1625	1629	1634	rBV5	9976	16775	0.20%	0.021%
20	12.928	1667	1673	1679	rVB4	15103	22457	0.27%	0.028%
21	13.028	1688	1690	1698	rVB8	4452	9127	0.11%	0.011%
22	13.222	1720	1723	1729	rVB6	8444	12182	0.15%	0.015%
23	13.740	1804	1811	1822	rBV	3365768	4600639	55.19%	5.656%
24	13.840	1823	1828	1843	rVV	36628	90176	1.08%	0.111%
25	14.010	1847	1857	1871	rVV	3913247	5676026	68.09%	6.978%
26	14.110	1873	1874	1882	rVB8	5312	8420	0.10%	0.010%
27	14.316	1900	1909	1921	rBV	2310391	3281175	39.36%	4.034%
28	14.534	1940	1946	1964	rBV	140138	324853	3.90%	0.399%
29	14.681	1968	1971	1976	rVV7	8897	18833	0.23%	0.023%
30	14.757	1980	1984	1992	rVB9	9183	17587	0.21%	0.022%
31	15.134	2043	2048	2055	rBV	76821	108331	1.30%	0.133%
32	15.322	2073	2080	2087	rBV	4553801	6487060	77.82%	7.975%
33	15.445	2094	2101	2115	rBV	1277513	1761746	21.13%	2.166%
34	15.557	2115	2120	2126	rVB	52824	76454	0.92%	0.094%
35	15.892	2171	2177	2183	rBV10	6139	12565	0.15%	0.015%
36	16.022	2194	2199	2202	rBV7	8202	17386	0.21%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
 Data File : BP011153.D
 Acq On : 28 Jul 2022 05:12
 Operator : CG/JU
 Sample : N3871-21
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJ18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.110	2211	2214	2218	rVB5	15309	21213	0.25%	0.026%
38	16.763	2318	2325	2330	rBV5	9545	20257	0.24%	0.025%
39	16.863	2338	2342	2345	rBV6	14016	21539	0.26%	0.026%
40	17.081	2373	2379	2390	rBV	2306921	3322298	39.86%	4.084%
41	17.181	2390	2396	2410	rVV2	4576386	6568159	78.80%	8.075%
42	17.392	2426	2432	2436	rBV4	8819	13636	0.16%	0.017%
43	17.780	2494	2498	2502	rVB4	23113	31455	0.38%	0.039%
44	17.992	2530	2534	2538	rBV4	28407	40009	0.48%	0.049%
45	18.063	2543	2546	2549	rVV2	13551	15352	0.18%	0.019%
46	19.010	2703	2707	2712	rBV3	57841	84497	1.01%	0.104%
47	19.080	2715	2719	2723	rVV	54060	69851	0.84%	0.086%
48	19.386	2769	2771	2774	rVB2	18255	15653	0.19%	0.019%
49	19.439	2774	2780	2788	rBV	5884396	7420636	89.02%	9.123%
50	20.933	3031	3034	3042	rBV2	112437	226051	2.71%	0.278%
51	21.204	3075	3080	3089	rBV	2955187	3651143	43.80%	4.489%
52	23.386	3444	3451	3459	rBV2	4238074	8335732	100.00%	10.248%
53	23.533	3470	3476	3486	rVB2	2083650	3976910	47.71%	4.889%




Sum of corrected areas: 81341215

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011153.D
Acq On : 28 Jul 2022 05:12
Operator : CG/JU
Sample : N3871-21
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

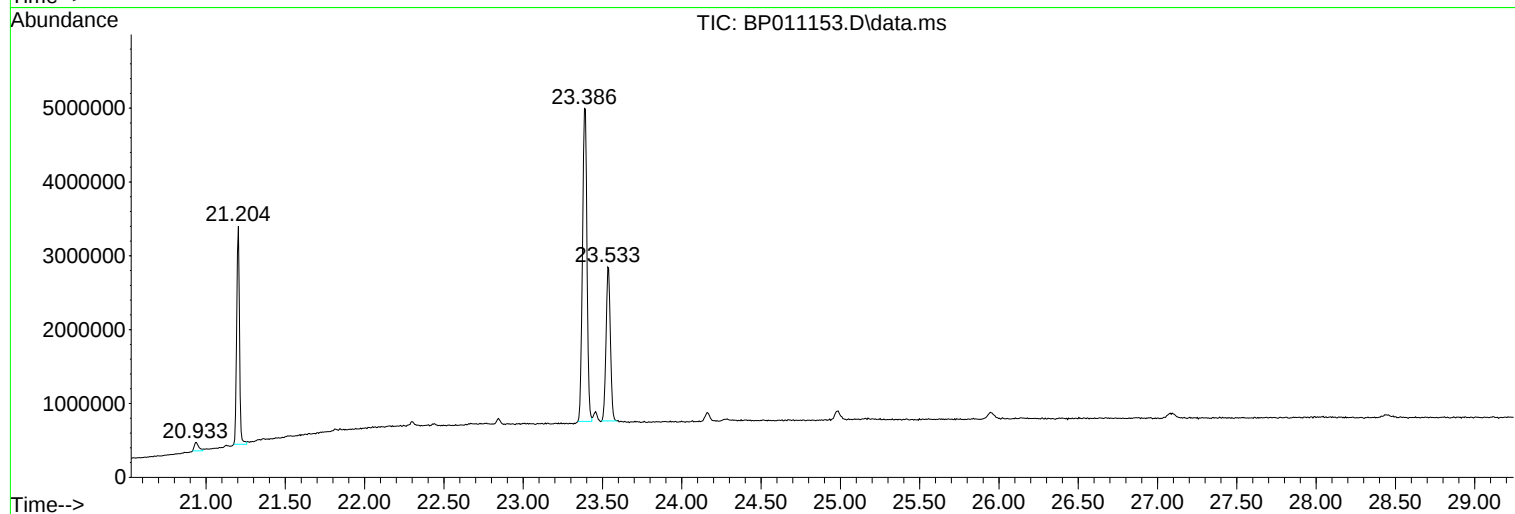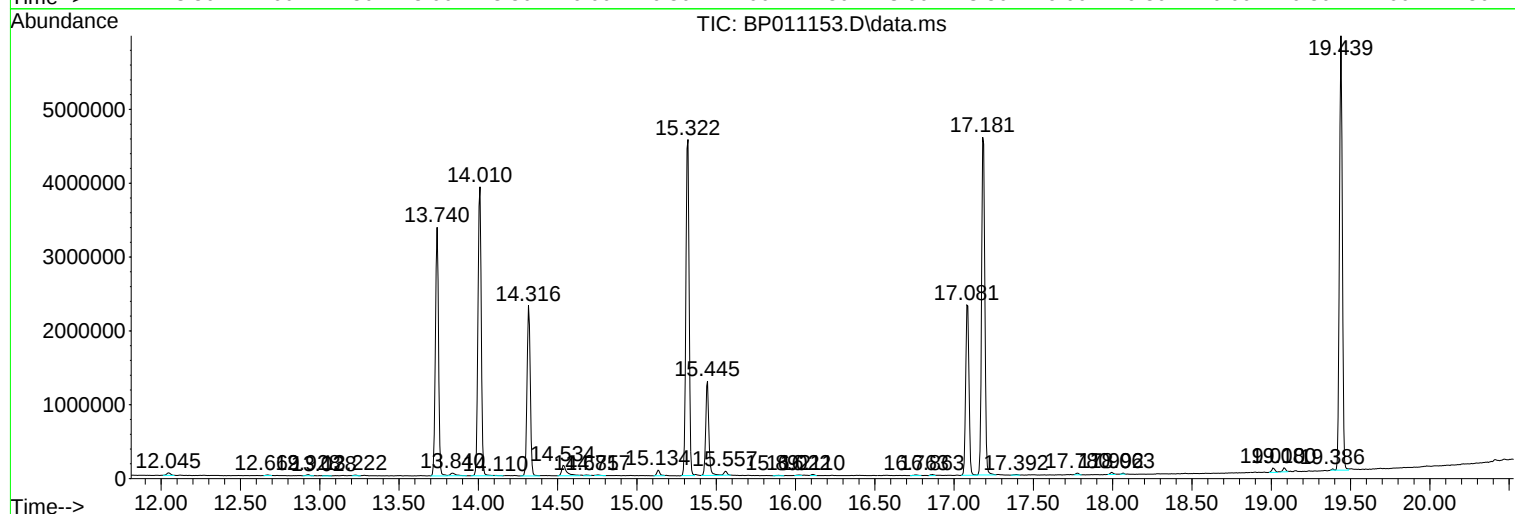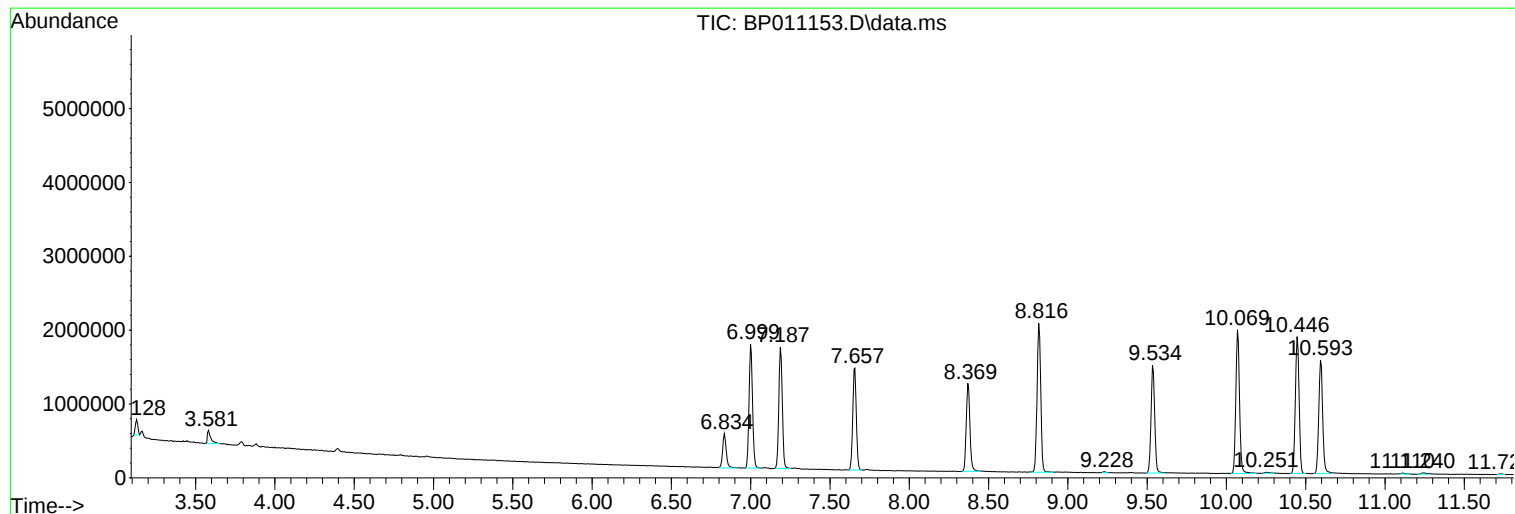

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011153.D
Acq On : 28 Jul 2022 05:12
Operator : CG/JU
Sample : N3871-21
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072722\
Data File : BP011153.D
Acq On : 28 Jul 2022 05:12
Operator : CG/JU
Sample : N3871-21
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJ18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------