

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072822\
 Data File : BP011158.D
 Acq On : 28 Jul 2022 12:45
 Operator : CG/JU
 Sample : SSTD01025
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010625

Quant Time: Jul 28 14:11:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 14:10:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.652	152	272369	20.000	ng/u1	0.00
20) Naphthalene-d8	10.440	136	1144918	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.316	164	581589	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.087	188	1047513	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.210	240	1052649	20.000	ng/u1	# 0.00
88) Perylene-d12	23.557	264	1147206	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.152	96	23188	3.069	ng/uL	0.00
4) Pyridine-d5	3.564	84	148206	7.589	ng/u1	0.00
7) Phenol-d5	6.828	99	196226	8.777	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	150519	10.470	ng/u1	0.00
11) 2-Chlorophenol-d4	7.181	132	166307	9.206	ng/u1	0.00
15) 4-Methylphenol-d8	8.364	113	156817	8.761	ng/u1	0.00
21) Nitrobenzene-d5	8.811	128	78036	9.353	ng/u1	0.00
24) 2-Nitrophenol-d4	9.534	143	69445	8.411	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	131279	8.695	ng/u1	0.00
31) 4-Chloroaniline-d4	10.593	131	204083	8.199	ng/u1	0.00
46) Dimethylphthalate-d6	13.740	166	350475	8.817	ng/u1	0.00
49) Acenaphthylene-d8	14.004	160	447043	9.532	ng/u1	0.00
54) 4-Nitrophenol-d4	14.534	143	47370	5.888	ng/u1	0.00
60) Fluorene-d10	15.316	176	307708	9.107	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	33771	6.515	ng/u1	0.00
73) Anthracene-d10	17.187	188	428531	9.623	ng/u1	0.00
81) Pyrene-d10	19.445	212	476804	8.624	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.404	264	510466	9.264	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.181	88	23333	2.943	ng/uL	94
5) Pyridine	3.581	79	158862	7.894	ng/u1#	79
6) Benzaldehyde	6.799	77	129368	11.912	ng/u1	96
8) Phenol	6.852	94	217984	9.172	ng/u1	91
10) Bis(2-Chloroethyl)ether	7.087	93	183736	9.741	ng/u1	94
12) 2-Chlorophenol	7.216	128	173174	9.273	ng/u1	98
13) 2-Methylphenol	8.099	108	155074	8.824	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.234	45	3665	0.142	ng/u1#	49
16) Acetophenone	8.475	105	267506	9.873	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.463	70	136670	10.053	ng/u1	97
18) 4-Methylphenol	8.428	108	167202	8.910	ng/u1	99
19) Hexachloroethane	8.716	117	81611	11.043	ng/u1#	72
22) Nitrobenzene	8.852	77	208275	10.615	ng/u1	99
23) Isophorone	9.381	82	356032	9.695	ng/u1	97
25) 2-Nitrophenol	9.563	139	81545	8.799	ng/u1	92
26) 2,4-Dimethylphenol	9.628	107	183875	9.383	ng/u1	99
27) Bis(2-Chloroethoxy)met...	9.869	93	231308	9.518	ng/u1	99
29) 2,4-Dichlorophenol	10.093	162	140268	8.976	ng/u1	96
30) Naphthalene	10.493	128	568846	9.750	ng/u1	99
32) 4-Chloroaniline	10.616	127	204262	8.296	ng/u1	97
33) Hexachlorobutadiene	10.775	225	91109	10.016	ng/u1	95
34) Caprolactam	11.410	113	35500	6.482	ng/u1	95
35) 4-Chloro-3-methylphenol	11.752	107	144934	8.206	ng/u1	99
36) 2-Methylnaphthalene	12.116	142	341026	9.016	ng/u1	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072822\
 Data File : BP011158.D
 Acq On : 28 Jul 2022 12:45
 Operator : CG/JU
 Sample : SSTD01025
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010625

Quant Time: Jul 28 14:11:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 14:10:09 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.340	142	341921	9.019	ng/ul#	98
39) 1,2,4,5-Tetrachloroben...	12.487	216	152285	9.928	ng/ul#	97
40) Hexachlorocyclopentadiene	12.463	237	91011	9.580	ng/ul	96
41) 2,4,6-Trichlorophenol	12.740	196	86170	8.530	ng/ul	100
42) 2,4,5-Trichlorophenol	12.804	196	92180	8.539	ng/ul	98
43) 1,1'-Biphenyl	13.146	154	430123	9.912	ng/ul#	97
44) 2-Chloronaphthalene	13.181	162	327084	10.035	ng/ul	96
45) 2-Nitroaniline	13.399	65	74376	7.832	ng/ul	96
47) Dimethylphthalate	13.787	163	359814	8.971	ng/ul	99
48) 2,6-Dinitrotoluene	13.904	165	51914	7.149	ng/ul#	85
50) Acenaphthylene	14.034	152	521369	9.907	ng/ul	99
51) 3-Nitroaniline	14.240	138	53629	6.147	ng/ul	95
52) Acenaphthene	14.381	153	338767	9.717	ng/ul	98
53) 2,4-Dinitrophenol	14.446	184	20260	4.769	ng/ul	98
55) 4-Nitrophenol	14.551	109	42500	6.900	ng/ul#	77
56) Dibenzofuran	14.722	168	468148	9.732	ng/ul	98
57) 2,4-Dinitrotoluene	14.693	165	78749	7.603	ng/ul	96
58) 2,3,4,6-Tetrachlorophenol	14.951	232	67208	7.950	ng/ul#	84
59) Diethylphthalate	15.163	149	355074	8.620	ng/ul	97
61) Fluorene	15.375	166	364122	9.432	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.375	204	166755	9.383	ng/ul	91
63) 4-Nitroaniline	15.410	138	32786	4.089	ng/ul	85
66) 4,6-Dinitro-2-methylph...	15.457	198	36137	6.796	ng/ul#	77
67) N-Nitrosodiphenylamine	15.593	169	289505	9.675	ng/ul	95
68) 4-Bromophenyl-phenylether	16.281	248	88263	9.342	ng/ul	94
69) Hexachlorobenzene	16.381	284	106324	9.697	ng/ul#	89
70) Atrazine	16.563	200	83736	8.089	ng/ul	98
71) Pentachlorophenol	16.734	266	51233	7.587	ng/ul	97
72) Phenanthrene	17.128	178	543034	9.950	ng/ul	99
74) Anthracene	17.222	178	539466	9.937	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.099	216	161643	10.779	ng/ul	99
76) Pentachlorobenzene	14.634	250	134715	10.248	ng/ul	97
77) Carbazole	17.504	167	463866	9.130	ng/ul	99
78) Di-n-butylphthalate	18.075	149	521989	8.219	ng/ul	100
80) Fluoranthene	19.116	202	583150	9.019	ng/ul#	85
82) Pyrene	19.475	202	629721	9.439	ng/ul#	84
83) Butylbenzylphthalate	20.369	149	218092	7.328	ng/ul#	92
84) 3,3'-Dichlorobenzidine	21.139	252	154662	8.298	ng/ul#	98
85) Benzo(a)anthracene	21.198	228	594346	9.271	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.139	149	351211	7.909	ng/ul#	94
87) Chrysene	21.245	228	611159	9.709	ng/ul	99
89) Di-n-octyl phthalate	22.051	149	601929	7.824	ng/ul	100
90) Benzo(b)fluoranthene	22.839	252	646755	9.130	ng/ul#	95
91) Benzo(k)fluoranthene	22.886	252	645995	9.709	ng/ul#	94
93) Benzo(a)pyrene	23.451	252	646654	9.506	ng/ul#	93
94) Indeno(1,2,3-cd)pyrene	25.974	276	784245	9.920	ng/ul#	88
95) Dibenzo(a,h)anthracene	25.998	278	679044	9.926	ng/ul#	91
96) Benzo(g,h,i)perylene	26.715	276	674740	10.021	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072822\
 Data File : BP011158.D
 Acq On : 28 Jul 2022 12:45
 Operator : CG/JU
 Sample : SST010625
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST010625

Quant Time: Jul 28 14:11:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 14:10:09 2022
 Response via : Initial Calibration




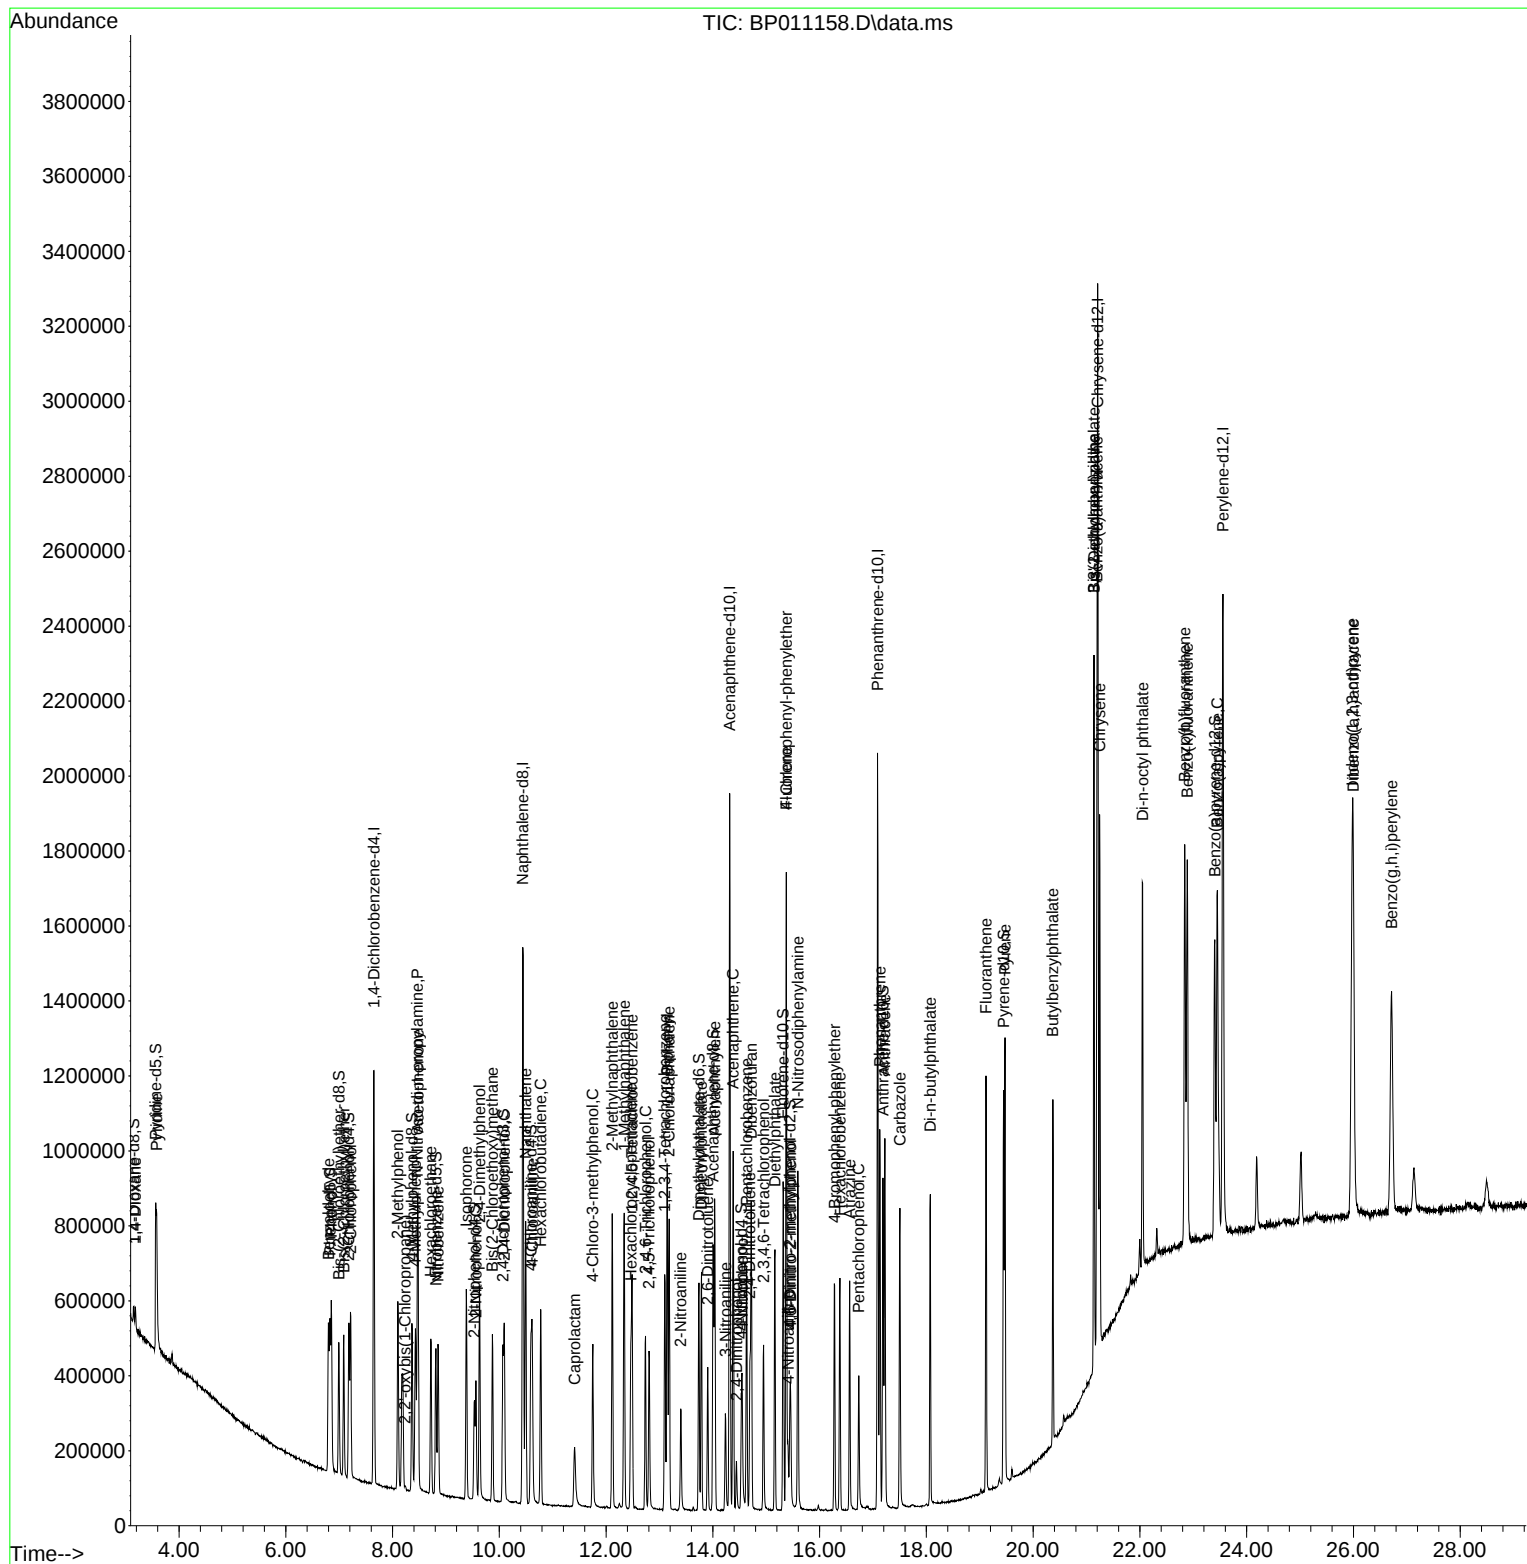




#2
1,4-Dioxane
Concen: 2.943 ng/uL
RT: 3.181 min Scan# 1
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion: 88 Resp: 23333
Ion Ratio Lower Upper
88 100
43 41.3 35.8 53.6
58 79.7 68.1 102.1



#5
Pyridine
Concen: 7.894 ng/uL
RT: 3.581 min Scan# 84
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion: 79 Resp: 158862
Ion Ratio Lower Upper
79 100
52 78.9 83.8 125.8#
51 42.2 41.0 61.4


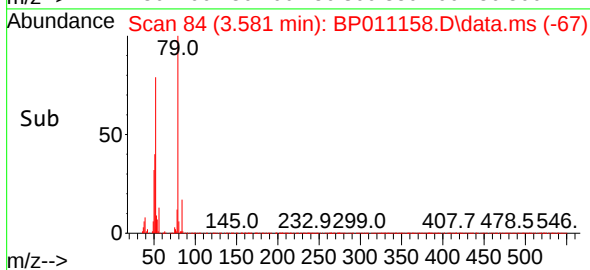






#6
Benzaldehyde
Concen: 11.912 ng/ul
RT: 6.799 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion: 77 Resp: 129368
Ion Ratio Lower Upper
77 100
105 91.8 76.0 114.0
106 87.4 73.2 109.8



#8
Phenol
Concen: 9.172 ng/ul
RT: 6.852 min Scan# 640
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion: 94 Resp: 217984
Ion Ratio Lower Upper
94 100
65 29.9 27.4 41.2
66 39.6 37.4 56.2




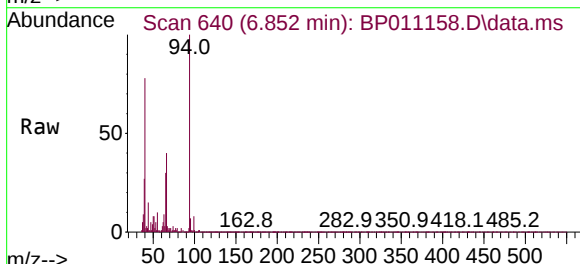




#10
 Bis(2-Chloroethyl)ether
 Concen: 9.741 ng/ul
 RT: 7.087 min Scan# 680
 Delta R.T. 0.000 min
 Lab File: BP011158.D
 Acq: 28 Jul 2022 12:45




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010625


Tgt Ion:	93	Resp:	183736
Ion	Ratio	Lower	Upper
93	100		
63	84.5	72.4	108.6
95	32.0	27.3	40.9

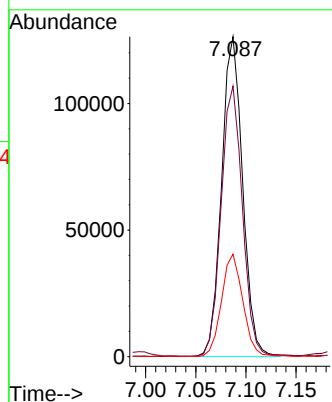

#12
 2-Chlorophenol
 Concen: 9.273 ng/ul
 RT: 7.216 min Scan# 702
 Delta R.T. 0.000 min
 Lab File: BP011158.D
 Acq: 28 Jul 2022 12:45

Tgt Ion:	128	Resp:	173174
Ion	Ratio	Lower	Upper
128	100		
64	54.0	44.8	67.2
130	32.7	25.8	38.6





#13

2-Methylphenol

Concen: 8.824 ng/ul

RT: 8.099 min Scan# 81

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45

Instrument :

BNA_P

ClientSampleId :





SSTD010625

Tgt Ion:108 Resp: 155074

Ion Ratio Lower Upper

108 100

107 88.8 71.4 107.0

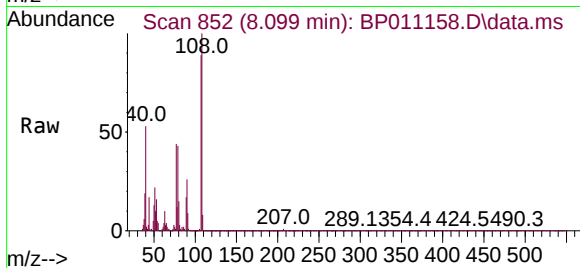

#14

2,2'-oxybis(1-Chloropropane)

Concen: 0.142 ng/ul

RT: 8.234 min Scan# 875

Delta R.T. 0.041 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45




Tgt Ion: 45 Resp: 3665


Ion Ratio Lower Upper

45 100

77 40.0 11.2 16.8#

79 19.1 6.9 10.3#


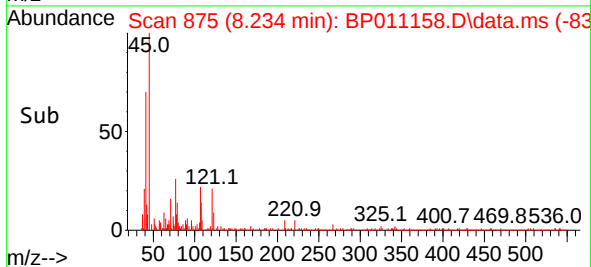

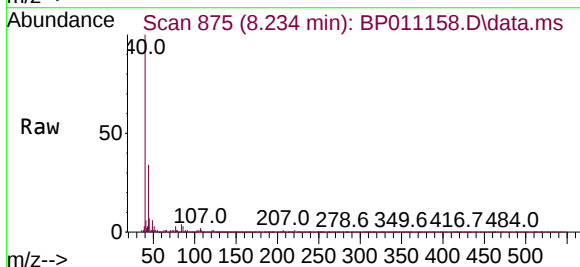




#16
Acetophenone
Concen: 9.873 ng/ul
RT: 8.475 min Scan# 916
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:105 Resp: 267506
Ion Ratio Lower Upper
105 100
77 83.9 67.5 101.3
51 34.9 29.6 44.4



#17
N-Nitroso-di-n-propylamine
Concen: 10.053 ng/ul
RT: 8.463 min Scan# 914
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion: 70 Resp: 136670
Ion Ratio Lower Upper
70 100
42 65.2 53.8 80.8
101 8.3 7.8 11.6
130 18.1 15.4 23.2



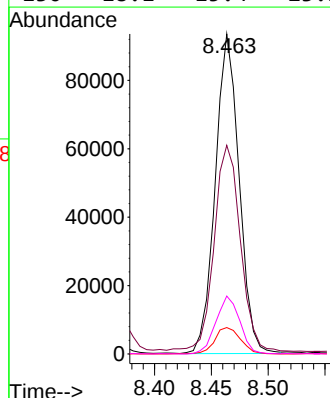





#18
4-Methylphenol
Concen: 8.910 ng/ul
RT: 8.428 min Scan# 908
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:108 Resp: 167202
Ion Ratio Lower Upper
108 100
107 111.1 88.3 132.5



#19
Hexachloroethane
Concen: 11.043 ng/ul
RT: 8.716 min Scan# 957
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:117 Resp: 81611
Ion Ratio Lower Upper
117 100
201 77.7 85.7 128.5#
199 49.0 57.4 86.0#




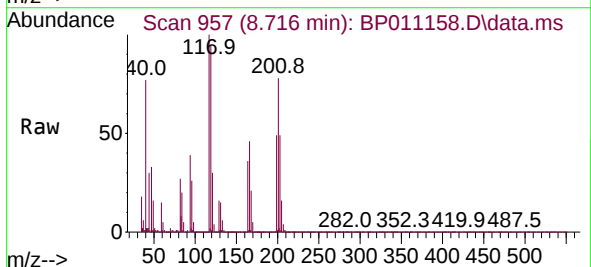




#22
Nitrobenzene
Concen: 10.615 ng/ul
RT: 8.852 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion: 77 Resp: 208275
Ion Ratio Lower Upper
77 100
123 39.6 31.5 47.3
65 13.9 11.4 17.2



#23
Isophorone
Concen: 9.695 ng/ul
RT: 9.381 min Scan# 1070
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion: 82 Resp: 356032
Ion Ratio Lower Upper
82 100
95 6.8 6.6 10.0
138 15.9 13.8 20.6



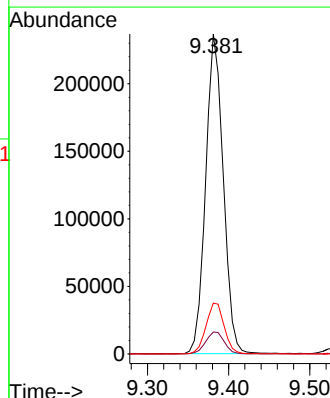





#25
2-Nitrophenol
Concen: 8.799 ng/ul
RT: 9.563 min Scan# 1101
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion	Ratio	Lower	Upper
139	100		
65	62.2	54.2	81.4
109	31.5	30.6	45.8



#26
2,4-Dimethylphenol
Concen: 9.383 ng/ul
RT: 9.628 min Scan# 1112
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion	Ratio	Lower	Upper
107	100		
121	48.7	39.1	58.7
122	81.6	66.1	99.1





#27

Bis(2-Chloroethoxy)methane

Concen: 9.518 ng/ul

RT: 9.869 min Scan# 1153

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD010625





Tgt Ion: 93 Resp: 231308

Ion Ratio Lower Upper

93 100

95 32.4 26.6 39.8

123 10.3 7.8 11.8

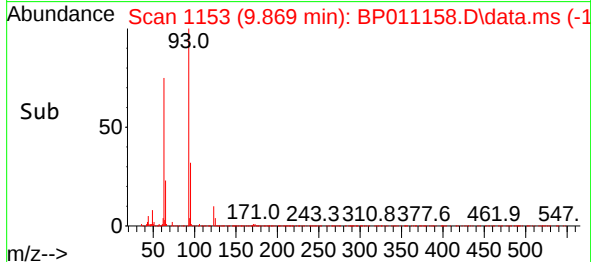

#29

2,4-Dichlorophenol

Concen: 8.976 ng/ul

RT: 10.093 min Scan# 1191

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45




Tgt Ion: 162 Resp: 140268


Ion Ratio Lower Upper

162 100

164 61.6 52.5 78.7

98 38.4 31.4 47.0


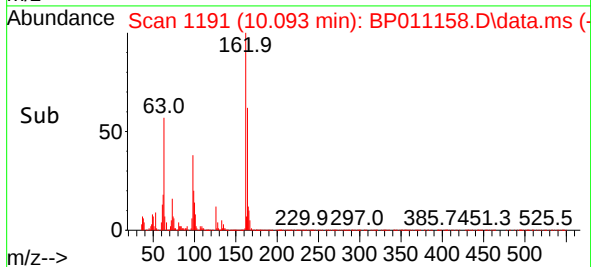

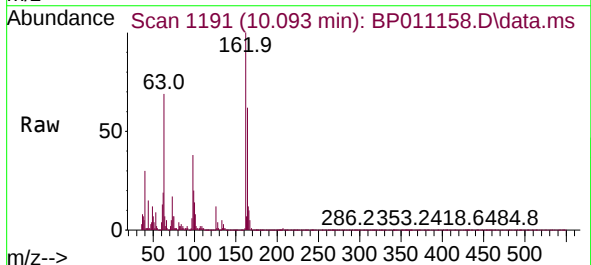




#30
Naphthalene
Concen: 9.750 ng/ul
RT: 10.493 min Scan# 1259
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:128 Resp: 568846
Ion Ratio Lower Upper
128 100
129 10.6 8.7 13.1
127 13.0 10.2 15.4



#32
4-Chloroaniline
Concen: 8.296 ng/ul
RT: 10.616 min Scan# 1280
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:127 Resp: 204262
Ion Ratio Lower Upper
127 100
129 31.0 26.2 39.2


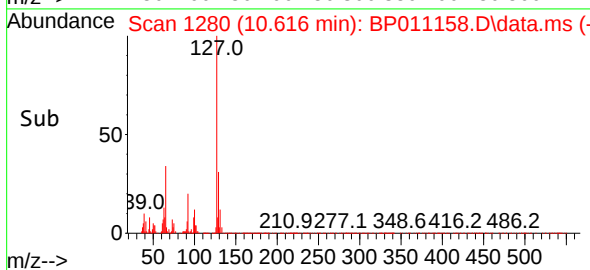






#33
Hexachlorobutadiene
Concen: 10.016 ng/ul
RT: 10.775 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:225 Resp: 91109
Ion Ratio Lower Upper
225 100
223 60.6 53.7 80.5
227 60.5 49.4 74.2



#34
Caprolactam
Concen: 6.482 ng/ul
RT: 11.410 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:113 Resp: 35500
Ion Ratio Lower Upper
113 100
55 197.0 153.8 230.8
56 145.9 110.2 165.4


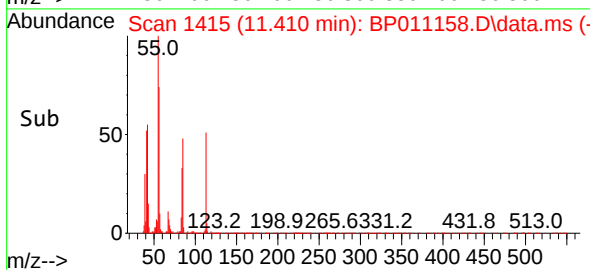






#35
4-Chloro-3-methylphenol
Concen: 8.206 ng/ul
RT: 11.752 min Scan# 1473
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:107 Resp: 144934
Ion Ratio Lower Upper
107 100
144 23.9 18.6 27.8
142 73.2 59.6 89.4

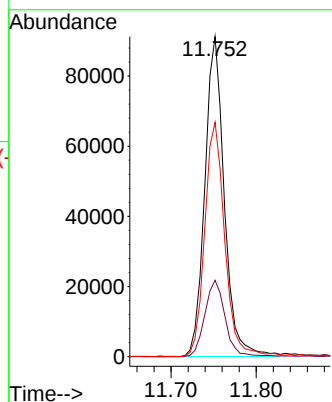

#36
2-Methylnaphthalene
Concen: 9.016 ng/ul
RT: 12.116 min Scan# 1535
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:142 Resp: 341026
Ion Ratio Lower Upper
142 100
141 91.8 70.1 105.1



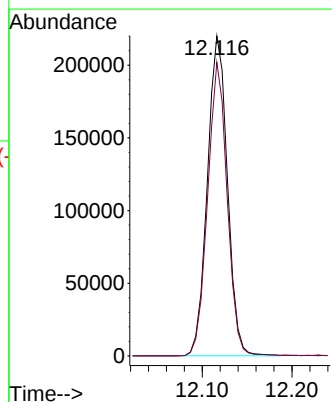





#37
1-Methylnaphthalene
Concen: 9.019 ng/ul
RT: 12.340 min Scan# 1573
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:142 Resp: 341921
Ion Ratio Lower Upper
142 100
141 93.0 73.3 109.9
116 3.8 4.0 6.0#



#39
1,2,4,5-Tetrachlorobenzene
Concen: 9.928 ng/ul
RT: 12.487 min Scan# 1598
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:216 Resp: 152285
Ion Ratio Lower Upper
216 100
214 78.2 63.0 94.6
179 23.5 18.1 27.1
108 23.5 13.6 20.4#

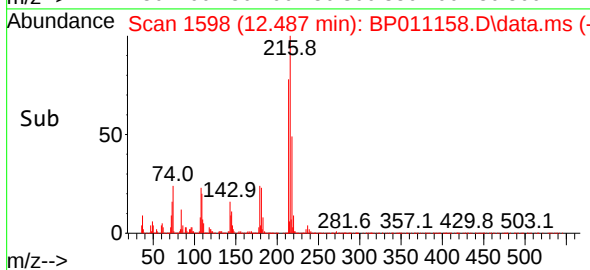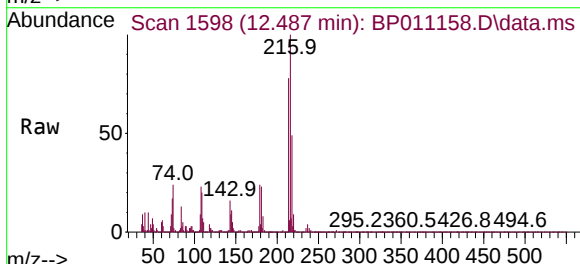

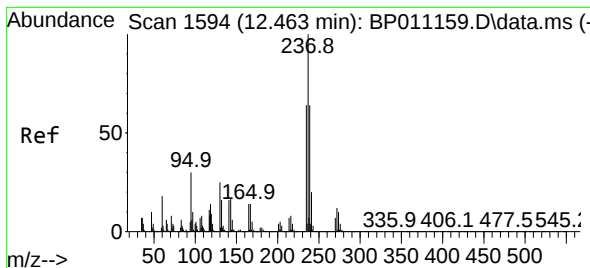

#40

Hexachlorocyclopentadiene

Concen: 9.580 ng/ul

RT: 12.463 min Scan# 1594

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45





Instrument :

BNA_P

ClientSampleId :

SSTD010625

Tgt Ion:237	Resp:	91011
Ion Ratio	Lower	Upper
237	100	
235	62.6	52.8 79.2
272	13.9	11.5 17.3

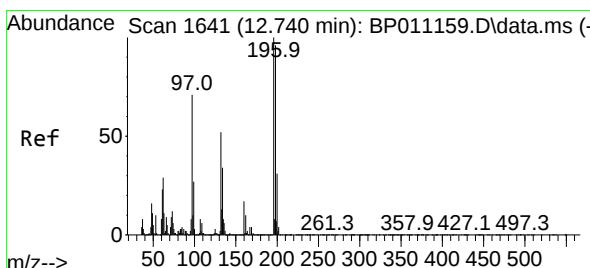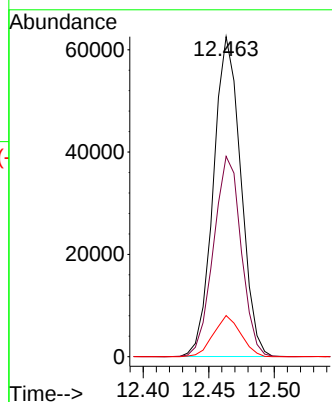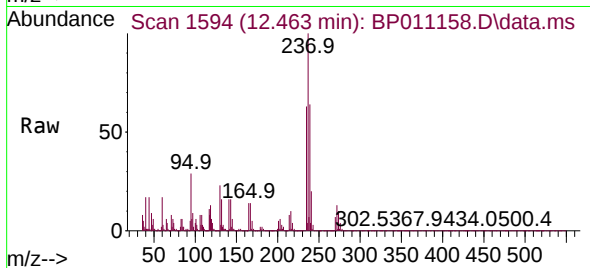

#41

2,4,6-Trichlorophenol

Concen: 8.530 ng/ul




RT: 12.740 min Scan# 1641


Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45

Tgt Ion:196	Resp:	86170
Ion Ratio	Lower	Upper
196	100	
198	98.0	78.2 117.4
200	31.7	25.0 37.6


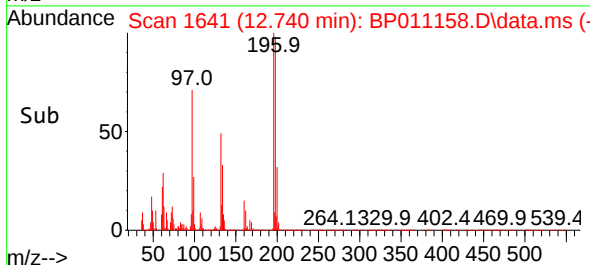

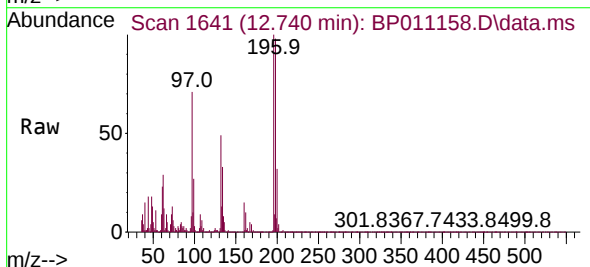




#42
2,4,5-Trichlorophenol
Concen: 8.539 ng/ul
RT: 12.804 min Scan# 1652
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:196 Resp: 92180
Ion Ratio Lower Upper
196 100
198 94.0 77.0 115.4
200 31.2 24.8 37.2



#43
1,1'-Biphenyl
Concen: 9.912 ng/ul
RT: 13.146 min Scan# 1710
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:154 Resp: 430123
Ion Ratio Lower Upper
154 100
153 40.7 31.9 47.9
76 15.8 9.2 13.8#



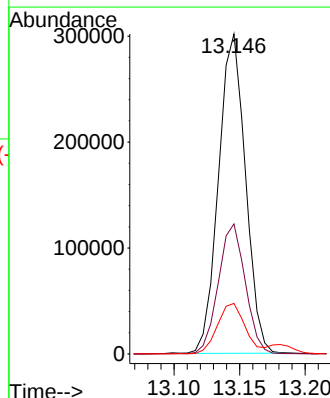





#44
2-Chloronaphthalene
Concen: 10.035 ng/ul
RT: 13.181 min Scan# 1716
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:162 Resp: 327084
Ion Ratio Lower Upper
162 100
164 33.0 25.5 38.3
127 43.4 31.9 47.9



#45
2-Nitroaniline
Concen: 7.832 ng/ul
RT: 13.399 min Scan# 1753
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion: 65 Resp: 74376
Ion Ratio Lower Upper
65 100
92 65.7 49.0 73.6
138 81.3 66.4 99.6



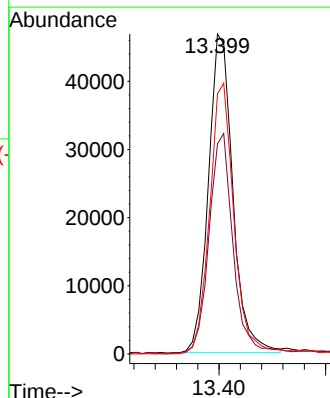
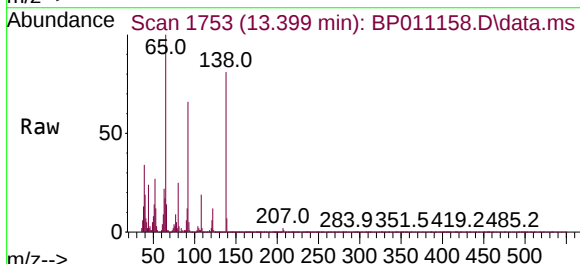




#47
Dimethylphthalate
Concen: 8.971 ng/ul
RT: 13.787 min Scan# 1819
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:163 Resp: 359814
Ion Ratio Lower Upper
163 100
194 3.8 3.4 5.2
164 9.7 7.6 11.4



#48
2,6-Dinitrotoluene
Concen: 7.149 ng/ul
RT: 13.904 min Scan# 1839
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:165 Resp: 51914
Ion Ratio Lower Upper
165 100
89 78.7 52.9 79.3
121 30.1 19.4 29.2#


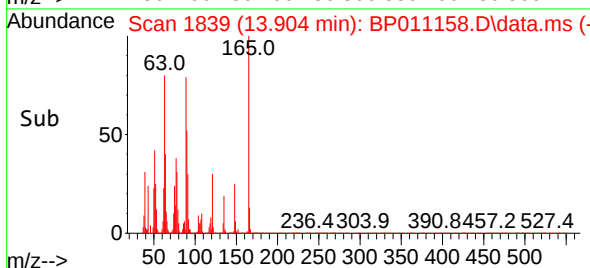
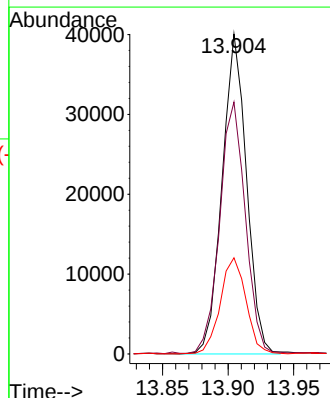





#50
Acenaphthylene
Concen: 9.907 ng/ul
RT: 14.034 min Scan# 1861
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:152 Resp: 521369
Ion Ratio Lower Upper
152 100
151 19.7 16.5 24.7
153 12.9 10.1 15.1



#51
3-Nitroaniline
Concen: 6.147 ng/ul
RT: 14.240 min Scan# 1896
Delta R.T. 0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:138 Resp: 53629
Ion Ratio Lower Upper
138 100
108 15.4 11.0 16.4
92 124.9 104.6 156.8




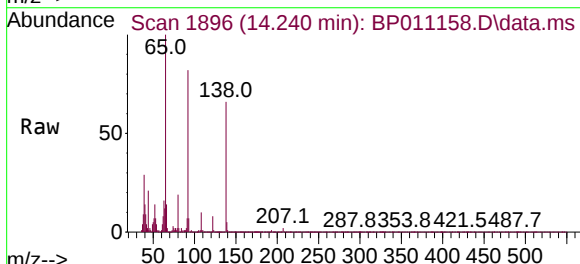




#52
Acenaphthene
Concen: 9.717 ng/ul
RT: 14.381 min Scan# 1920
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:153 Resp: 338767
Ion Ratio Lower Upper
153 100
152 48.2 36.2 54.2
154 88.7 70.8 106.2

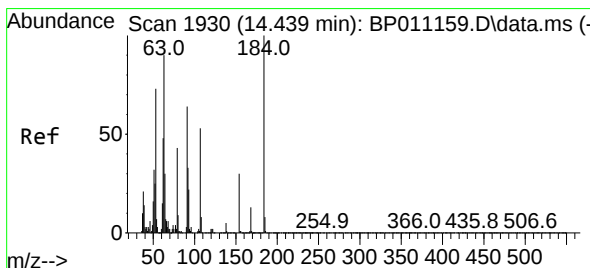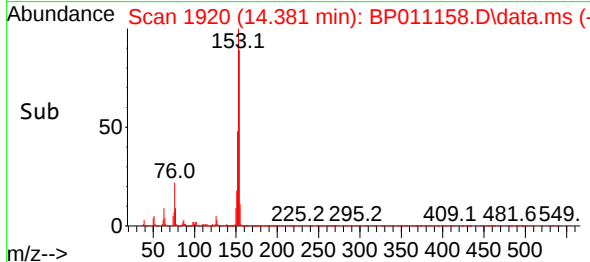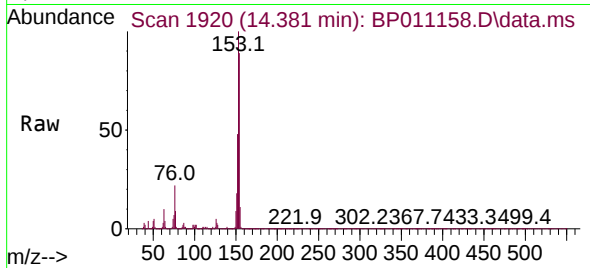

#53
2,4-Dinitrophenol
Concen: 4.769 ng/ul
RT: 14.446 min Scan# 1931
Delta R.T. 0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:184 Resp: 20260
Ion Ratio Lower Upper
184 100
63 90.7 73.8 110.6
154 68.9 57.2 85.8


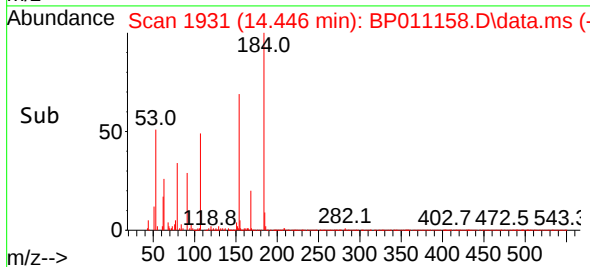

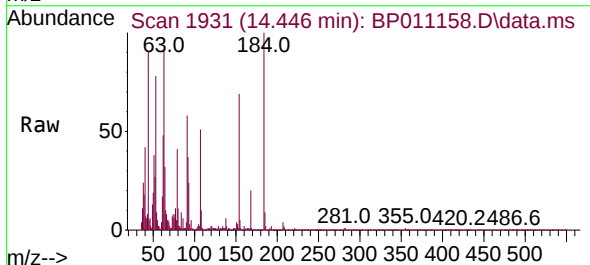




#55
4-Nitrophenol
Concen: 6.900 ng/ul
RT: 14.551 min Scan# 1949
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:109 Resp: 42500
Ion Ratio Lower Upper
109 100
139 128.9 75.6 113.4#
65 150.9 107.6 161.4

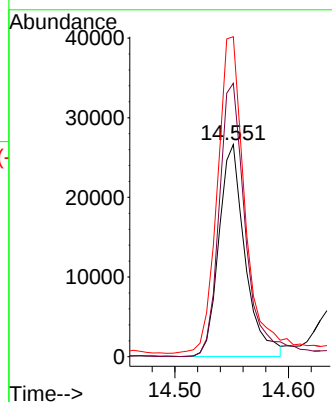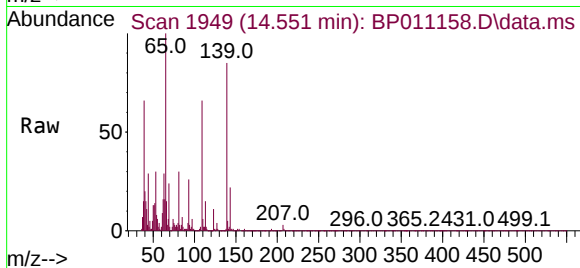

#56
Dibenzofuran
Concen: 9.732 ng/ul
RT: 14.722 min Scan# 1978
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:168 Resp: 468148
Ion Ratio Lower Upper
168 100
139 40.0 32.8 49.2


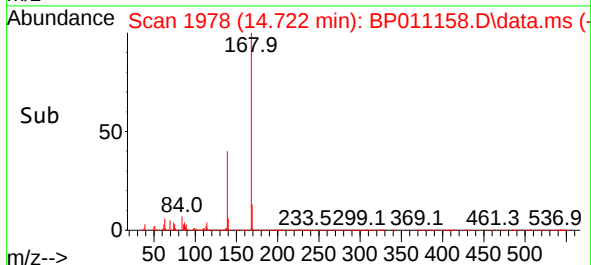

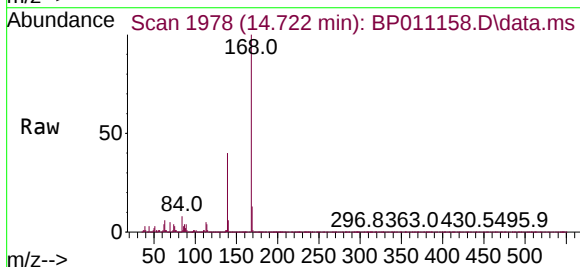




#57
2,4-Dinitrotoluene
Concen: 7.603 ng/ul
RT: 14.693 min Scan# 1973
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:165 Resp: 78749
Ion Ratio Lower Upper
165 100
63 61.7 47.0 70.6
182 2.8 2.2 3.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 7.950 ng/ul
RT: 14.951 min Scan# 2017
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:232 Resp: 67208
Ion Ratio Lower Upper
232 100
131 58.0 35.8 53.8#
130 3.0 1.8 2.8#
166 35.8 23.7 35.5#

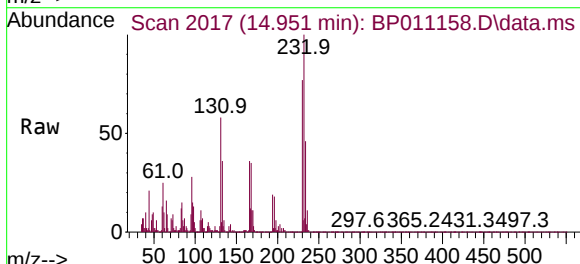



#59

Diethylphthalate

Concen: 8.620 ng/ul

RT: 15.163 min Scan# 2053

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD010625





Tgt Ion:149 Resp: 355074

Ion Ratio Lower Upper

149 100

177 20.3 17.6 26.4

150 11.8 10.3 15.5

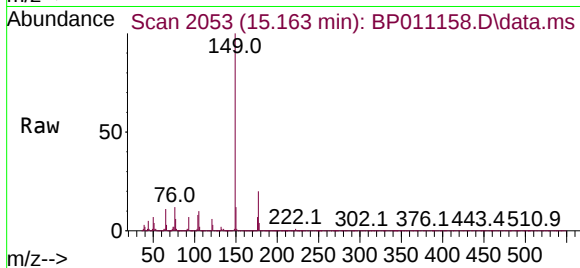

#61

Fluorene

Concen: 9.432 ng/ul

RT: 15.375 min Scan# 2089

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45




Tgt Ion:166 Resp: 364122


Ion Ratio Lower Upper

166 100

165 97.3 77.4 116.2

167 13.8 10.8 16.2









#62
4-Chlorophenyl-phenylether
Concen: 9.383 ng/ul
RT: 15.375 min Scan# 2089
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:204 Resp: 166755
Ion Ratio Lower Upper
204 100
206 32.1 26.0 39.0
141 71.6 49.3 73.9



#63
4-Nitroaniline
Concen: 4.089 ng/ul
RT: 15.410 min Scan# 2095
Delta R.T. 0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:138 Resp: 32786
Ion Ratio Lower Upper
138 100
92 63.4 46.2 69.2
108 87.7 85.8 128.8


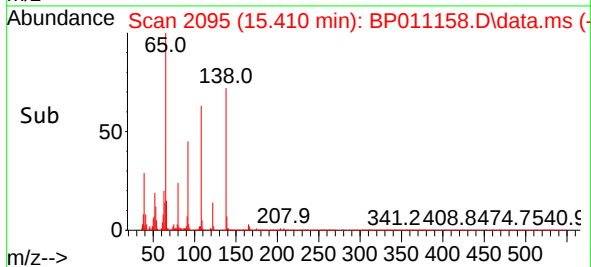

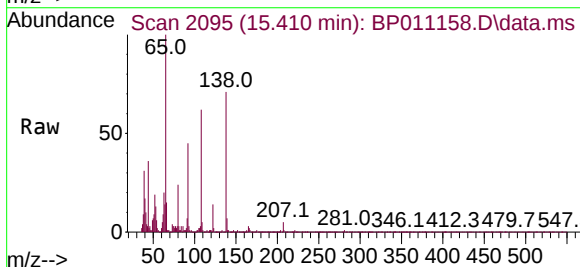




#66
4,6-Dinitro-2-methylphenol
Concen: 6.796 ng/ul
RT: 15.457 min Scan# 2103
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:198 Resp: 36137
Ion Ratio Lower Upper
198 100
182 10.7 4.3 6.5#
77 42.9 23.7 35.5#

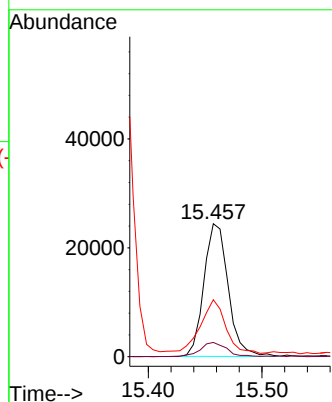

#67
N-Nitrosodiphenylamine
Concen: 9.675 ng/ul
RT: 15.593 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:169 Resp: 289505
Ion Ratio Lower Upper
169 100
168 69.0 52.6 78.8
167 39.1 27.8 41.6









#68
4-Bromophenyl-phenylether
Concen: 9.342 ng/ul
RT: 16.281 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:248 Resp: 88263
Ion Ratio Lower Upper
248 100
250 100.2 80.8 121.2
141 90.1 63.9 95.9



#69
Hexachlorobenzene
Concen: 9.697 ng/ul
RT: 16.381 min Scan# 2260
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:284 Resp: 106324
Ion Ratio Lower Upper
284 100
142 44.8 27.8 41.6#
249 29.9 25.4 38.2

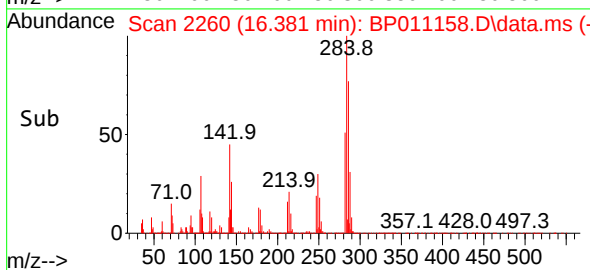



#70

Atrazine

Concen: 8.089 ng/ul

RT: 16.563 min Scan# 2291

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD010625





Tgt Ion:200 Resp: 83736

Ion Ratio Lower Upper

200 100

173 26.6 20.7 31.1

215 47.1 38.6 57.8



#71

Pentachlorophenol

Concen: 7.587 ng/ul

RT: 16.734 min Scan# 2320

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45




Tgt Ion:266 Resp: 51233


Ion Ratio Lower Upper

266 100

264 63.7 51.4 77.2

268 63.2 53.5 80.3









#72
Phenanthrene
Concen: 9.950 ng/ul
RT: 17.128 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:178 Resp: 543034
Ion Ratio Lower Upper
178 100
179 15.4 12.7 19.1
176 19.1 14.6 22.0



#74
Anthracene
Concen: 9.937 ng/ul
RT: 17.222 min Scan# 2403
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:178 Resp: 539466
Ion Ratio Lower Upper
178 100
179 15.1 12.2 18.2
176 18.9 14.5 21.7

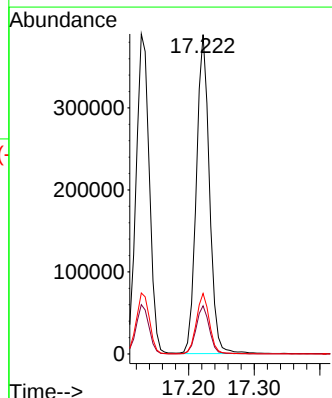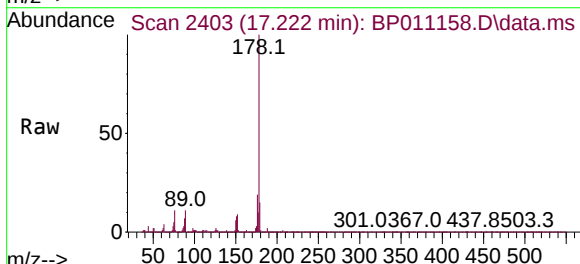



#75

1,2,3,4-Tetrachlorobenzene

Concen: 10.779 ng/uL

RT: 13.099 min Scan# 1702

Delta R.T. -0.006 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD010625





Tgt Ion:216 Resp: 161643

Ion Ratio Lower Upper

216 100

214 79.5 65.0 97.4

218 48.8 39.1 58.7

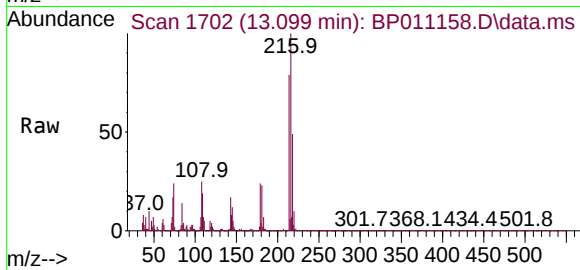

#76

Pentachlorobenzene

Concen: 10.248 ng/uL

RT: 14.634 min Scan# 1963

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45




Tgt Ion:250 Resp: 134715


Ion Ratio Lower Upper

250 100

248 65.8 49.8 74.6

252 65.6 51.2 76.8




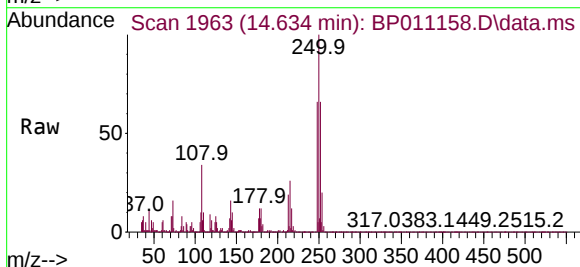




#77
 Carbazole
 Concen: 9.130 ng/ul
 RT: 17.504 min Scan# 2451
 Delta R.T. 0.006 min
 Lab File: BP011158.D
 Acq: 28 Jul 2022 12:45




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010625


Tgt Ion:	167	Resp:	463866
Ion	Ratio	Lower	Upper
167	100		
166	21.5	16.9	25.3
139	13.3	10.6	16.0



#78
 Di-n-butylphthalate
 Concen: 8.219 ng/ul
 RT: 18.075 min Scan# 2548
 Delta R.T. 0.006 min
 Lab File: BP011158.D
 Acq: 28 Jul 2022 12:45

Tgt Ion:	149	Resp:	521989
Ion	Ratio	Lower	Upper
149	100		
150	9.0	7.1	10.7
104	5.9	4.6	6.8




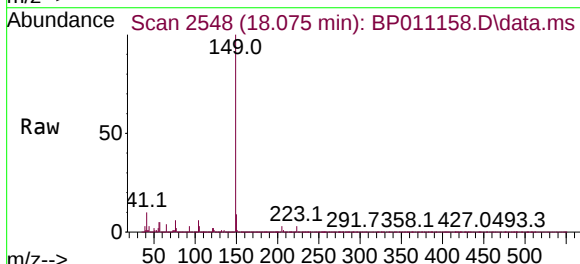




#80
Fluoranthene
Concen: 9.019 ng/ul
RT: 19.116 min Scan# 2725
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:202 Resp: 583150
Ion Ratio Lower Upper
202 100
101 15.2 7.1 10.7#
100 11.4 5.7 8.5#



#82
Pyrene
Concen: 9.439 ng/ul
RT: 19.475 min Scan# 2786
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:202 Resp: 629721
Ion Ratio Lower Upper
202 100
101 16.2 7.9 11.9#
100 13.8 6.7 10.1#





#83

Butylbenzylphthalate

Concen: 7.328 ng/ul

RT: 20.369 min Scan# 2938

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD010625





Tgt Ion:149 Resp: 218092

Ion Ratio Lower Upper

149 100

91 81.7 60.0 90.0

206 17.3 17.4 26.2#

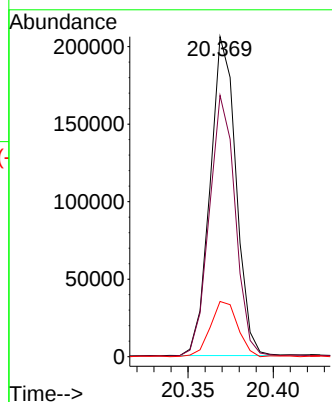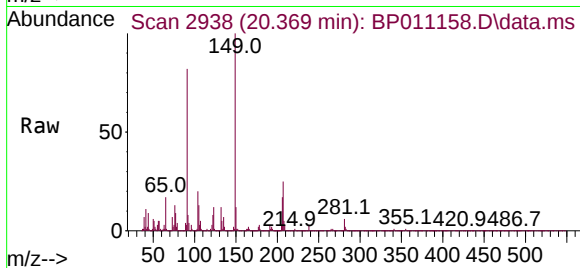

#84

3,3'-Dichlorobenzidine

Concen: 8.298 ng/ul

RT: 21.139 min Scan# 3069

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45




Tgt Ion:252 Resp: 154662


Ion Ratio Lower Upper

252 100

254 63.9 51.0 76.4

126 15.9 8.6 12.8#









#85
Benzo(a)anthracene
Concen: 9.271 ng/ul
RT: 21.198 min Scan# 3079
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:228 Resp: 594346
Ion Ratio Lower Upper
228 100
229 19.2 15.0 22.4
226 27.1 20.6 31.0

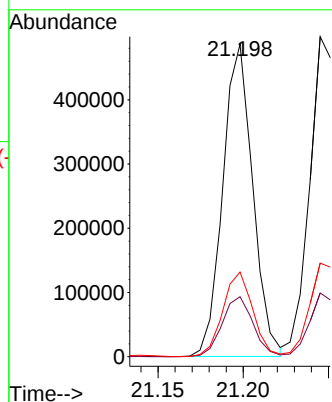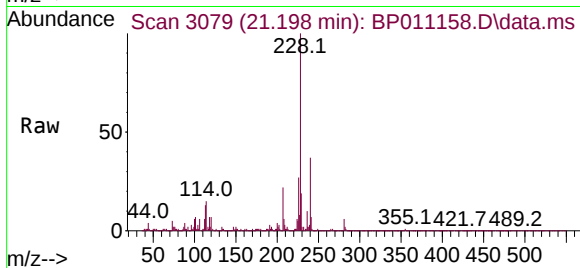

#86
Bis(2-ethylhexyl)phthalate
Concen: 7.909 ng/ul
RT: 21.139 min Scan# 3069
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:149 Resp: 351211
Ion Ratio Lower Upper
149 100
167 25.3 22.6 33.8
279 3.2 4.2 6.4#




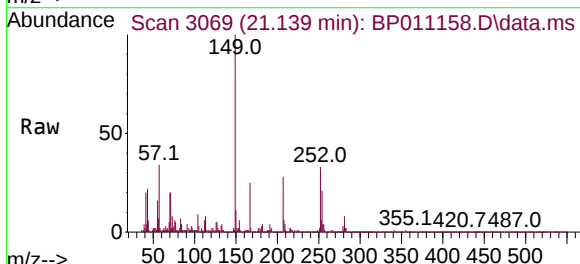




#87
Chrysene
Concen: 9.709 ng/ul
RT: 21.245 min Scan# 3087
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:228 Resp: 611159
Ion Ratio Lower Upper
228 100
226 29.3 23.6 35.4
229 19.9 15.6 23.4



#89
Di-n-octyl phthalate
Concen: 7.824 ng/ul
RT: 22.051 min Scan# 3224
Delta R.T. 0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:149 Resp: 601929









#90
Benzo(b)fluoranthene
Concen: 9.130 ng/ul
RT: 22.839 min Scan# 3358
Delta R.T. 0.000 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD010625


Tgt Ion:252 Resp: 646755
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.6
125 14.5 6.2 9.2#

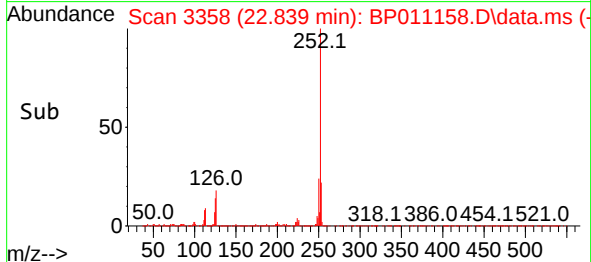

#91
Benzo(k)fluoranthene
Concen: 9.709 ng/ul
RT: 22.886 min Scan# 3366
Delta R.T. -0.006 min
Lab File: BP011158.D
Acq: 28 Jul 2022 12:45

Tgt Ion:252 Resp: 645995
Ion Ratio Lower Upper
252 100
253 22.2 17.0 25.4
125 14.1 6.2 9.4#

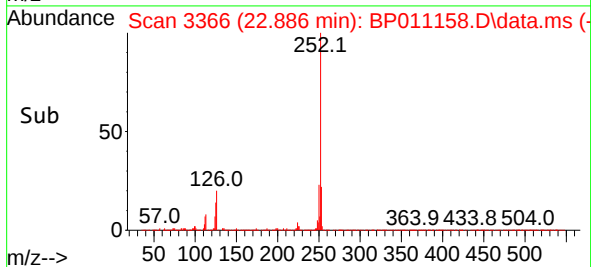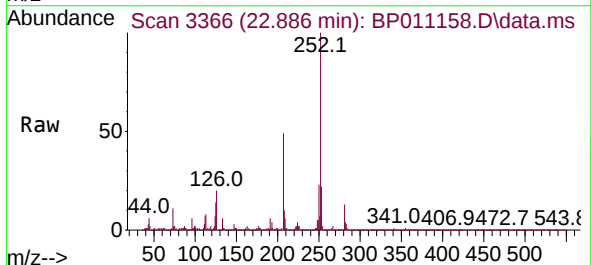



#93

Benzo(a)pyrene

Concen: 9.506 ng/ul

RT: 23.451 min Scan# 3462

Delta R.T. 0.000 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD010625





Tgt Ion:252 Resp: 646654

Ion Ratio Lower Upper

252 100

253 22.3 17.4 26.0

125 16.1 6.6 10.0#

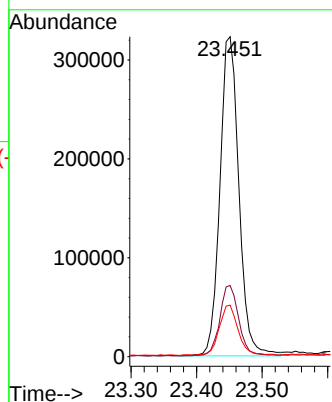

#94

Indeno(1,2,3-cd)pyrene

Concen: 9.920 ng/ul

RT: 25.974 min Scan# 3891

Delta R.T. -0.006 min

Lab File: BP011158.D

Acq: 28 Jul 2022 12:45




Tgt Ion:276 Resp: 784245


Ion Ratio Lower Upper

276 100

138 30.6 14.6 22.0#

277 24.4 19.6 29.4









#95
 Dibenzo(a,h)anthracene
 Concen: 9.926 ng/ul
 RT: 25.998 min Scan# 3895
 Delta R.T. -0.006 min
 Lab File: BP011158.D
 Acq: 28 Jul 2022 12:45

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010625

Tgt Ion:278 Resp: 679044
 Ion Ratio Lower Upper
 278 100
 139 22.0 9.4 14.2#
 279 23.2 18.9 28.3



#96
 Benzo(g,h,i)perylene
 Concen: 10.021 ng/ul
 RT: 26.715 min Scan# 4017
 Delta R.T. -0.006 min
 Lab File: BP011158.D
 Acq: 28 Jul 2022 12:45

Tgt Ion:276 Resp: 674740
 Ion Ratio Lower Upper
 276 100
 138 28.8 12.7 19.1#
 277 23.2 18.2 27.4

