

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072822\
 Data File : BP011163.D
 Acq On : 28 Jul 2022 15:38
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV630

Quant Time: Jul 28 16:23:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.652	152	297064	20.000	ng/ul	0.00
20) Naphthalene-d8	10.446	136	1328355	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.316	164	646430	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.086	188	1032449	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.210	240	931534	20.000	ng/ul	# 0.00
88) Perylene-d12	23.557	264	1029490	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.152	96	49090	7.568	ng/uL	0.00
4) Pyridine-d5	3.558	84	354571	19.321	ng/ul	0.00
7) Phenol-d5	6.828	99	505797	19.507	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	388936	21.213	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	417210	20.418	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	420768	19.838	ng/ul	0.00
21) Nitrobenzene-d5	8.810	128	214659	20.793	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	206570	20.890	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	352915	20.251	ng/ul	0.00
31) 4-Chloroaniline-d4	10.593	131	544929	19.289	ng/ul	0.00
46) Dimethylphthalate-d6	13.740	166	880082	19.983	ng/ul	0.00
49) Acenaphthylene-d8	14.010	160	1164388	21.039	ng/ul	0.00
54) 4-Nitrophenol-d4	14.534	143	129996	16.409	ng/ul	0.00
60) Fluorene-d10	15.322	176	721459	19.494	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	92767	17.824	ng/ul	0.00
73) Anthracene-d10	17.186	188	931354	20.473	ng/ul	0.00
81) Pyrene-d10	19.445	212	966659	19.312	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.404	264	1041436	20.367	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.187	88	49990	7.445	ng/uL#	82
5) Pyridine	3.581	79	349360	18.455	ng/ul#	74
6) Benzaldehyde	6.799	77	296564	23.711	ng/ul	98
8) Phenol	6.858	94	529063	19.019	ng/ul	91
10) Bis(2-Chloroethyl)ether	7.087	93	449418	19.926	ng/ul	94
12) 2-Chlorophenol	7.216	128	422884	19.906	ng/ul	96
13) 2-Methylphenol	8.099	108	396941	19.252	ng/ul	98
14) 2,2'-oxybis(1-Chloropr...	8.193	45	739256	19.569	ng/ul	97
16) Acetophenone	8.481	105	680492	20.625	ng/ul	96
17) N-Nitroso-di-n-propyla...	8.469	70	360137	20.649	ng/ul	99
18) 4-Methylphenol	8.428	108	428600	19.302	ng/ul	97
19) Hexachloroethane	8.716	117	188329	19.735	ng/ul#	71
22) Nitrobenzene	8.857	77	528905	19.927	ng/ul	96
23) Isophorone	9.387	82	951238	19.808	ng/ul	98
25) 2-Nitrophenol	9.563	139	222338	20.010	ng/ul	92
26) 2,4-Dimethylphenol	9.634	107	477736	20.014	ng/ul	98
27) Bis(2-Chloroethoxy)met...	9.869	93	595471	19.735	ng/ul	98
29) 2,4-Dichlorophenol	10.093	162	351902	19.525	ng/ul	98
30) Naphthalene	10.493	128	1382044	19.776	ng/ul	99
32) 4-Chloroaniline	10.616	127	532553	18.971	ng/ul	97
33) Hexachlorobutadiene	10.775	225	216438	19.662	ng/ul	95
34) Caprolactam	11.410	113	88287	14.729	ng/ul	90
35) 4-Chloro-3-methylphenol	11.751	107	374159	18.515	ng/ul	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072822\
 Data File : BP011163.D
 Acq On : 28 Jul 2022 15:38
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Quant Time: Jul 28 16:23:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.116	142	877530	19.842	ng/ul	99
37) 1-Methylnaphthalene	12.340	142	855323	19.305	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.487	216	375898	20.901	ng/ul#	98
40) Hexachlorocyclopentadiene	12.463	237	252583	21.302	ng/ul	95
41) 2,4,6-Trichlorophenol	12.740	196	231406	20.490	ng/ul	97
42) 2,4,5-Trichlorophenol	12.810	196	236495	19.782	ng/ul	99
43) 1,1'-Biphenyl	13.145	154	1068484	20.687	ng/ul#	96
44) 2-Chloronaphthalene	13.181	162	798300	20.674	ng/ul	97
45) 2-Nitroaniline	13.404	65	217376	19.370	ng/ul	92
47) Dimethylphthalate	13.787	163	851920	19.207	ng/ul	99
48) 2,6-Dinitrotoluene	13.904	165	163953	21.154	ng/ul	93
50) Acenaphthylene	14.034	152	1249966	20.217	ng/ul	98
51) 3-Nitroaniline	14.234	138	168434	20.123	ng/ul	98
52) Acenaphthene	14.381	153	805154	19.937	ng/ul	98
53) 2,4-Dinitrophenol	14.445	184	61127	13.985	ng/ul	97
55) 4-Nitrophenol	14.551	109	109610	16.102	ng/ul#	82
56) Dibenzofuran	14.722	168	1071657	19.522	ng/ul	99
57) 2,4-Dinitrotoluene	14.698	165	200197	18.514	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	14.951	232	168678	19.404	ng/ul#	81
59) Diethylphthalate	15.163	149	820125	18.500	ng/ul	97
61) Fluorene	15.375	166	816795	19.135	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.375	204	370179	19.054	ng/ul	89
63) 4-Nitroaniline	15.410	138	123989	17.424	ng/ul#	85
66) 4,6-Dinitro-2-methylph...	15.463	198	96141	18.189	ng/ul#	95
67) N-Nitrosodiphenylamine	15.592	169	653892	20.609	ng/ul	97
68) 4-Bromophenyl-phenylether	16.281	248	200852	20.273	ng/ul	92
69) Hexachlorobenzene	16.381	284	221399	19.535	ng/ul#	89
70) Atrazine	16.563	200	178038	17.844	ng/ul	94
71) Pentachlorophenol	16.733	266	116918	17.968	ng/ul	96
72) Phenanthrene	17.128	178	1108580	19.620	ng/ul	98
74) Anthracene	17.222	178	1118531	20.009	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.104	216	381708	21.446	ng/uL	97
76) Pentachlorobenzene	14.634	250	315476	21.505	ng/uL	98
77) Carbazole	17.504	167	957150	19.327	ng/ul	97
78) Di-n-butylphthalate	18.075	149	1152466	19.459	ng/ul	100
80) Fluoranthene	19.116	202	1127613	18.237	ng/ul#	84
82) Pyrene	19.475	202	1186209	18.669	ng/ul#	83
83) Butylbenzylphthalate	20.374	149	475199	18.677	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.139	252	326640	20.103	ng/ul#	98
85) Benzo(a)anthracene	21.198	228	1151539	19.886	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.139	149	772388	20.087	ng/ul#	94
87) Chrysene	21.251	228	1103414	19.167	ng/ul	100
89) Di-n-octyl phthalate	22.051	149	1310412	18.520	ng/ul	100
90) Benzo(b)fluoranthene	22.845	252	1296117	19.971	ng/ul#	95
91) Benzo(k)fluoranthene	22.892	252	1212587	19.686	ng/ul#	95
93) Benzo(a)pyrene	23.451	252	1214027	19.177	ng/ul#	94
94) Indeno(1,2,3-cd)pyrene	25.980	276	1506400	19.315	ng/ul#	87
95) Dibenzo(a,h)anthracene	25.998	278	1312165	19.616	ng/ul#	91
96) Benzo(g,h,i)perylene	26.721	276	1318289	19.544	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
BNA_P
ClientSampleId :
SICV630

Quant Time: Jul 28 16:23:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 16:05:22 2022
Response via : Initial Calibration



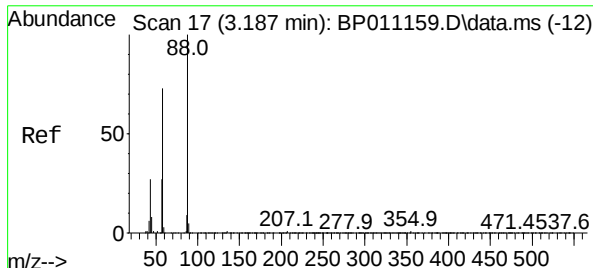

1,4-Dioxane

Concen: 7.445 ng/uL

RT: 3.187 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion: 88 Resp: 49990

Ion Ratio Lower Upper

88 100

43 30.7 35.8 53.6#

58 69.8 68.1 102.1

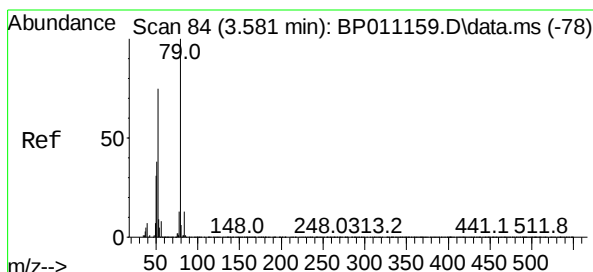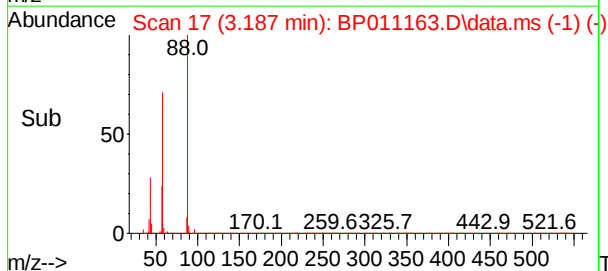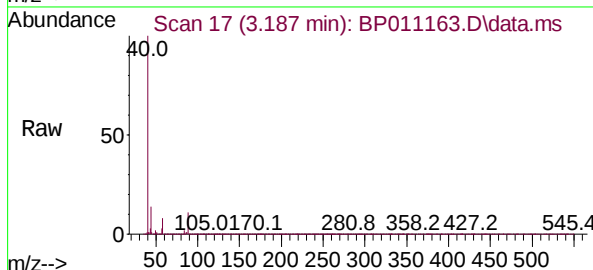

Pyridine

Concen: 18.455 ng/uL

RT: 3.581 min Scan# 84

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38




Tgt Ion: 79 Resp: 349360


Ion Ratio Lower Upper

79 100

52 74.0 83.8 125.8#

51 38.2 41.0 61.4#

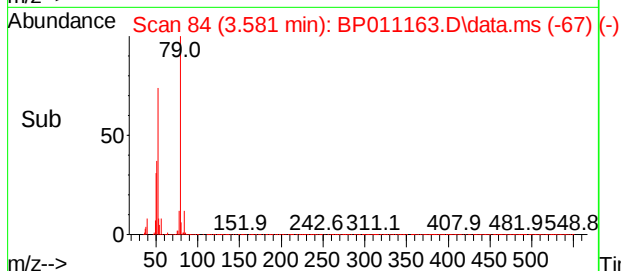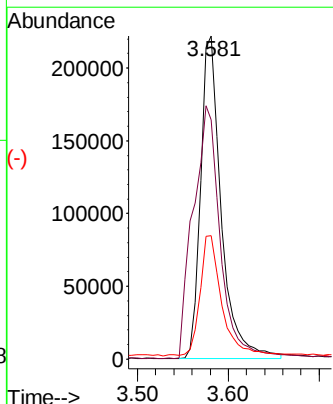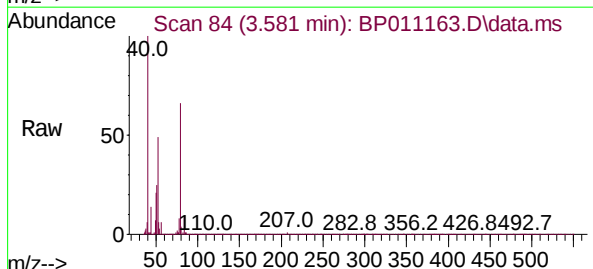

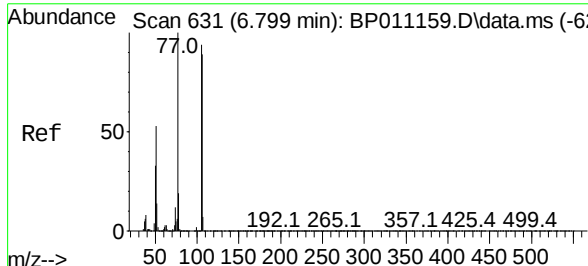

Benzaldehyde

Concen: 23.711 ng/ul

RT: 6.799 min Scan# 631

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :





BNA_P

ClientSampleId :

SICV630

Tgt Ion: 77 Resp: 296564

Ion	Ratio	Lower	Upper
77	100		
105	93.2	76.0	114.0
106	89.8	73.2	109.8

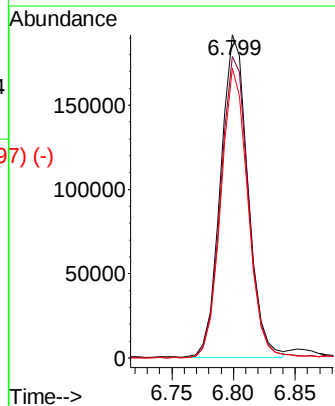

Phenol

Concen: 19.019 ng/ul

RT: 6.858 min Scan# 641




Delta R.T. 0.000 min


Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Tgt Ion: 94 Resp: 529063

Ion	Ratio	Lower	Upper
94	100		
65	30.6	27.4	41.2
66	39.8	37.4	56.2



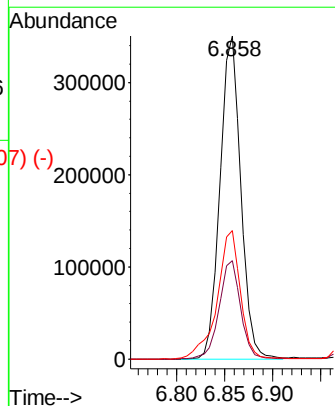



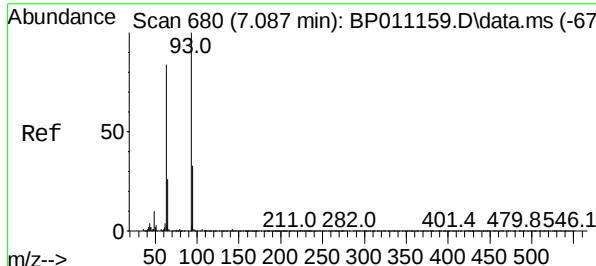

Scan 680 (7.087 min): BP011159.D\data.ms (-673) #10
 Bis(2-Chloroethyl)ether
 Concen: 19.926 ng/ul
 RT: 7.087 min Scan# 680
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	93	Resp:	449418
Ion	Ratio	Lower	Upper
93	100		
63	84.4	72.4	108.6
95	31.8	27.3	40.9

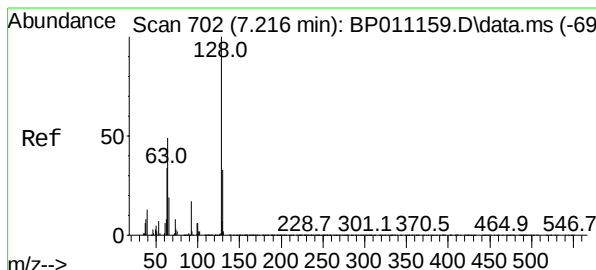

Scan 702 (7.216 min): BP011159.D\data.ms (-694) #12
 2-Chlorophenol
 Concen: 19.906 ng/ul
 RT: 7.216 min Scan# 702
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	128	Resp:	422884
Ion	Ratio	Lower	Upper
128	100		
64	52.1	44.8	67.2
130	33.3	25.8	38.6



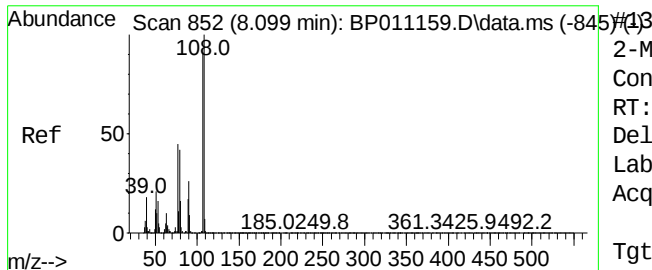

2-Methylphenol

Concen: 19.252 ng/ul

RT: 8.099 min Scan# 852

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :





SICV630

Tgt Ion:108 Resp: 396941

Ion Ratio Lower Upper

108 100

107 90.8 71.4 107.0

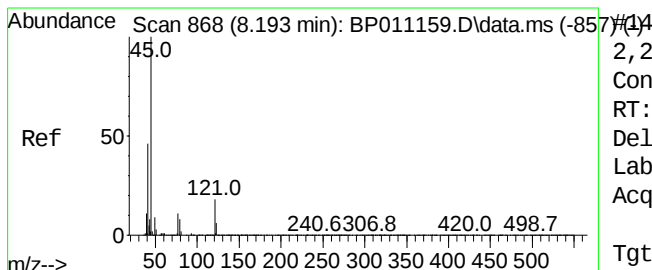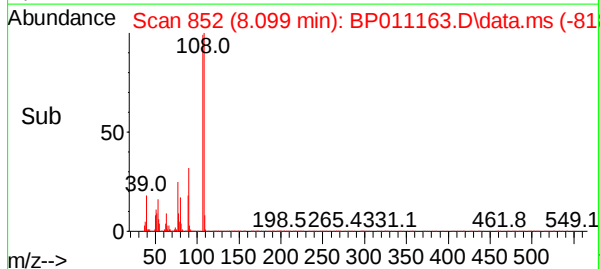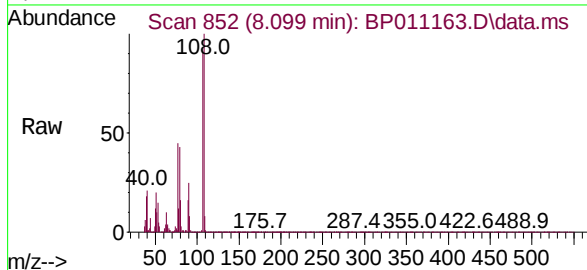

2,2'-oxybis(1-Chloropropane)

Concen: 19.569 ng/ul

RT: 8.193 min Scan# 868

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38




Tgt Ion: 45 Resp: 739256


Ion Ratio Lower Upper

45 100

77 12.9 11.2 16.8

79 9.9 6.9 10.3

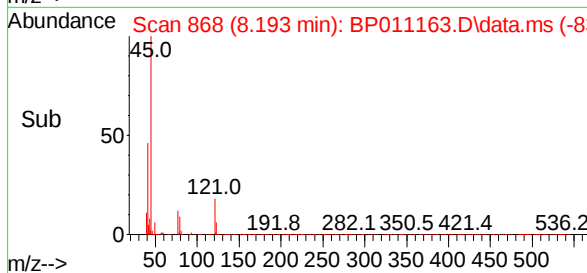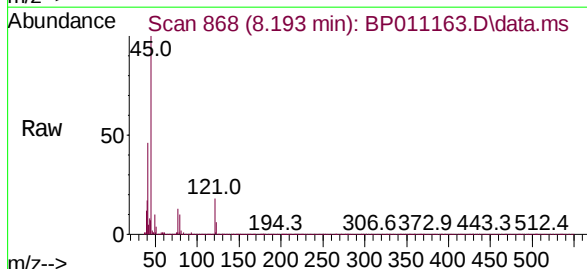

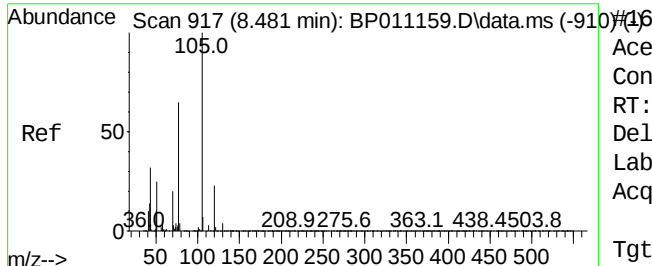

Acetophenone

Concen: 20.625 ng/ul

RT: 8.481 min Scan# 917

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:105 Resp: 680492

Ion Ratio Lower Upper

105 100

77 81.8 67.5 101.3

51 32.6 29.6 44.4

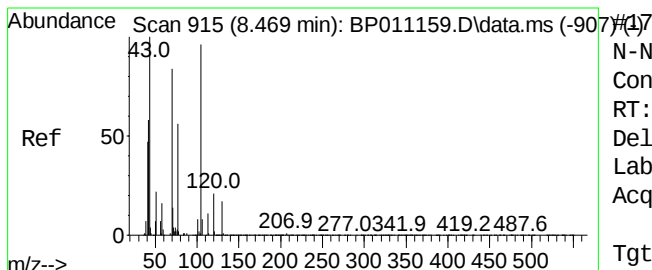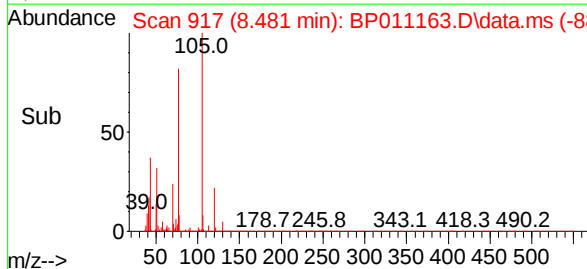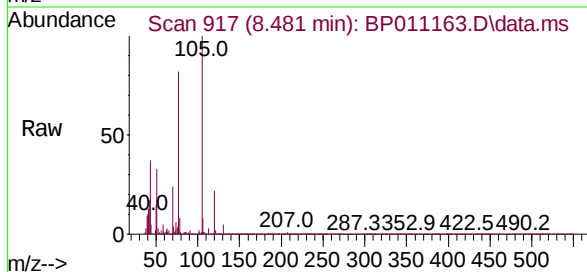

N-Nitroso-di-n-propylamine

Concen: 20.649 ng/ul

RT: 8.469 min Scan# 915

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Tgt Ion: 70 Resp: 360137




Ion Ratio Lower Upper


70 100

42 66.8 53.8 80.8

101 9.4 7.8 11.6

130 18.9 15.4 23.2

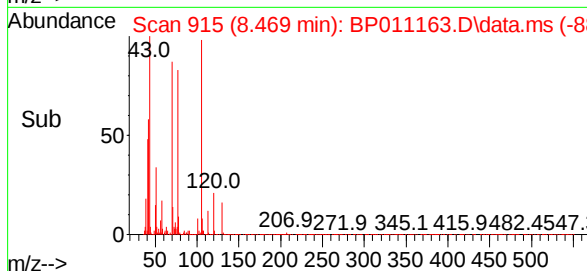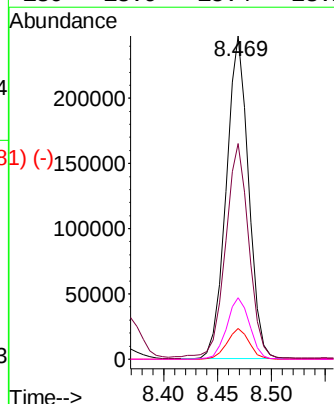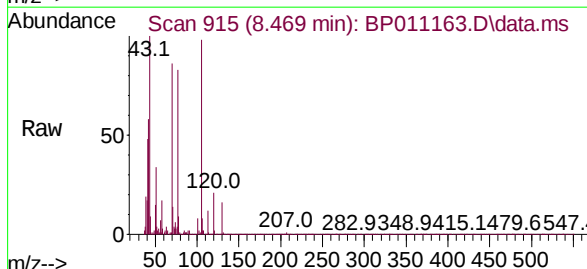

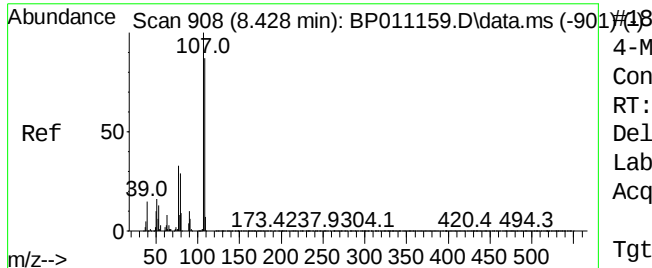

4-Methylphenol

Concen: 19.302 ng/ul

RT: 8.428 min Scan# 908

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :





SICV630

Tgt Ion:108 Resp: 428600

Ion Ratio Lower Upper

108 100

107 113.5 88.3 132.5

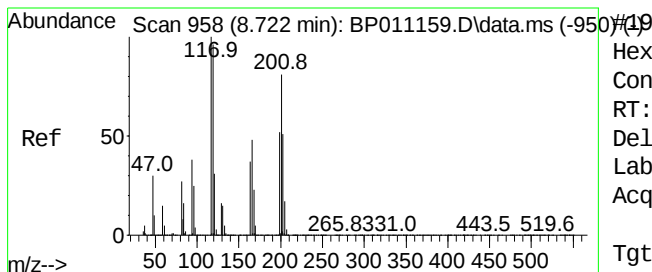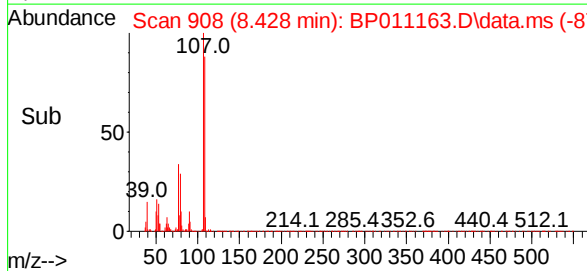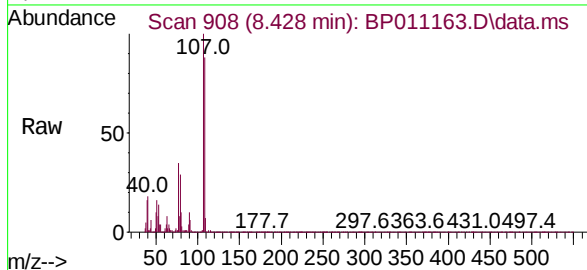

Hexachloroethane

Concen: 19.735 ng/ul

RT: 8.716 min Scan# 957

Delta R.T. -0.006 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38




Tgt Ion:117 Resp: 188329


Ion Ratio Lower Upper

117 100

201 76.5 85.7 128.5#

199 48.6 57.4 86.0#

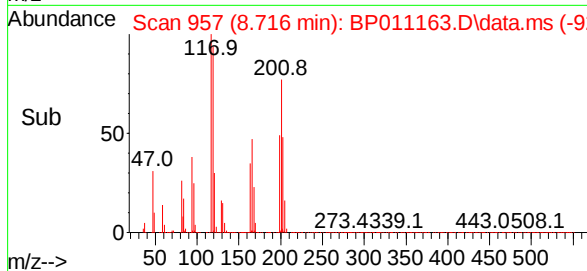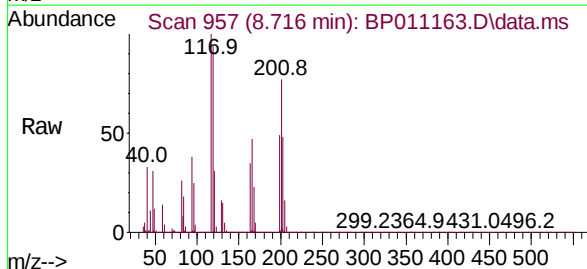

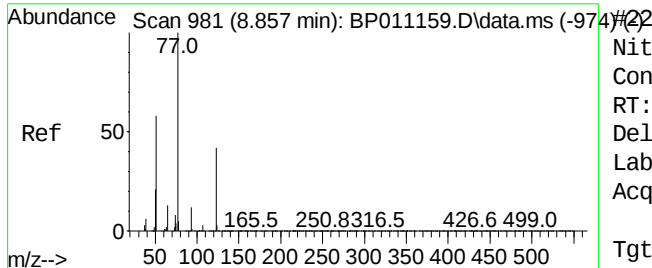

Nitrobenzene

Concen: 19.927 ng/ul

RT: 8.857 min Scan# 981

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion: 77 Resp: 528905

Ion Ratio Lower Upper

77 100

123 42.4 31.5 47.3

65 13.8 11.4 17.2

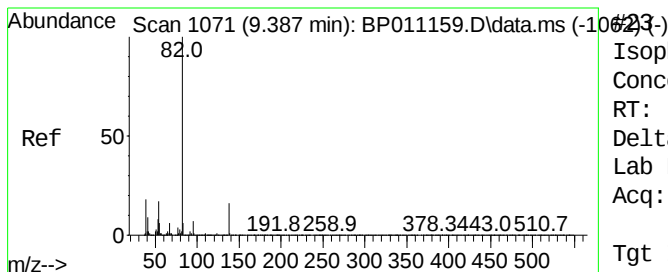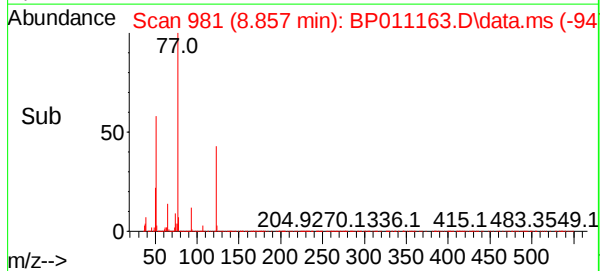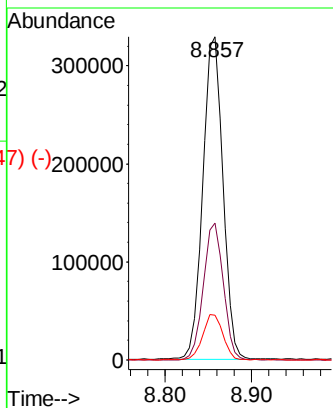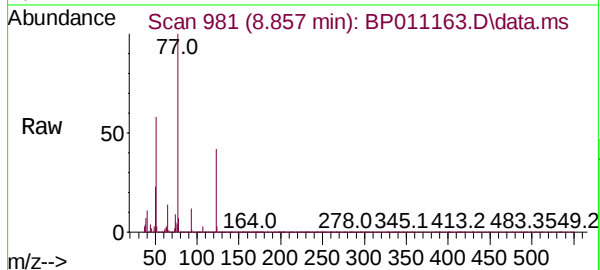

Isophorone

Concen: 19.808 ng/ul

RT: 9.387 min Scan# 1071

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38




Tgt Ion: 82 Resp: 951238


Ion Ratio Lower Upper

82 100

95 7.1 6.6 10.0

138 16.6 13.8 20.6

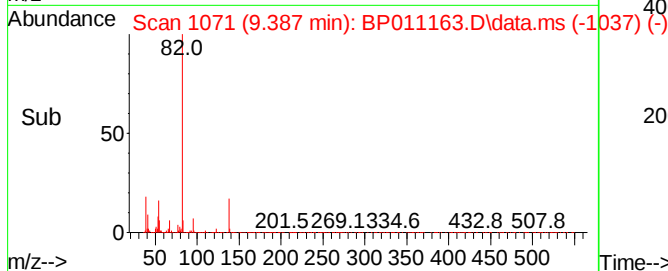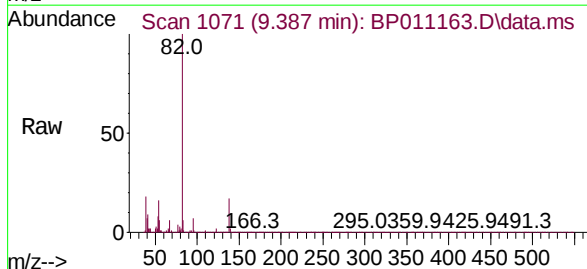

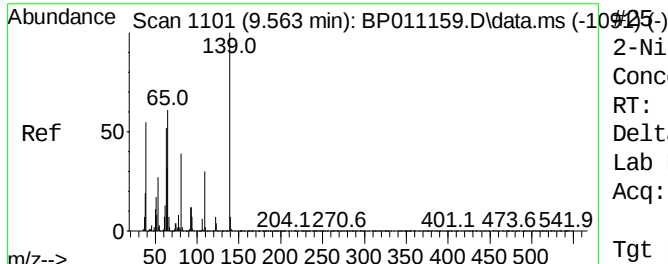

2-Nitrophenol

Concen: 20.010 ng/ul

RT: 9.563 min Scan# 1101

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:139 Resp: 222338

Ion Ratio Lower Upper

139 100

65 62.1 54.2 81.4

109 32.3 30.6 45.8

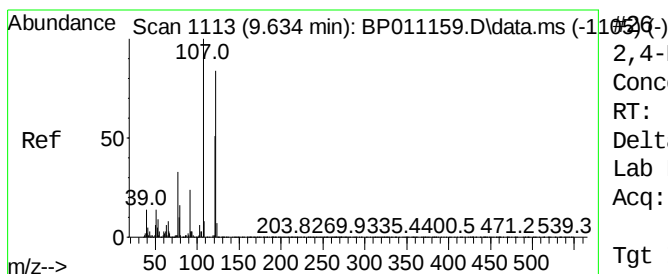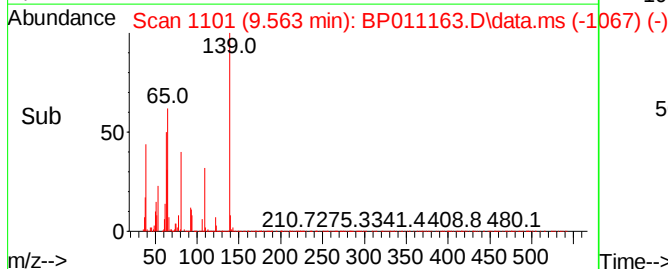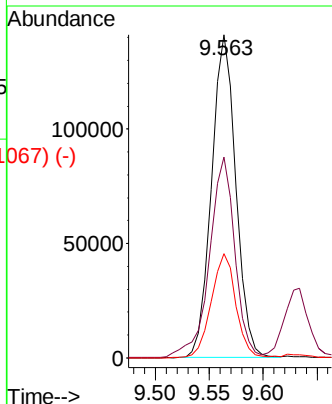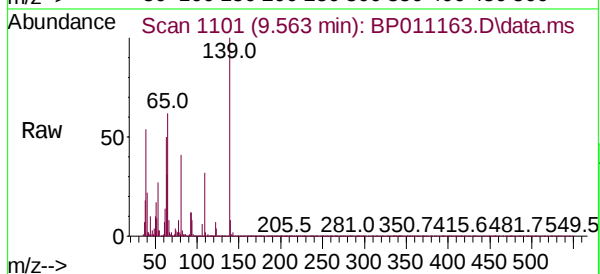

2,4-Dimethylphenol

Concen: 20.014 ng/ul

RT: 9.634 min Scan# 1113

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38




Tgt Ion:107 Resp: 477736

Ion Ratio Lower Upper

107 100

121 51.3 39.1 58.7

122 84.0 66.1 99.1

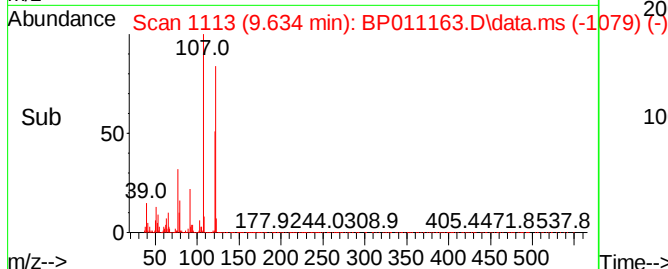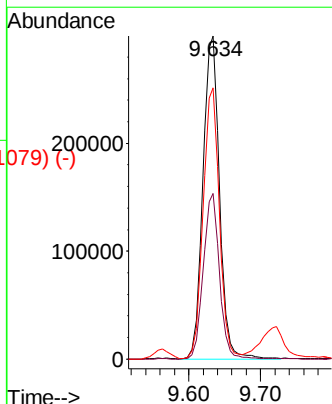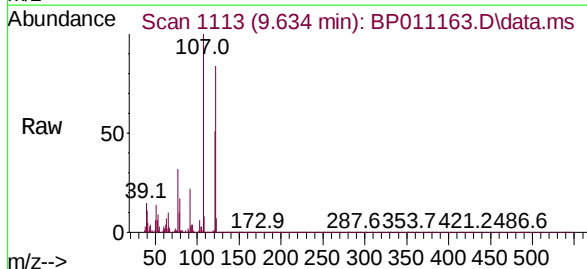

Abundance Scan 1153 (9.869 min): BP011159.D\data.ms (-1147) (-)

Bis(2-Chloroethoxy)methane

Concen: 19.735 ng/ul

RT: 9.869 min Scan# 1153

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630

Tgt Ion: 93 Resp: 595471

Ion Ratio Lower Upper

93 100

95 32.5 26.6 39.8

123 11.0 7.8 11.8

Abundance Scan 1153 (9.869 min): BP011163.D\data.ms

Ref 50

93.0

171.0 288.8 354.5 423.4 491.1

m/z-->

50 100 150 200 250 300 350 400 450 500

Abundance Scan 1153 (9.869 min): BP011163.D\data.ms (-1119) (-)

Ref 50

93.0

173.0 247.3 313.1 380.4 476.6 548.9

m/z-->

50 100 150 200 250 300 350 400 450 500

Abundance

9.869

300000

200000

100000

0

Time-->

9.80 9.85 9.90 9.95

Abundance Scan 1191 (10.093 min): BP011159.D\data.ms (-1129) (-)

2,4-Dichlorophenol

Concen: 19.525 ng/ul

RT: 10.093 min Scan# 1191

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Tgt Ion: 162 Resp: 351902

Ion Ratio Lower Upper

162 100

164 66.2 52.5 78.7

98 41.8 31.4 47.0

Abundance Scan 1191 (10.093 min): BP011163.D\data.ms

Ref 50

63.0

161.9

292.1 356.8 421.6 487.3

m/z-->

50 100 150 200 250 300 350 400 450 500

Abundance Scan 1191 (10.093 min): BP011163.D\data.ms (-1157) (-)

Ref 50

63.0

161.9

231.7 297.5 416.7 490.4

m/z-->

50 100 150 200 250 300 350 400 450 500

Abundance

10.093

200000

150000


100000

50000

0

Time-->





10.00 10.10 10.20

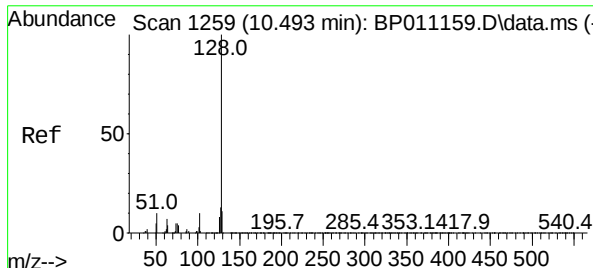

Scan 1259 (10.493 min): BP011159.D\data.ms (-1259) (-)
 Naphthalene
 Concen: 19.776 ng/ul
 RT: 10.493 min Scan# 1259
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	128	Resp:	1382044
Ion	Ratio	Lower	Upper
128	100		
129	11.2	8.7	13.1
127	13.2	10.2	15.4

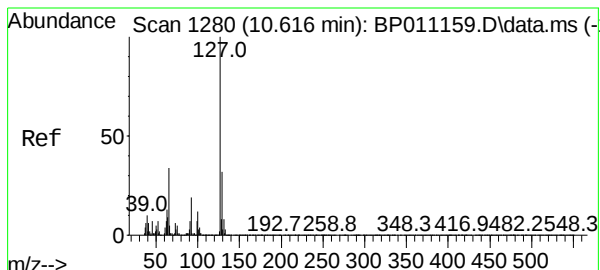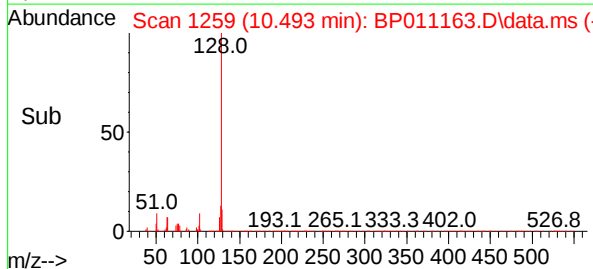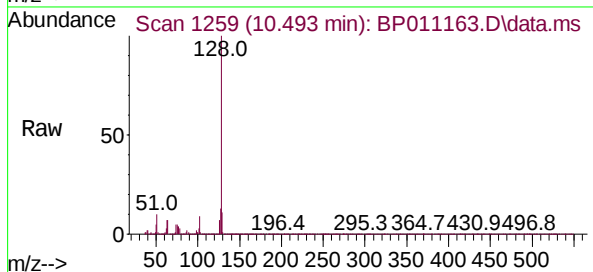

Scan 1280 (10.616 min): BP011159.D\data.ms (-1280) (-)
 4-Chloroaniline
 Concen: 18.971 ng/ul
 RT: 10.616 min Scan# 1280
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	127	Resp:	532553
Ion	Ratio	Lower	Upper
127	100		
129	31.2	26.2	39.2


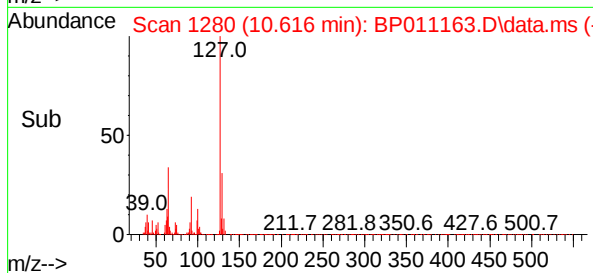

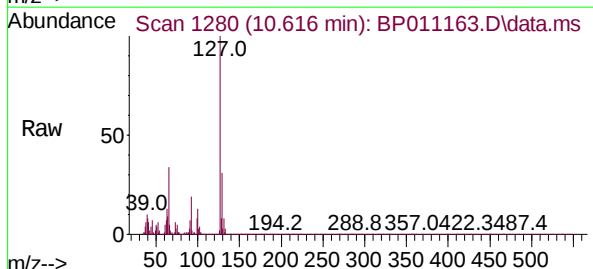


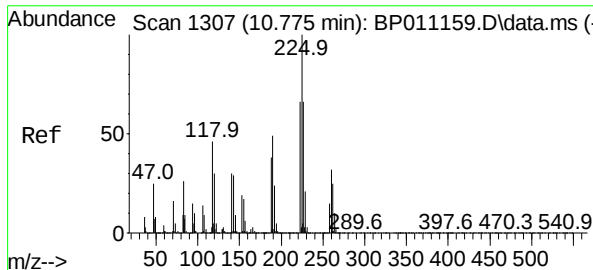

Scan 1307 (10.775 min): BP011159.D\data.ms (-1258) (-)
 Hexachlorobutadiene
 Concen: 19.662 ng/ul
 RT: 10.775 min Scan# 1307
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	225	Resp:	216438
Ion	Ratio	Lower	Upper
225	100		
223	61.7	53.7	80.5
227	63.5	49.4	74.2

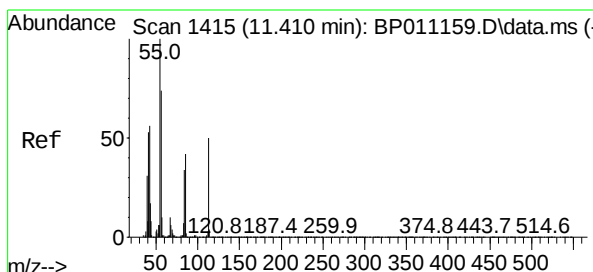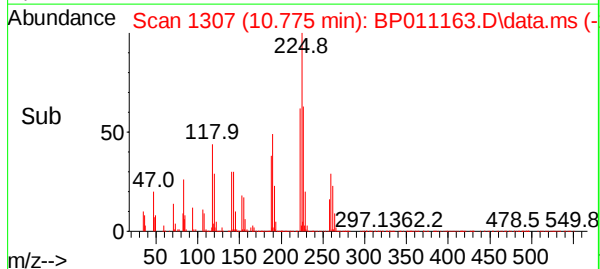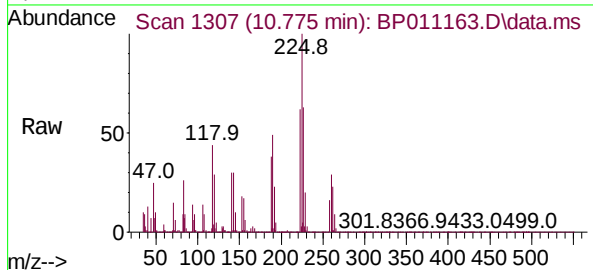

Scan 1415 (11.410 min): BP011159.D\data.ms (-1408) (-)
 Caprolactam
 Concen: 14.729 ng/ul
 RT: 11.410 min Scan# 1415
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	113	Resp:	88287
Ion	Ratio	Lower	Upper
113	100		
55	205.6	153.8	230.8
56	151.0	110.2	165.4


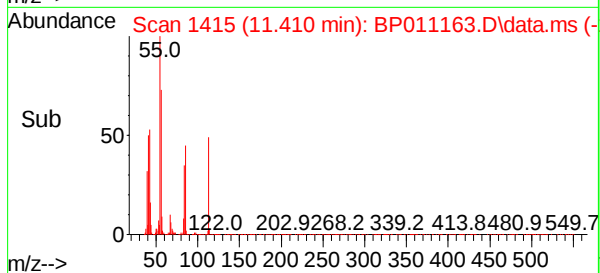

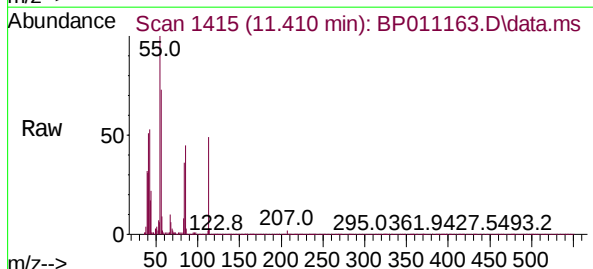




Scan 1473 (11.751 min): BP011159.D\data.ms (-1435) (-)
 4-Chloro-3-methylphenol
 Concen: 18.515 ng/ul
 RT: 11.751 min Scan# 1435
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 Client Sample Id :
 SICV630


Tgt Ion:	107	Resp:	374159
Ion	Ratio	Lower	Upper
107	100		
144	24.6	18.6	27.8
142	77.4	59.6	89.4

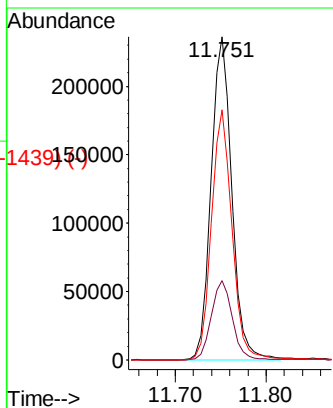

Scan 1535 (12.116 min): BP011159.D\data.ms (-1528) (-)
 2-Methylnaphthalene
 Concen: 19.842 ng/ul
 RT: 12.116 min Scan# 1535
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	142	Resp:	877530
Ion	Ratio	Lower	Upper
142	100		
141	88.7	70.1	105.1









Scan 1573 (12.340 min): BP011159.D\data.ms (-1537) (-)
 1-Methylnaphthalene
 Concen: 19.305 ng/ul
 RT: 12.340 min Scan# 1573
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	142	Resp:	855323
Ion Ratio	Lower	Upper	
142	100		
141	92.4	73.3	109.9
116	4.1	4.0	6.0



Scan 1598 (12.487 min): BP011159.D\data.ms (-1539) (-)
 1,2,4,5-Tetrachlorobenzene
 Concen: 20.901 ng/ul
 RT: 12.487 min Scan# 1598
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	216	Resp:	375898
Ion Ratio	Lower	Upper	
216	100		
214	79.0	63.0	94.6
179	22.7	18.1	27.1
108	23.6	13.6	20.4#



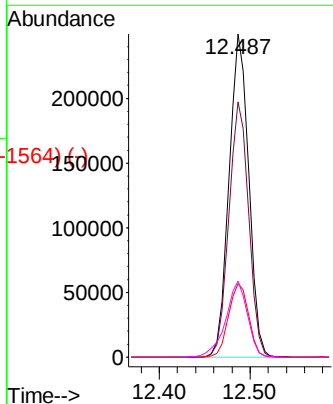



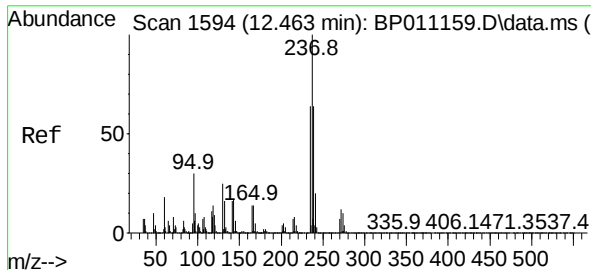

Hexachlorocyclopentadiene
 Concen: 21.302 ng/ul
 RT: 12.463 min Scan# 1594
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	237	Resp:	252583
Ion	Ratio	Lower	Upper
237	100		
235	62.3	52.8	79.2
272	12.0	11.5	17.3

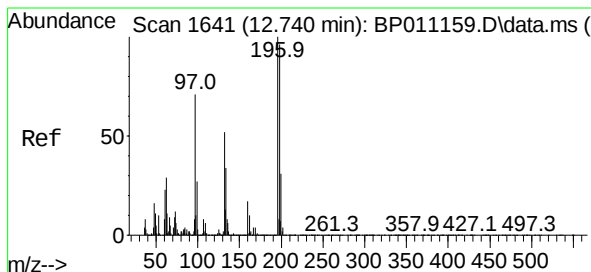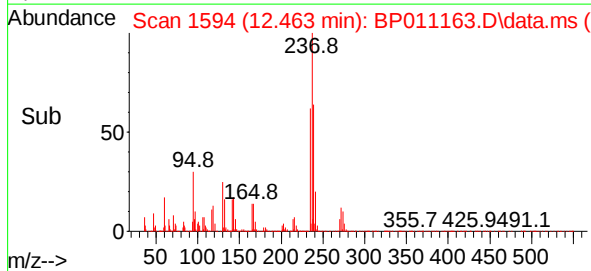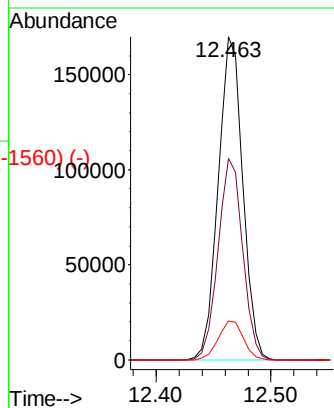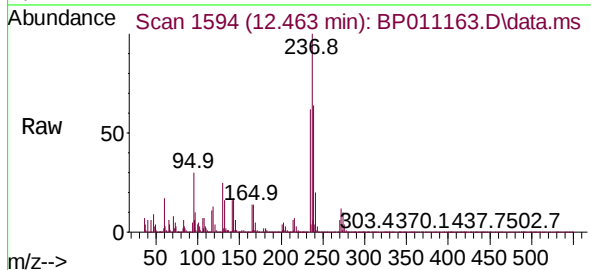

2,4,6-Trichlorophenol
 Concen: 20.490 ng/ul
 RT: 12.740 min Scan# 1641
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	196	Resp:	231406
Ion	Ratio	Lower	Upper
196	100		
198	95.0	78.2	117.4
200	30.4	25.0	37.6


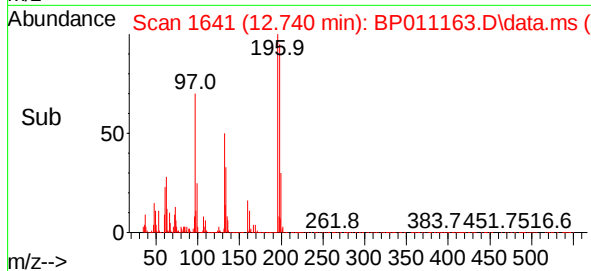

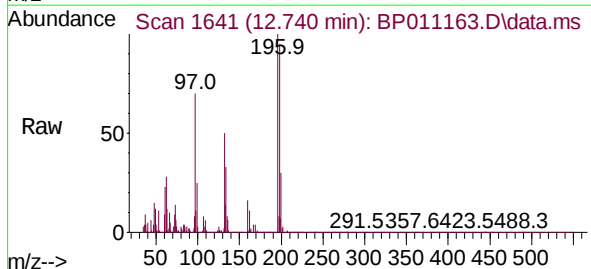




2,4,5-Trichlorophenol
Concen: 19.782 ng/ul
RT: 12.810 min Scan# 1653
Delta R.T. 0.006 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38




Instrument :
BNA_P
ClientSampleId :
SICV630

Tgt Ion:	196	Resp:	236495
Ion	Ratio	Lower	Upper
196	100		
198	97.7	77.0	115.4
200	31.5	24.8	37.2



1,1'-Biphenyl
Concen: 20.687 ng/ul
RT: 13.145 min Scan# 1710
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38

Tgt Ion:	154	Resp:	1068484
Ion	Ratio	Lower	Upper
154	100		
153	41.2	31.9	47.9
76	15.5	9.2	13.8#



Abundance Scan 1716 (13.181 min): BP011159.D\data.ms (-1700) (-)

2-Chloronaphthalene

Concen: 20.674 ng/ul

RT: 13.181 min Scan# 1700

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630

Tgt Ion:162 Resp: 798300

Ion Ratio Lower Upper

162 100

164 31.7 25.5 38.3

127 43.1 31.9 47.9

Abundance Scan 1716 (13.181 min): BP011163.D\data.ms

Ref 50

Raw 50

Sub 50

m/z--> 50 100 150 200 250 300 350 400 450 500

63.0 162.0 228.3 302.2 368.4 437.6 502.0

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance Scan 1716 (13.181 min): BP011163.D\data.ms (-1682) (-)

Ref 50

Raw 50

Sub 50

m/z--> 50 100 150 200 250 300 350 400 450 500

63.0 161.9 228.3 294.8 415.7 490.8

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance

500000

400000

300000

200000

100000

0

Time--> 13.10 13.20

Abundance Scan 1753 (13.398 min): BP011159.D\data.ms (-1745) (-)

2-Nitroaniline

Concen: 19.370 ng/ul

RT: 13.404 min Scan# 1754

Delta R.T. 0.006 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Tgt Ion: 65 Resp: 217376

Ion Ratio Lower Upper

65 100

92 65.2 49.0 73.6

138 91.7 66.4 99.6

Abundance Scan 1754 (13.404 min): BP011163.D\data.ms

Ref 50

Raw 50

Sub 50

m/z--> 50 100 150 200 250 300 350 400 450 500

65.0 138.0 206.9 295.3 364.5 429.1 495.2

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance Scan 1754 (13.404 min): BP011163.D\data.ms (-1719) (-)

Ref 50

Raw 50

Sub 50

m/z--> 50 100 150 200 250 300 350 400 450 500

65.0 137.9 238.4 304.1 424.4 499.9

m/z--> 50 100 150 200 250 300 350 400 450 500


Abundance

100000

50000

0





Time--> 13.30 13.40



Dimethylphthalate
 Concen: 19.207 ng/ul
 RT: 13.787 min Scan# 1819
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	163	Resp:	851920
Ion	Ratio	Lower	Upper
163	100		
194	3.6	3.4	5.2
164	9.9	7.6	11.4



2,6-Dinitrotoluene
 Concen: 21.154 ng/ul
 RT: 13.904 min Scan# 1839
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	165	Resp:	163953
Ion	Ratio	Lower	Upper
165	100		
89	72.7	52.9	79.3
121	26.4	19.4	29.2









Acenaphthylene
Concen: 20.217 ng/ul
RT: 14.034 min Scan# 1861
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:	152	Resp:	1249966
Ion	Ratio	Lower	Upper
152	100		
151	19.9	16.5	24.7
153	13.4	10.1	15.1

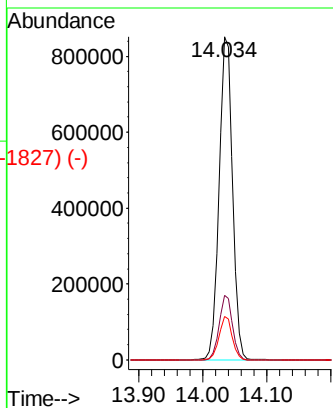

3-Nitroaniline
Concen: 20.123 ng/ul
RT: 14.234 min Scan# 1895
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38

Tgt Ion:	138	Resp:	168434
Ion	Ratio	Lower	Upper
138	100		
108	12.3	11.0	16.4
92	132.4	104.6	156.8



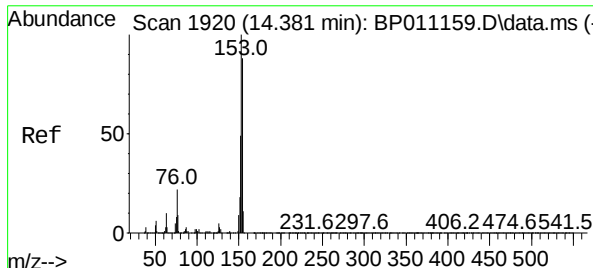

Acenaphthene

Concen: 19.937 ng/ul

RT: 14.381 min Scan# 1920

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:153 Resp: 805154

Ion Ratio Lower Upper

153 100

152 48.6 36.2 54.2

154 88.6 70.8 106.2

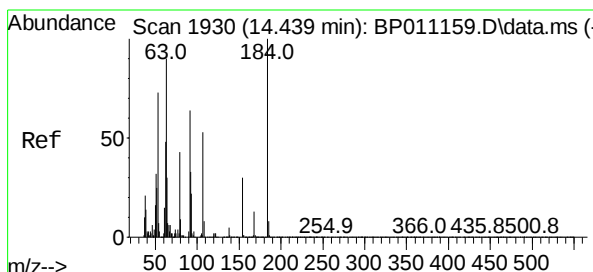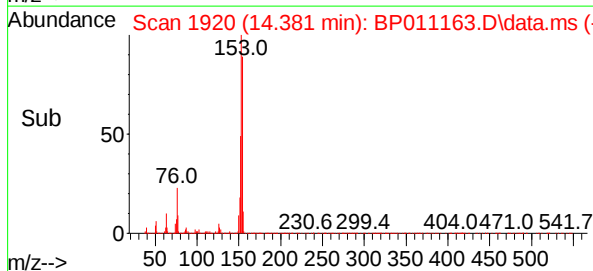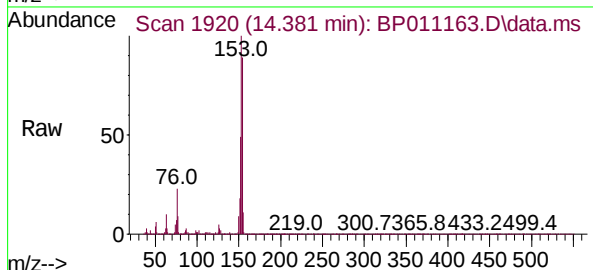

2,4-Dinitrophenol

Concen: 13.985 ng/ul

RT: 14.445 min Scan# 1931

Delta R.T. 0.006 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38




Tgt Ion:184 Resp: 61127


Ion Ratio Lower Upper

184 100

63 88.6 73.8 110.6

154 68.9 57.2 85.8


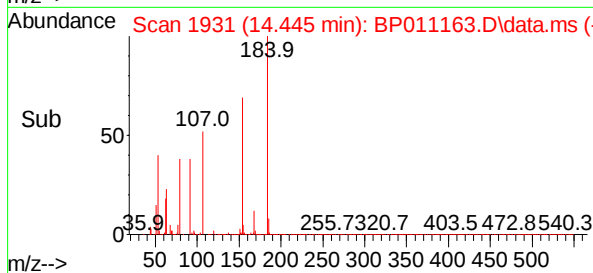

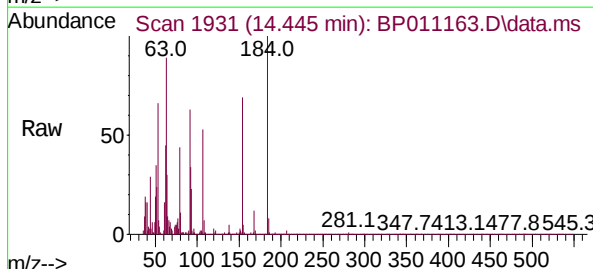


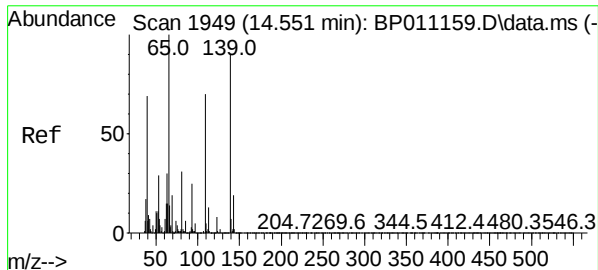

4-Nitrophenol
Concen: 16.102 ng/ul
RT: 14.551 min Scan# 1949
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:109 Resp: 109610
Ion Ratio Lower Upper
109 100
139 125.5 75.6 113.4#
65 144.1 107.6 161.4

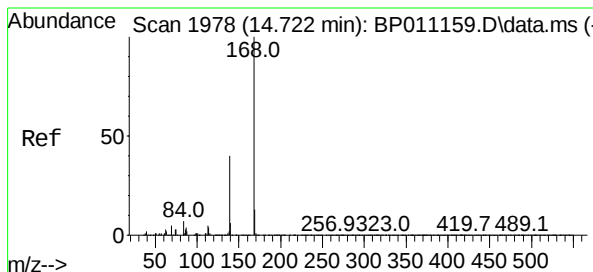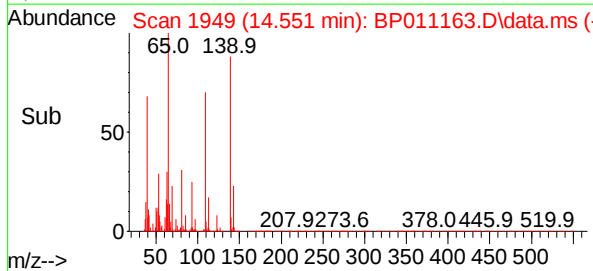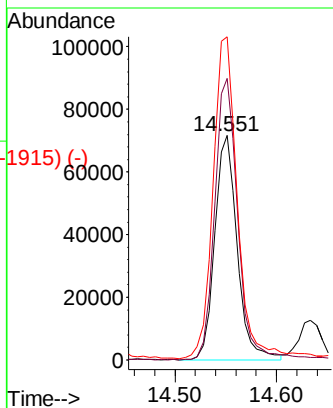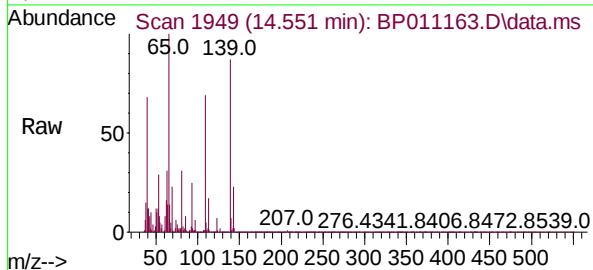

Dibenzofuran
Concen: 19.522 ng/ul
RT: 14.722 min Scan# 1978
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38

Tgt Ion:168 Resp: 1071657
Ion Ratio Lower Upper
168 100
139 41.5 32.8 49.2


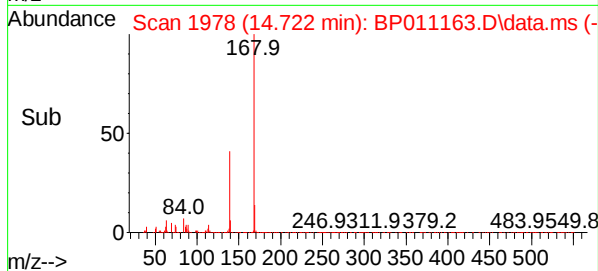

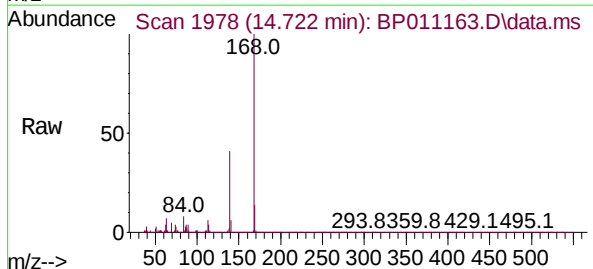




2,4-Dinitrotoluene
Concen: 18.514 ng/ul
RT: 14.698 min Scan# 1974
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:	165	Resp:	200197
Ion Ratio	Lower	Upper	
165	100		
63	56.3	47.0	70.6
182	2.3	2.2	3.2



2,3,4,6-Tetrachlorophenol
Concen: 19.404 ng/ul
RT: 14.951 min Scan# 2017
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38

Tgt Ion:	232	Resp:	168678
Ion Ratio	Lower	Upper	
232	100		
131	59.6	35.8	53.8#
130	3.0	1.8	2.8#
166	37.0	23.7	35.5#



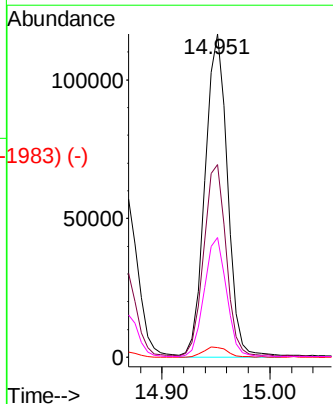





Diethylphthalate
 Concen: 18.500 ng/ul
 RT: 15.163 min Scan# 2053
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	149	Resp:	820125
Ion	Ratio	Lower	Upper
149	100		
177	20.1	17.6	26.4
150	12.1	10.3	15.5

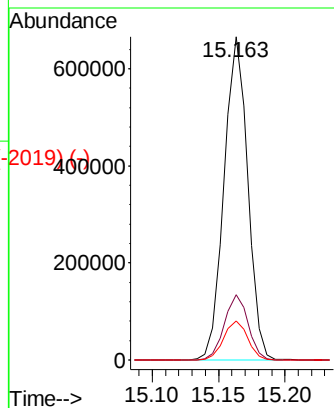

Fluorene
 Concen: 19.135 ng/ul
 RT: 15.375 min Scan# 2089
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	166	Resp:	816795
Ion	Ratio	Lower	Upper
166	100		
165	96.7	77.4	116.2
167	13.5	10.8	16.2







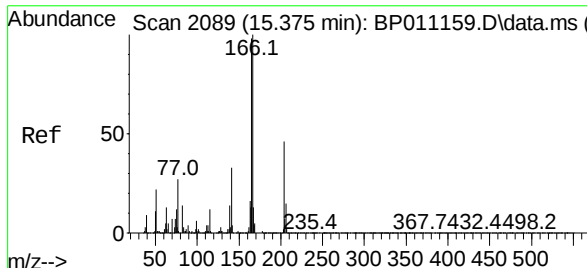

4-Chlorophenyl-phenylether
 Concen: 19.054 ng/ul
 RT: 15.375 min Scan# 2089
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	204	Resp:	370179
Ion	Ratio	Lower	Upper
204	100		
206	33.3	26.0	39.0
141	73.9	49.3	73.9

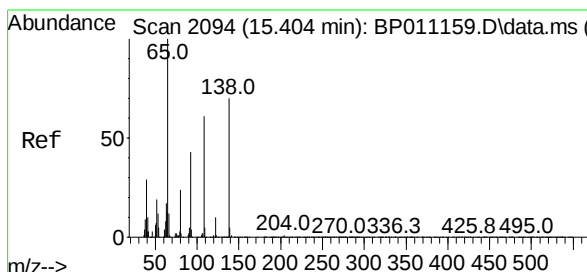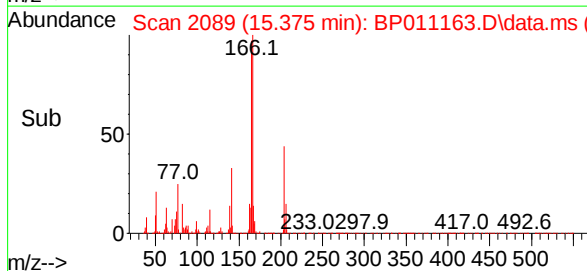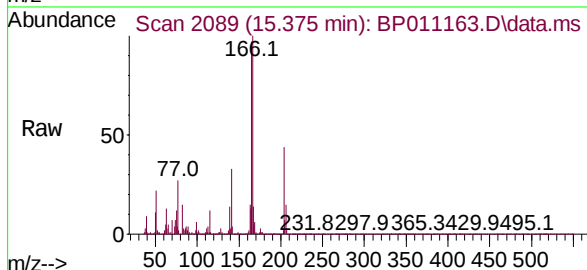

4-Nitroaniline
 Concen: 17.424 ng/ul
 RT: 15.410 min Scan# 2095
 Delta R.T. 0.006 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	138	Resp:	123989
Ion	Ratio	Lower	Upper
138	100		
92	59.2	46.2	69.2
108	84.7	85.8	128.8#


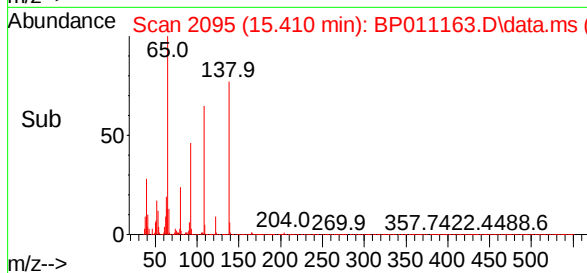

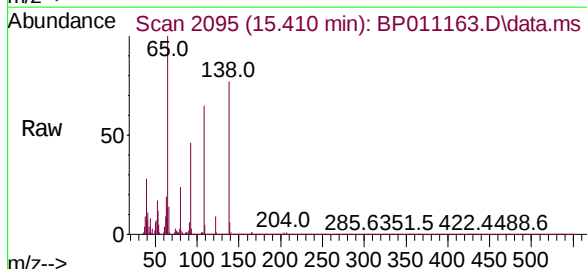


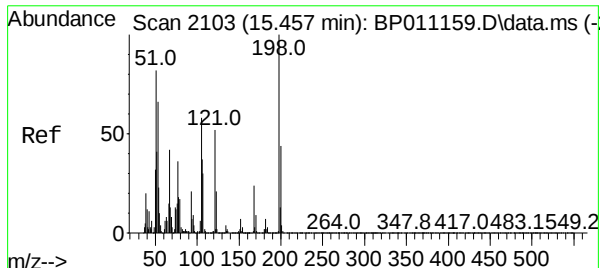

4,6-Dinitro-2-methylphenol
 Concen: 18.189 ng/ul
 RT: 15.463 min Scan# 2103
 Delta R.T. 0.006 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:198 Resp: 96141
 Ion Ratio Lower Upper
 198 100
 182 6.7 4.3 6.5#
 77 32.2 23.7 35.5

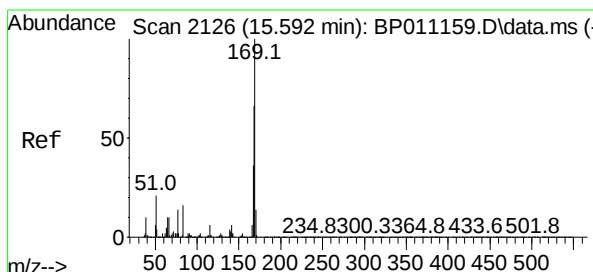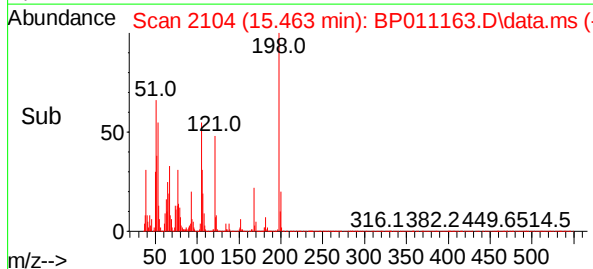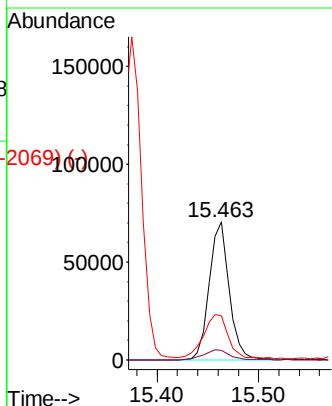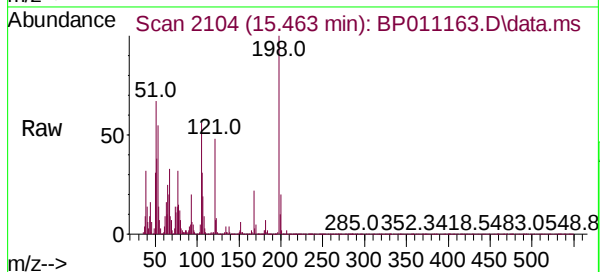

N-Nitrosodiphenylamine
 Concen: 20.609 ng/ul
 RT: 15.592 min Scan# 2126
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:169 Resp: 653892
 Ion Ratio Lower Upper
 169 100
 168 68.2 52.6 78.8
 167 36.2 27.8 41.6


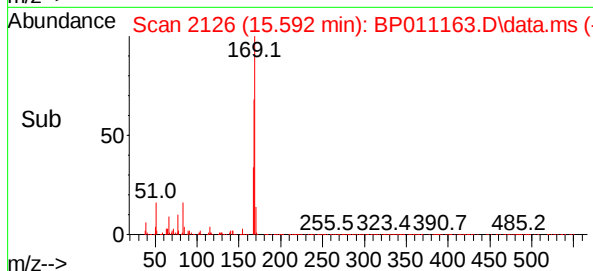
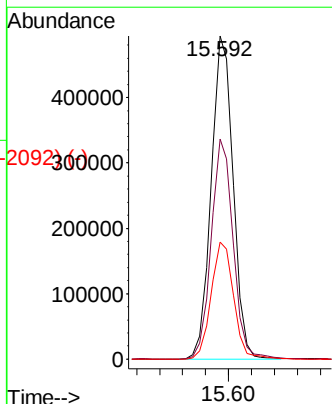
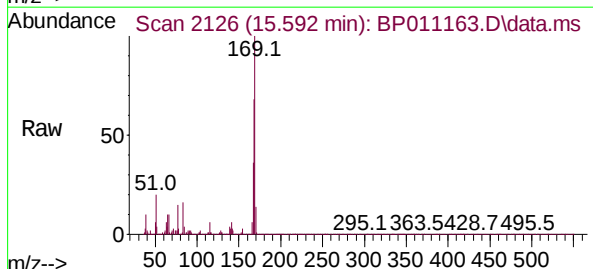


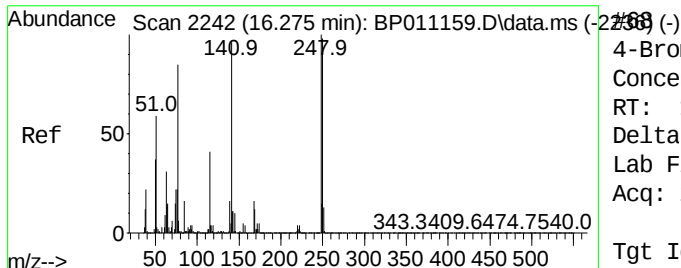

4-Bromophenyl-phenylether
Concen: 20.273 ng/ul
RT: 16.281 min Scan# 2242
Delta R.T. 0.006 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38




Instrument :
BNA_P
ClientSampleId :
SICV630

Tgt Ion:	248	Resp:	200852
Ion	Ratio	Lower	Upper
248	100		
250	98.1	80.8	121.2
141	92.2	63.9	95.9

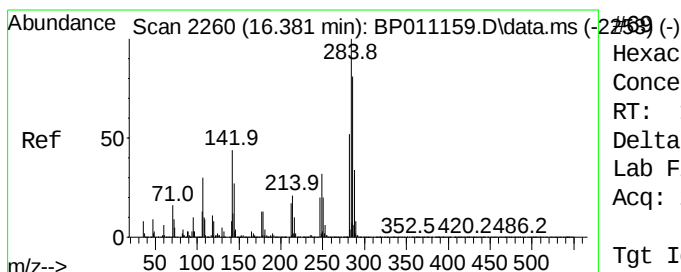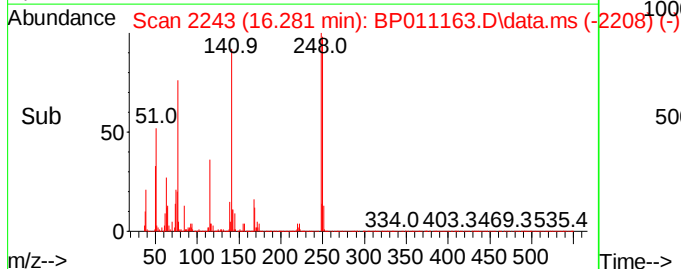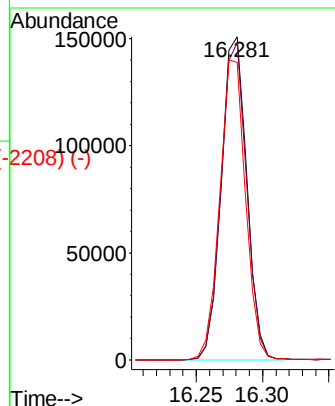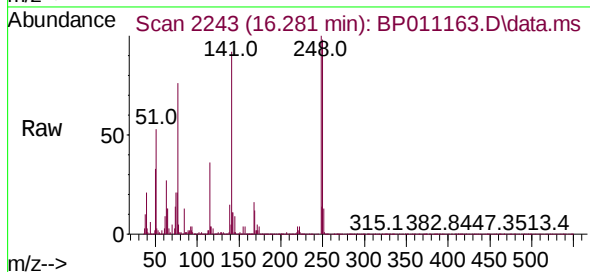

Hexachlorobenzene
Concen: 19.535 ng/ul
RT: 16.381 min Scan# 2260
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38

Tgt Ion:	284	Resp:	221399
Ion	Ratio	Lower	Upper
284	100		
142	45.8	27.8	41.6#
249	32.8	25.4	38.2

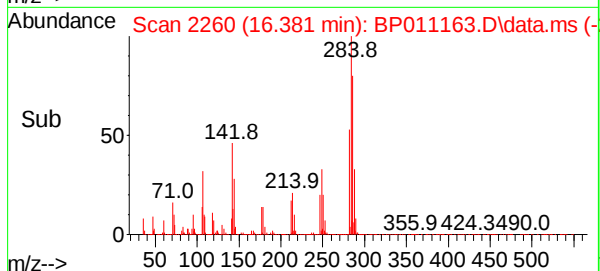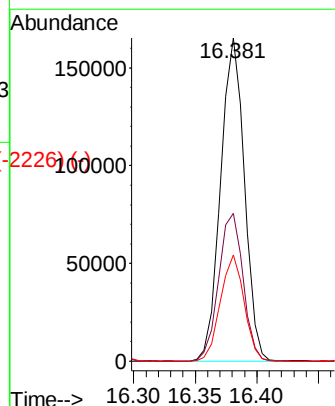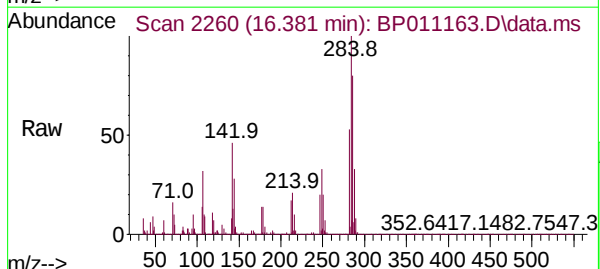

Abundance Scan 2291 (16.563 min): BP011159.D\data.ms (-2257) (-)

Atrazine

Concen: 17.844 ng/ul

RT: 16.563 min Scan# 2291

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630

Tgt Ion:200 Resp: 178038

Ion Ratio Lower Upper

200 100

173 29.9 20.7 31.1

215 45.3 38.6 57.8

Abundance Scan 2291 (16.563 min): BP011163.D\data.ms

Ref

58.0 131.9 200.1 325.7391.7457.7525.4

m/z-->

Raw

58.1 132.0 200.1 295.4363.0430.8496.7

m/z-->

Abundance Scan 2291 (16.563 min): BP011163.D\data.ms (-2257) (-)

Sub

58.1 131.9 200.1 265.7330.4401.8466.8531.5

m/z-->

Abundance

16.563

100000

50000

0

Time-->

16.50 16.60

Abundance Scan 2320 (16.733 min): BP011159.D\data.ms (-2273) (-)

Pentachlorophenol

Concen: 17.968 ng/ul

RT: 16.733 min Scan# 2320

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Tgt Ion:266 Resp: 116918

Ion Ratio Lower Upper

266 100

264 59.2 51.4 77.2

268 65.5 53.5 80.3

Abundance Scan 2320 (16.733 min): BP011163.D\data.ms

Ref

94.9 164.9 265.9 330.8397.6463.1530.4

m/z-->

Raw

94.9 164.9 265.9 331.4396.8462.4527.7

m/z-->

Abundance Scan 2320 (16.733 min): BP011163.D\data.ms (-2286) (-)

Sub

94.8 164.8 265.9 342.5409.4477.9543.9

m/z-->

Abundance

16.733

80000

60000


40000

20000

0

Time-->





16.70 16.80



Scan 2387 (17.128 min): BP011159.D\data.ms (-2353) (-)
 Phenanthrene
 Concen: 19.620 ng/ul
 RT: 17.128 min Scan# 2387
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 Client Sample Id :
 SICV630


Tgt Ion:	178	Resp:	1108580
Ion	Ratio	Lower	Upper
178	100		
179	14.9	12.7	19.1
176	19.1	14.6	22.0



Scan 2403 (17.222 min): BP011159.D\data.ms (-2356) (-)
 Anthracene
 Concen: 20.009 ng/ul
 RT: 17.222 min Scan# 2403
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	178	Resp:	1118531
Ion	Ratio	Lower	Upper
178	100		
179	14.9	12.2	18.2
176	18.8	14.5	21.7









Scan 1703 (13.104 min): BP011159.D\data.ms (-1695) (-)
 1,2,3,4-Tetrachlorobenzene
 Concen: 21.446 ng/uL
 RT: 13.104 min Scan# 1695
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630

Tgt Ion:	216	Resp:	381708
Ion	Ratio	Lower	Upper
216	100		
214	78.5	65.0	97.4
218	47.1	39.1	58.7

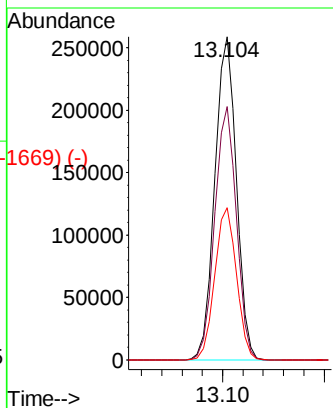


Scan 1963 (14.634 min): BP011159.D\data.ms (-1956) (-)
 Pentachlorobenzene
 Concen: 21.505 ng/uL
 RT: 14.634 min Scan# 1963
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	250	Resp:	315476
Ion	Ratio	Lower	Upper
250	100		
248	65.6	49.8	74.6
252	64.0	51.2	76.8






Abundance Scan 2450 (17.498 min): BP011159.D\data.ms (-2447) (-)

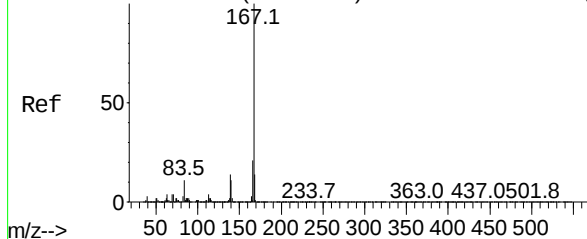


Carbazole
Concen: 19.327 ng/ul
RT: 17.504 min Scan# 2451
Delta R.T. 0.006 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38

Instrument :
BNA_P
ClientSampleId :
SICV630

Tgt Ion:	167	Resp:	957150
Ion	Ratio	Lower	Upper
167	100		
166	22.1	16.9	25.3
139	14.5	10.6	16.0

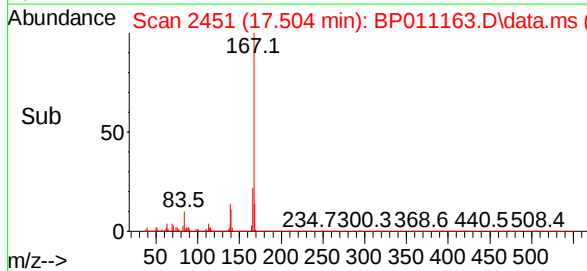
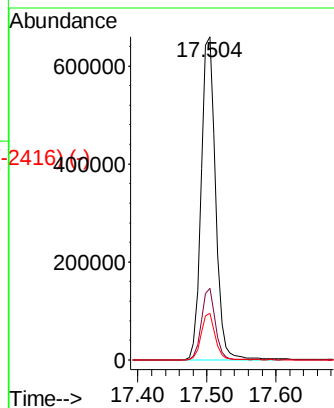
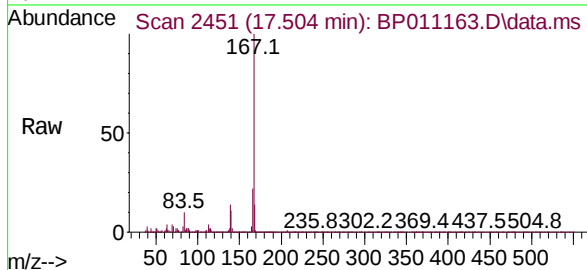


Abundance Scan 2547 (18.069 min): BP011159.D\data.ms (-2547) (-)

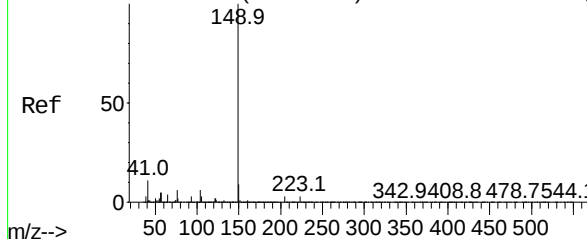


Di-n-butylphthalate
Concen: 19.459 ng/ul
RT: 18.075 min Scan# 2548
Delta R.T. 0.006 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38

Tgt Ion:	149	Resp:	1152466
Ion	Ratio	Lower	Upper
149	100		
150	9.1	7.1	10.7
104	5.6	4.6	6.8

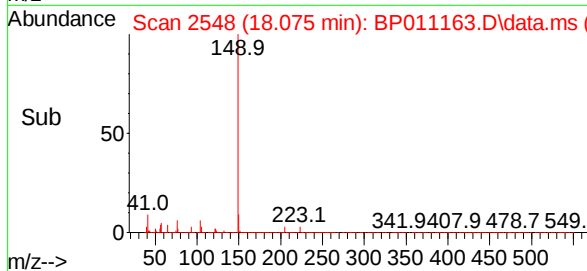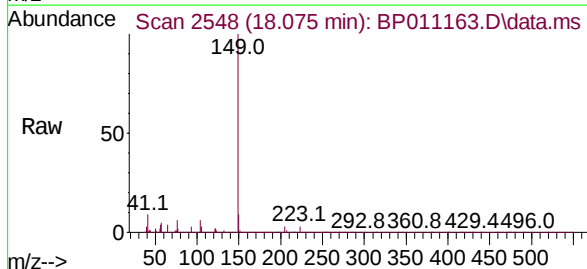

Abundance Scan 2725 (19.116 min): BP011159.D\data.ms (-2718) (-)

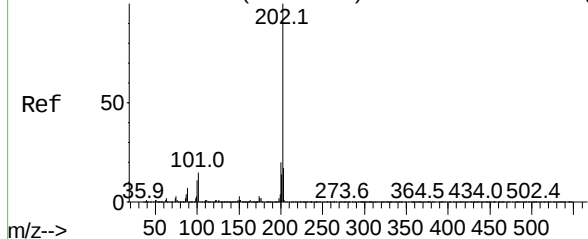

Fluoranthene

Concen: 18.237 ng/ul

RT: 19.116 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38

Instrument :

BNA_P

ClientSampleId :

SICV630



Tgt Ion:202 Resp: 1127613

Ion Ratio Lower Upper


202 100

101 15.2 7.1 10.7#


100 12.0 5.7 8.5#



Abundance Scan 2725 (19.116 min): BP011163.D\data.ms (-2691) (-)

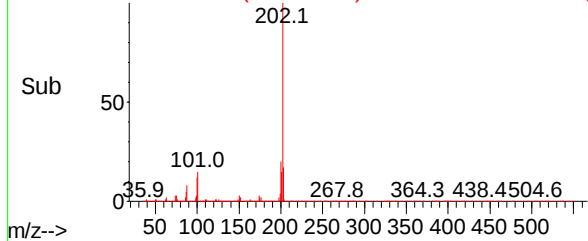

Abundance Scan 2786 (19.474 min): BP011159.D\data.ms (-2782) (-)

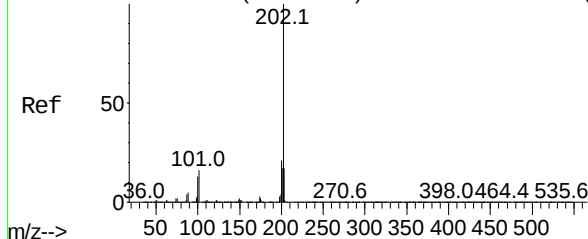

Pyrene

Concen: 18.669 ng/ul

RT: 19.475 min Scan# 2786

Delta R.T. 0.000 min

Lab File: BP011163.D

Acq: 28 Jul 2022 15:38



Tgt Ion:202 Resp: 1186209

Ion Ratio Lower Upper


202 100


101 16.8 7.9 11.9#

100 14.0 6.7 10.1#



Abundance Scan 2786 (19.475 min): BP011163.D\data.ms (-2752) (-)




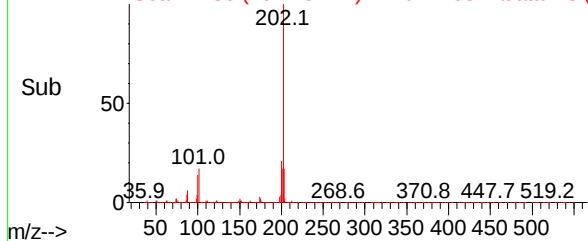




Butylbenzylphthalate
 Concen: 18.677 ng/ul
 RT: 20.374 min Scan# 2938
 Delta R.T. 0.006 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	149	Resp:	475199
Ion	Ratio	Lower	Upper
149	100		
91	76.8	60.0	90.0
206	18.2	17.4	26.2

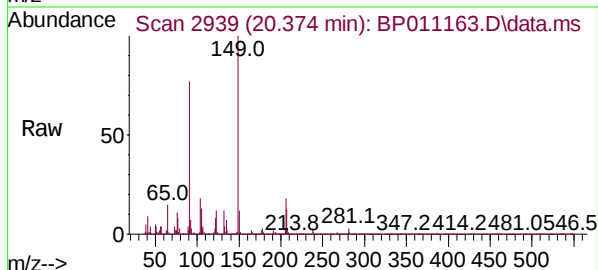

3,3'-Dichlorobenzidine
 Concen: 20.103 ng/ul
 RT: 21.139 min Scan# 3069
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	252	Resp:	326640
Ion	Ratio	Lower	Upper
252	100		
254	64.5	51.0	76.4
126	14.1	8.6	12.8#



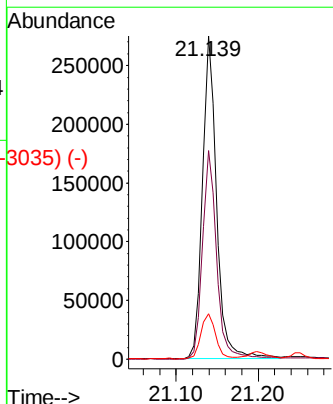
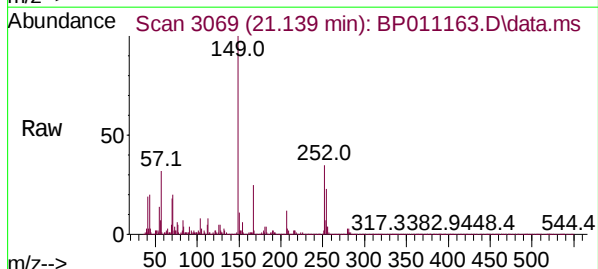




Scan 3079 (21.198 min): BP011159.D\data.ms (-30785) (-)
 Benzo(a)anthracene
 Concen: 19.886 ng/ul
 RT: 21.198 min Scan# 30785
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument : BNA_P
 ClientSampleId : SICV630


Tgt Ion:	228	Resp:	1151539
Ion	Ratio	Lower	Upper
228	100		
229	19.8	15.0	22.4
226	27.1	20.6	31.0

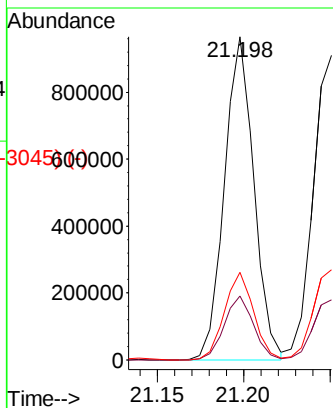

Scan 3069 (21.139 min): BP011159.D\data.ms (-30686) (-)
 Bis(2-ethylhexyl)phthalate
 Concen: 20.087 ng/ul
 RT: 21.139 min Scan# 3069
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	149	Resp:	772388
Ion	Ratio	Lower	Upper
149	100		
167	25.2	22.6	33.8
279	3.3	4.2	6.4#









Scan 3087 (21.245 min): BP011159.D\data.ms (-3087) (-)
 Chrysene
 Concen: 19.167 ng/ul
 RT: 21.251 min Scan# 3088
 Delta R.T. 0.006 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	228	Resp:	1103414
Ion	Ratio	Lower	Upper
228	100		
226	29.7	23.6	35.4
229	19.7	15.6	23.4

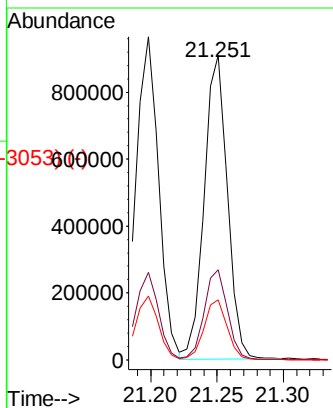

Scan 3223 (22.045 min): BP011159.D\data.ms (-3223) (-)
 Di-n-octyl phthalate
 Concen: 18.520 ng/ul
 RT: 22.051 min Scan# 3224
 Delta R.T. 0.006 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:149 Resp: 1310412



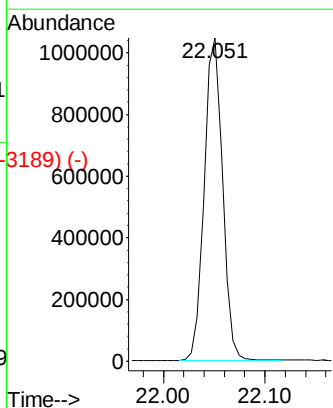





Benzo(b)fluoranthene
Concen: 19.971 ng/u1
RT: 22.845 min Scan# 3359
Delta R.T. 0.006 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:	252	Resp:	1296117
Ion	Ratio	Lower	Upper
252	100		
253	21.3	17.8	26.6
125	13.2	6.2	9.2#



Benzo(k)fluoranthene
Concen: 19.686 ng/u1
RT: 22.892 min Scan# 3367
Delta R.T. 0.000 min
Lab File: BP011163.D
Acq: 28 Jul 2022 15:38

Tgt Ion:	252	Resp:	1212587
Ion	Ratio	Lower	Upper
252	100		
253	21.7	17.0	25.4
125	13.1	6.2	9.4#









Benzo(a)pyrene
 Concen: 19.177 ng/ul
 RT: 23.451 min Scan# 3462
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:	252	Resp:	1214027
Ion	Ratio	Lower	Upper
252	100		
253	21.8	17.4	26.0
125	15.6	6.6	10.0#

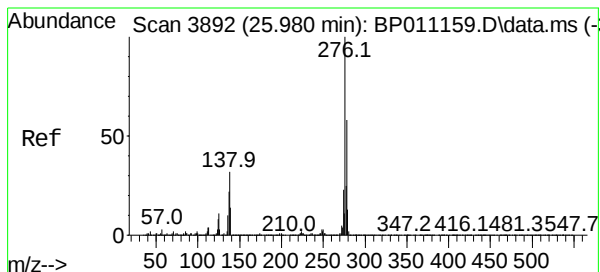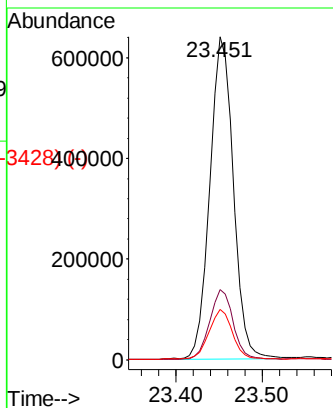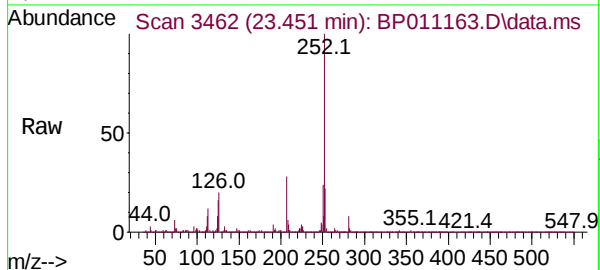

Indeno(1,2,3-cd)pyrene
 Concen: 19.315 ng/ul
 RT: 25.980 min Scan# 3892
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	276	Resp:	1506400
Ion	Ratio	Lower	Upper
276	100		
138	31.5	14.6	22.0#
277	24.4	19.6	29.4



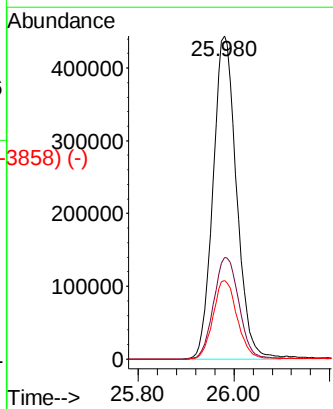
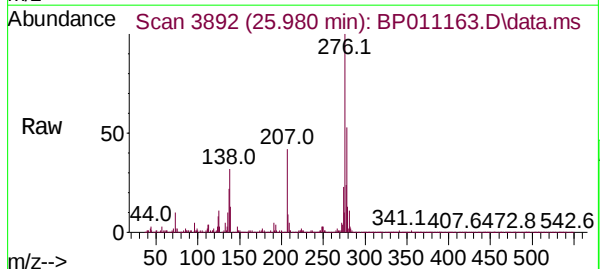


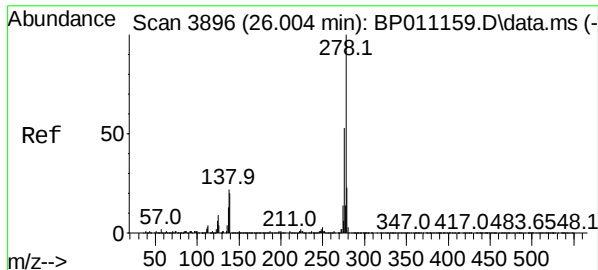

Scan 3896 (26.004 min): BP011159.D\data.ms (-3896) (-)
 Dibenzo(a,h)anthracene
 Concen: 19.616 ng/ul
 RT: 25.998 min Scan# 4095
 Delta R.T. -0.006 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Instrument :
 BNA_P
 ClientSampleId :
 SICV630

Tgt Ion:	278	Resp:	1312165
Ion	Ratio	Lower	Upper
278	100		
139	22.0	9.4	14.2#
279	23.5	18.9	28.3

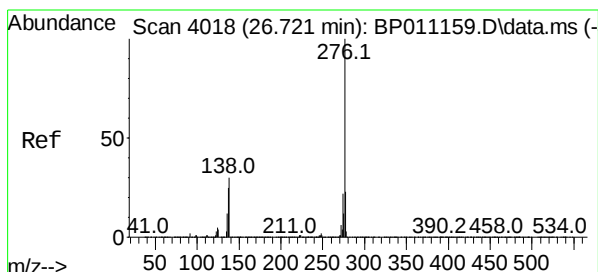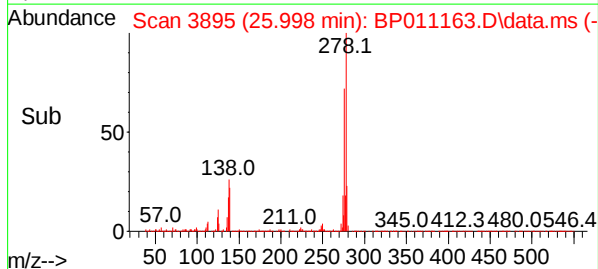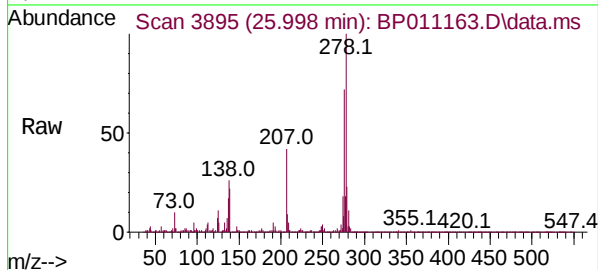

Scan 4018 (26.721 min): BP011159.D\data.ms (-4018) (-)
 Benzo(g,h,i)perylene
 Concen: 19.544 ng/ul
 RT: 26.721 min Scan# 4018
 Delta R.T. 0.000 min
 Lab File: BP011163.D
 Acq: 28 Jul 2022 15:38

Tgt Ion:	276	Resp:	1318289
Ion	Ratio	Lower	Upper
276	100		
138	28.5	12.7	19.1#
277	23.5	18.2	27.4

