

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072921\
 Data File : BP006425.D
 Acq On : 29 Jul 2021 17:42
 Operator : CG/JU
 Sample : M3141-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEP0

Quant Time: Jul 29 18:14:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 29 16:44:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	345939	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	1511030	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	888733	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	1721997	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1498961	20.000	ng/ul	0.00
88) Perylene-d12	23.598	264	1305889	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	20093	2.168	ng/uL	0.00
4) Pyridine-d5	3.705	84	205771	7.479	ng/ul	0.00
7) Phenol-d5	6.952	99	350313	10.782	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	232775	11.515	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	271467	11.246	ng/ul	0.00
15) 4-Methylphenol-d8	8.487	113	278388	10.896	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	135532	12.046	ng/ul	0.00
24) 2-Nitrophenol-d4	9.652	143	133262	12.405	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	229863	10.919	ng/ul	0.00
31) 4-Chloroaniline-d4	10.705	131	354341	10.224	ng/ul	0.00
46) Dimethylphthalate-d6	13.828	166	770196	12.176	ng/ul	0.00
49) Acenaphthylene-d8	14.099	160	922587	11.872	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	100466	7.999	ng/ul	0.00
60) Fluorene-d10	15.398	176	633444	11.913	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	70343	7.328	ng/ul	0.00
73) Anthracene-d10	17.257	188	966849	12.438	ng/ul	0.00
81) Pyrene-d10	19.498	212	1046650	13.575	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.445	264	737934	11.120	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	36065	1.086	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072921\
Data File : BP006425.D
Acq On : 29 Jul 2021 17:42
Operator : CG/JU
Sample : M3141-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEP0

Quant Time: Jul 29 18:14:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 29 16:44:32 2021
Response via : Initial Calibration

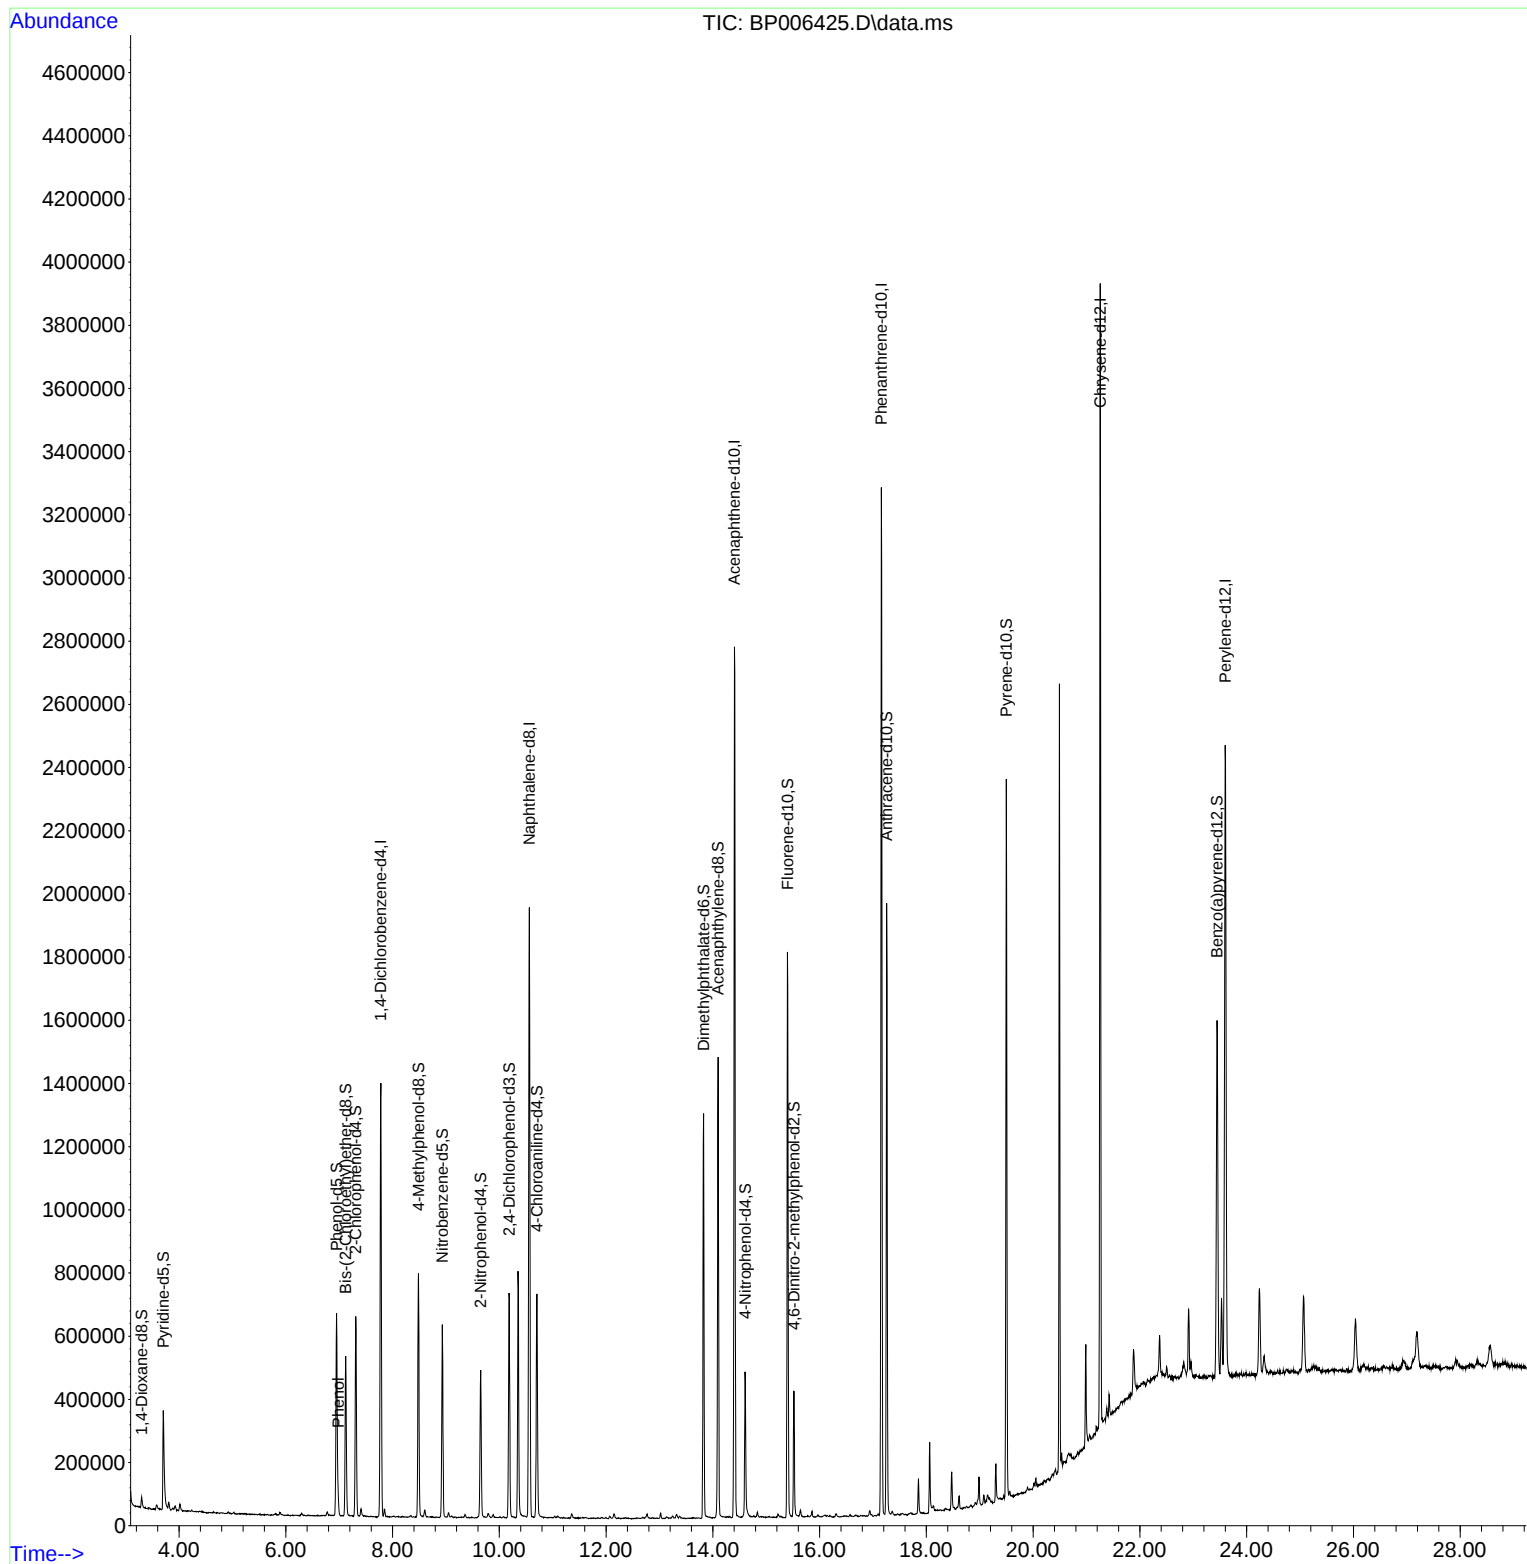

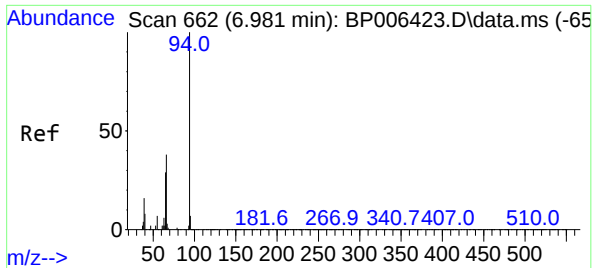

#8
Phenol
Concen: 1.086 ng/ul
RT: 6.981 min Scan# 662
Delta R.T. 0.000 min
Lab File: BP006425.D
Acq: 29 Jul 2021 17:42

Instrument :
BNA_P
ClientSampleId :
BGEPO

Tgt Ion: 94 Resp: 36065
Ion Ratio Lower Upper
94 100
65 27.9 23.4 35.0
66 39.8 31.1 46.7

