

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072921\  
 Data File : BP006426.D  
 Acq On : 29 Jul 2021 18:16  
 Operator : CG/JU  
 Sample : M3141-16  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 BGER5

Quant Time: Jul 30 01:13:59 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SFAM-EPA-BP072421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jul 29 11:29:11 2021  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	335332	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	1470477	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	853709	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	1638134	20.000	ng/ul	0.00
79) Chrysene-d12	21.256	240	1441934	20.000	ng/ul	0.00
88) Perylene-d12	23.603	264	1275738	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	54085	6.020	ng/uL	0.00
4) Pyridine-d5	3.699	84	828201	31.055	ng/ul	0.00
7) Phenol-d5	6.951	99	1064568	33.802	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	694038	35.418	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	824802	35.251	ng/ul	0.00
15) 4-Methylphenol-d8	8.487	113	875113	35.334	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	418419	38.215	ng/ul	0.00
24) 2-Nitrophenol-d4	9.651	143	428906	41.026	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.186	165	718499	35.072	ng/ul	0.00
31) 4-Chloroaniline-d4	10.704	131	1143180	33.895	ng/ul	0.00
46) Dimethylphthalate-d6	13.827	166	2300969	37.870	ng/ul	0.00
49) Acenaphthylene-d8	14.098	160	2848451	38.158	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	379627	31.467	ng/ul	0.00
60) Fluorene-d10	15.404	176	1890243	37.006	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.521	200	252775	27.679	ng/ul	0.00
73) Anthracene-d10	17.257	188	2841916	38.431	ng/ul	0.00
81) Pyrene-d10	19.504	212	3060562	41.267	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.450	264	2456060	37.885	ng/ul	0.00
Target Compounds						
8) Phenol	6.981	94	88570	2.751	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072921\  
 Data File : BP006426.D  
 Acq On : 29 Jul 2021 18:16  
 Operator : CG/JU  
 Sample : M3141-16  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

**Instrument :**  
 BNA\_P  
**ClientSampleId :**  
 BGER5


Quant Time: Jul 30 01:13:59 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SFAM-EPA-BP072421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jul 29 11:29:11 2021  
 Response via : Initial Calibration

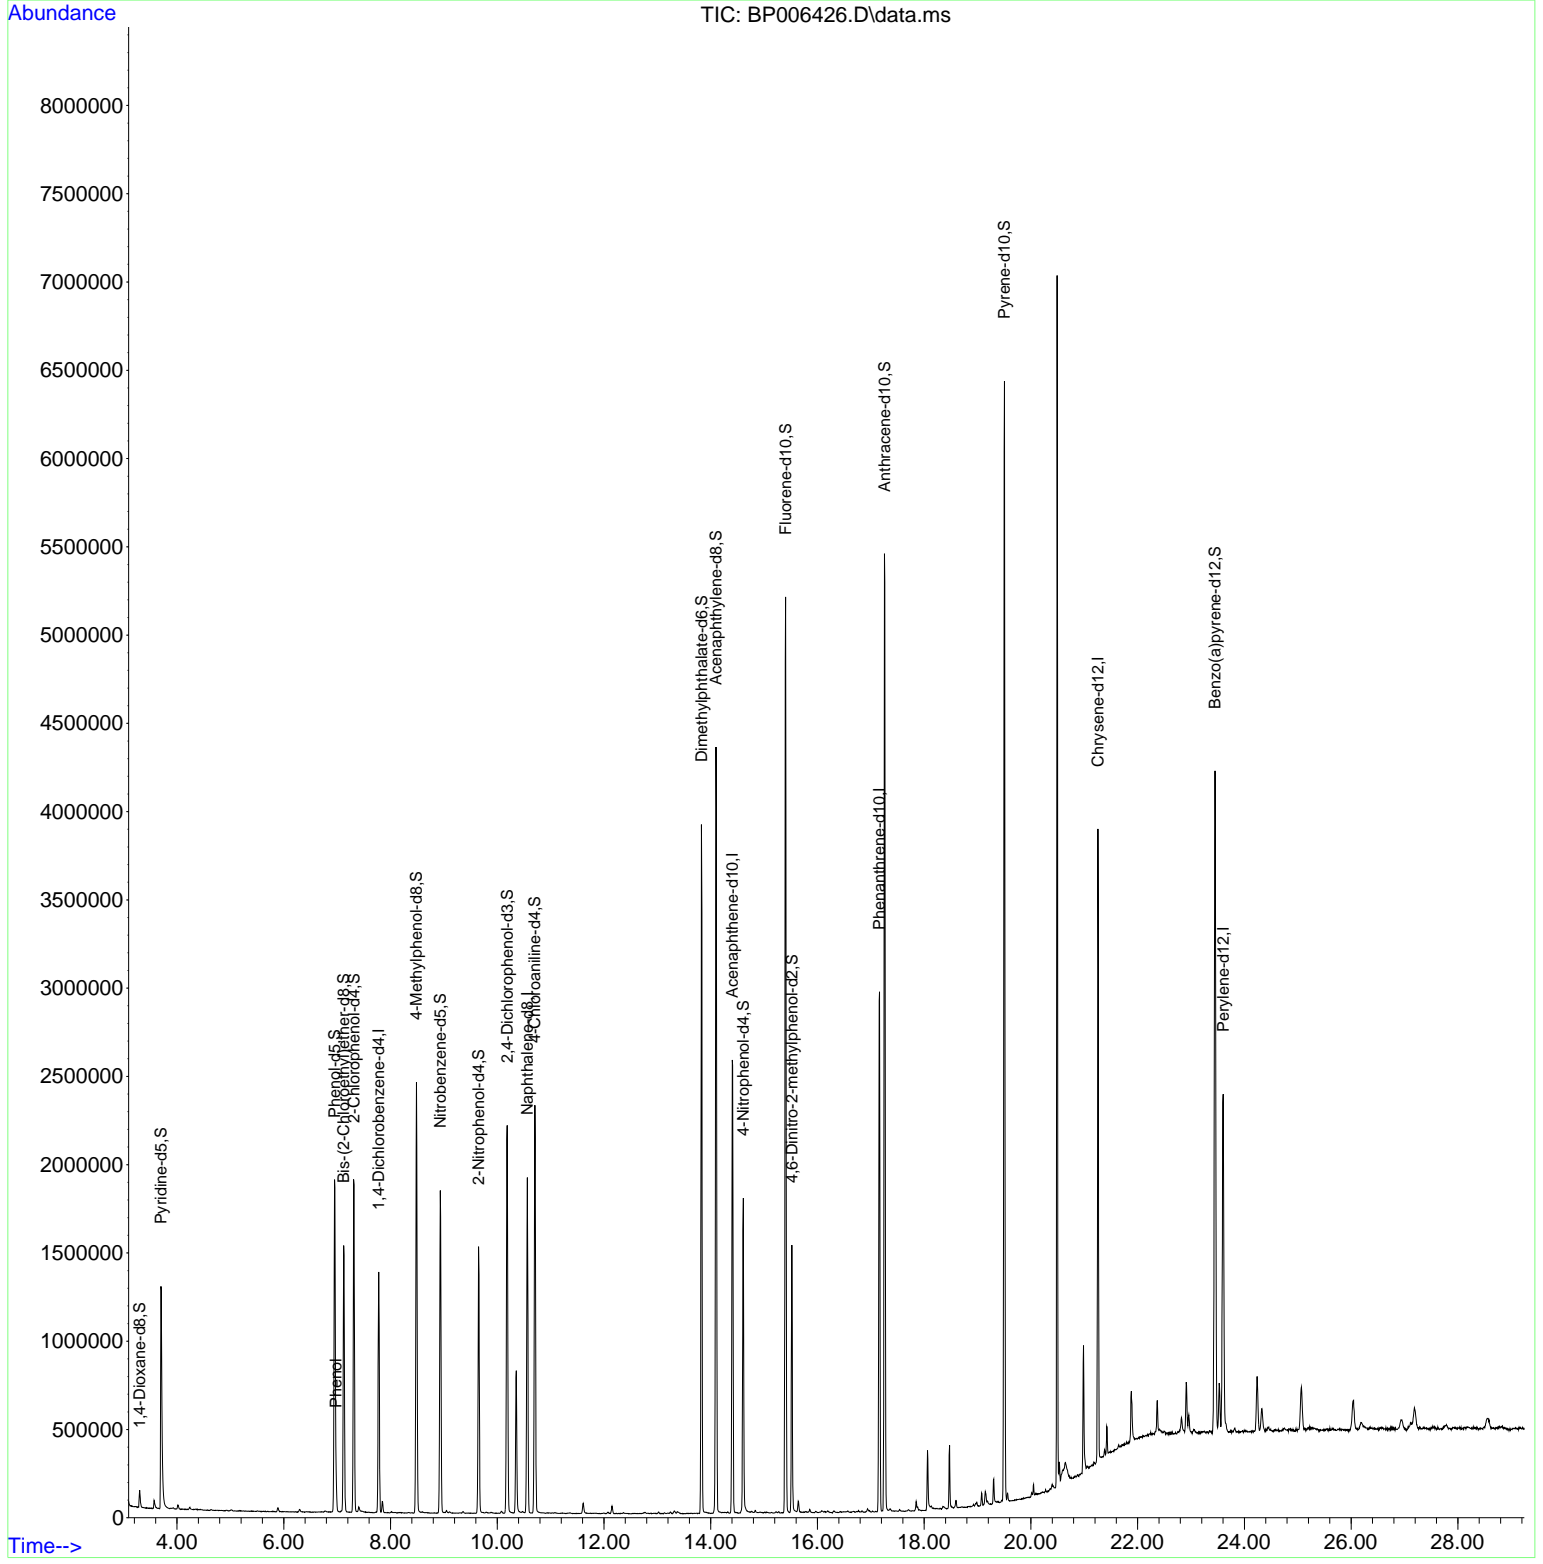

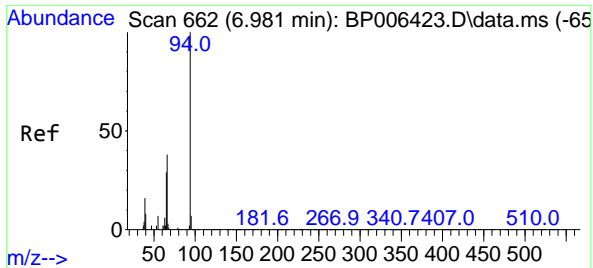

#8  
 Phenol  
 Concen: 2.751 ng/ul  
 RT: 6.981 min Scan# 662  
 Delta R.T. -0.000 min  
 Lab File: BP006426.D  
 Acq: 29 Jul 2021 18:16

**Instrument :**  
 BNA\_P  
**ClientSampled :**  
 BGER5

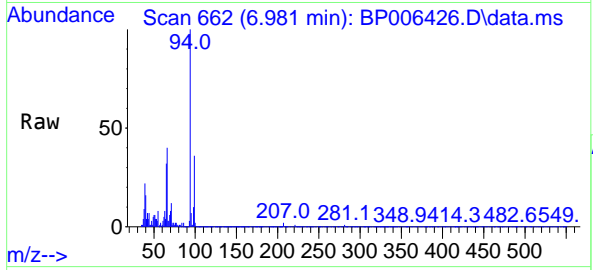

Tgt Ion: 94 Resp: 88570

Ion	Ratio	Lower	Upper
94	100		
65	31.5	23.4	35.0
66	39.6	31.1	46.7

