

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072921\
 Data File : BP006427.D
 Acq On : 29 Jul 2021 18:50
 Operator : CG/JU
 Sample : M3141-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEQ4

Quant Time: Jul 30 01:14:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 29 11:29:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	304851	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	1311244	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	750371	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	1460414	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1374844	20.000	ng/ul	0.00
88) Perylene-d12	23.598	264	1239329	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	64295	7.873	ng/uL	0.00
4) Pyridine-d5	3.699	84	952897	39.303	ng/ul	0.00
7) Phenol-d5	6.952	99	1153168	40.277	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	739689	41.521	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	898932	42.261	ng/ul	0.00
15) 4-Methylphenol-d8	8.487	113	934556	41.507	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	445142	45.593	ng/ul	0.00
24) 2-Nitrophenol-d4	9.652	143	457726	49.099	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	757379	41.459	ng/ul	0.00
31) 4-Chloroaniline-d4	10.705	131	1204811	40.060	ng/ul	0.00
46) Dimethylphthalate-d6	13.828	166	2368726	44.354	ng/ul	0.00
49) Acenaphthylene-d8	14.098	160	2971194	45.283	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	396047	37.349	ng/ul	0.00
60) Fluorene-d10	15.404	176	1972350	43.932	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	274729	33.744	ng/ul	0.00
73) Anthracene-d10	17.257	188	2977556	45.166	ng/ul	0.00
81) Pyrene-d10	19.498	212	3282443	46.418	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.451	264	2761146	43.842	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	57856	1.977	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072921\
Data File : BP006427.D
Acq On : 29 Jul 2021 18:50
Operator : CG/JU
Sample : M3141-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEQ4

Quant Time: Jul 30 01:14:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 29 11:29:11 2021
Response via : Initial Calibration

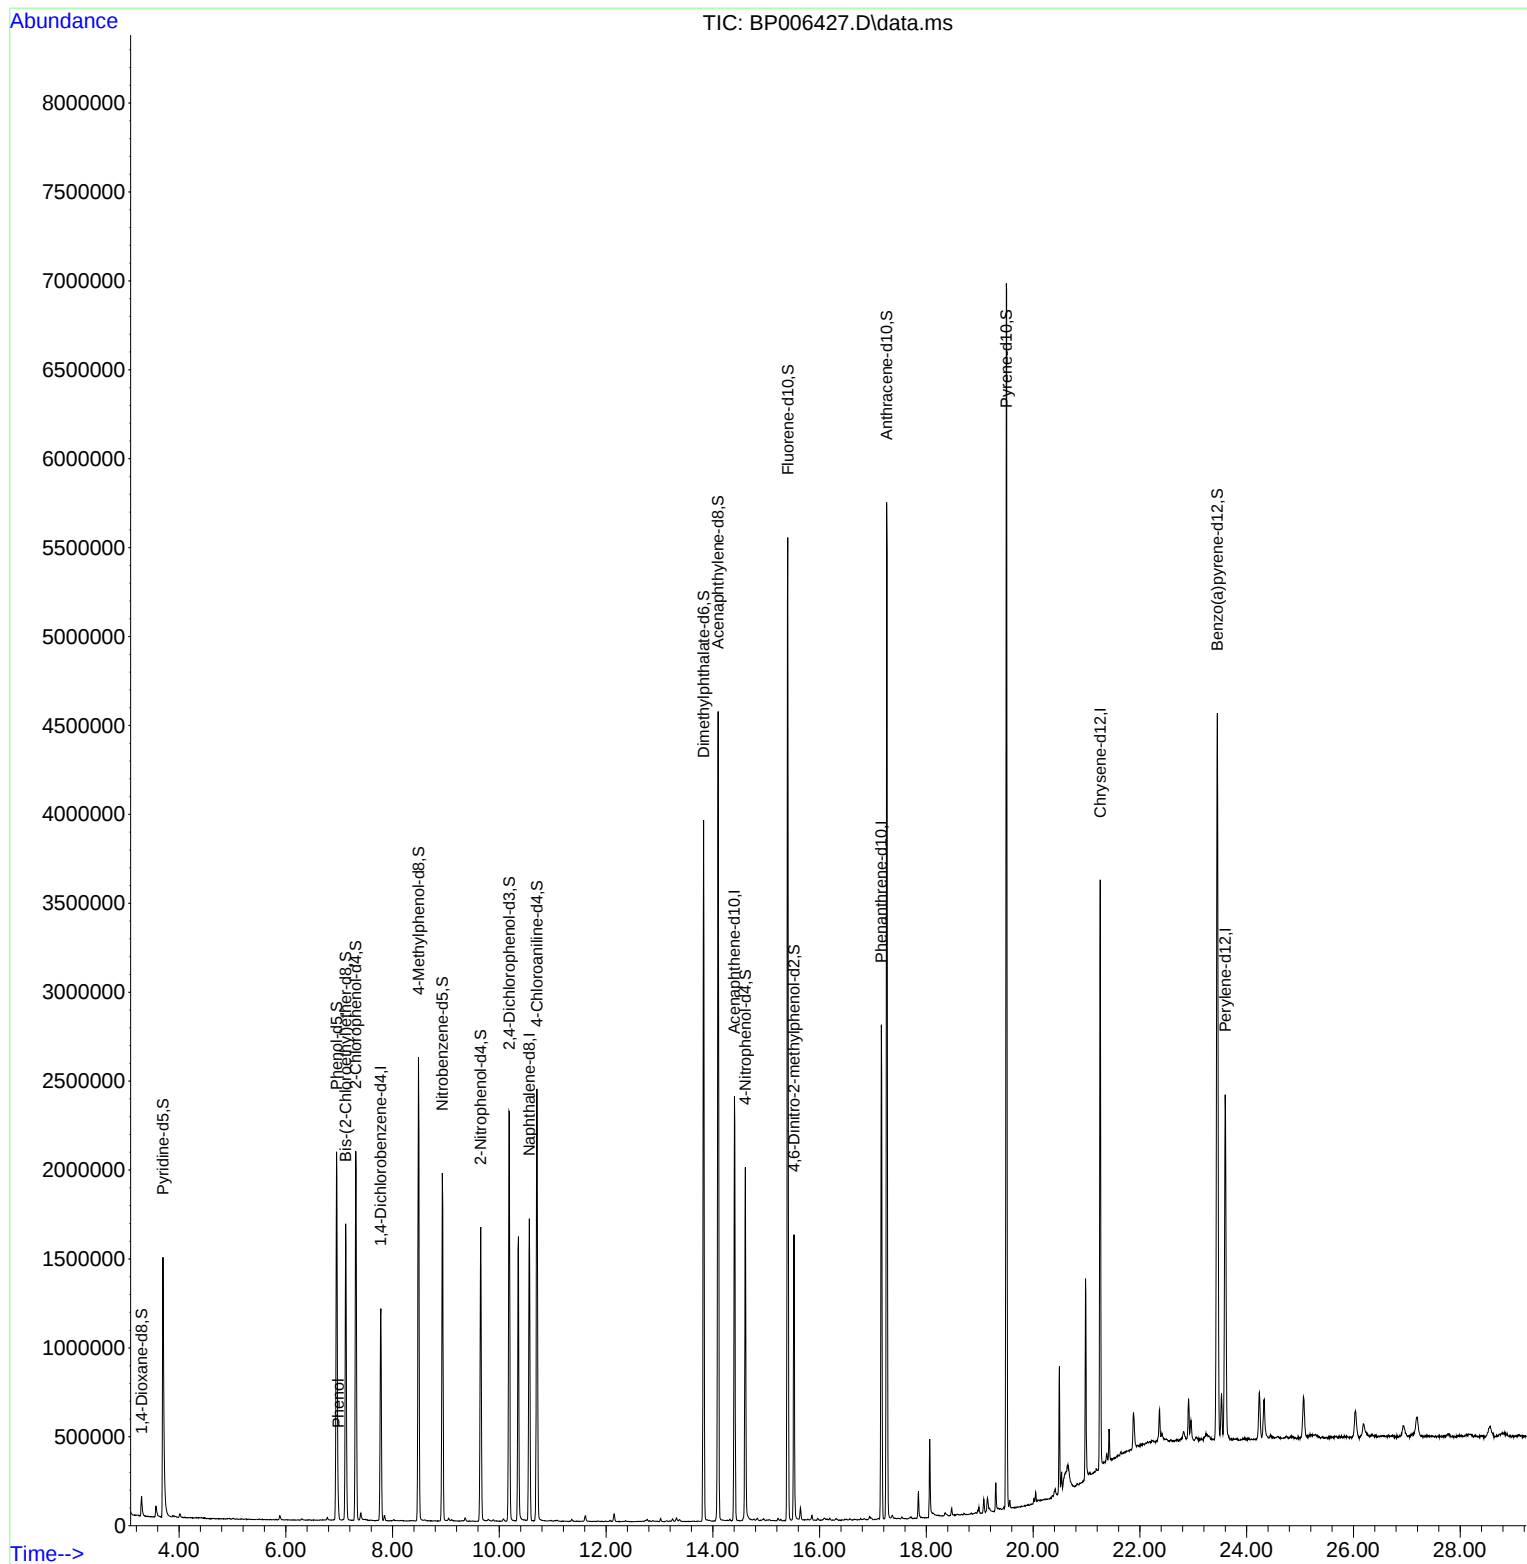

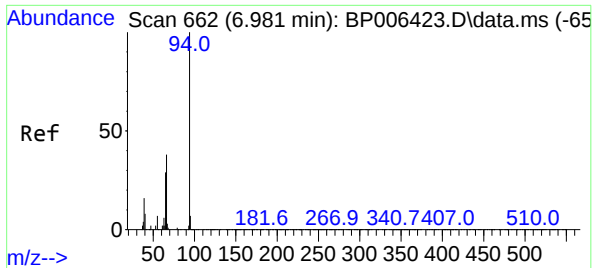

#8
Phenol
Concen: 1.977 ng/ul
RT: 6.981 min Scan# 662
Delta R.T. 0.000 min
Lab File: BP006427.D
Acq: 29 Jul 2021 18:50

Instrument :
BNA_P
ClientSampleId :
BGEQ4

Tgt Ion: 94 Resp: 57856
Ion Ratio Lower Upper
94 100
65 30.6 23.4 35.0
66 38.6 31.1 46.7

