

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072921\
 Data File : BP006428.D
 Acq On : 29 Jul 2021 19:24
 Operator : CG/JU
 Sample : M3141-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEQ1

Quant Time: Jul 30 01:14:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 29 11:29:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	321653	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	1356487	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	762638	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	1446560	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1220122	20.000	ng/ul	0.00
88) Perylene-d12	23.604	264	1037660	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	72220	8.381	ng/uL	0.00
4) Pyridine-d5	3.699	84	1060765	41.467	ng/ul	0.00
7) Phenol-d5	6.952	99	1334024	44.159	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	854086	45.438	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	1019553	45.427	ng/ul	0.00
15) 4-Methylphenol-d8	8.487	113	1065848	44.865	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	511452	50.637	ng/ul	0.00
24) 2-Nitrophenol-d4	9.651	143	531364	55.097	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	860889	45.553	ng/ul	0.00
31) 4-Chloroaniline-d4	10.704	131	1368693	43.991	ng/ul	0.00
46) Dimethylphthalate-d6	13.828	166	2629002	48.435	ng/ul	0.00
49) Acenaphthylene-d8	14.098	160	3309468	49.627	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	483989	44.908	ng/ul	0.00
60) Fluorene-d10	15.404	176	2152073	47.164	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	328277	40.708	ng/ul	0.00
73) Anthracene-d10	17.257	188	3190696	48.862	ng/ul	0.00
81) Pyrene-d10	19.504	212	3346504	53.325	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.451	264	2522312	47.834	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	57241	1.854	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072921\
Data File : BP006428.D
Acq On : 29 Jul 2021 19:24
Operator : CG/JU
Sample : M3141-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEQ1

Quant Time: Jul 30 01:14:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 29 11:29:11 2021
Response via : Initial Calibration

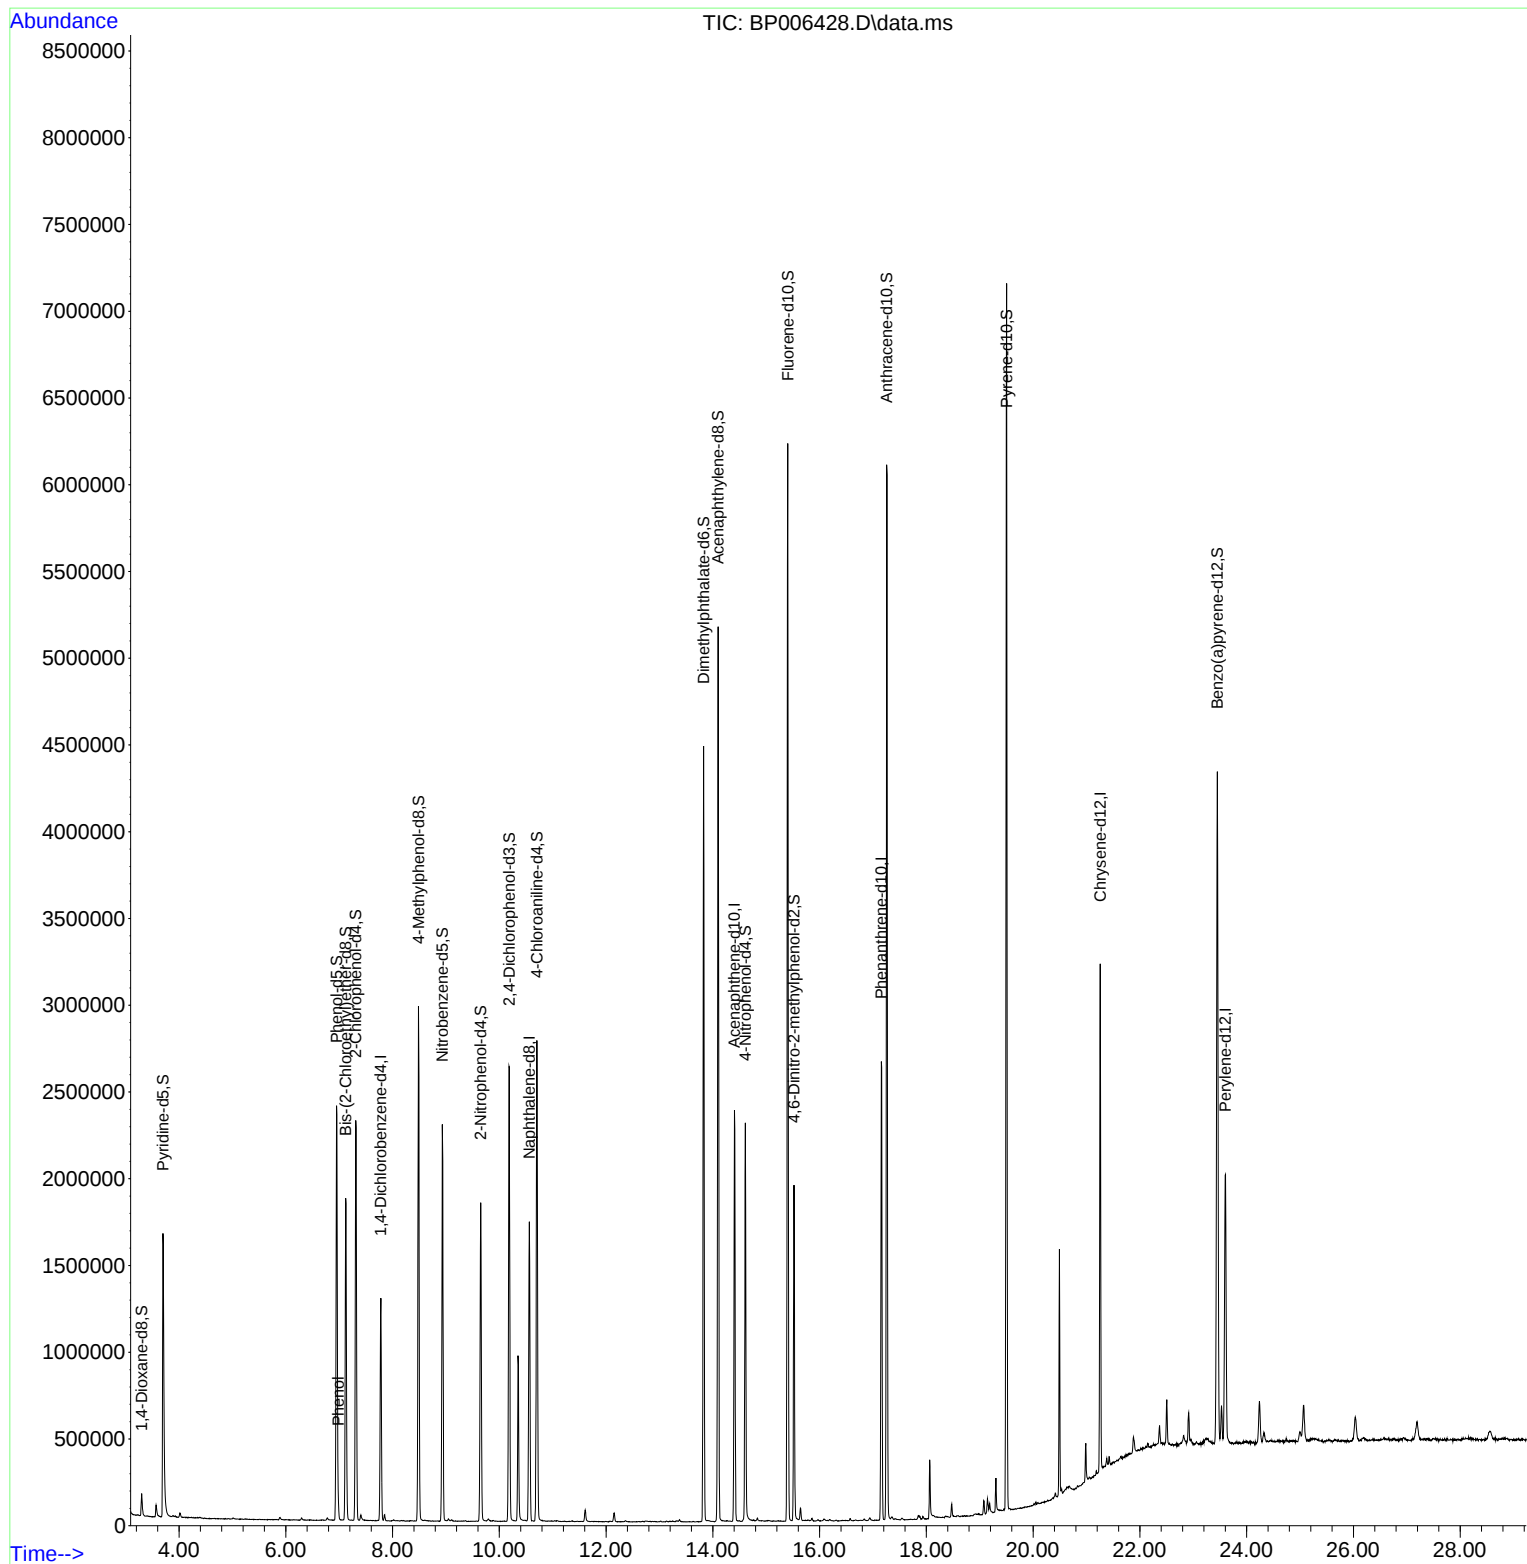

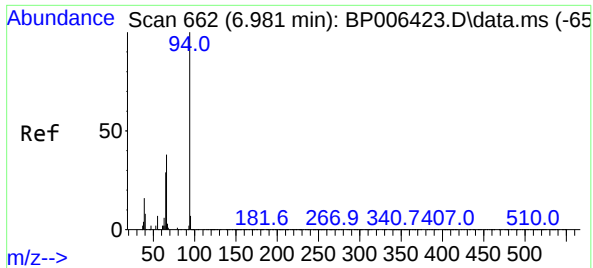

#8
Phenol
Concen: 1.854 ng/ul
RT: 6.981 min Scan# 662
Delta R.T. -0.000 min
Lab File: BP006428.D
Acq: 29 Jul 2021 19:24

Instrument :
BNA_P
ClientSampleId :
BGEQ1

Tgt Ion: 94 Resp: 57241
Ion Ratio Lower Upper
94 100
65 31.5 23.4 35.0
66 41.5 31.1 46.7

