

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072921\
 Data File : BP006432.D
 Acq On : 29 Jul 2021 21:41
 Operator : CG/JU
 Sample : M3141-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEP4

Quant Time: Jul 30 01:15:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 29 11:29:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	313352	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	1320104	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	739120	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	1382699	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1163159	20.000	ng/ul	0.00
88) Perylene-d12	23.598	264	999979	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	57065	6.798	ng/uL	0.00
4) Pyridine-d5	3.699	84	834765	33.497	ng/ul	0.00
7) Phenol-d5	6.952	99	1046705	35.566	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	685322	37.426	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	815056	37.278	ng/ul	0.00
15) 4-Methylphenol-d8	8.487	113	837524	36.188	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	408616	41.571	ng/ul	0.00
24) 2-Nitrophenol-d4	9.652	143	413296	44.036	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	677927	36.861	ng/ul	0.00
31) 4-Chloroaniline-d4	10.704	131	1055034	34.844	ng/ul	0.00
46) Dimethylphthalate-d6	13.828	166	2093179	39.791	ng/ul	0.00
49) Acenaphthylene-d8	14.098	160	2622093	40.571	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	316829	30.333	ng/ul	0.00
60) Fluorene-d10	15.404	176	1740029	39.347	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	217314	28.192	ng/ul	0.00
73) Anthracene-d10	17.257	188	2556905	40.965	ng/ul	0.00
81) Pyrene-d10	19.498	212	2689481	44.954	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.451	264	1999927	39.356	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	61370	2.040	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072921\
Data File : BP006432.D
Acq On : 29 Jul 2021 21:41
Operator : CG/JU
Sample : M3141-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEP4

Quant Time: Jul 30 01:15:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 29 11:29:11 2021
Response via : Initial Calibration

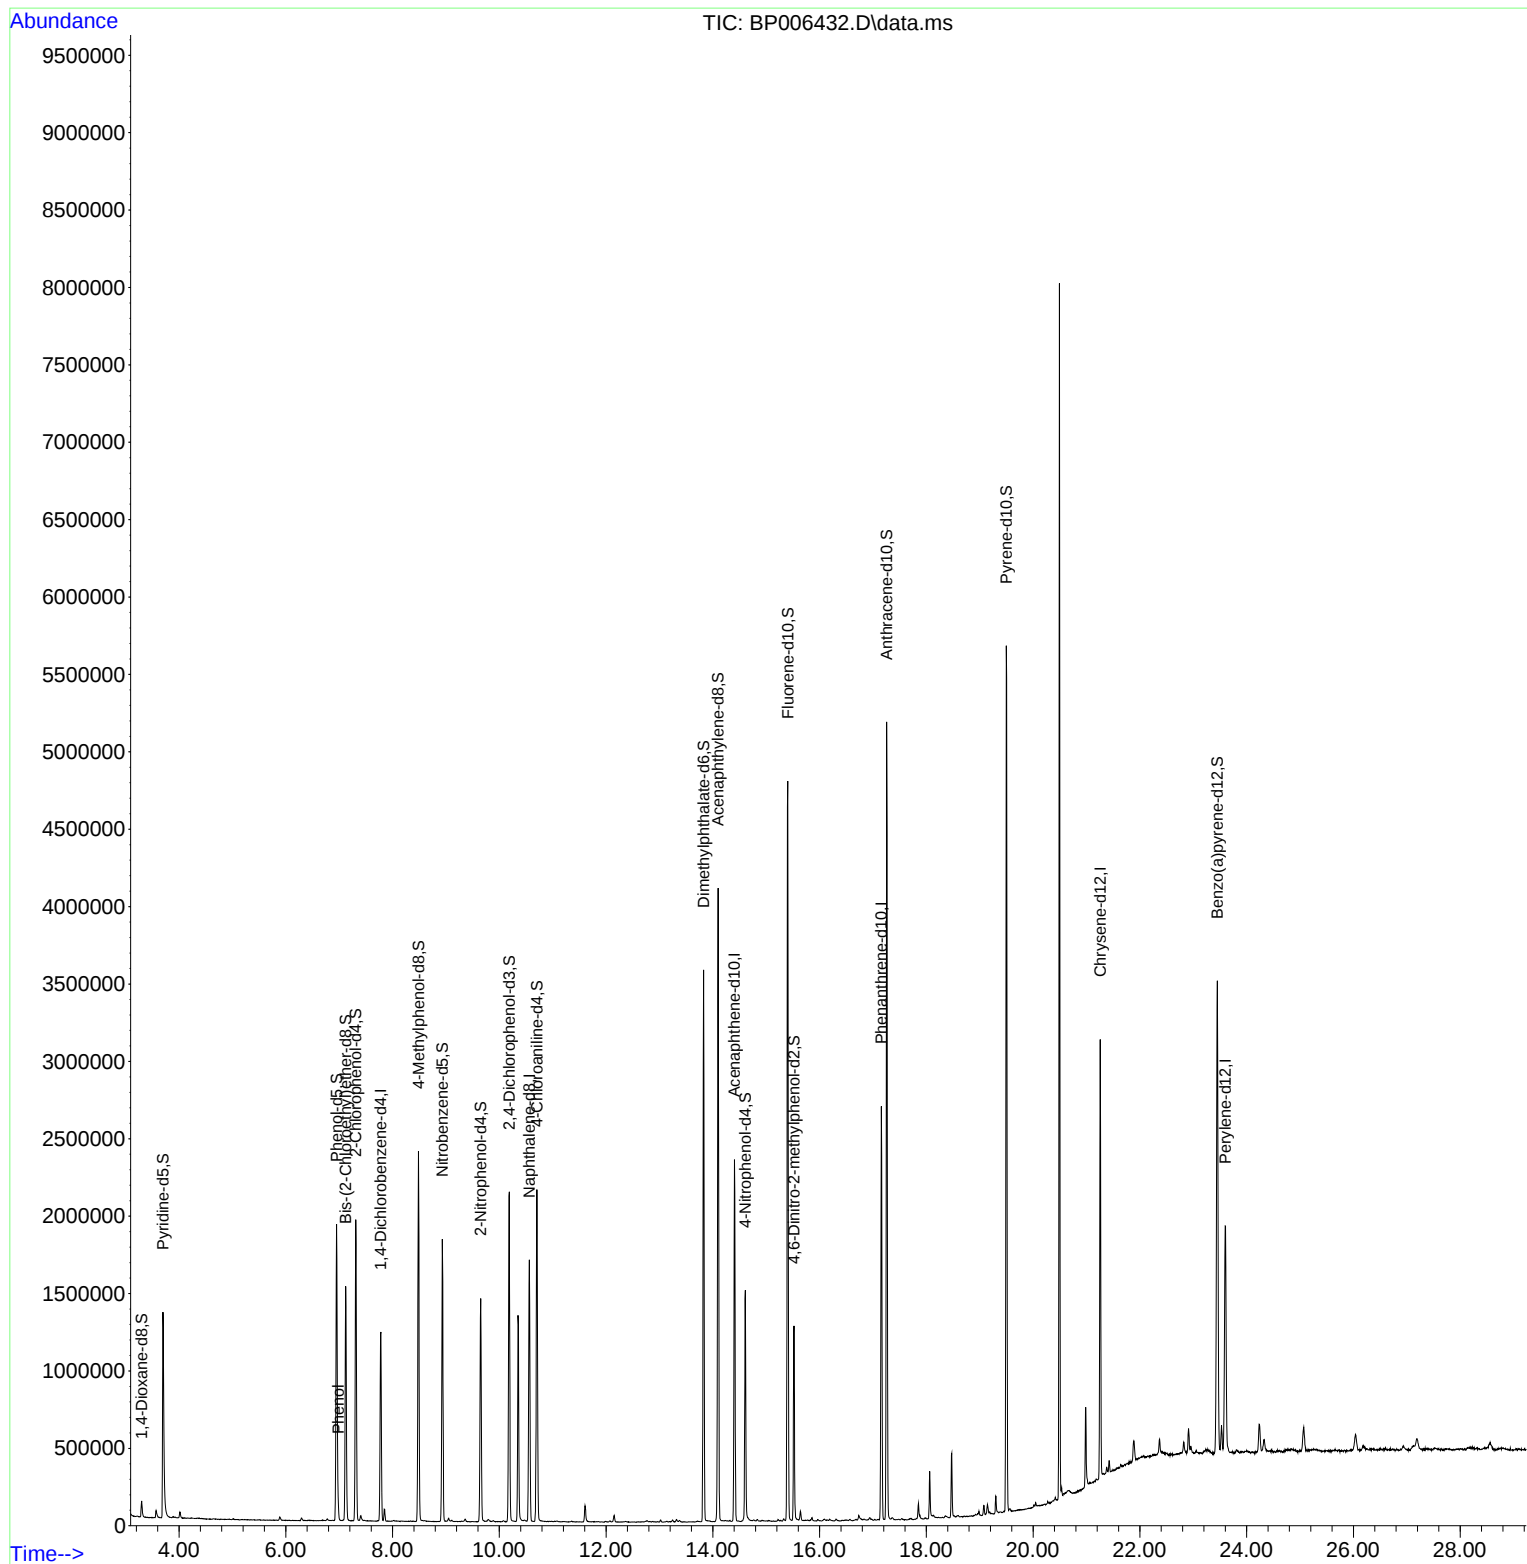

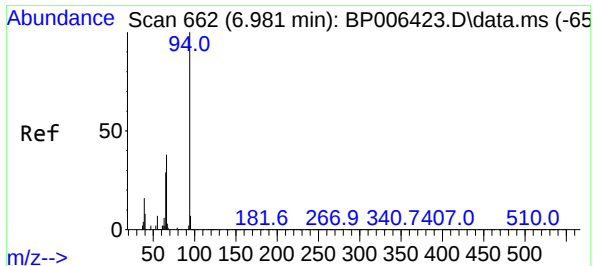

#8
Phenol
Concen: 2.040 ng/ul
RT: 6.981 min Scan# 662
Delta R.T. 0.000 min
Lab File: BP006432.D
Acq: 29 Jul 2021 21:41

Instrument :
BNA_P
ClientSampleId :
BGEP4

Tgt Ion: 94 Resp: 61370
Ion Ratio Lower Upper
94 100
65 29.1 23.4 35.0
66 41.3 31.1 46.7

