
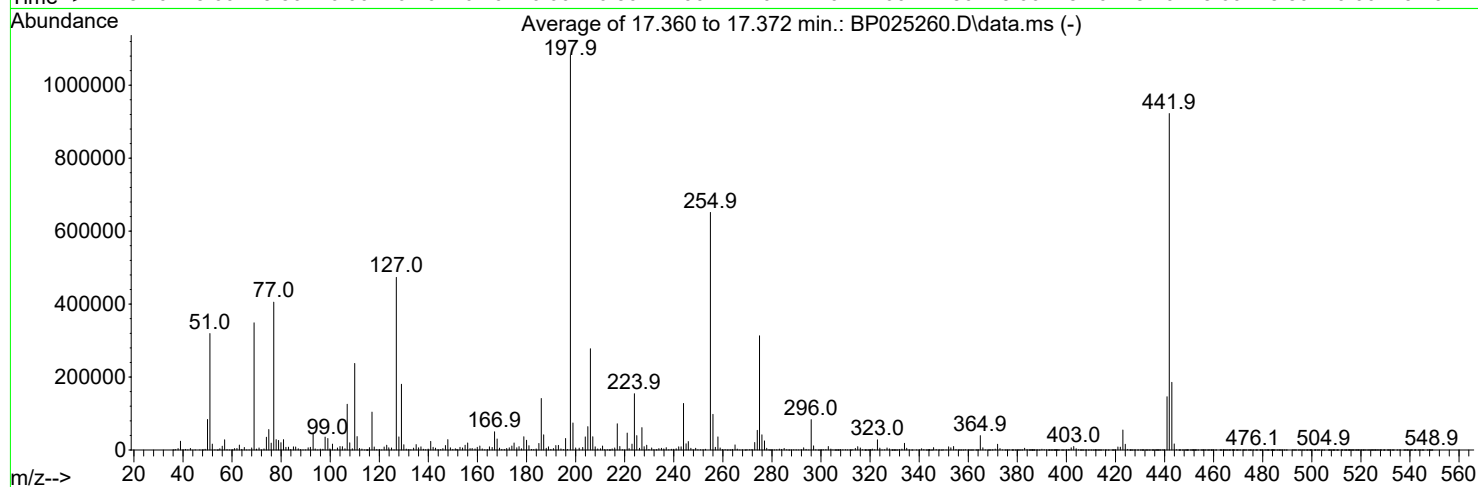


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072925\
Data File : BP025260.D
Acq On : 29 Jul 2025 13:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 29 15:28:11 2025

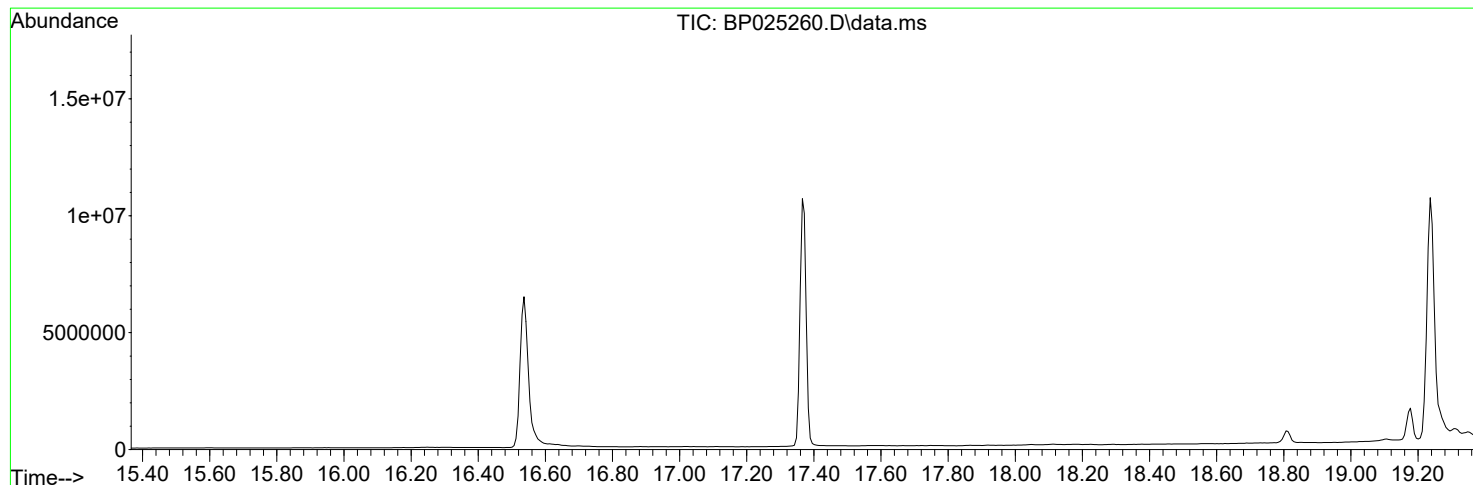

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	5858	PASS
69	69	100	100	100.0	348909	PASS
70	69	0.00	2	0.7	2560	PASS
197	198	0.00	2	0.1	1439	PASS
198	198	100	100	100.0	1082412	PASS
199	198	5	9	6.8	74143	PASS
365	198	1	100	3.6	39353	PASS
441	443	0.01	150	78.7	146115	PASS
442	442	100	100	100.0	922363	PASS
443	442	15	24	20.1	185746	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/29/2025	BNA_P	<u>BP025260.D</u>
Compound Name	Response	Retention Time
DDT	4574040	20.536
DDD	83023	20.118
DDE	3950	19.536
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
86973	4661013	1.87

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072925\
Data File : BP025260.D
Acq On : 29 Jul 2025 13:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 29 17:44:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

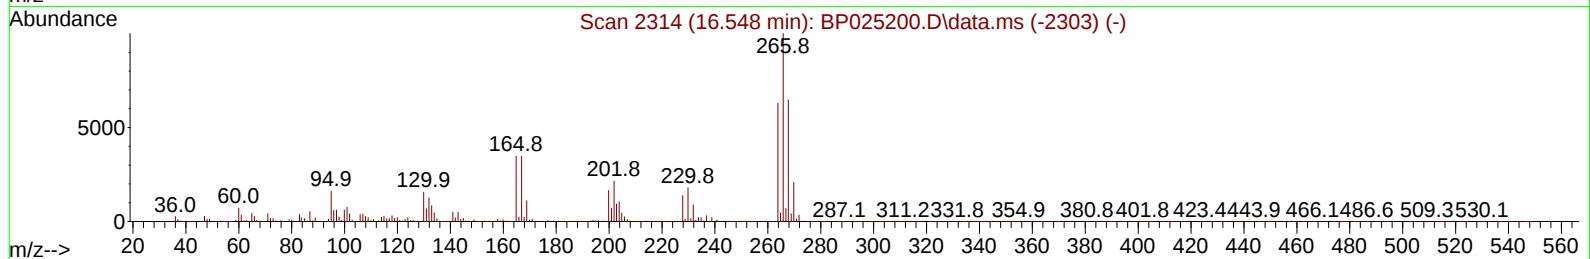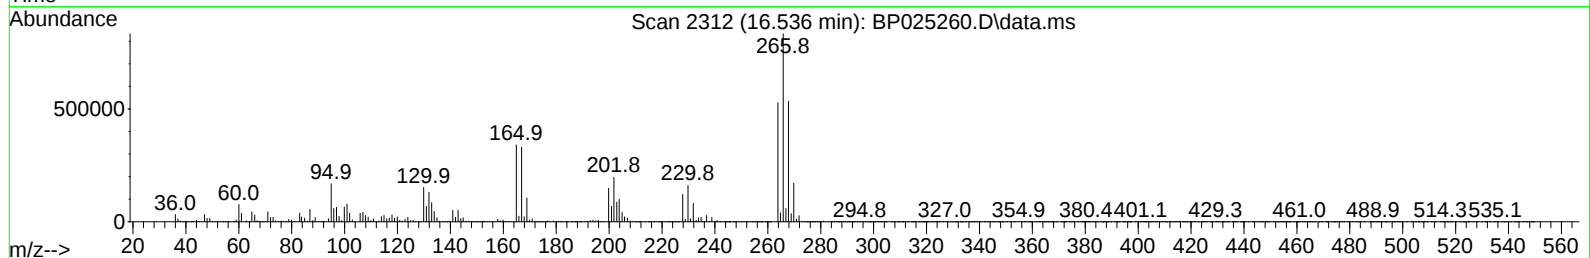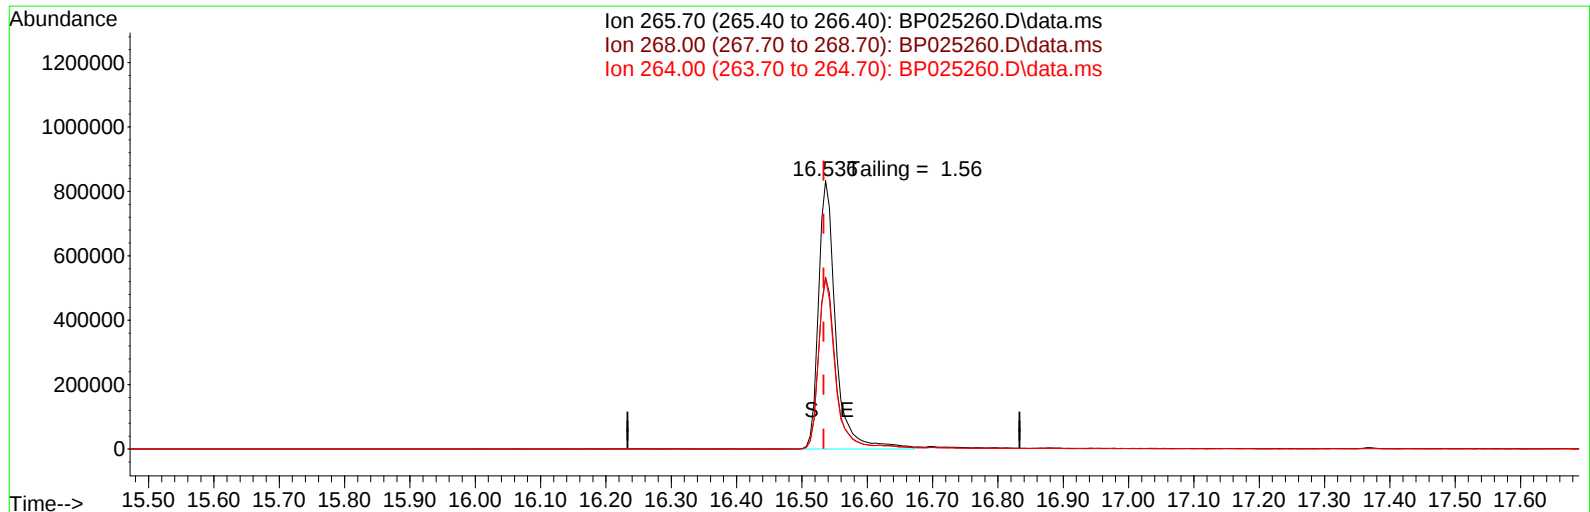

TIC: BP025260.D\data.ms

(70) Pentachlorophenol (C)

16.536min (+ 0.003) 164713.90 ng




response 1533754

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.06
264.00	62.90	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072925\
Data File : BP025260.D
Acq On : 29 Jul 2025 13:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 29 17:44:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

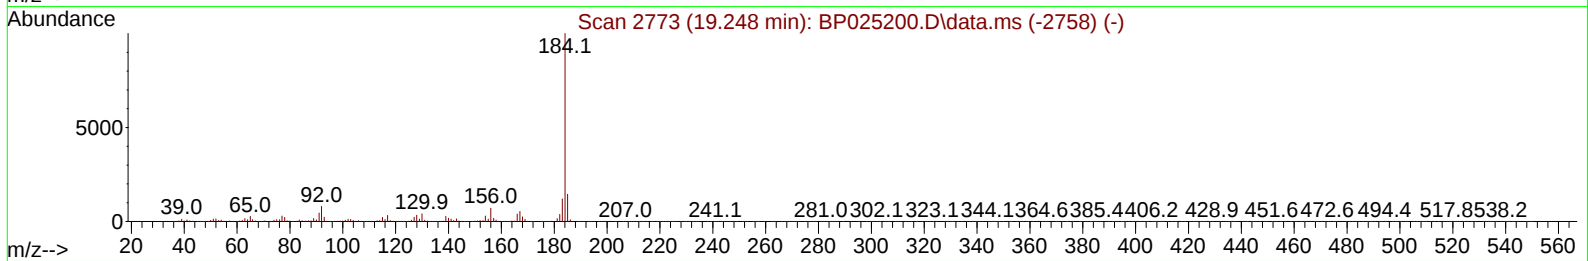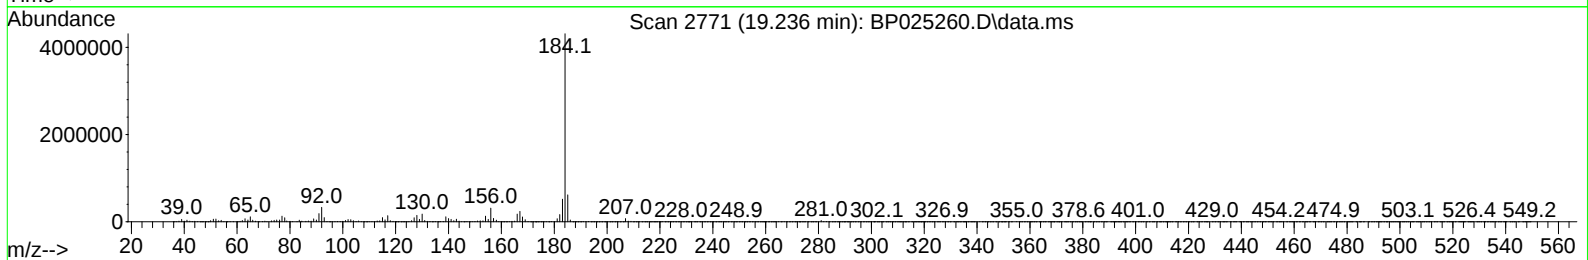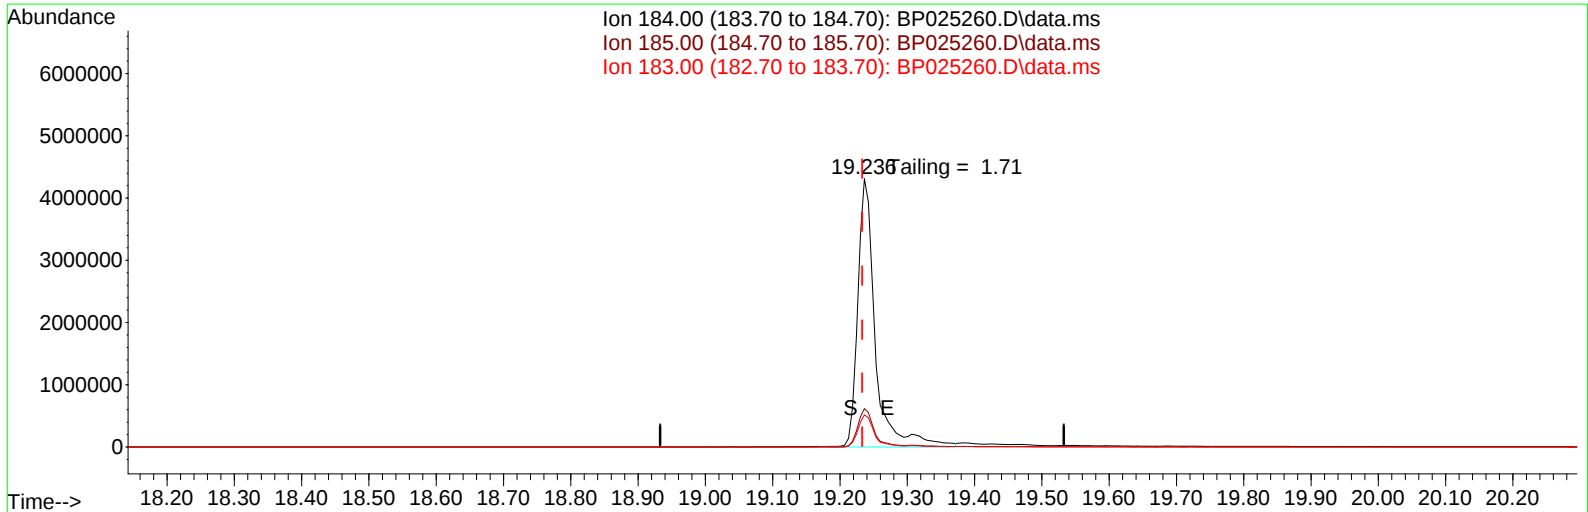

TIC: BP025260.D\data.ms

(77) Benzidine

19.236min (+ 0.003) 66020.40 ng

response 7278014

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.33
183.00	12.00	12.02
0.00	0.00	0.00