




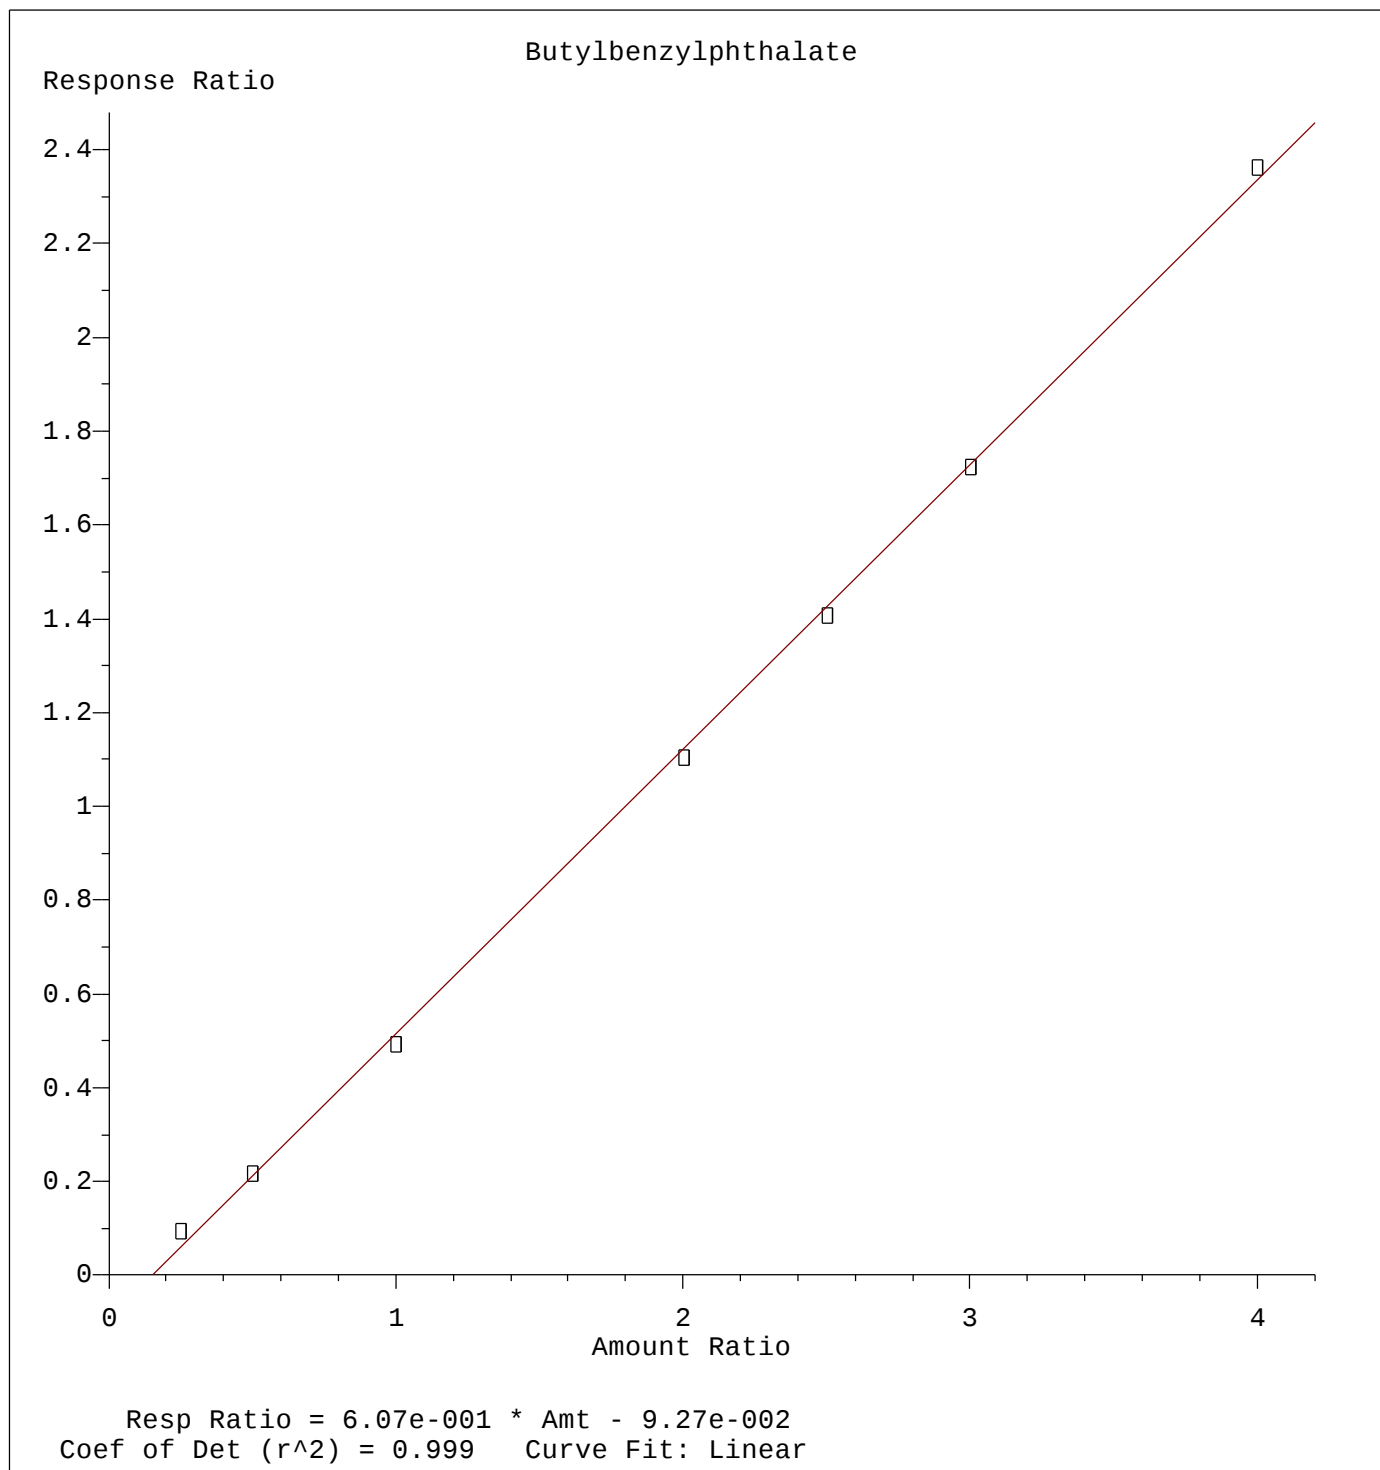

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020

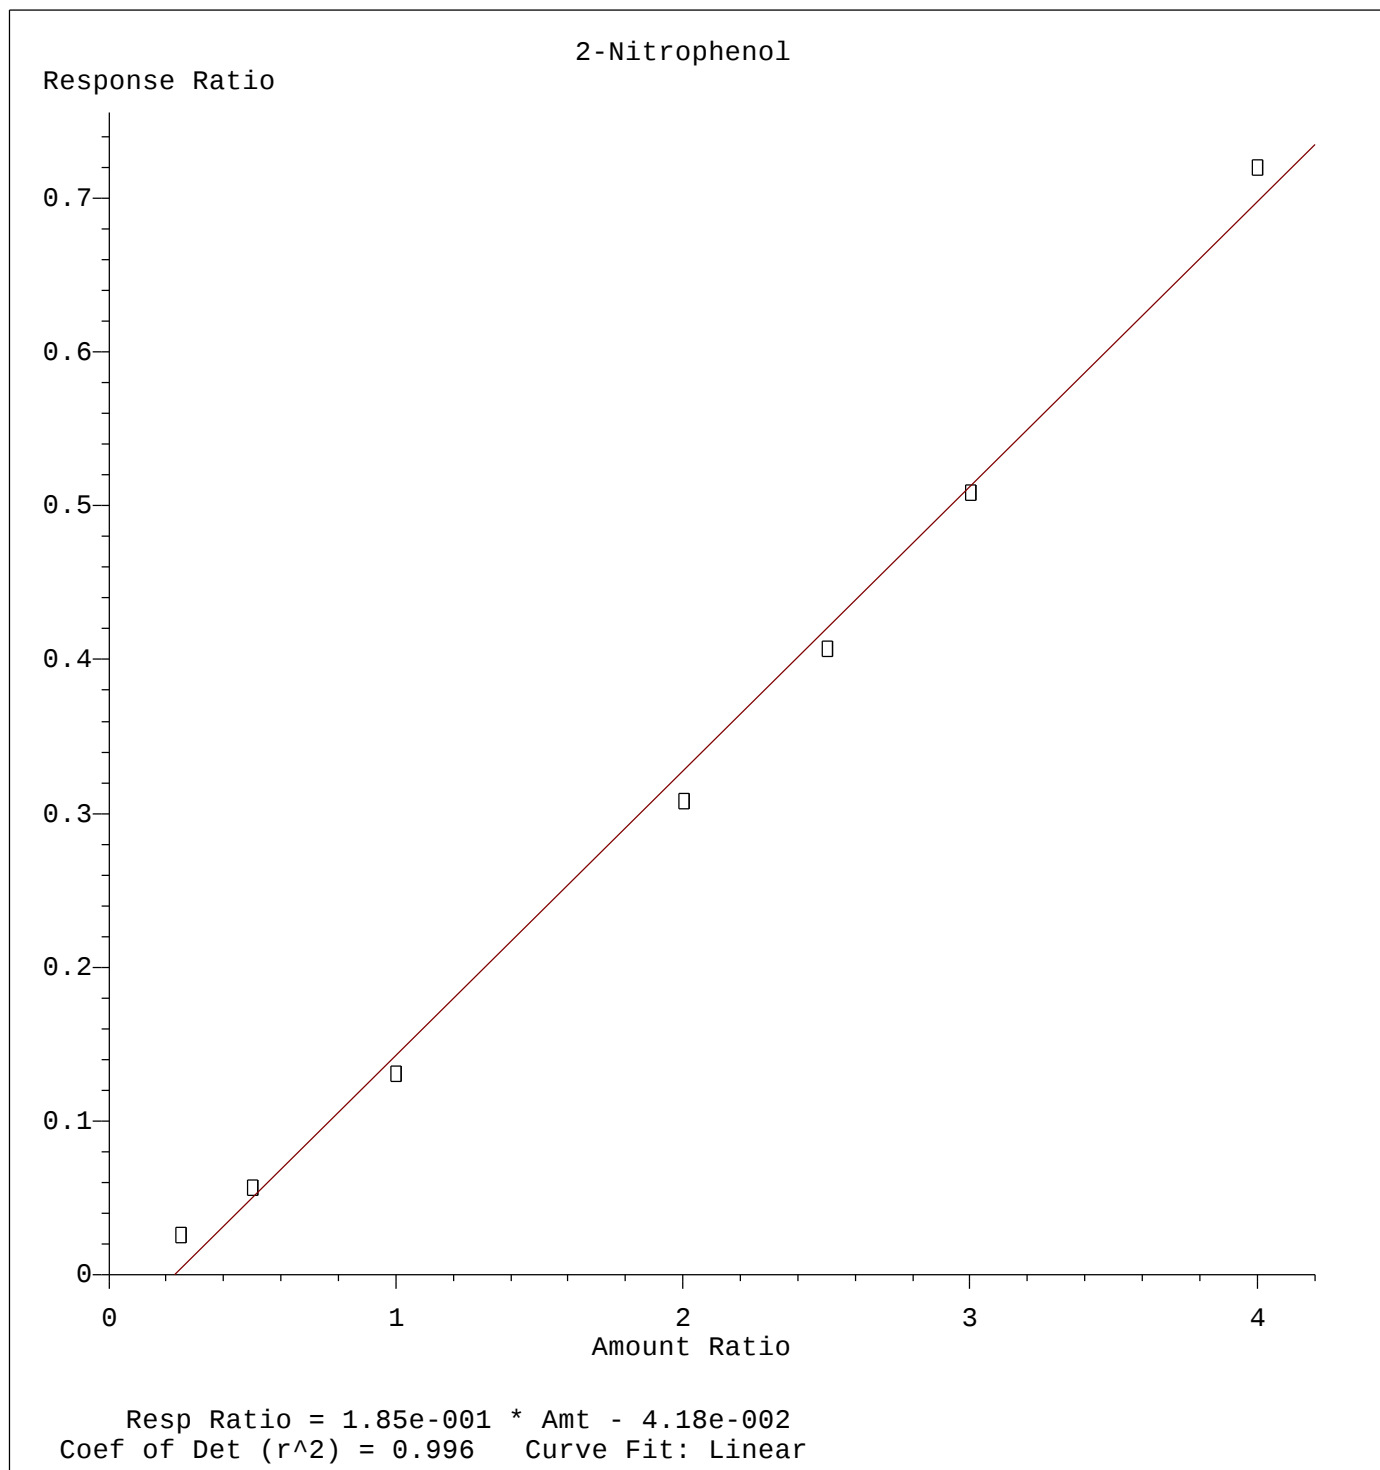


Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020

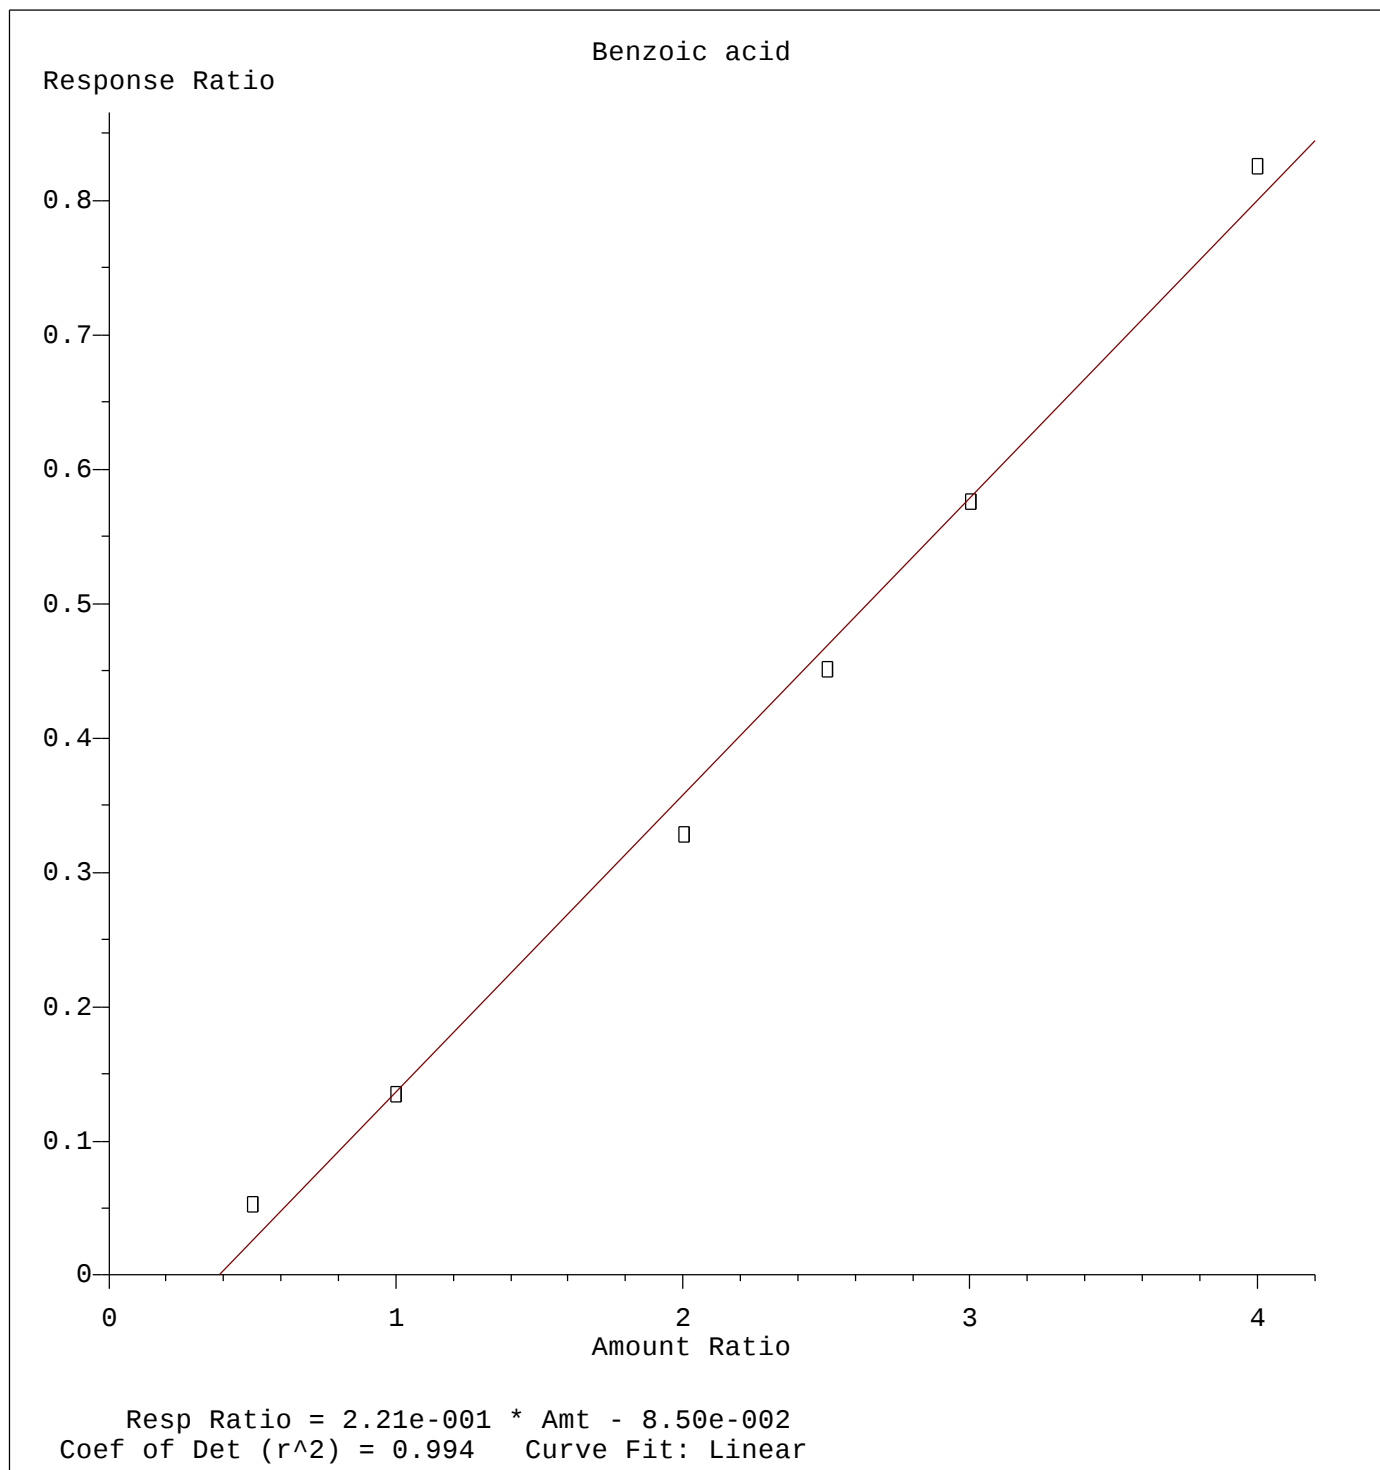

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020

2-Nitroaniline

Response Ratio

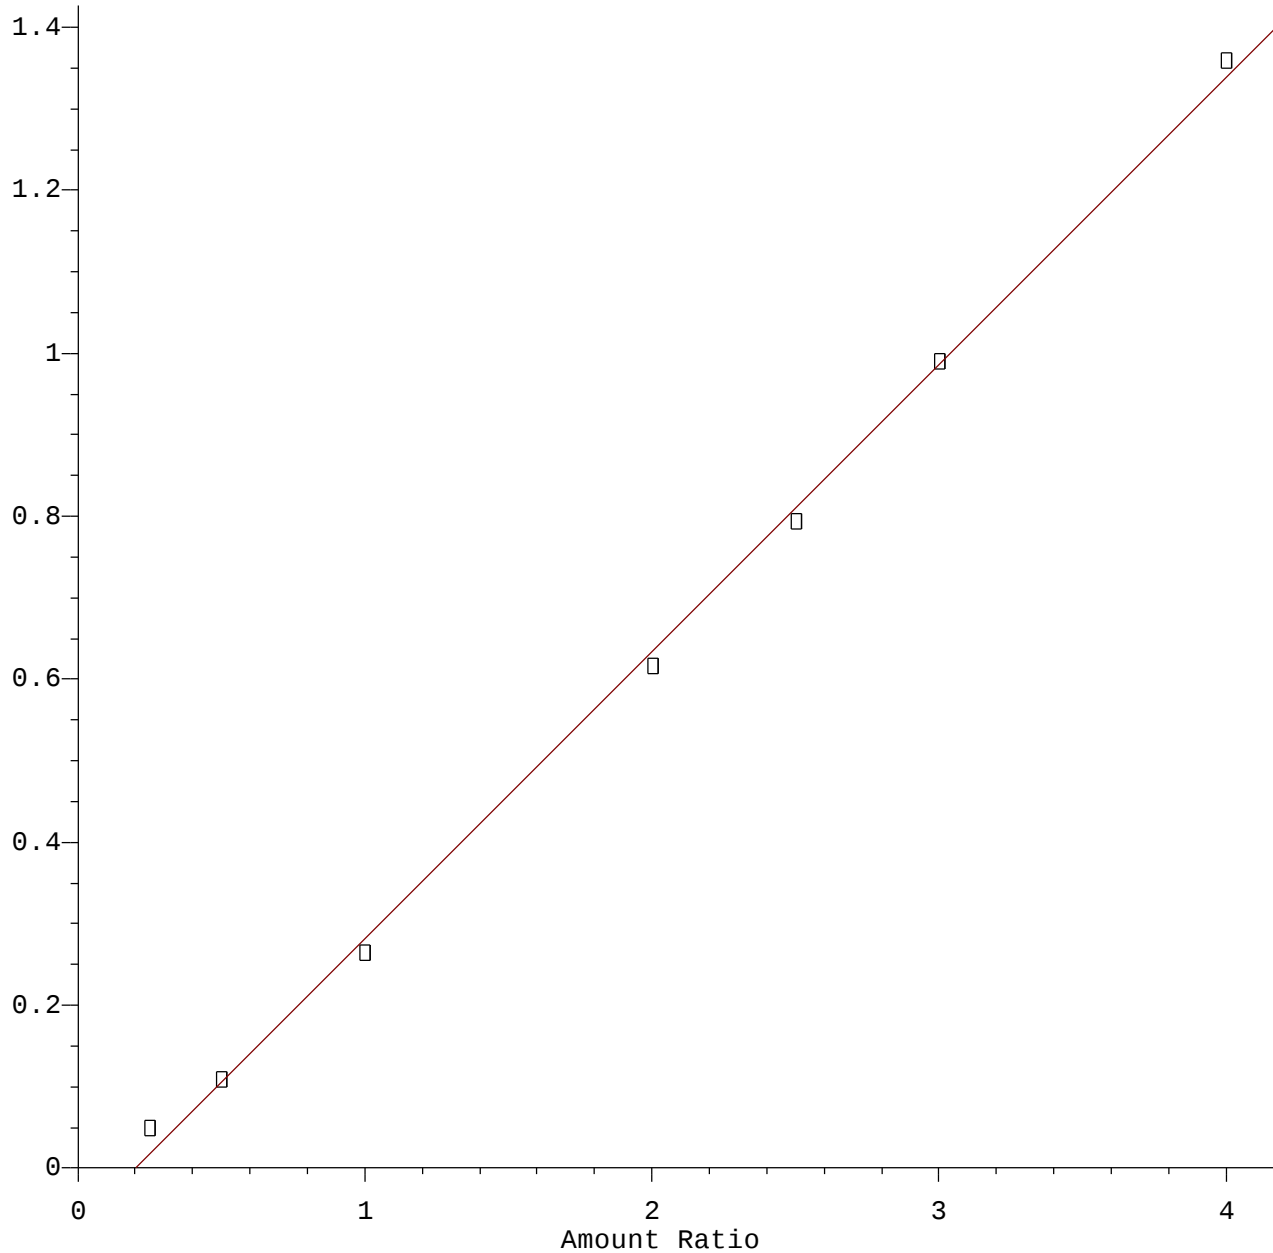


Resp Ratio = $3.52 \times 10^{-1} \times \text{Amt} - 6.99 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020


2,6-Dinitrotoluene

Response Ratio

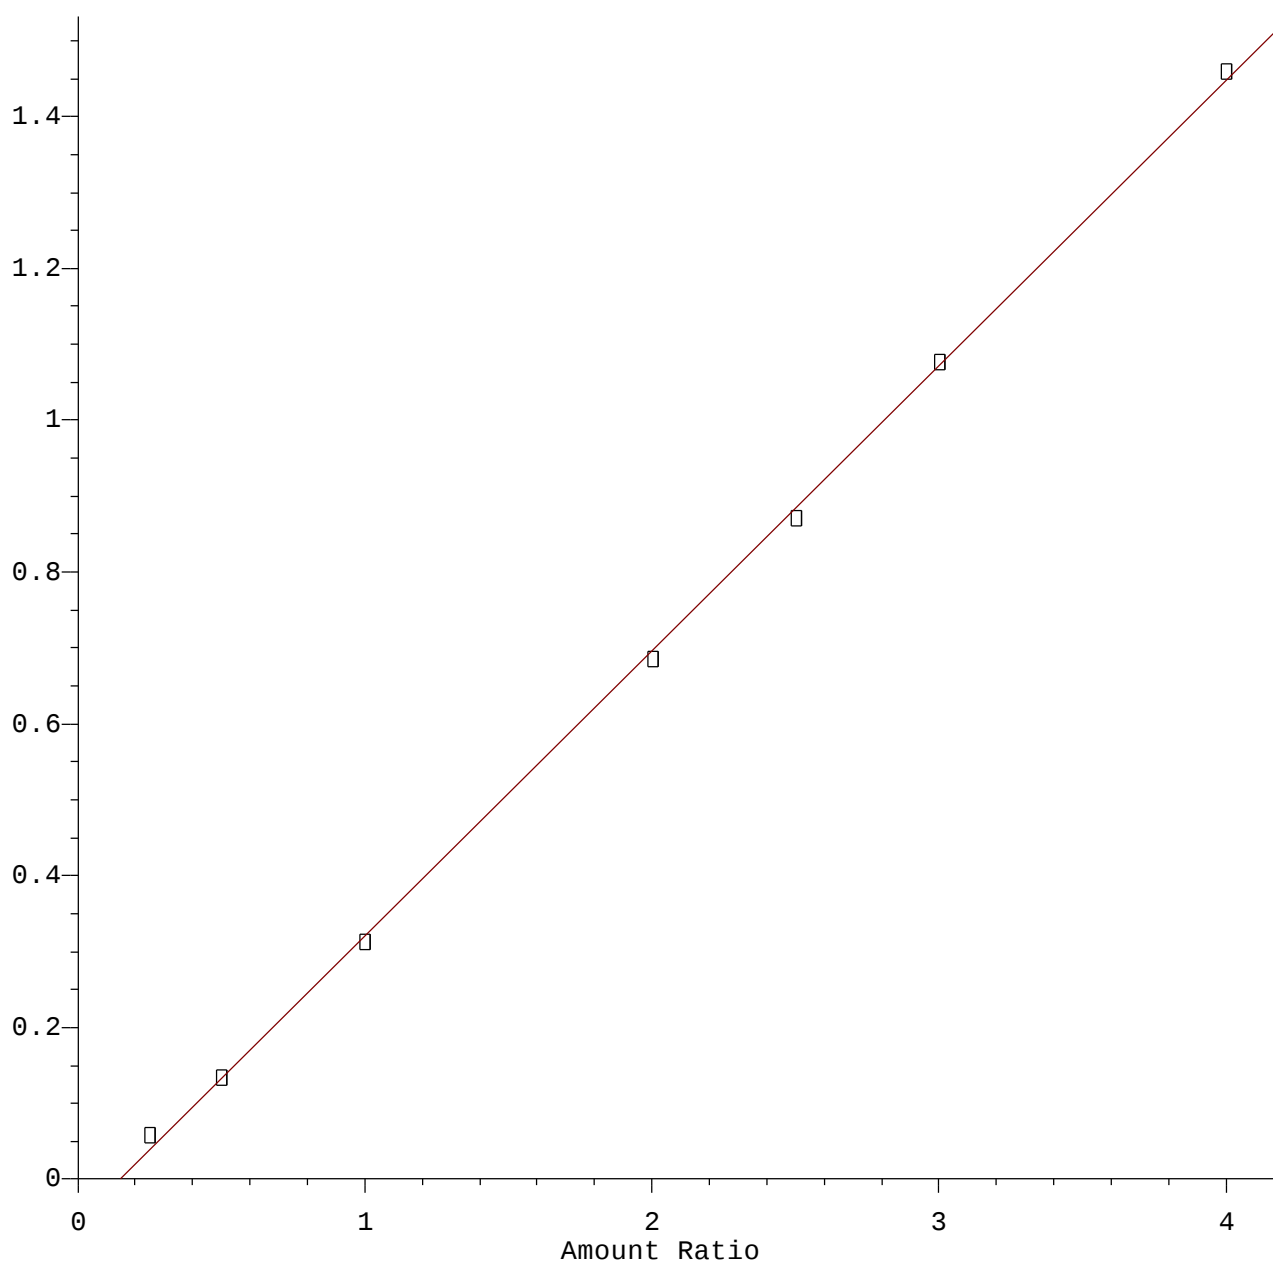

Resp Ratio = $3.75 \times 10^{-1} \times \text{Amt} - 5.44 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020

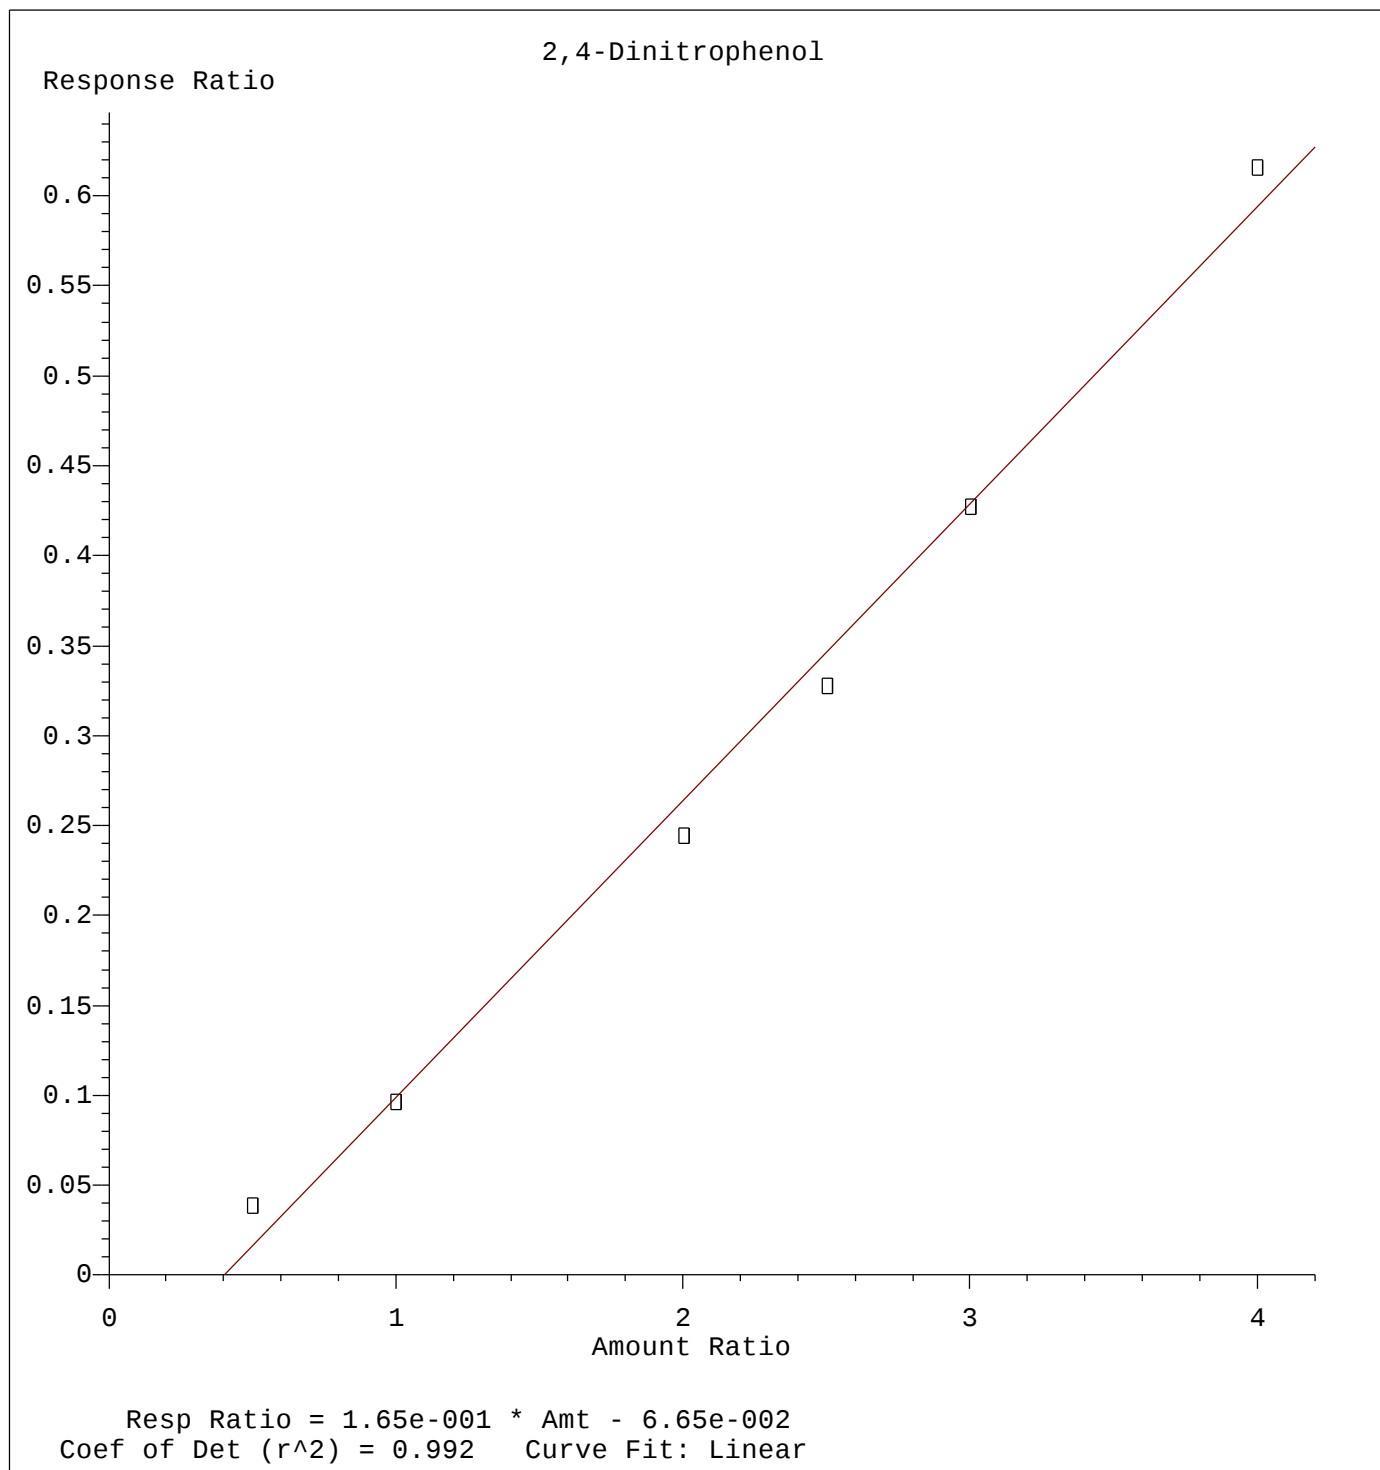

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020


2,4-Dinitrotoluene

Response Ratio

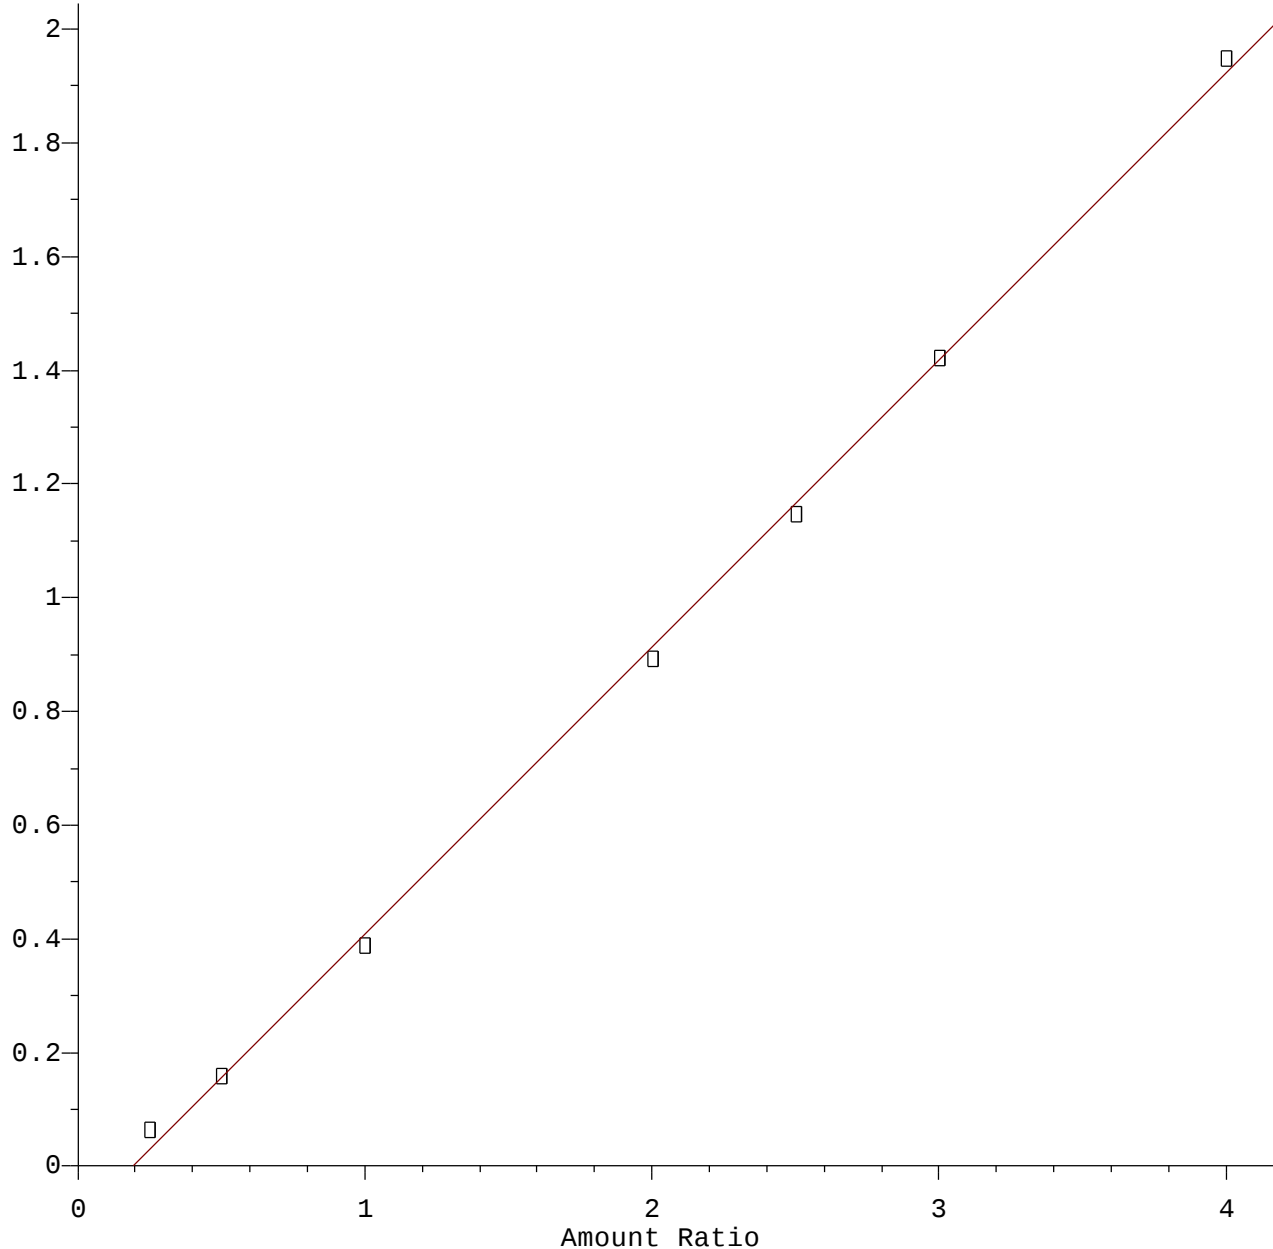


Resp Ratio = $5.05 \times 10^{-1} \times \text{Amt} - 9.60 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020

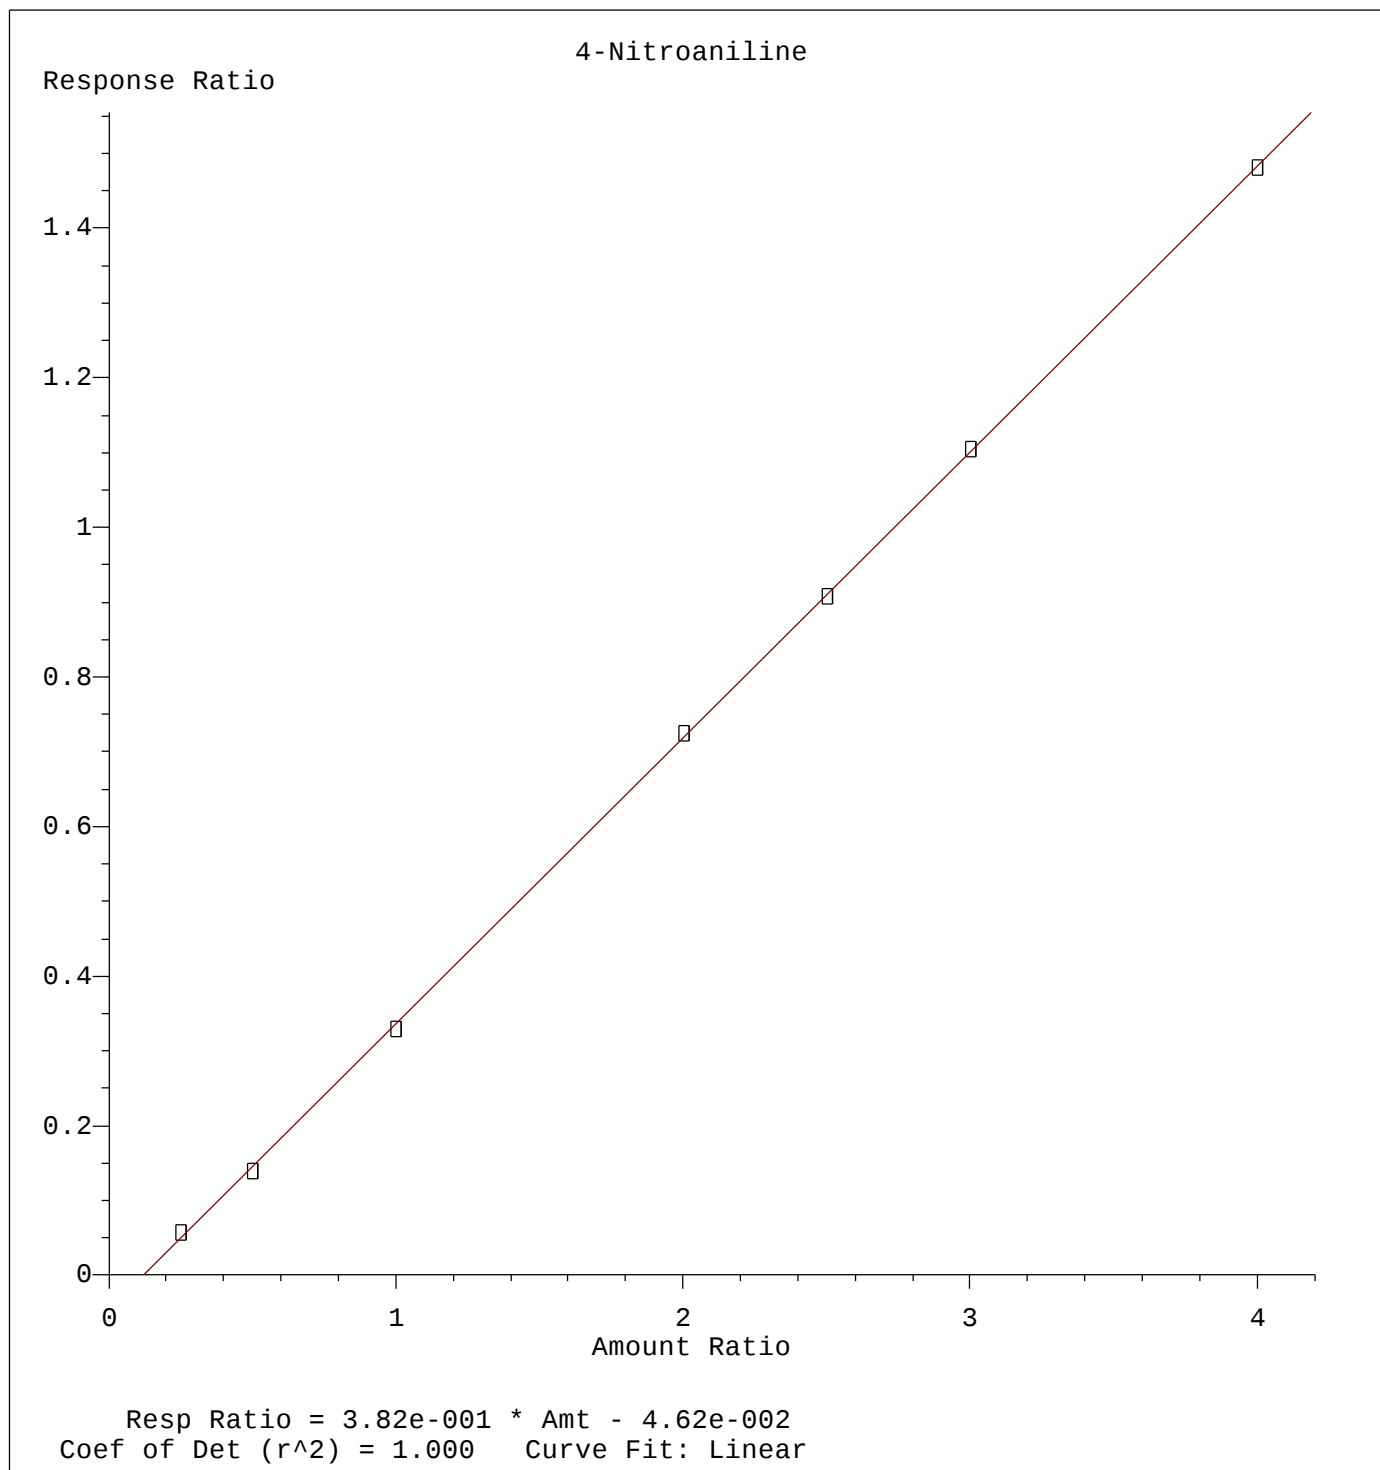

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020

4,6-Dinitro-2-methylphenol

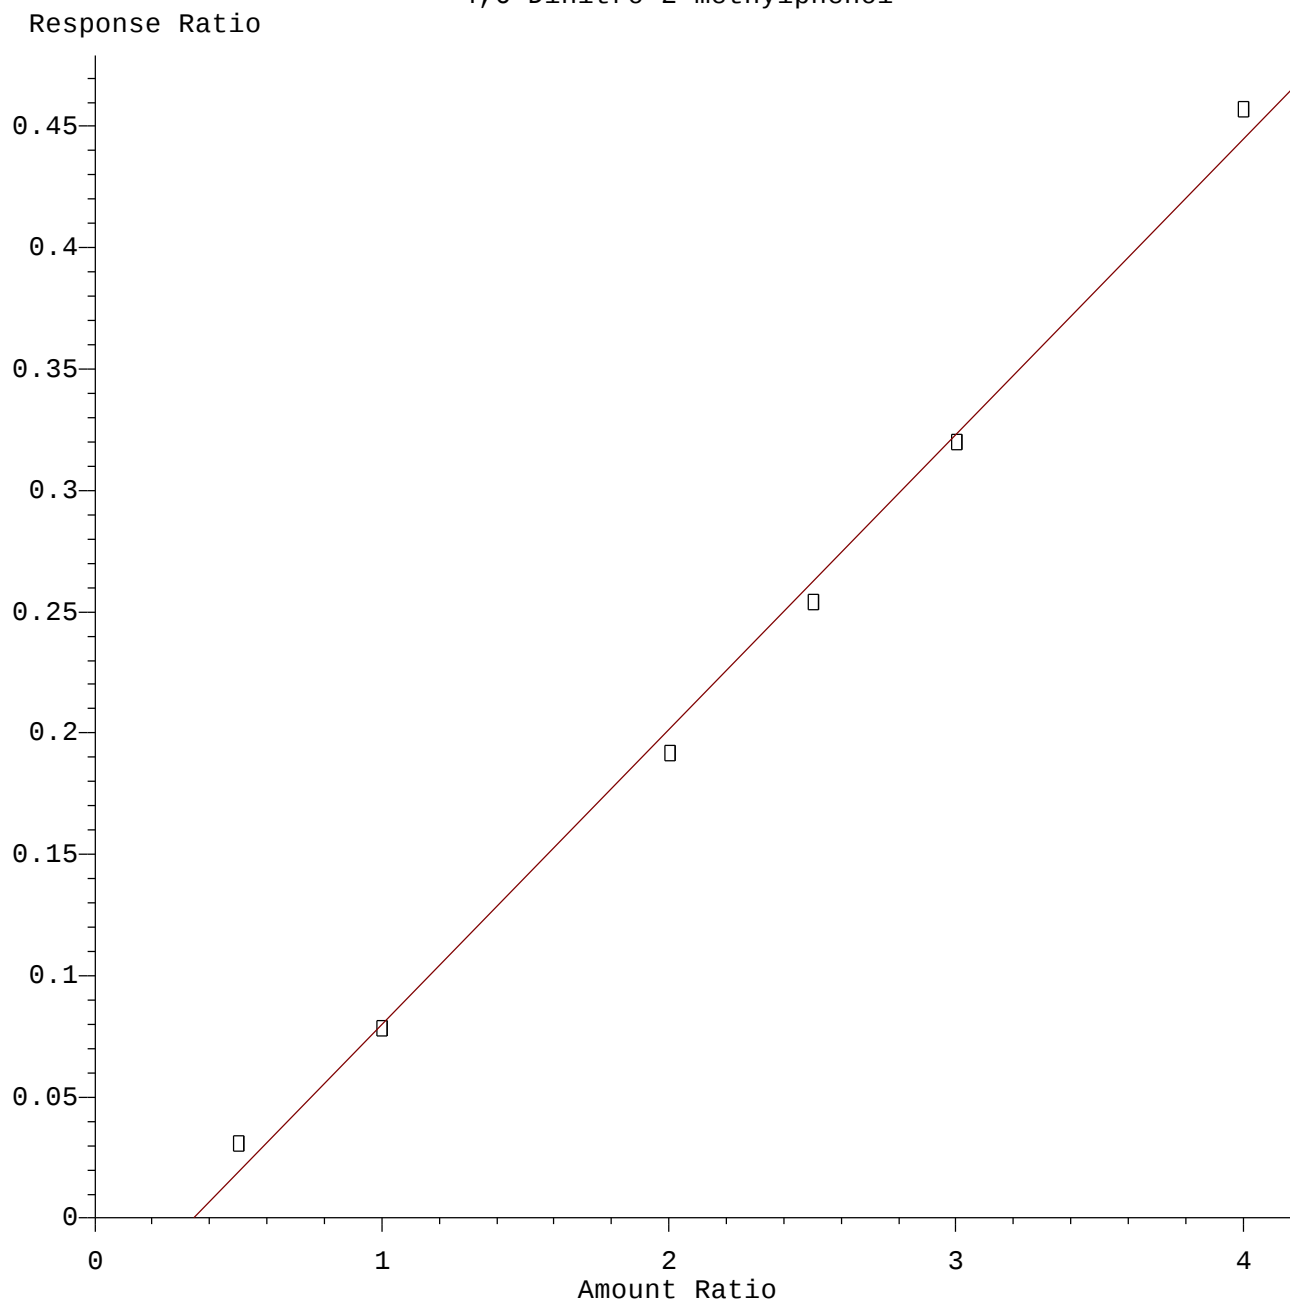


Resp Ratio = $1.22 \times 10^{-1} \times \text{Amt} - 4.20 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020

3-Nitroaniline

Response Ratio

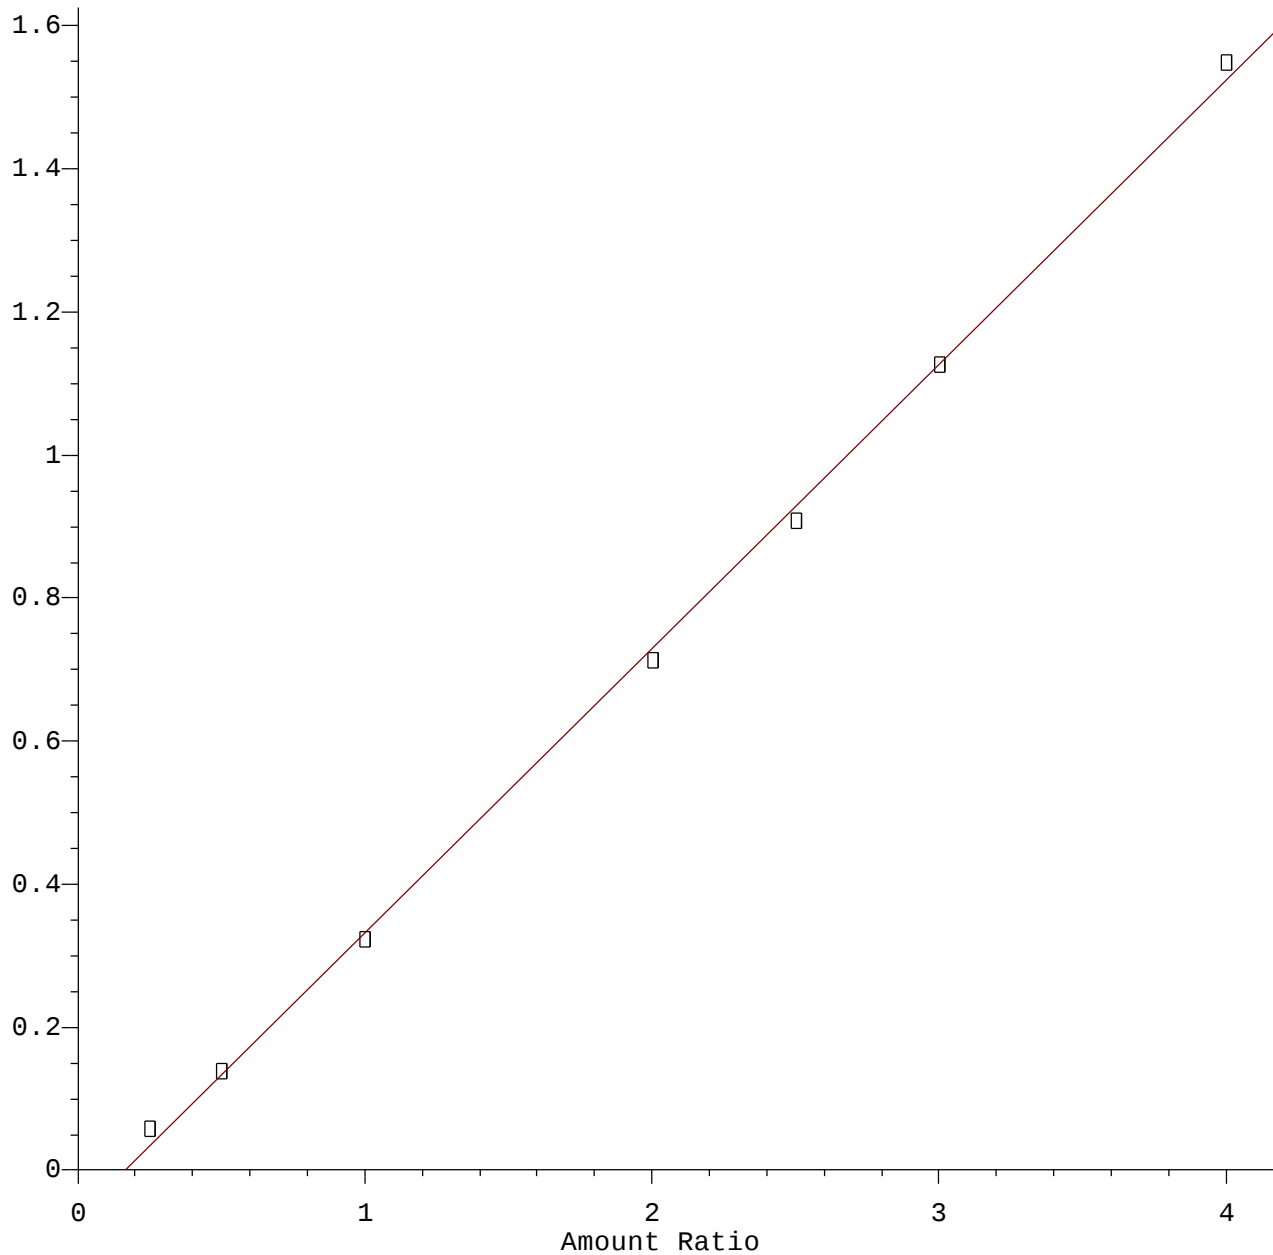

Resp Ratio = 3.97e-001 * Amt - 6.50e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Calibration Table Last Updated: Thu Jul 30 15:30:34 2020