
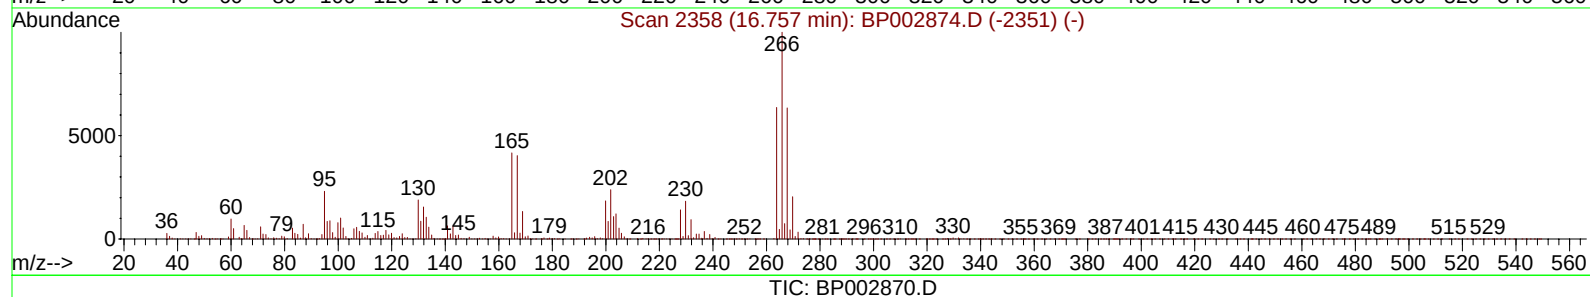
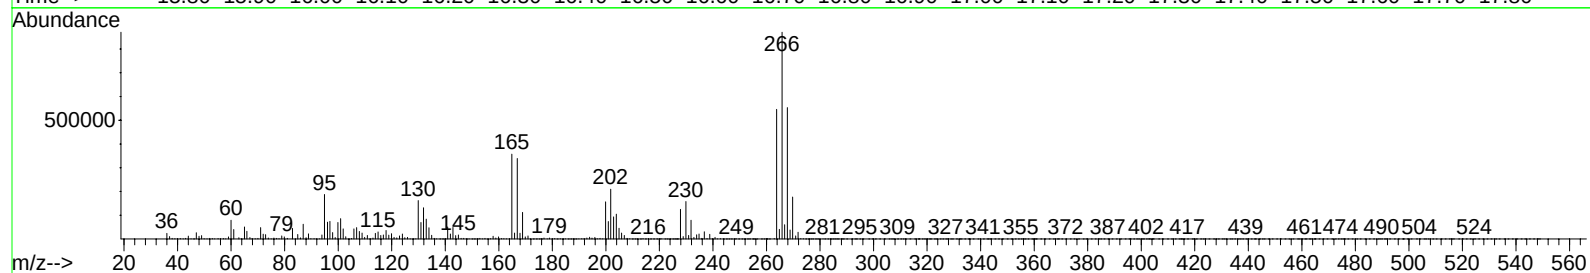


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073020\
 Data File : BP002870.D
 Acq On : 30 Jul 2020 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 18:29:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 15:30:34 2020
 Response via : Initial Calibration

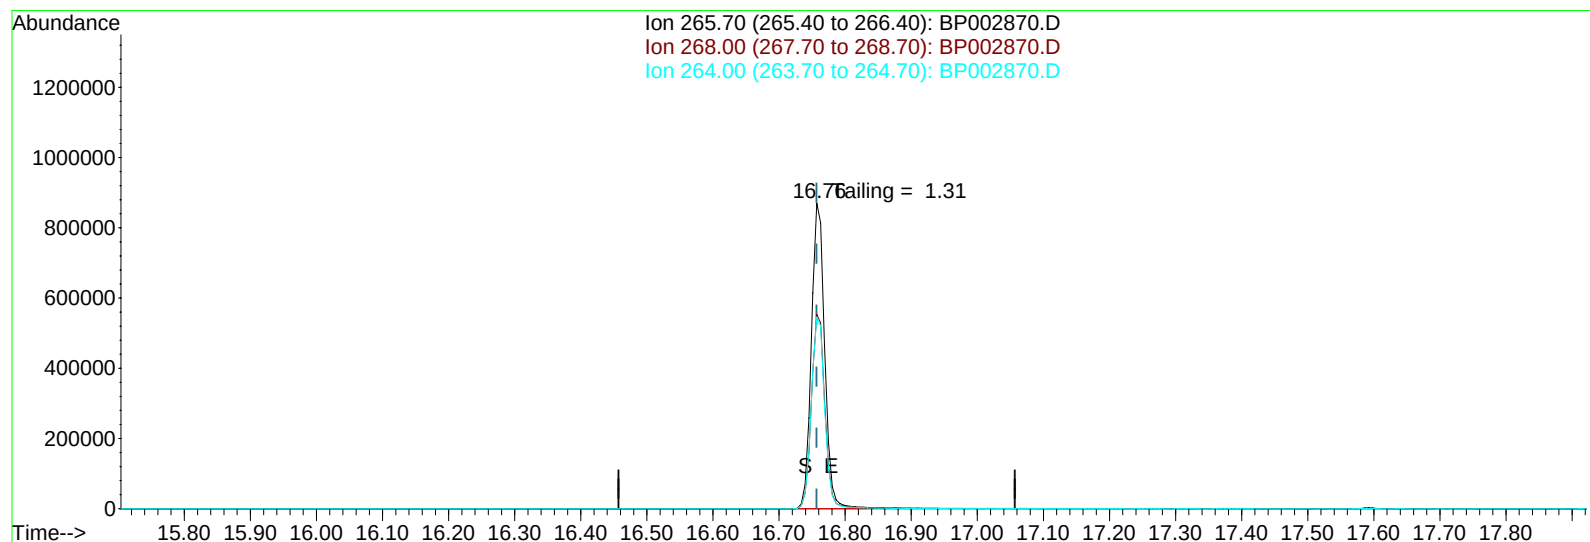

(70) Pentachlorophenol (C)




16.757min (0.000) 73722.11ng

response 1226541

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	63.51
264.00	63.60	62.70
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073020\
 Data File : BP002870.D
 Acq On : 30 Jul 2020 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 18:29:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 15:30:34 2020
 Response via : Initial Calibration

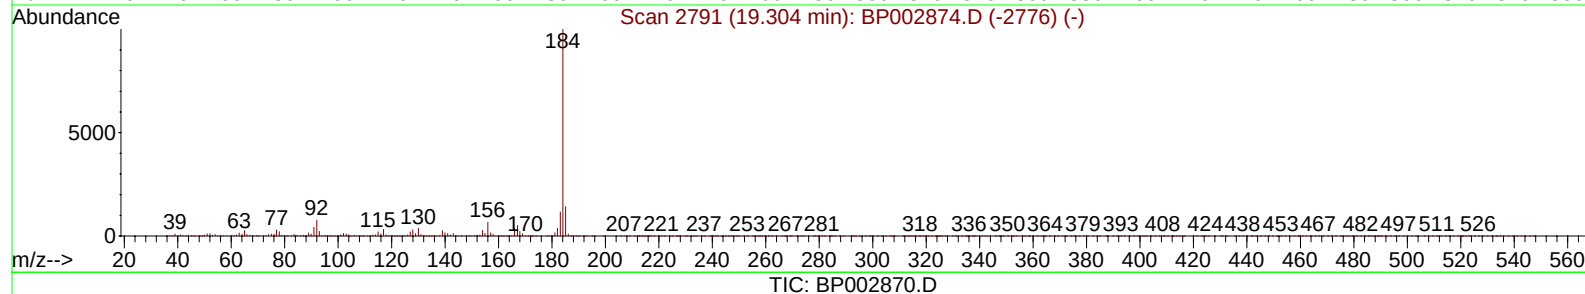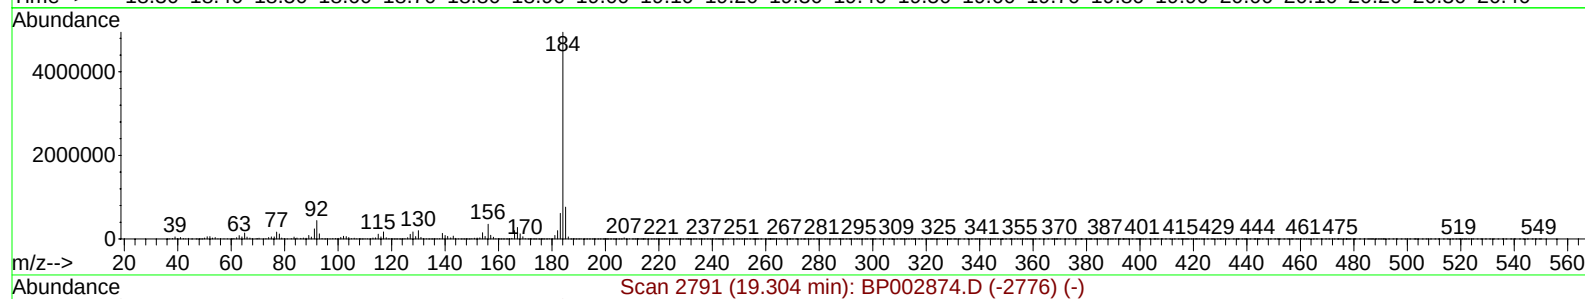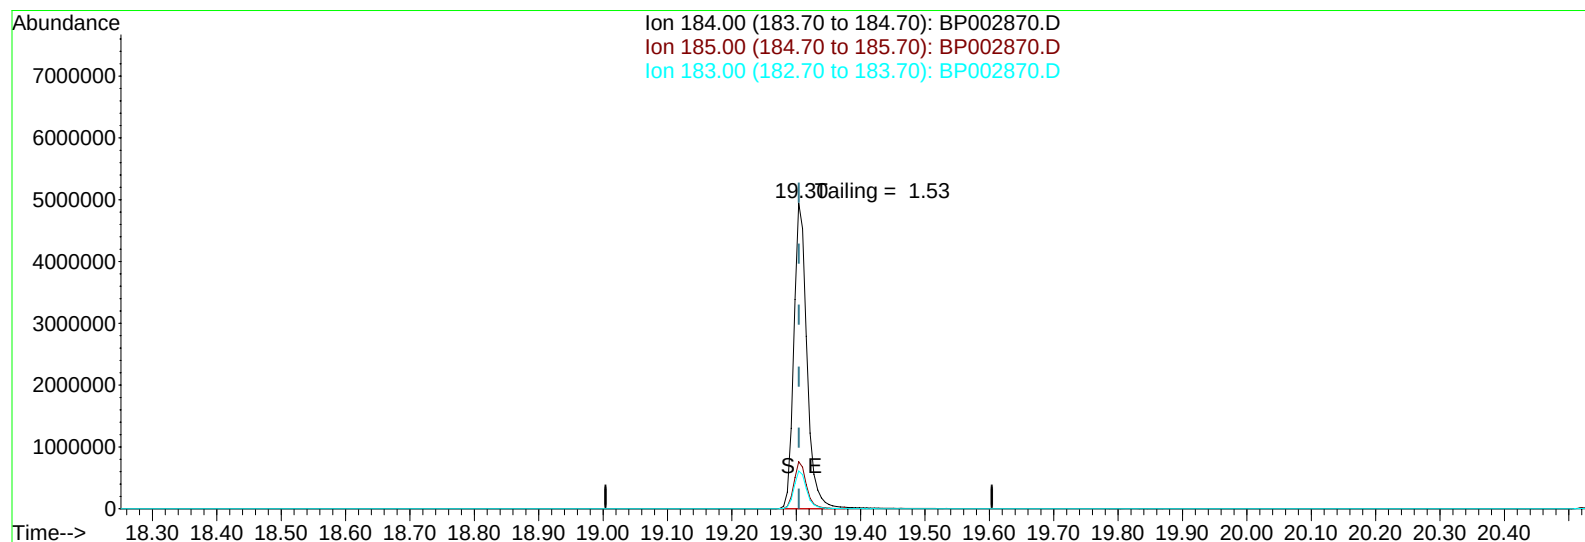

(77) Benzidine

19.304min (0.000) 104654.52ng

response 7084655

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	15.40
183.00	11.60	12.36
0.00	0.00	0.00