


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073020\
 Data File : BP002870.D
 Acq On : 30 Jul 2020 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 15:30:34 2020

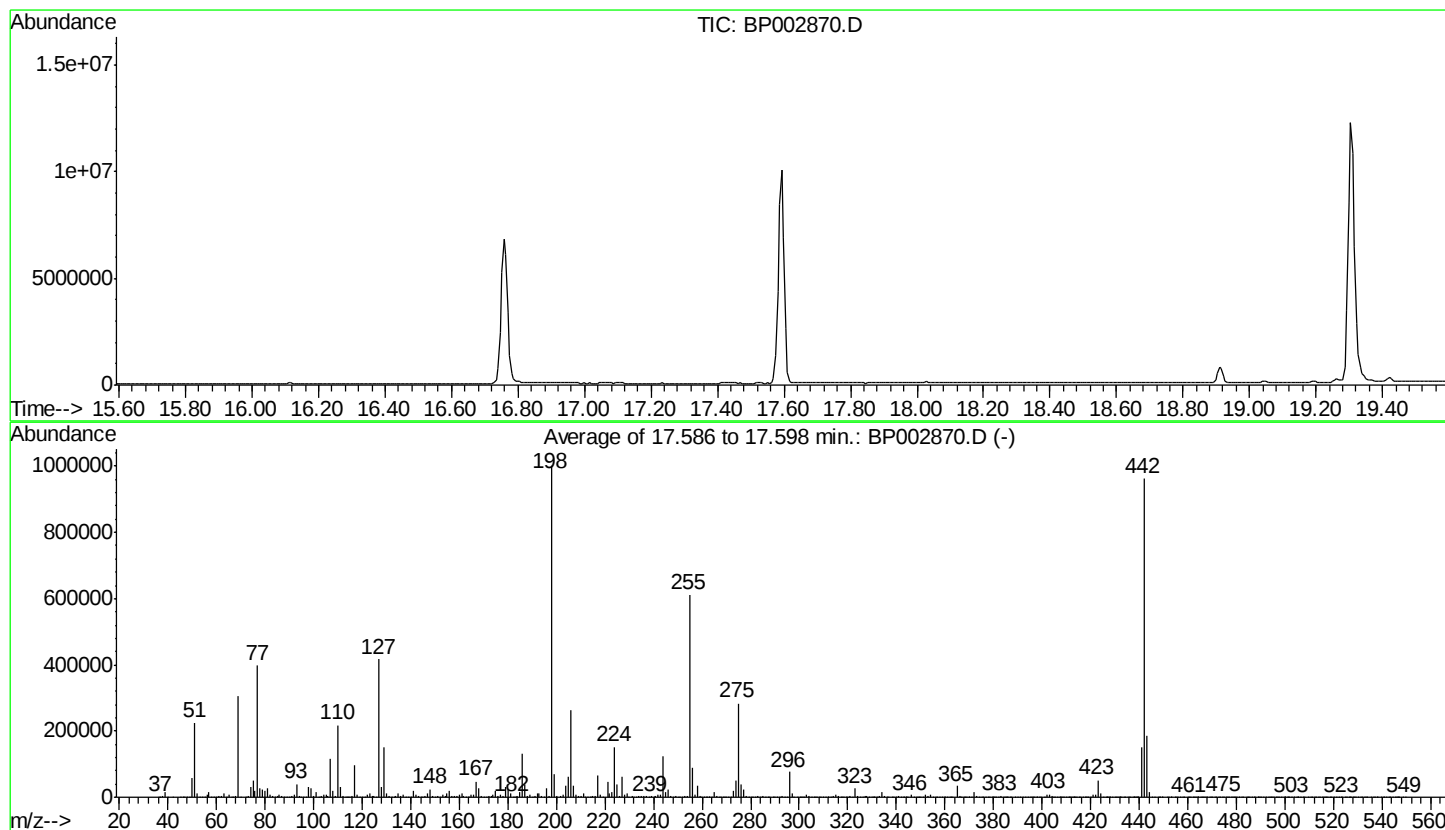

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	224620	PASS
68	69	0.00	2	1.5	4619	PASS
69	198	0.00	100	30.7	307370	PASS
70	69	0.00	2	0.5	1555	PASS
127	198	10	80	41.6	416706	PASS
197	198	0.00	2	0.3	2700	PASS
198	198	100	100	100.0	1001742	PASS
199	198	5	9	6.8	68145	PASS
275	198	10	60	28.2	282775	PASS
365	198	1	100	3.5	34712	PASS
441	198	0.01	100	14.9	149392	PASS
442	198	50	100	95.9	961109	PASS
443	442	15	24	19.3	185633	PASS