

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
 Data File : BP002892.D
 Acq On : 31 Jul 2020 14:08
 Operator : CG/JU
 Sample : PB130646BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jul 31 14:52:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 15:30:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	604214	20.00	ng	0.00
21) Naphthalene-d8	10.50	136	2331746	20.00	ng	0.00
39) Acenaphthene-d10	14.35	164	1409957	20.00	ng	0.00
64) Phenanthrene-d10	17.10	188	2984622	20.00	ng	0.00
76) Chrysene-d12	21.20	240	2463558	20.00	ng	0.00
86) Perylene-d12	23.46	264	2052514	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	4615463	116.91	ng	0.00
7) Phenol-d6	6.89	99	5805888	105.93	ng	0.00
23) Nitrobenzene-d5	8.86	82	3543239	82.30	ng	0.00
42) 2,4,6-Tribromophenol	15.84	330	2113709	120.62	ng	0.00
45) 2-Fluorobiphenyl	12.97	172	7848901	76.06	ng	0.00
79) Terphenyl-d14	19.69	244	9708048	78.89	ng	0.00
Target Compounds						
26) 2-Nitrophenol	9.61	139	19	4.521	ng	# 1
32) Benzoic acid	9.80	122	24	7.687	ng	# 1
48) 2-Nitroaniline	13.41	65	82	3.975	ng	# 43
51) 2,6-Dinitrotoluene	13.91	165	49	2.901	ng	# 7
53) 3-Nitroaniline	14.26	138	83	3.276	ng	# 1
54) 2,4-Dinitrophenol	14.43	184	16	8.059	ng	# 1
57) 2,4-Dinitrotoluene	14.70	165	129	3.809	ng	# 64
62) 4-Nitroaniline	15.38	138	176	2.423	ng	# 71
65) 4,6-Dinitro-2-methylphenol	15.48	198	10	6.901	ng	# 1
80) Butylbenzylphthalate	20.39	149	413	3.063	ng	# 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
Data File : BP002892.D
Acq On : 31 Jul 2020 14:08
Operator : CG/JU
Sample : PB130646BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Jul 31 14:52:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 15:30:34 2020
Response via : Initial Calibration

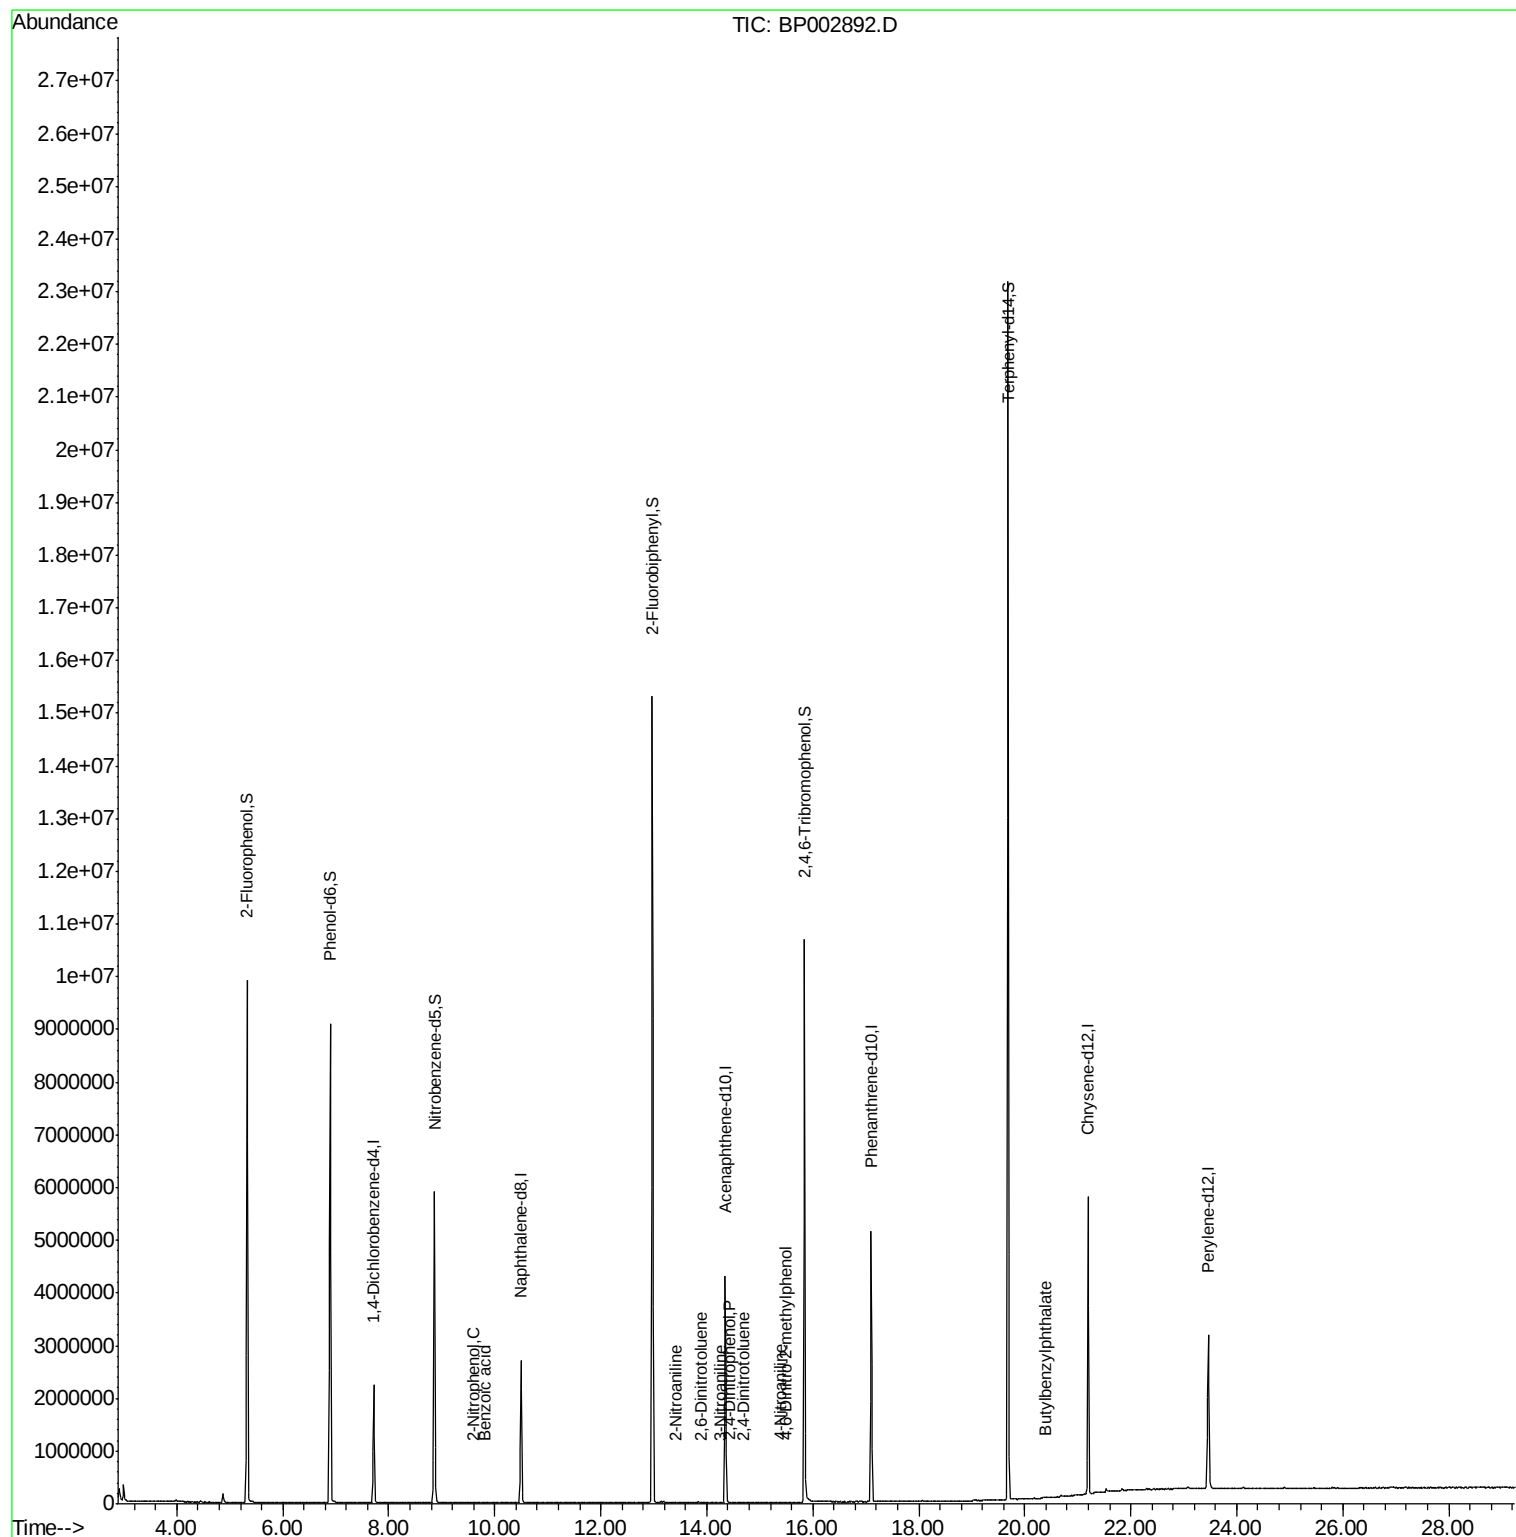

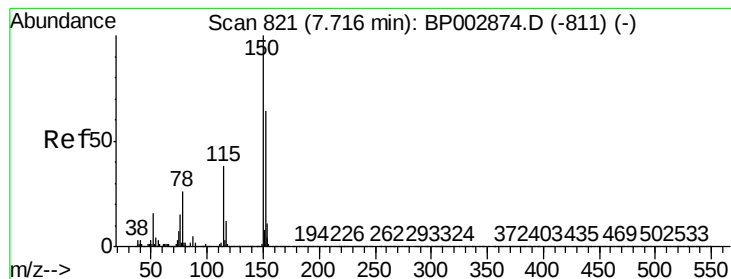


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.72 min Scan# 821
Delta R.T. -0.00 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Instrument :
BNA_P
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.4	124.8	187.2
115	57.2	47.4	71.2




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

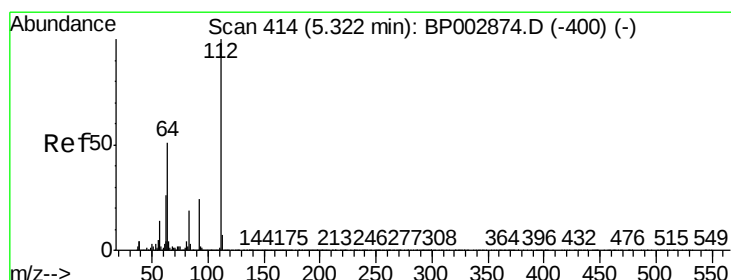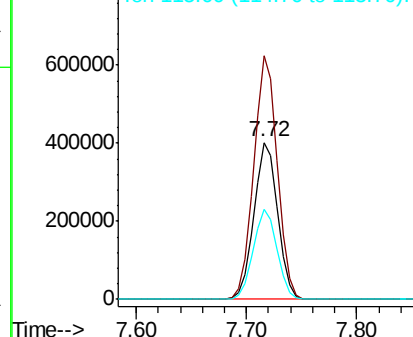



#5


2-Fluorophenol
Concen: 116.911 ng
RT: 5.33 min Scan# 415
Delta R.T. 0.01 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Tgt Ion	Ratio	Lower	Upper
112	100		
64	50.4	41.0	61.6
63	25.6	20.7	31.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

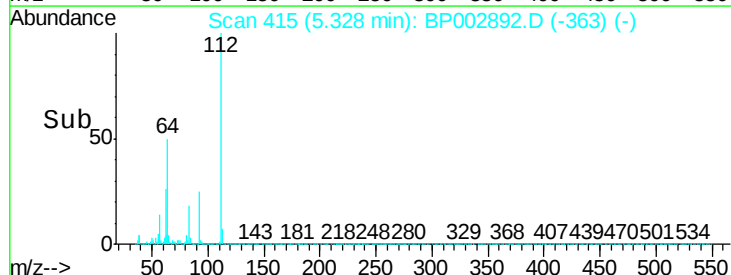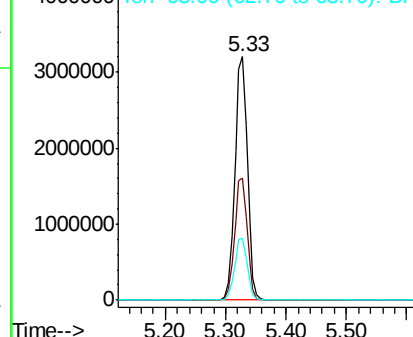

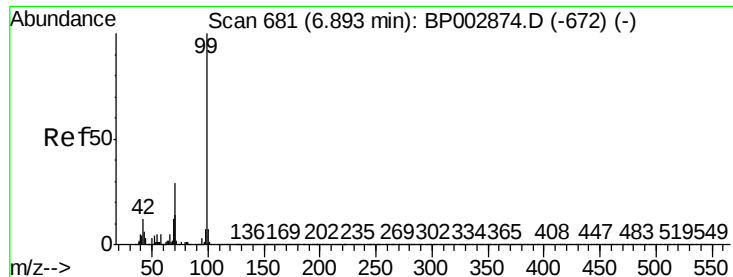

#7

Phenol-d6

Concen: 105.927 ng

RT: 6.89 min Scan# 681

Delta R.T. -0.00 min

Lab File: BP002892.D

Acq: 31 Jul 2020 14:08





Instrument :

BNA_P

ClientSampleId :

Tot Ion: 99 Resp: 5805888

Ion	Ratio	Lower	Upper
99	100		
42	11.8	9.3	13.9
71	30.3	23.5	35.3

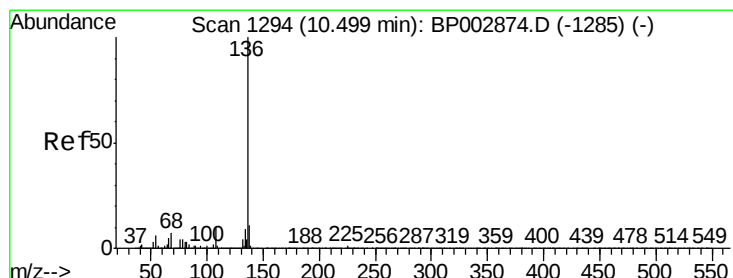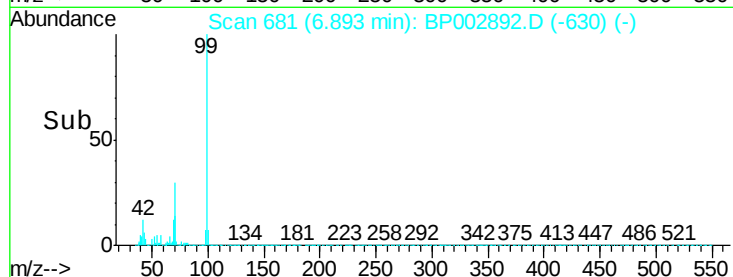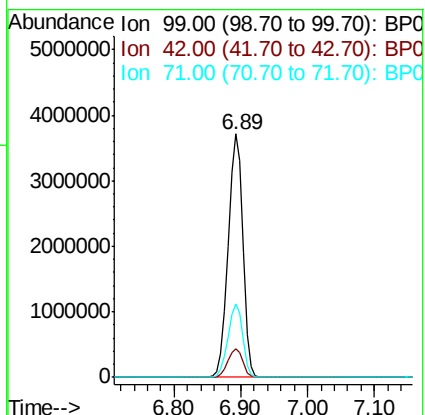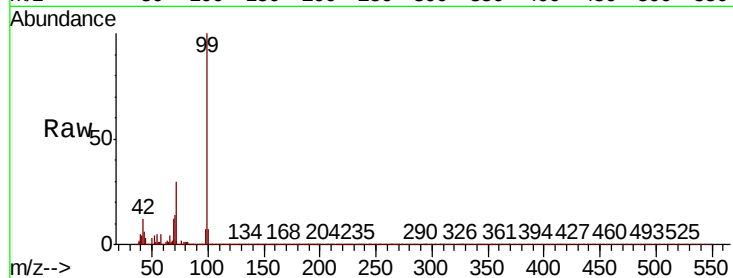

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.50 min Scan# 1294




Delta R.T. -0.00 min

Lab File: BP002892.D

Acq: 31 Jul 2020 14:08

Tgt Ion: 136 Resp: 2331746

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.6	13.0
54	6.0	5.1	7.7
68	6.2	5.3	7.9


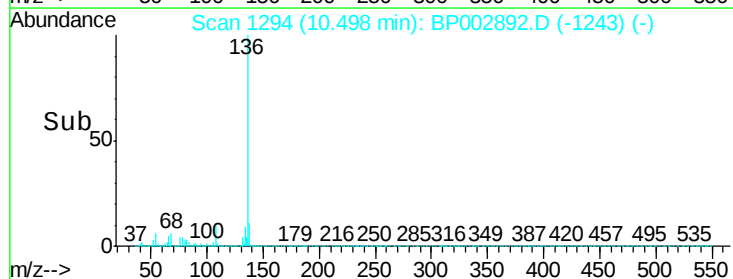
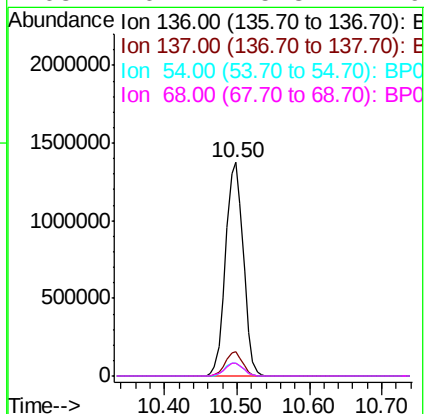
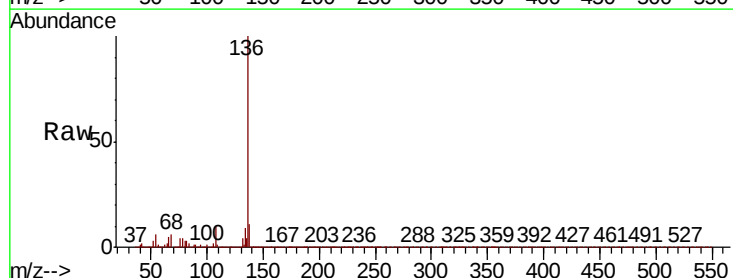




#23
Nitrobenzene-d5
Concen: 82.303 ng
RT: 8.86 min Scan# 1016
Delta R.T. -0.00 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08




Instrument :
BNA_P
ClientSampled :


Tot Ion: 82 Resp: 3543239
Ion Ratio Lower Upper
82 100
128 44.8 34.6 52.0
54 36.8 29.5 44.3

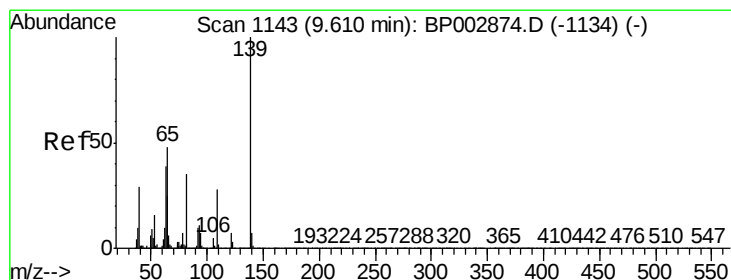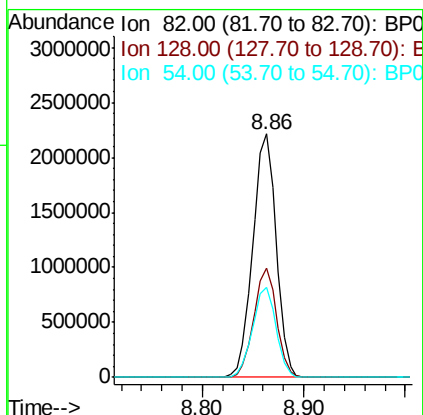

#26
2-Nitrophenol
Concen: 4.521 ng
RT: 9.61 min Scan# 1143
Delta R.T. 0.00 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Tgt Ion:139 Resp: 19
Ion Ratio Lower Upper
139 100
109 354.5 22.2 33.2#
65 795.5 38.9 58.3#



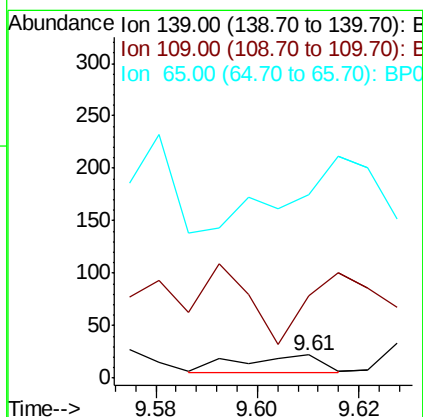
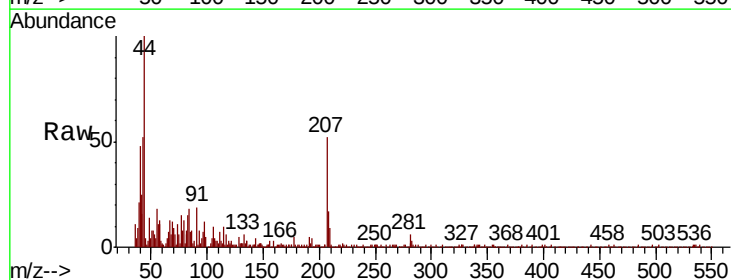


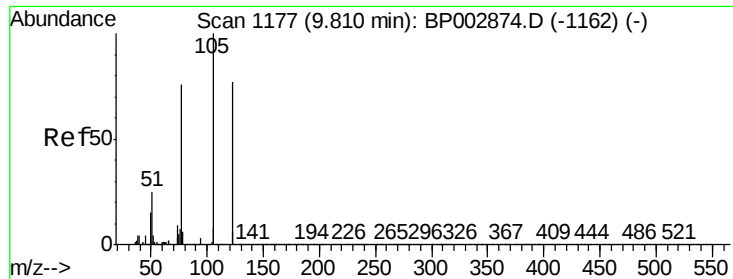

#32
Benzoic acid
Concen: 7.687 ng
RT: 9.80 min Scan# 1176
Delta R.T. -0.01 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08




Instrument :
BNA_P
ClientSampled :


Tot Ion	Ratio	Lower	Upper
122	100		
105	333.0	103.4	143.4#
77	323.4	74.6	114.6#

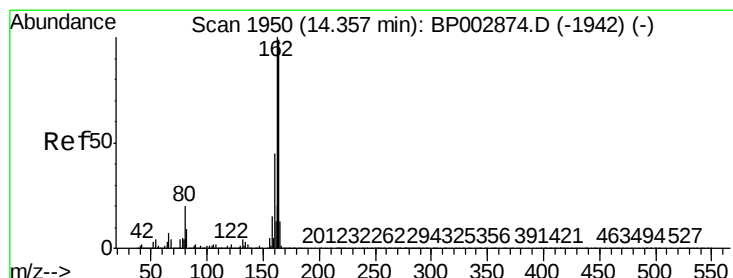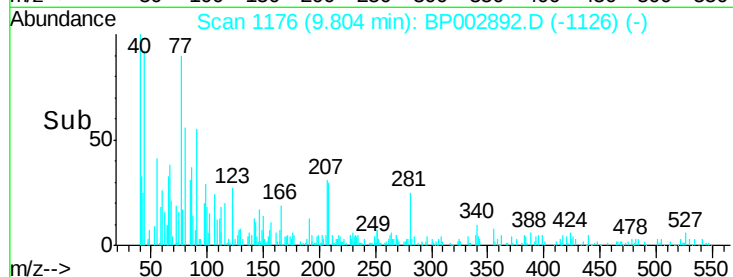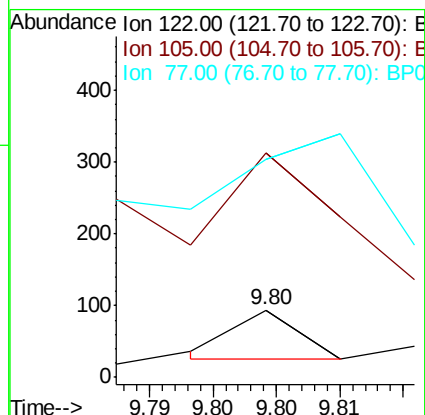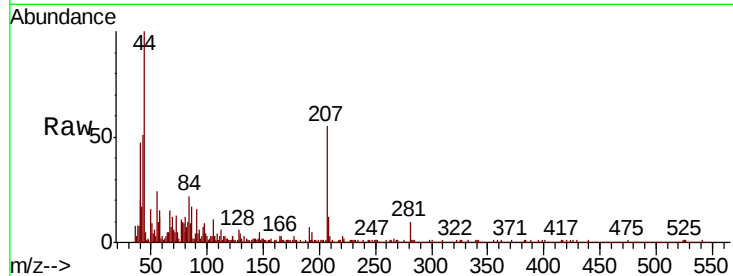

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.35 min Scan# 1949
Delta R.T. -0.01 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.7	81.0	121.6
160	45.5	36.2	54.4


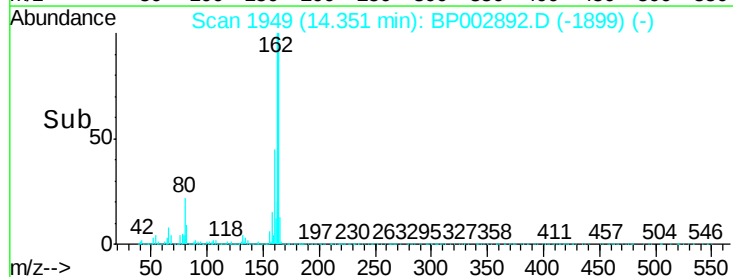
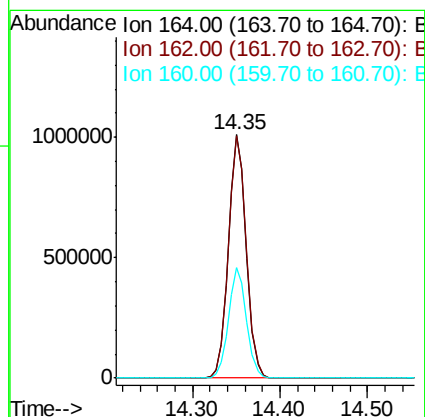
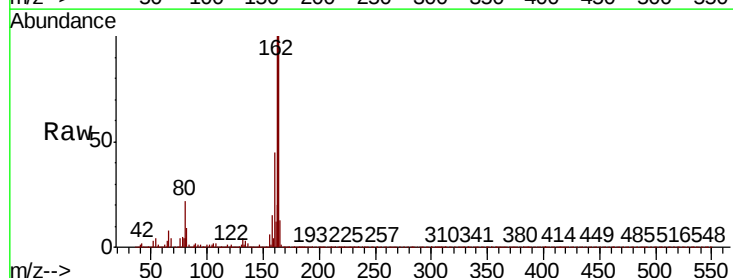


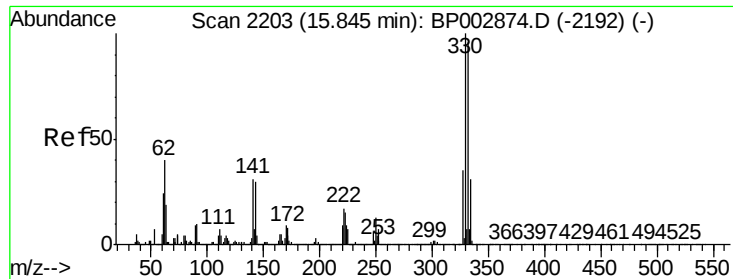

#42
2,4,6-Tribromophenol
Concen: 120.617 ng
RT: 15.84 min Scan# 2203
Delta R.T. -0.00 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08




Instrument :
BNA_P
ClientSampleId :


Tot Ion:330 Resp: 2113709
Ion Ratio Lower Upper
330 100
332 96.2 77.1 115.7
141 29.3 24.6 37.0

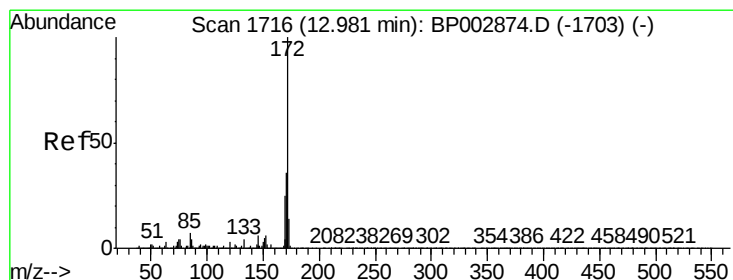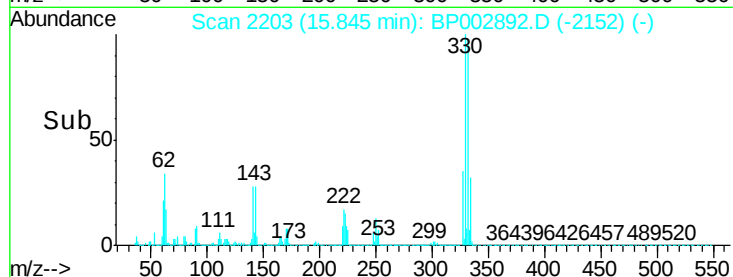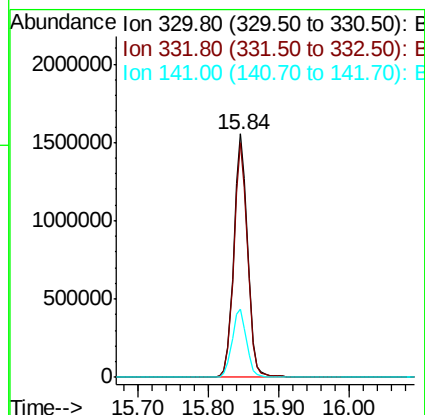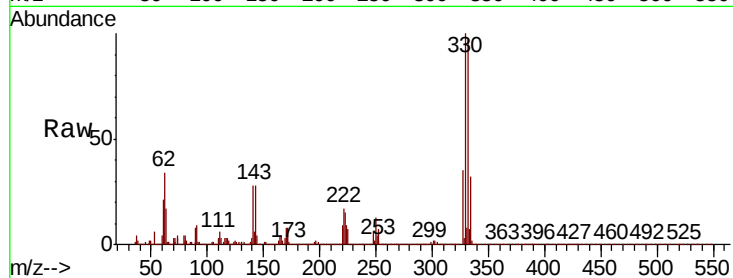

#45
2-Fluorobiphenyl
Concen: 76.059 ng
RT: 12.97 min Scan# 1715
Delta R.T. -0.01 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Tgt Ion:172 Resp: 7848901
Ion Ratio Lower Upper
172 100
171 37.0 29.1 43.7
170 25.0 19.6 29.4

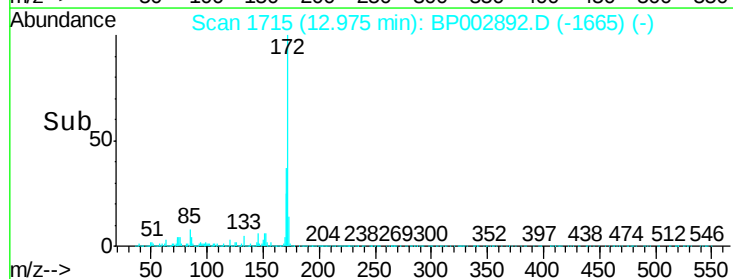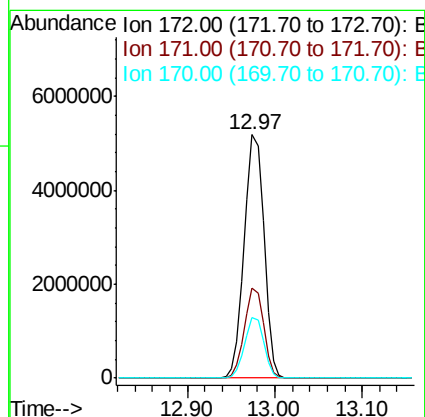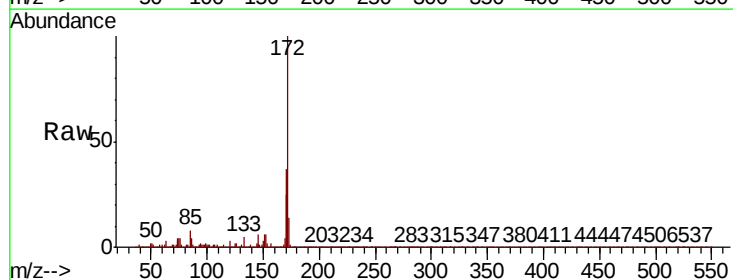

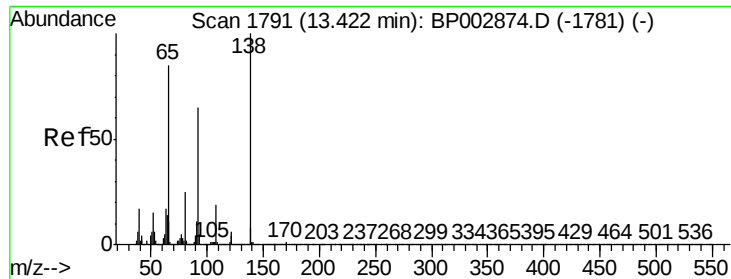

#48

2-Nitroaniline

Concen: 3.975 ng

RT: 13.41 min Scan# 1789

Delta R.T. -0.01 min

Lab File: BP002892.D

Acq: 31 Jul 2020 14:08

Instrument :

BNA_P

ClientSampleId :





Tot Ion: 65 Resp: 82

Ion Ratio Lower Upper

65 100

92 70.2 61.4 92.0

138 19.4 94.2 141.4#

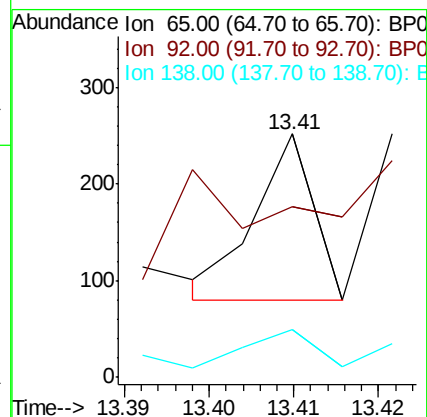

#51

2,6-Dinitrotoluene

Concen: 2.901 ng

RT: 13.91 min Scan# 1874

Delta R.T. -0.01 min

Lab File: BP002892.D

Acq: 31 Jul 2020 14:08




Tgt Ion: 165 Resp: 49


Ion Ratio Lower Upper

165 100

63 130.5 40.3 60.5#

89 112.2 46.5 69.7#



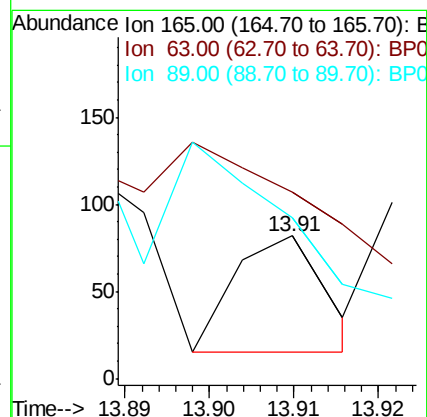



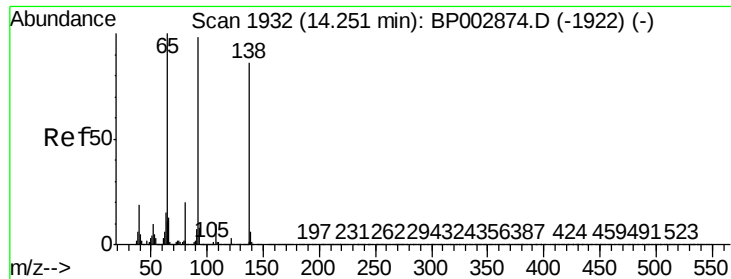

#53
3-Nitroaniline
Concen: 3.276 ng
RT: 14.26 min Scan# 1934
Delta R.T. 0.01 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08




Instrument :
BNA_P
ClientSampleId :


Tot Ion:138 Resp: 83
Ion Ratio Lower Upper
138 100
108 140.6 9.4 14.0#
92 634.4 91.0 136.6#

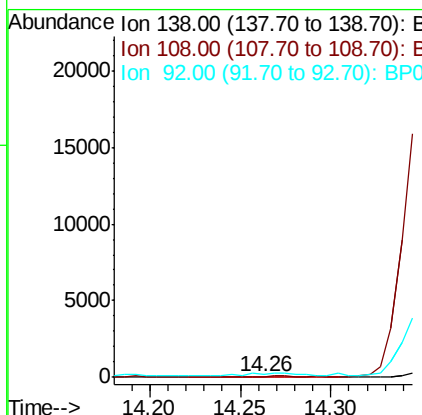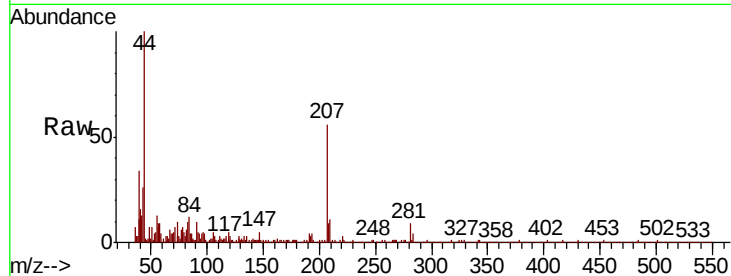

#54
2,4-Dinitrophenol
Concen: 8.059 ng
RT: 14.43 min Scan# 1963
Delta R.T. -0.02 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Tgt Ion:184 Resp: 16
Ion Ratio Lower Upper
184 100
63 323.1 50.3 75.5#
154 438.5 50.6 76.0#

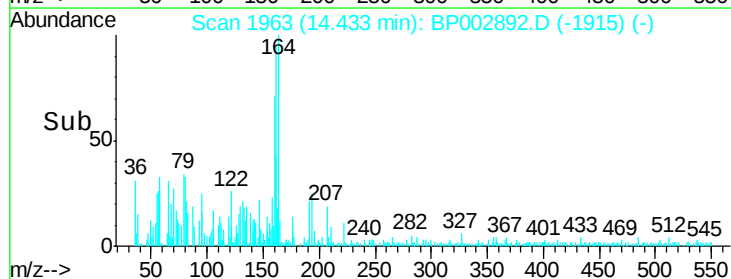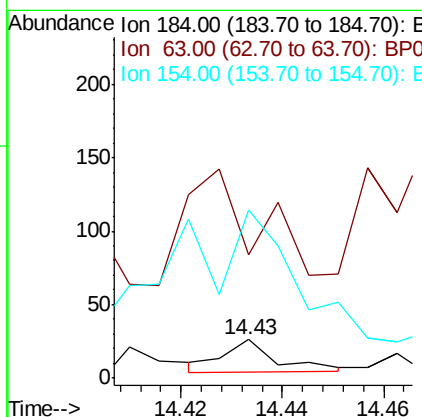

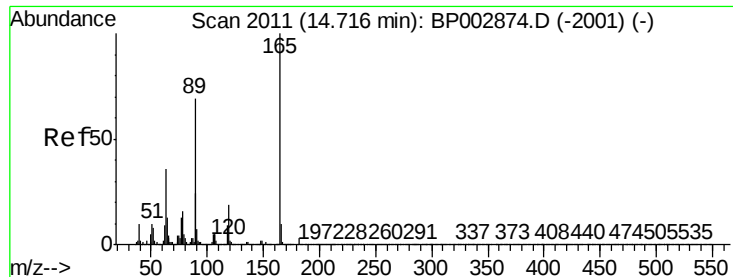

#57

2,4-Dinitrotoluene

Concen: 3.809 ng

RT: 14.70 min Scan# 2008

Delta R.T. -0.02 min

Lab File: BP002892.D





Acq: 31 Jul 2020 14:08

Instrument :

BNA_P

ClientSampled :

Tot Ion:	165	Resp:	129
Ion	Ratio	Lower	Upper
165	100		
63	72.4	29.0	43.4#
89	88.8	55.5	83.3#
182	1.7	2.2	3.4#

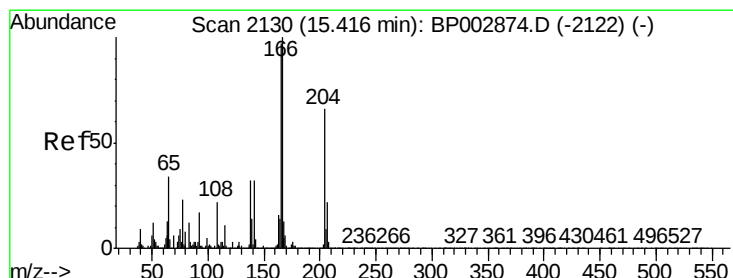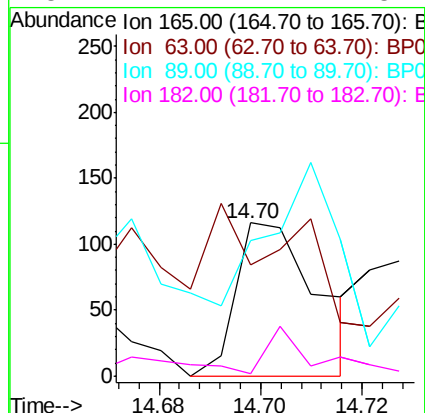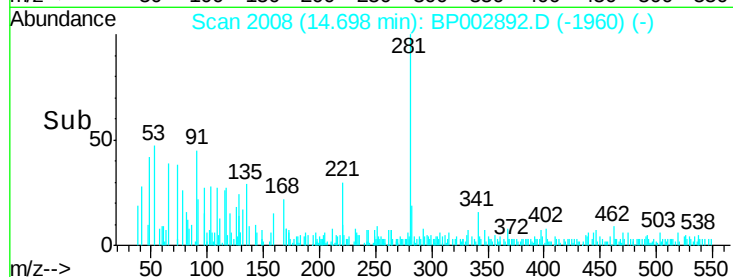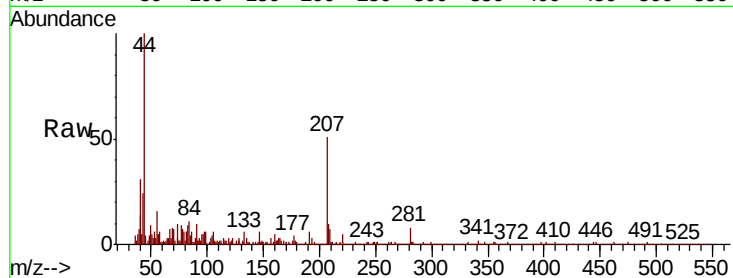

#62

4-Nitroaniline

Concen: 2.423 ng




RT: 15.38 min Scan# 2124


Delta R.T. -0.03 min

Lab File: BP002892.D

Acq: 31 Jul 2020 14:08

Tgt Ion:	138	Resp:	176
Ion	Ratio	Lower	Upper
138	100		
92	55.1	32.2	72.2
108	31.4	50.0	90.0#

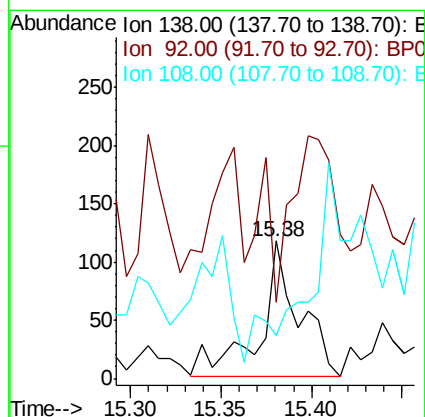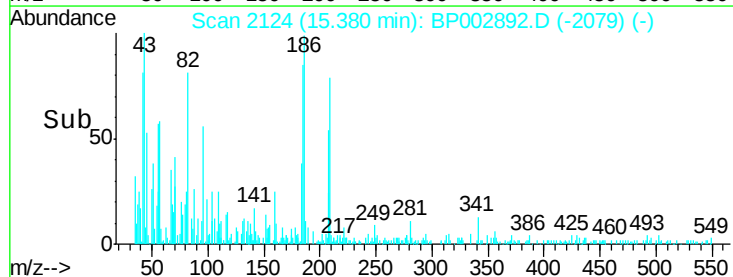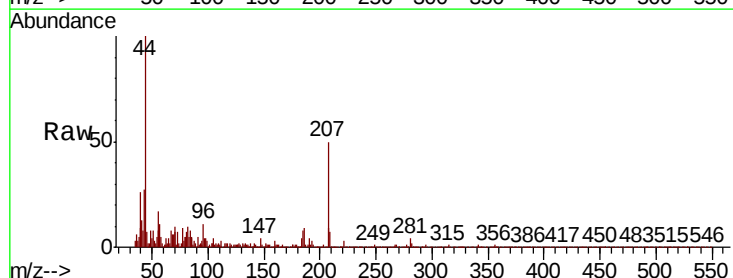



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.10 min Scan# 2417

Delta R.T. -0.01 min

Lab File: BP002892.D

Acq: 31 Jul 2020 14:08

Instrument :

BNA_P

ClientSampled :


Tot Ion:188 Resp: 2984622

Ion Ratio Lower Upper

188 100

94 9.7 7.8 11.6




80 10.3 8.0 12.0



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

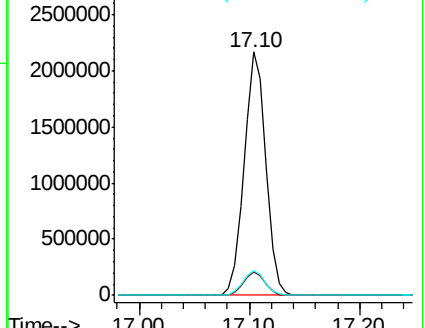

#65

4,6-Dinitro-2-methylphenol

Concen: 6.901 ng

RT: 15.48 min Scan# 2141

Delta R.T. 0.00 min

Lab File: BP002892.D

Acq: 31 Jul 2020 14:08


Tgt Ion:198 Resp: 10

Ion Ratio Lower Upper

198 100

51 920.0 11.6 51.6#



105 835.0 23.8 63.8#




Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BP0

Ion 105.00 (104.70 to 105.70): E




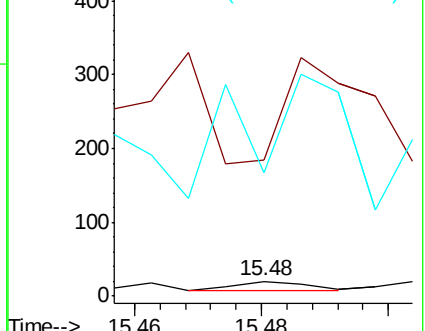


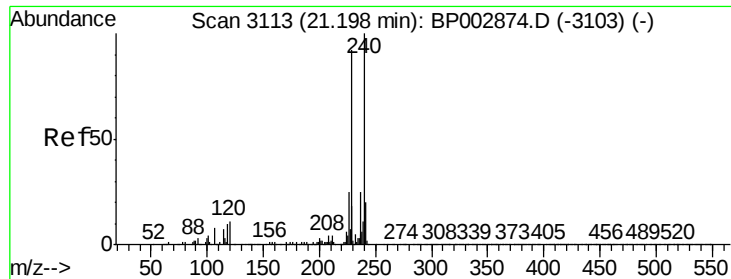

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.20 min Scan# 3113
Delta R.T. -0.00 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08




Instrument :
BNA_P
ClientSampleId :


Tot Ion:240 Resp: 2463558
Ion Ratio Lower Upper
240 100
120 10.4 8.9 13.3
236 26.1 20.3 30.5

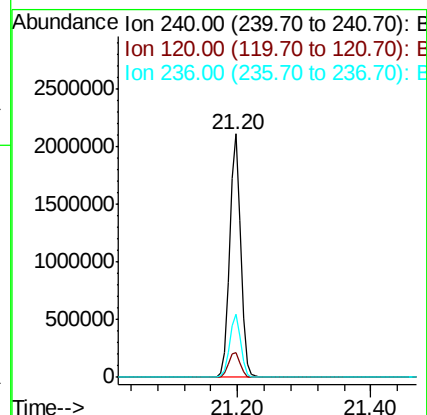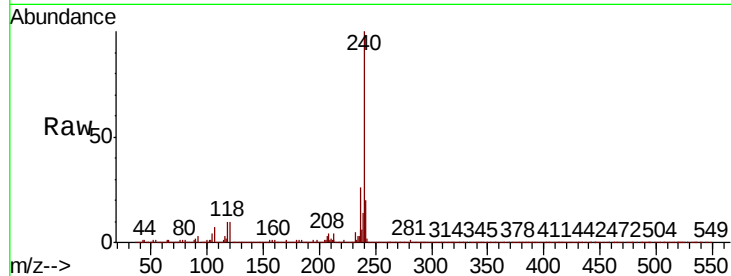

#79
Terphenyl-d14
Concen: 78.890 ng
RT: 19.69 min Scan# 2856
Delta R.T. -0.00 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Tgt Ion:244 Resp: 9708048
Ion Ratio Lower Upper
244 100
212 8.3 6.4 9.6
122 11.4 9.4 14.2

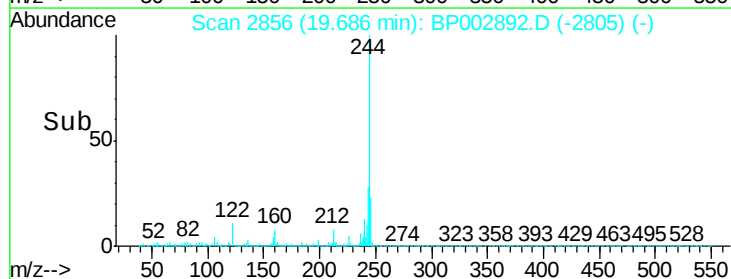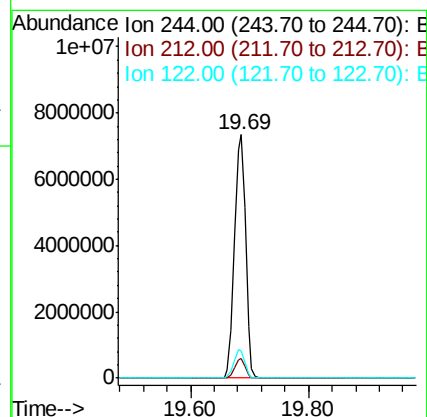







#80
Butylbenzylphthalate
Concen: 3.063 ng
RT: 20.39 min Scan# 2975
Delta R.T. 0.02 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Instrument :
BNA_P
ClientSampled :

Tot Ion:149 Resp: 413
Ion Ratio Lower Upper
149 100
91 132.8 60.5 90.7#
206 30.7 17.5 26.3#




Abundance Ion 149.00 (148.70 to 149.70): E
Ion 91.00 (90.70 to 91.70): BP0
Ion 206.00 (205.70 to 206.70): E

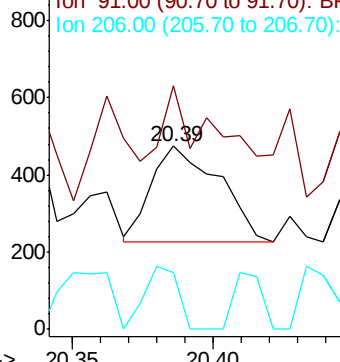

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.46 min Scan# 3498
Delta R.T. -0.01 min
Lab File: BP002892.D
Acq: 31 Jul 2020 14:08

Tgt Ion:264 Resp: 2052514
Ion Ratio Lower Upper
264 100
260 24.2 19.0 28.6
265 22.2 17.0 25.4



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

