

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
 Data File : BP002901.D
 Acq On : 31 Jul 2020 19:59
 Operator : CG/JU
 Sample : L3518-38
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-11

Quant Time: Jul 31 23:20:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 15:30:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	559562	20.00	ng	0.00
21) Naphthalene-d8	10.50	136	2173485	20.00	ng	0.00
39) Acenaphthene-d10	14.35	164	1255275	20.00	ng	0.00
64) Phenanthrene-d10	17.10	188	2526054	20.00	ng	0.00
76) Chrysene-d12	21.20	240	1989655	20.00	ng	0.00
86) Perylene-d12	23.46	264	1764625	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.33	112	3897103	106.59	ng	0.00
7) Phenol-d6	6.89	99	4390501	86.50	ng	0.00
23) Nitrobenzene-d5	8.86	82	3427365	85.41	ng	0.00
42) 2,4,6-Tribromophenol	15.85	330	1930407	123.73	ng	0.00
45) 2-Fluorobiphenyl	12.97	172	6837438	74.42	ng	0.00
79) Terphenyl-d14	19.68	244	8912613	89.68	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.02	88	66211	4.219	ng	# 1
26) 2-Nitrophenol	9.60	139	101	4.526	ng	# 1
32) Benzoic acid	9.85	122	196	7.694	ng	# 80
48) 2-Nitroaniline	13.42	65	73	3.975	ng	# 46
51) 2,6-Dinitrotoluene	13.90	165	302	2.912	ng	# 39
53) 3-Nitroaniline	14.26	138	69	3.276	ng	# 1
54) 2,4-Dinitrophenol	14.46	184	70	8.064	ng	# 1
57) 2,4-Dinitrotoluene	14.73	165	333	3.816	ng	# 8
62) 4-Nitroaniline	15.40	138	421	2.434	ng	# 85
65) 4,6-Dinitro-2-methylphenol	15.47	198	34	6.902	ng	# 1
80) Butylbenzylphthalate	20.37	149	986	3.074	ng	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
Data File : BP002901.D
Acq On : 31 Jul 2020 19:59
Operator : CG/JU
Sample : L3518-38
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-11

Quant Time: Jul 31 23:20:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 15:30:34 2020
Response via : Initial Calibration

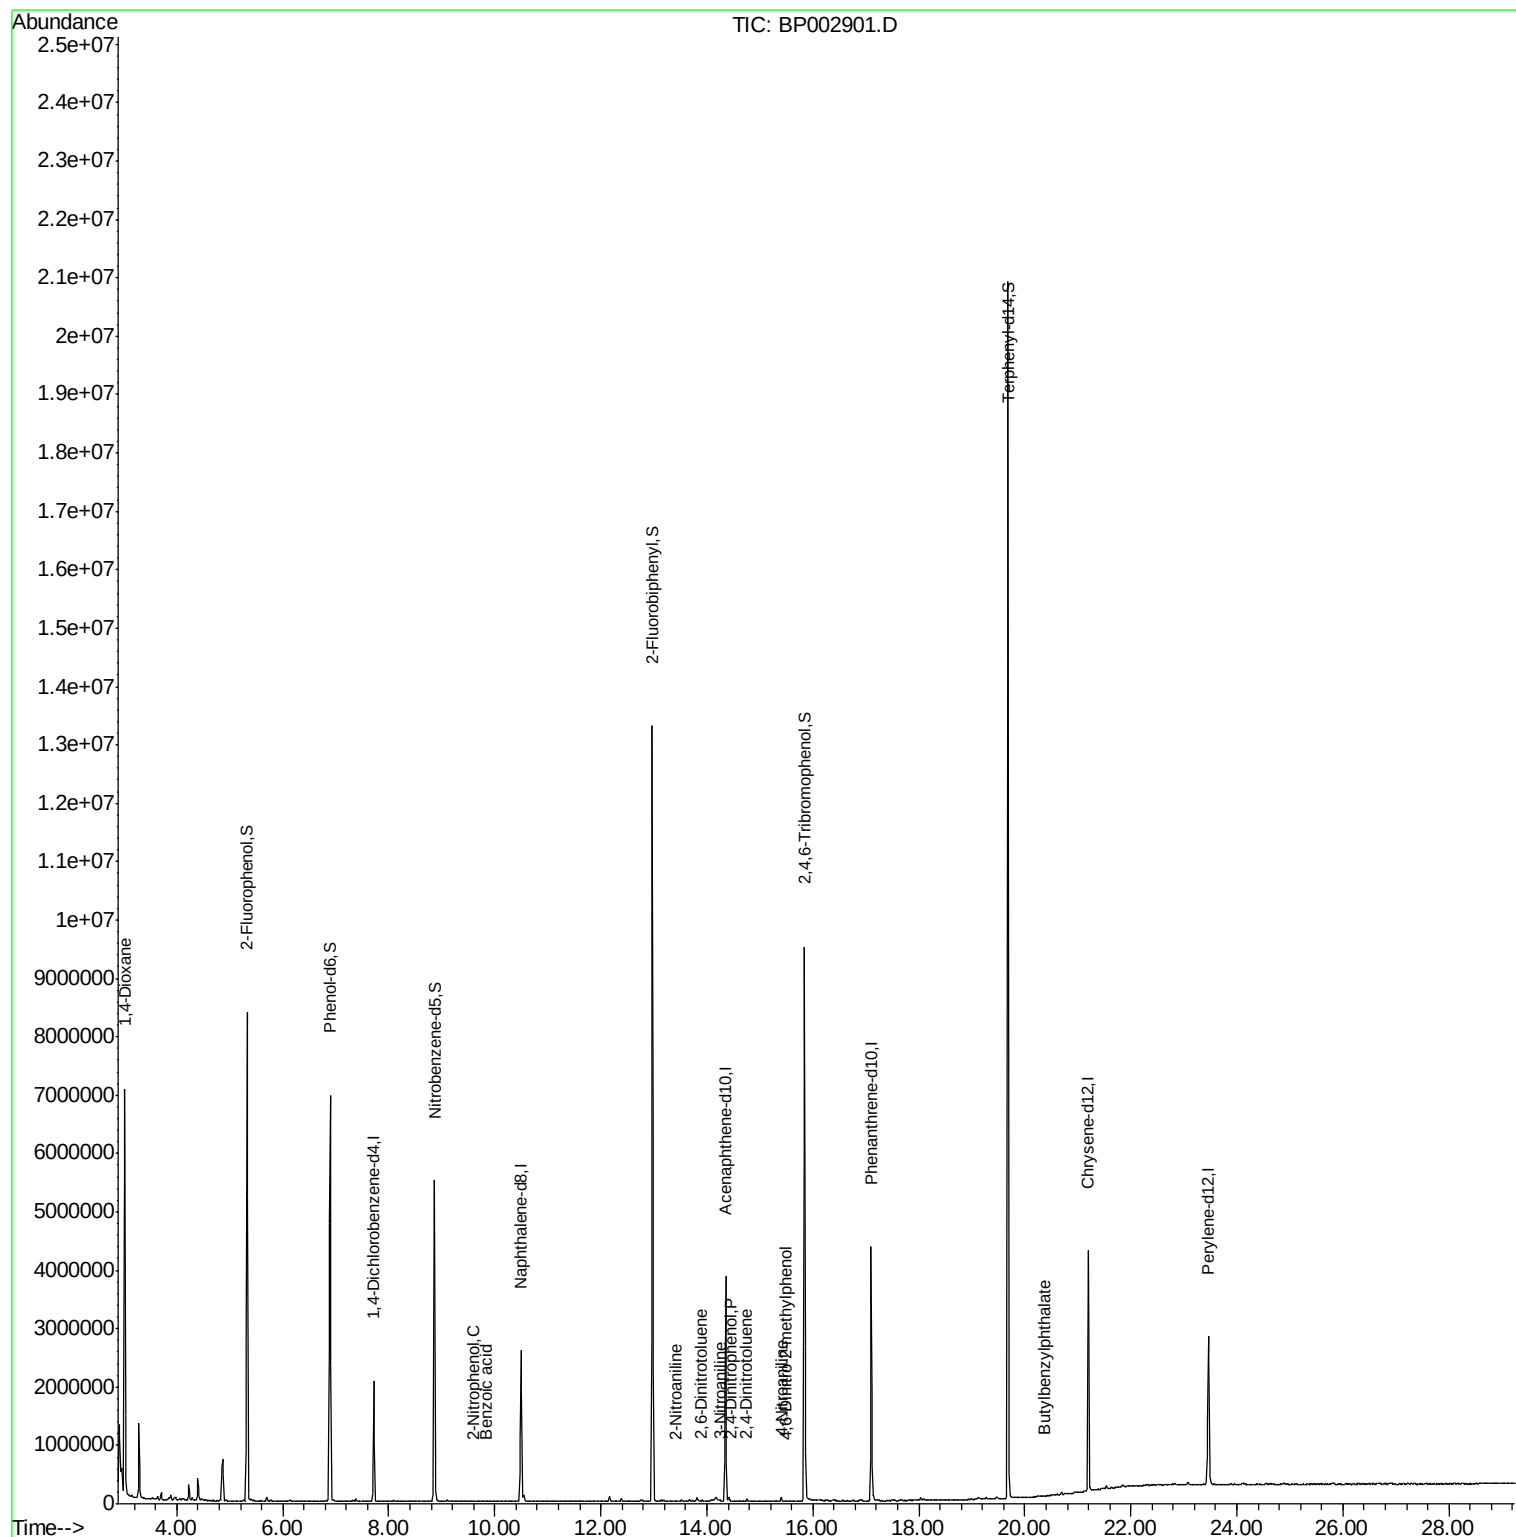







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.72 min Scan# 821
Delta R.T. 0.00 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59

Instrument :
BNA_P
ClientSampleId :
TP-11




Tot Ion	Ratio	Lower	Upper
152	100		
150	156.3	124.8	187.2
115	58.2	47.4	71.2

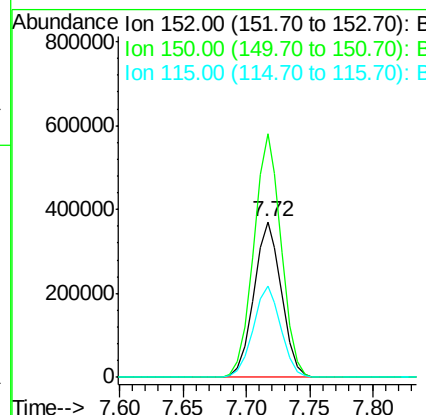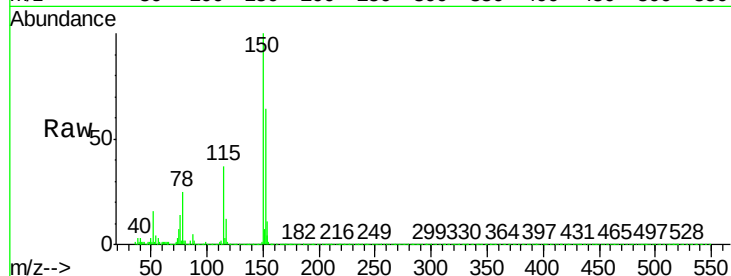


#2

1,4-Dioxane
Concen: 4.219 ng
RT: 3.02 min Scan# 22
Delta R.T. -0.26 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59

Tgt Ion	Ratio	Lower	Upper
88	100		
58	25.4	47.4	71.0#
43	1741.2	15.2	22.8#

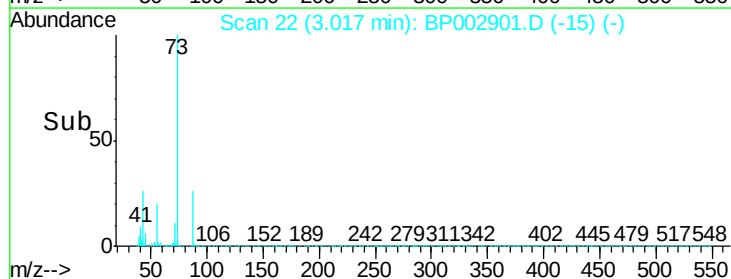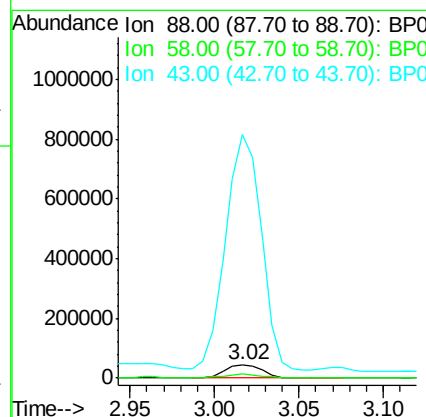



#5

2-Fluorophenol

Concen: 106.592 ng

RT: 5.33 min Scan# 415

Delta R.T. 0.01 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59

Instrument :

BNA_P

ClientSampleId :

TP-11


Tot Ion:112 Resp: 3897103

Ion Ratio Lower Upper

112 100

64 49.5 41.0 61.6




63 25.3 20.7 31.1



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

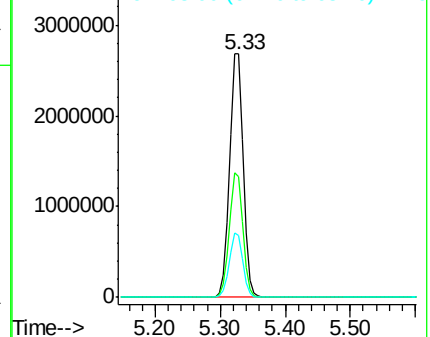

#7

Phenol-d6

Concen: 86.495 ng

RT: 6.89 min Scan# 681

Delta R.T. 0.00 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59


Tgt Ion: 99 Resp: 4390501

Ion Ratio Lower Upper

99 100

42 11.6 9.3 13.9



71 29.7 23.5 35.3




Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0




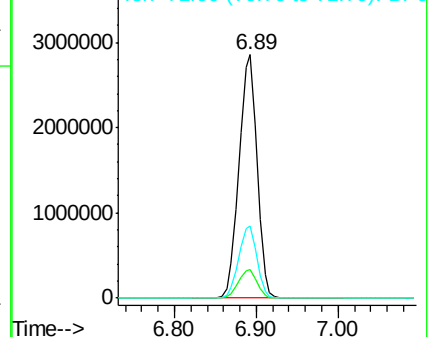




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.50 min Scan# 1294
Delta R.T. 0.00 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59




Instrument :
BNA_P
ClientSampleId :
TP-11


Tot Ion:136	Resp: 2173485
Ion Ratio	Lower Upper
136 100	
137 10.8	8.6 13.0
54 6.1	5.1 7.7
68 6.3	5.3 7.9

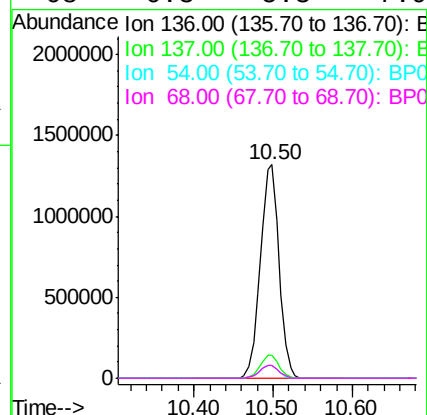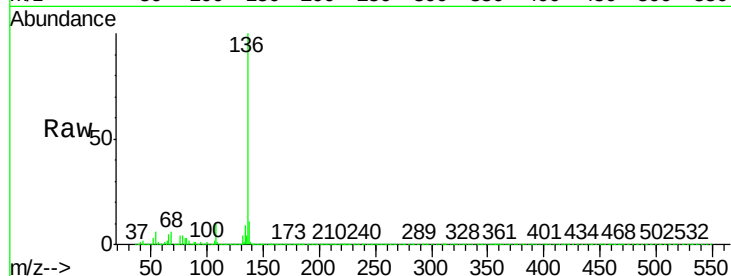

#23
Nitrobenzene-d5
Concen: 85.409 ng
RT: 8.86 min Scan# 1016
Delta R.T. 0.00 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59

Tgt Ion: 82	Resp: 3427365
Ion Ratio	Lower Upper
82 100	
128 44.4	34.6 52.0
54 36.1	29.5 44.3


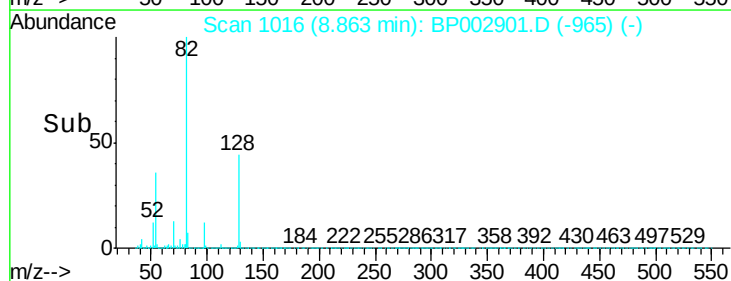
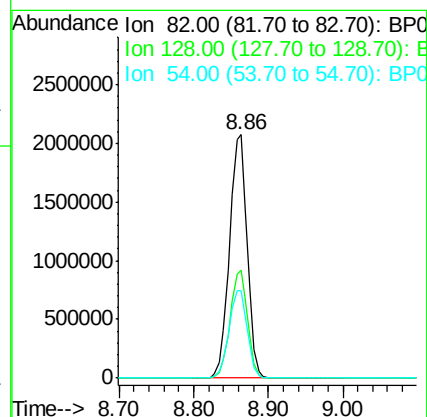



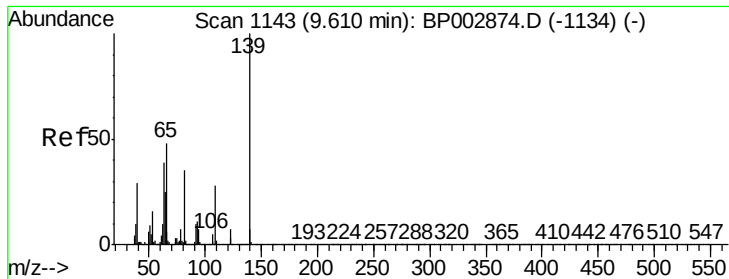

#26
2-Nitrophenol
Concen: 4.526 ng
RT: 9.60 min Scan# 1142
Delta R.T. -0.01 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59




Instrument :
BNA_P
ClientSampled :
TP-11


Tot Ion	Ratio	Lower	Upper
139	100		
109	92.3	22.2	33.2#
65	129.0	38.9	58.3#

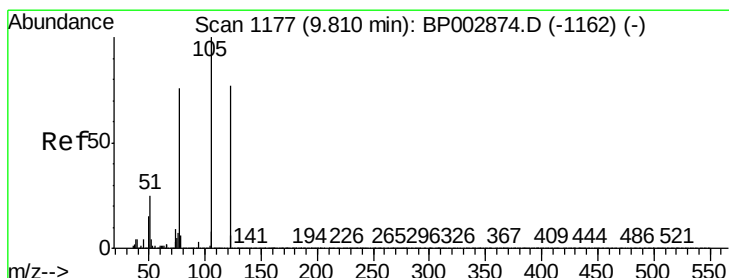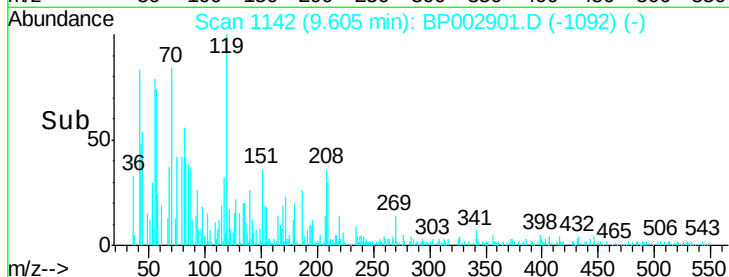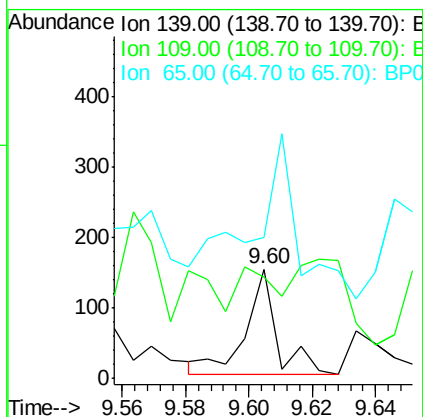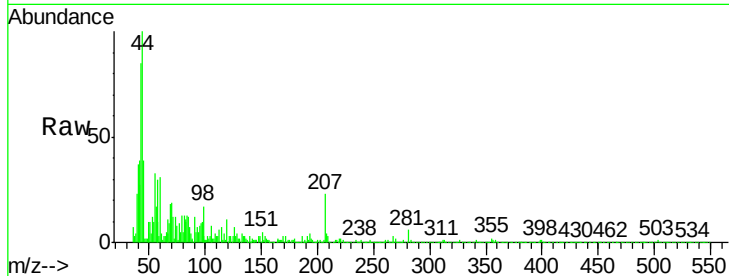

#32
Benzoic acid
Concen: 7.694 ng
RT: 9.85 min Scan# 1183
Delta R.T. 0.04 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59

Tgt Ion	Ratio	Lower	Upper
122	100		
105	116.5	103.4	143.4
77	132.1	74.6	114.6#

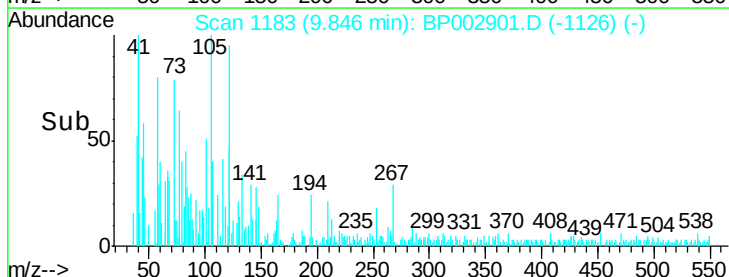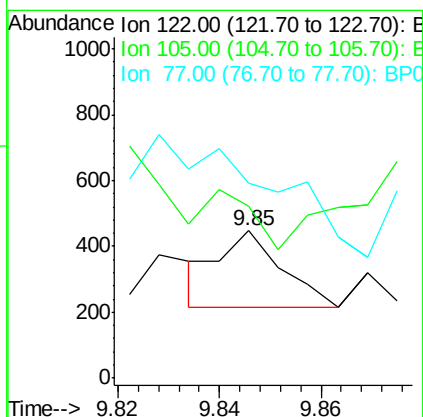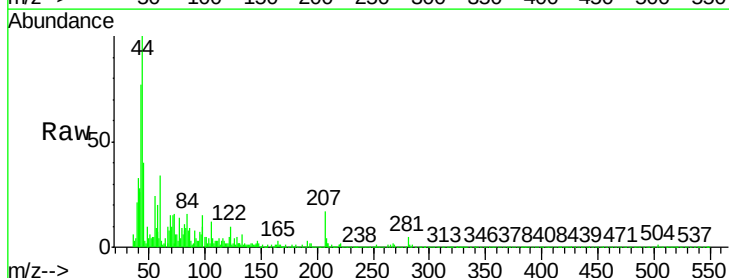

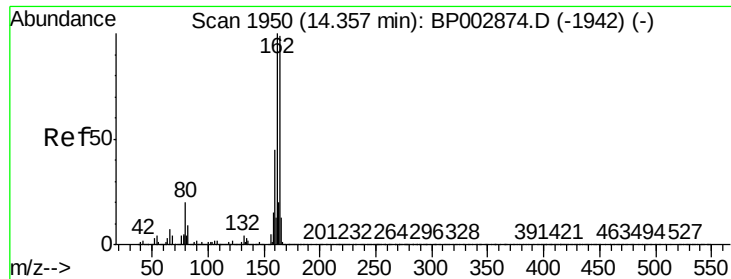

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.35 min Scan# 1949

Delta R.T. -0.01 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59

Instrument :

BNA_P

ClientSampleId :

TP-11


Tot Ion:164 Resp: 1255275

Ion Ratio Lower Upper

164 100

162 99.2 81.0 121.6




160 45.2 36.2 54.4

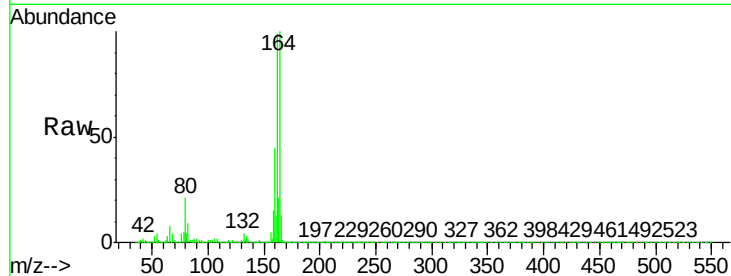

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

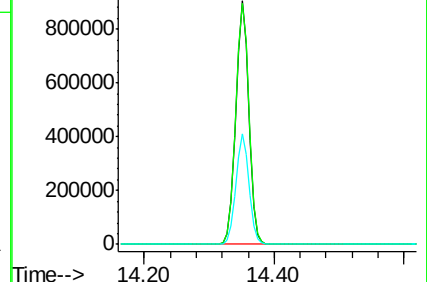

#42

2,4,6-Tribromophenol

Concen: 123.731 ng

RT: 15.85 min Scan# 2203

Delta R.T. 0.00 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59


Tgt Ion:330 Resp: 1930407

Ion Ratio Lower Upper

330 100

332 96.5 77.1 115.7



141 29.7 24.6 37.0




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



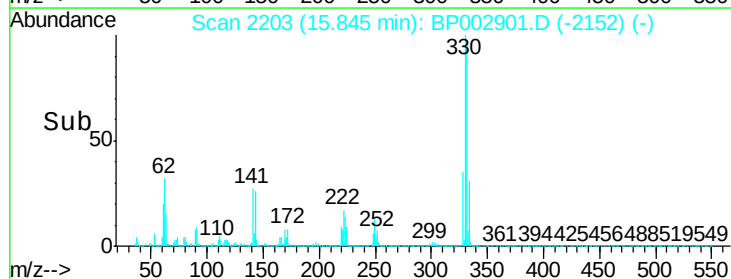
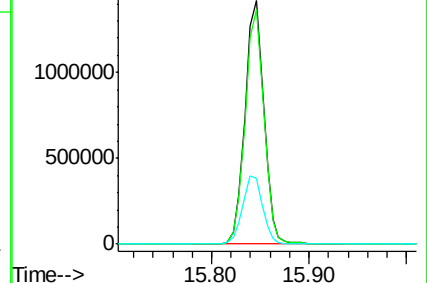


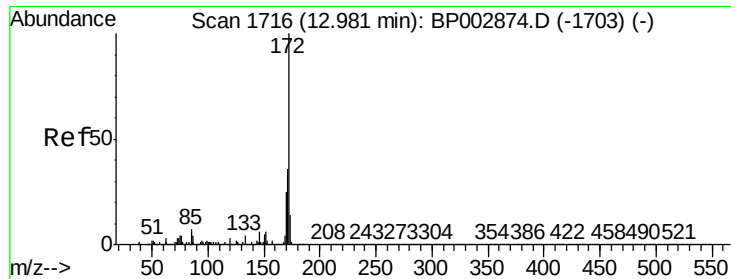

#45
2-Fluorobiphenyl
Concen: 74.422 ng
RT: 12.97 min Scan# 1715
Delta R.T. -0.01 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59




Instrument :
BNA_P
ClientSampleId :
TP-11


Tot Ion:172 Resp: 6837438
Ion Ratio Lower Upper
172 100
171 36.5 29.1 43.7
170 24.7 19.6 29.4

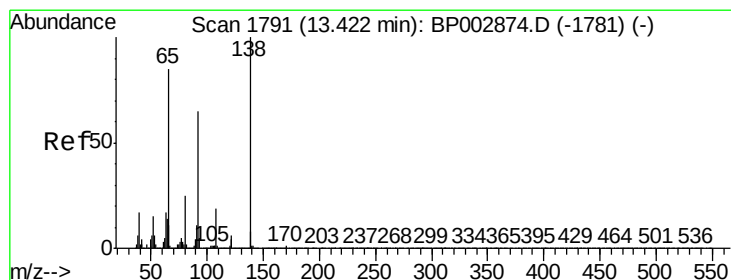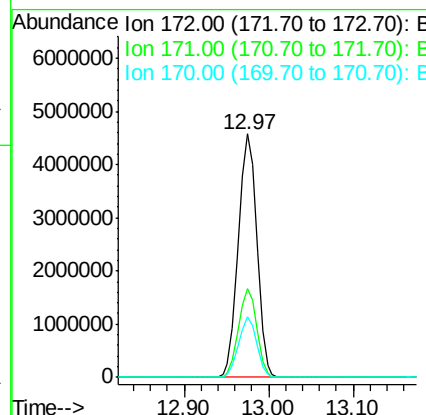

#48
2-Nitroaniline
Concen: 3.975 ng
RT: 13.42 min Scan# 1791
Delta R.T. 0.00 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59

Tgt Ion: 65 Resp: 73
Ion Ratio Lower Upper
65 100
92 63.0 61.4 92.0
138 32.1 94.2 141.4#

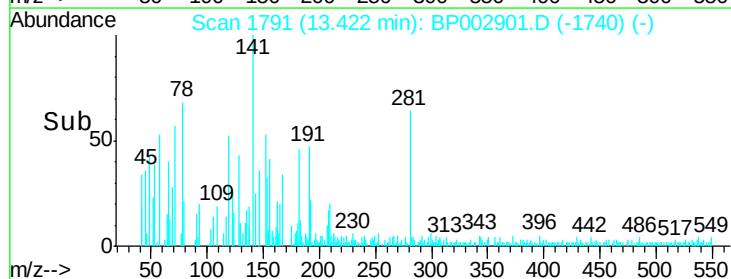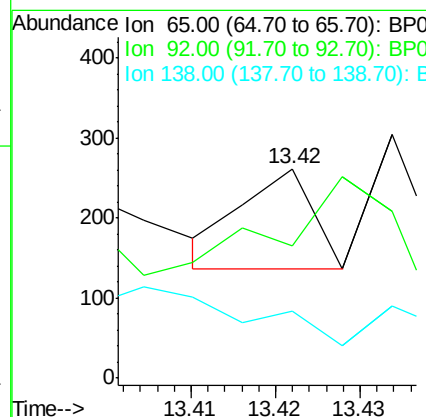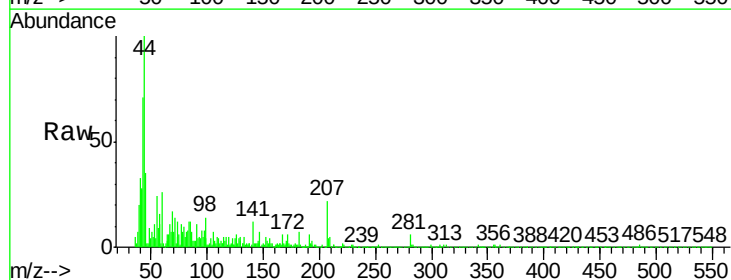

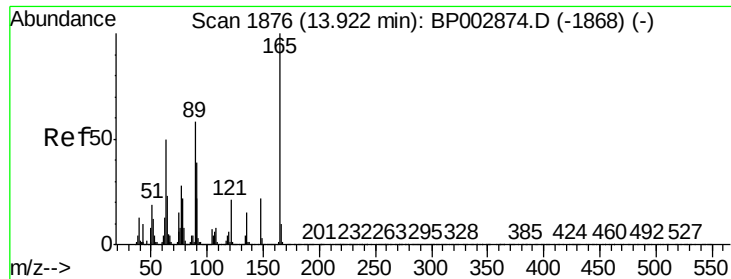

#51

2,6-Dinitrotoluene

Concen: 2.912 ng

RT: 13.90 min Scan# 1872

Delta R.T. -0.02 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59





Instrument :

BNA_P

ClientSampled :

TP-11

Tot Ion:165	Resp:	302
Ion Ratio	Lower	Upper
165	100	
63	90.5	40.3 60.5#
89	105.4	46.5 69.7#

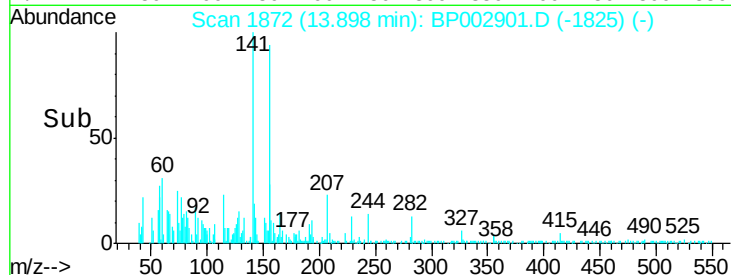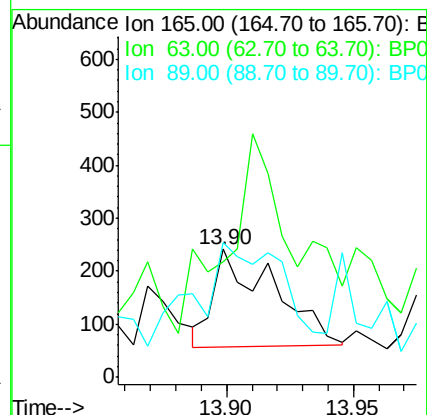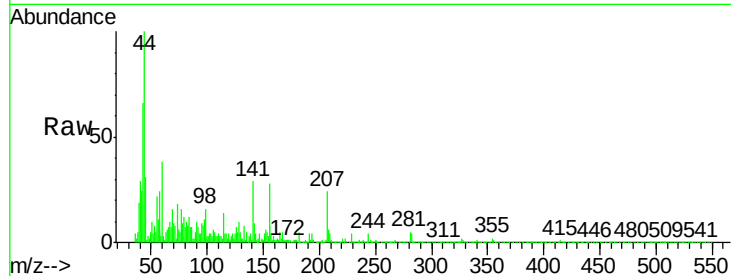

#53

3-Nitroaniline

Concen: 3.276 ng




RT: 14.26 min Scan# 1934


Delta R.T. 0.01 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59

Tgt Ion:138	Resp:	69
Ion Ratio	Lower	Upper
138	100	
108	129.8	9.4 14.0#
92	209.5	91.0 136.6#



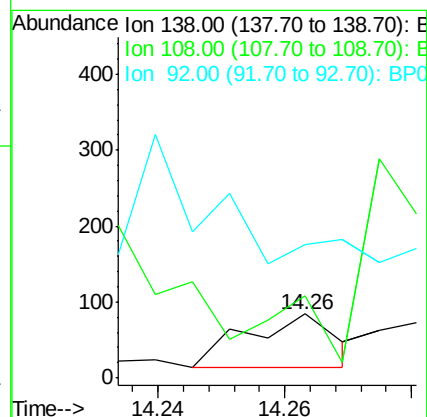



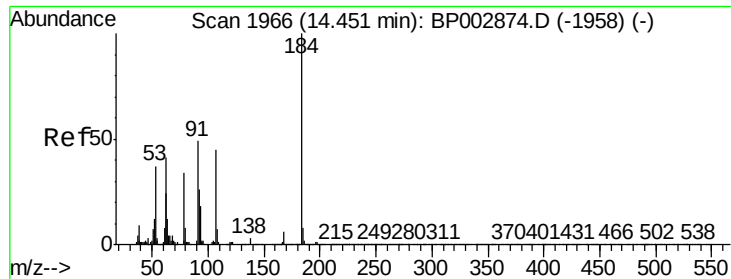

#54
2,4-Dinitrophenol
Concen: 8.064 ng
RT: 14.46 min Scan# 1968
Delta R.T. 0.01 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59




Instrument :
BNA_P
ClientSampleId :
TP-11


Tot Ion:184 Resp: 70
Ion Ratio Lower Upper
184 100
63 350.8 50.3 75.5#
154 212.3 50.6 76.0#

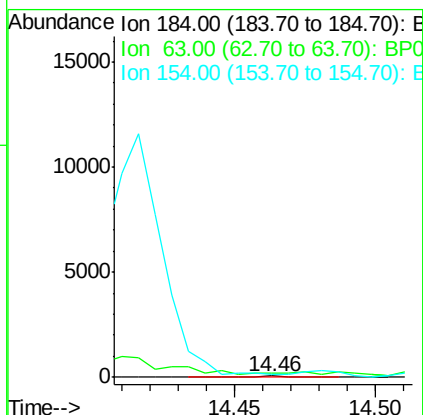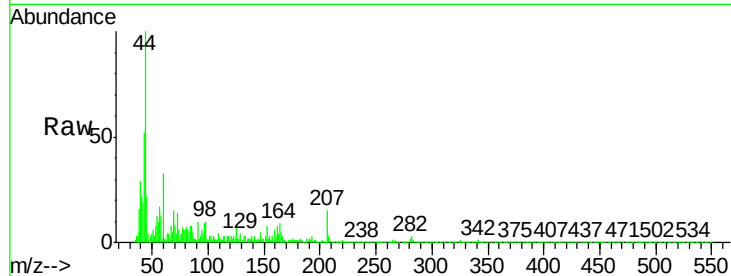

#57
2,4-Dinitrotoluene
Concen: 3.816 ng
RT: 14.73 min Scan# 2014
Delta R.T. 0.02 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59

Tgt Ion:165 Resp: 333
Ion Ratio Lower Upper
165 100
63 152.4 29.0 43.4#
89 94.8 55.5 83.3#
182 80.3 2.2 3.4#

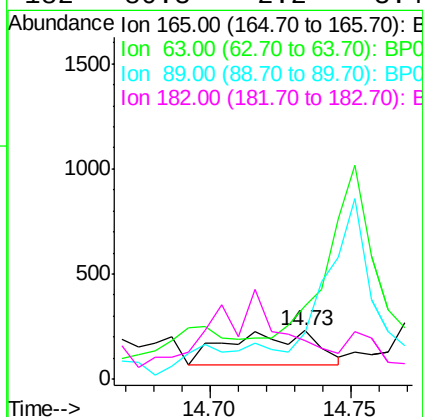



#62

4-Nitroaniline

Concen: 2.434 ng

RT: 15.40 min Scan# 2128

Delta R.T. -0.01 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59

Instrument :

BNA_P

ClientSampled :

TP-11


Tot Ion:138 Resp: 421

Ion Ratio Lower Upper

138 100

92 55.7 32.2 72.2

108 51.8 50.0 90.0




Abundance Ion 138.00 (137.70 to 138.70): E


Ion 92.00 (91.70 to 92.70): BP0

Ion 108.00 (107.70 to 108.70): E

Time-->



Time-->



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.10 min Scan# 2417

Delta R.T. -0.01 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59


Tgt Ion:188 Resp: 2526054

Ion Ratio Lower Upper

188 100

94 10.0 7.8 11.6

80 10.4 8.0 12.0




Abundance Ion 188.00 (187.70 to 188.70): E


Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

Time-->







Time-->

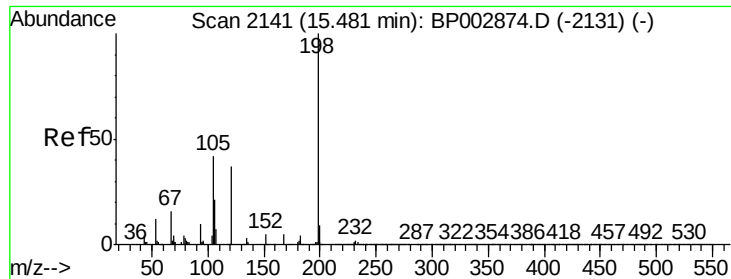

#65
4,6-Dinitro-2-methylphenol
Concen: 6.902 ng
RT: 15.47 min Scan# 2140
Delta R.T. -0.01 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59




Instrument :
BNA_P
ClientSampleId :
TP-11


Tot Ion:198 Resp: 34
Ion Ratio Lower Upper
198 100
51 1374.1 11.6 51.6#
105 1025.9 23.8 63.8#

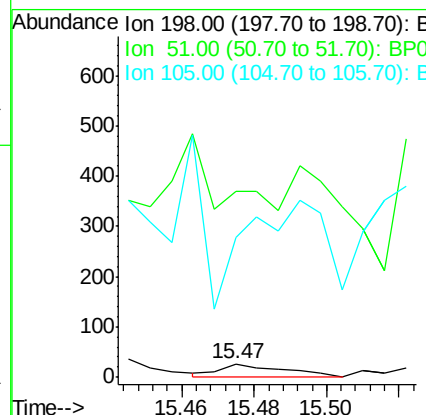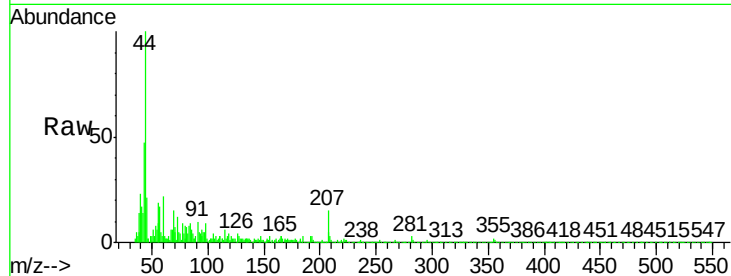

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.20 min Scan# 3113
Delta R.T. 0.00 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59

Tgt Ion:240 Resp: 1989655
Ion Ratio Lower Upper
240 100
120 10.2 8.9 13.3
236 25.6 20.3 30.5

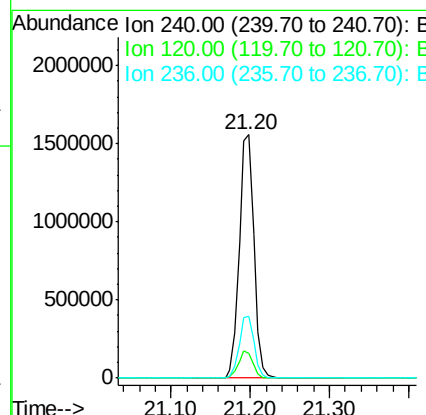

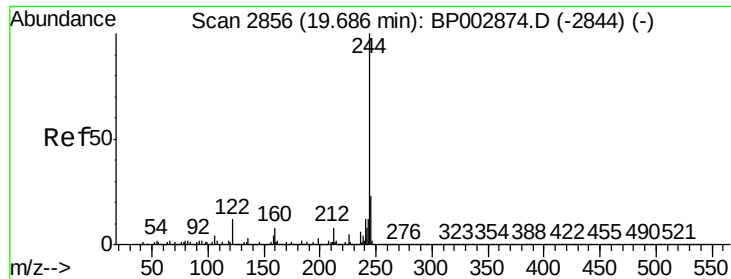

#79

Terphenyl-d14

Concen: 89.677 ng

RT: 19.68 min Scan# 2856

Delta R.T. -0.01 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59

Instrument :

BNA_P

ClientSampled :

TP-11


Tot Ion:244 Resp: 8912613

Ion Ratio Lower Upper

244 100

212 8.2 6.4 9.6




122 12.1 9.4 14.2

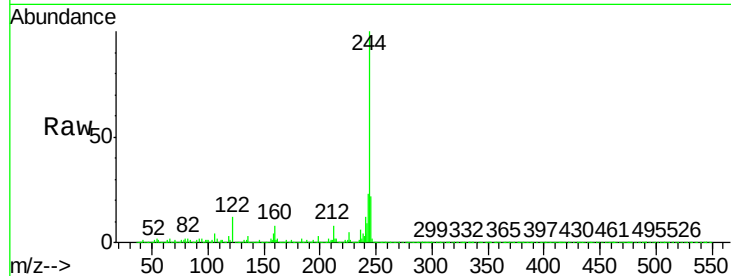

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

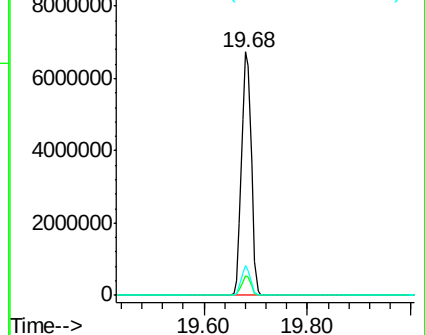

#80

Butylbenzylphthalate

Concen: 3.074 ng

RT: 20.37 min Scan# 2972

Delta R.T. 0.00 min

Lab File: BP002901.D

Acq: 31 Jul 2020 19:59


Tgt Ion:149 Resp: 986

Ion Ratio Lower Upper

149 100

91 99.6 60.5 90.7#



206 19.6 17.5 26.3




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BP0

Ion 206.00 (205.70 to 206.70): E

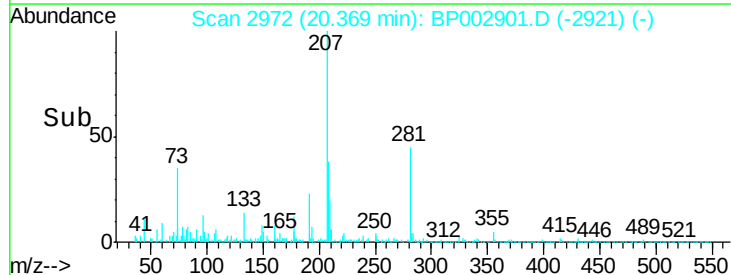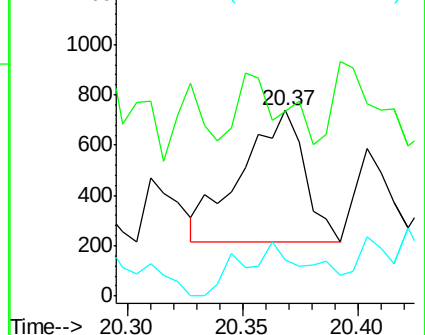



#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.46 min Scan# 3498
Delta R.T. -0.01 min
Lab File: BP002901.D
Acq: 31 Jul 2020 19:59

Instrument :
BNA_P
ClientSampleId :
TP-11

Tot Ion:264 Resp: 1764625

Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.0	28.6
265	21.8	17.0	25.4

