
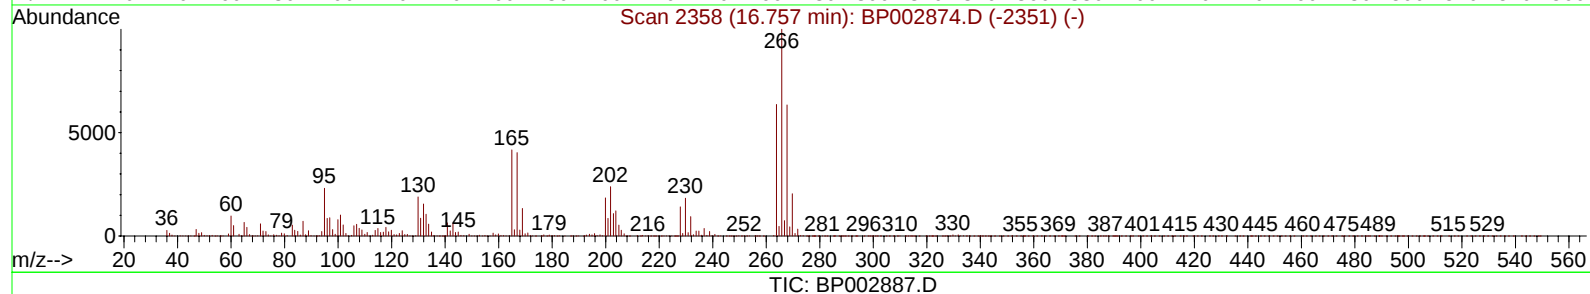
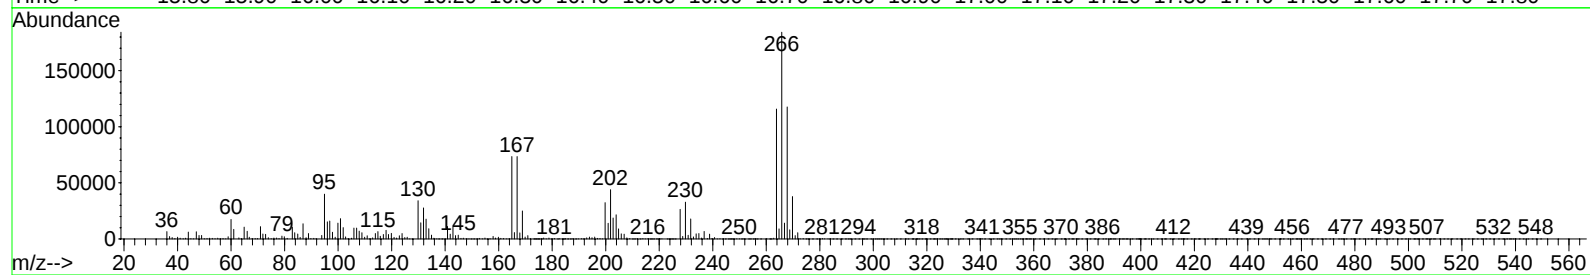


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
Data File : BP002887.D
Acq On : 31 Jul 2020 10:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 17:42:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 15:30:34 2020
Response via : Initial Calibration

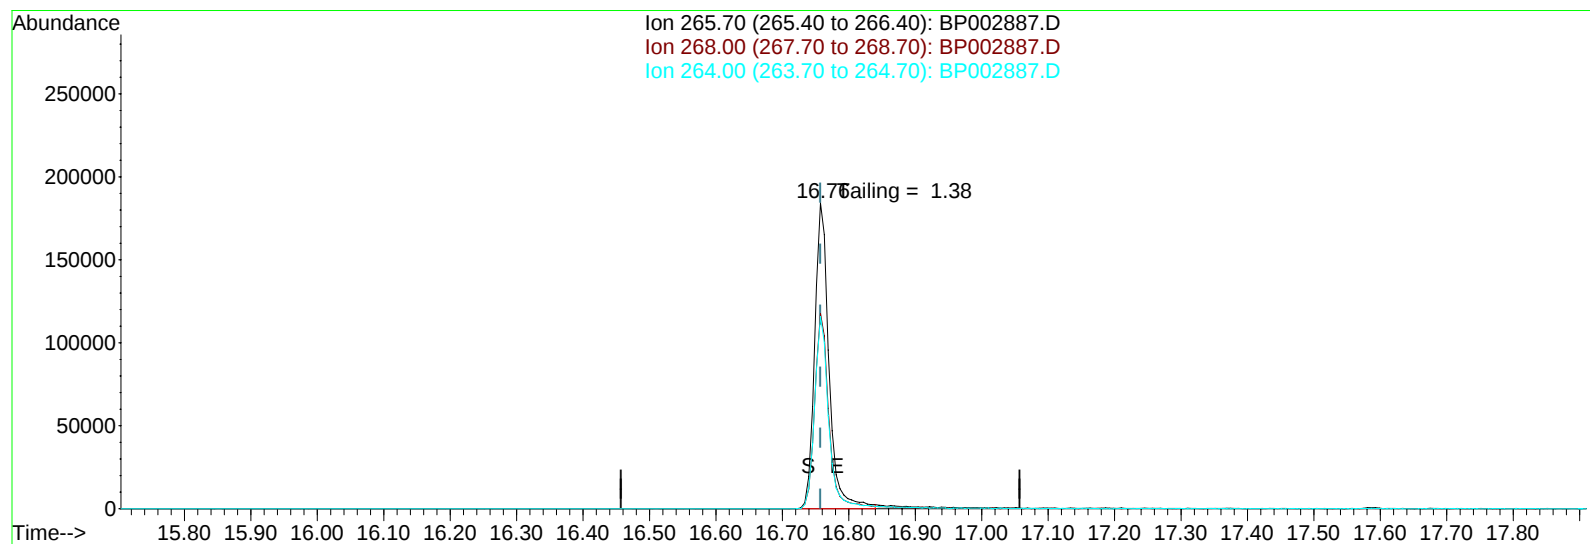

(70) Pentachlorophenol (C)




16.757min (+0.000) 365652.57ng

response 282829

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	63.89
264.00	63.60	62.83
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
 Data File : BP002887.D
 Acq On : 31 Jul 2020 10:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 17:42:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 15:30:34 2020
 Response via : Initial Calibration

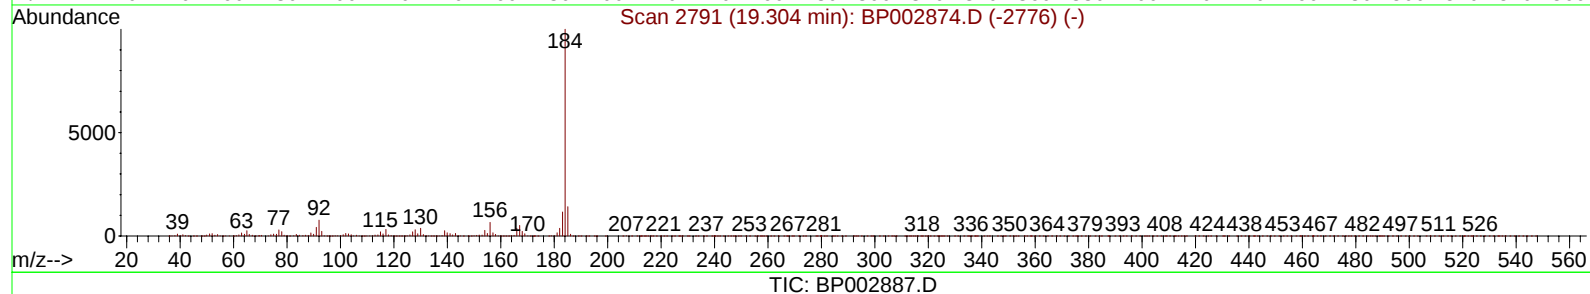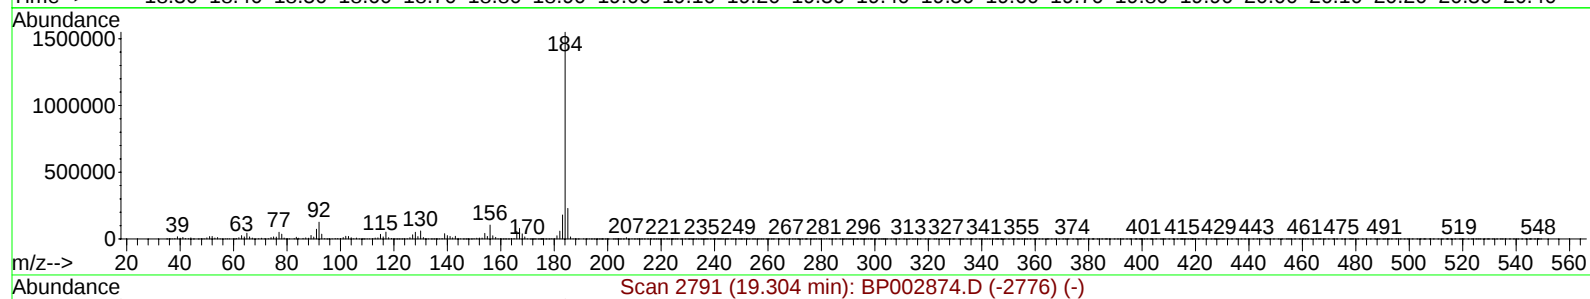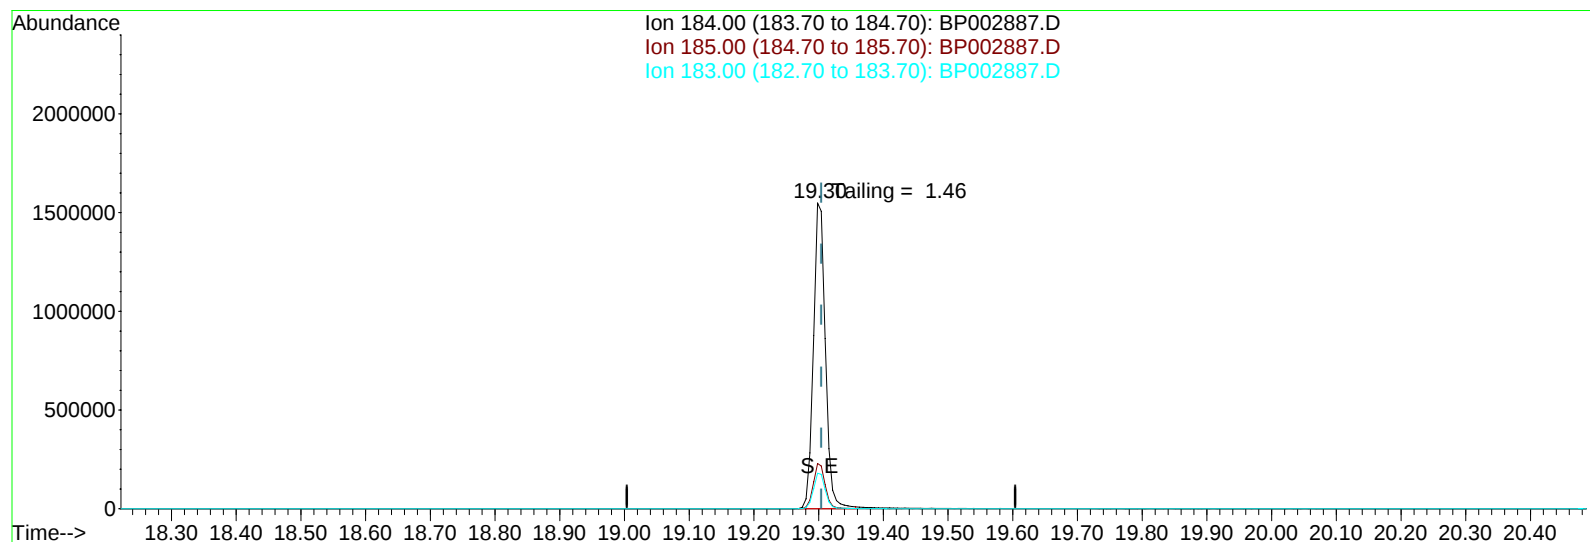

(77) Benzidine

19.298min (-0.006) 737842.82ng

response 2024949

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.82
183.00	11.60	11.63
0.00	0.00	0.00