

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
 Data File : BP002892.D
 Acq On : 31 Jul 2020 14:08
 Operator : CG/JU
 Sample : PB130646BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB130646BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.999	15	19	29	rVB	295196	344916	1.17%	0.248%
2	5.328	408	415	430	rBV	9908346	14323108	48.45%	10.305%
3	6.893	672	681	699	rBV	9087899	14351714	48.55%	10.325%
4	7.716	814	821	830	rBV	2220308	3344105	11.31%	2.406%
5	8.863	1008	1016	1029	rBV	5896556	9529044	32.23%	6.856%
6	10.498	1285	1294	1306	rBV	2707535	4603805	15.57%	3.312%
7	12.975	1707	1715	1726	rBV	15296404	22512275	76.15%	16.197%
8	14.351	1942	1949	1958	rBV2	4307887	6134657	20.75%	4.414%
9	15.845	2196	2203	2227	rBV	10679739	14978106	50.67%	10.776%
10	17.104	2410	2417	2428	rBV	5145531	7118128	24.08%	5.121%
11	19.686	2850	2856	2870	rBV	23106897	29562828	100.00%	21.269%
12	21.198	3107	3113	3121	rBV	5645016	6644722	22.48%	4.781%
13	23.462	3491	3498	3512	rVB2	2907736	5545560	18.76%	3.990%




Sum of corrected areas: 138992968

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
Data File : BP002892.D
Acq On : 31 Jul 2020 14:08
Operator : CG/JU
Sample : PB130646BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130646BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

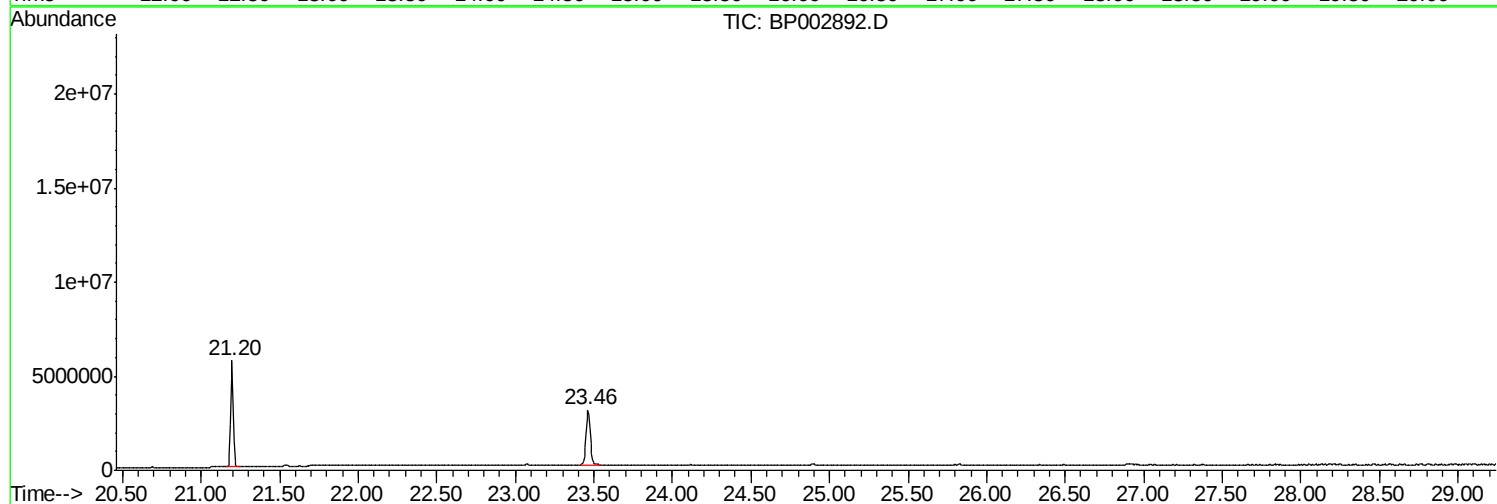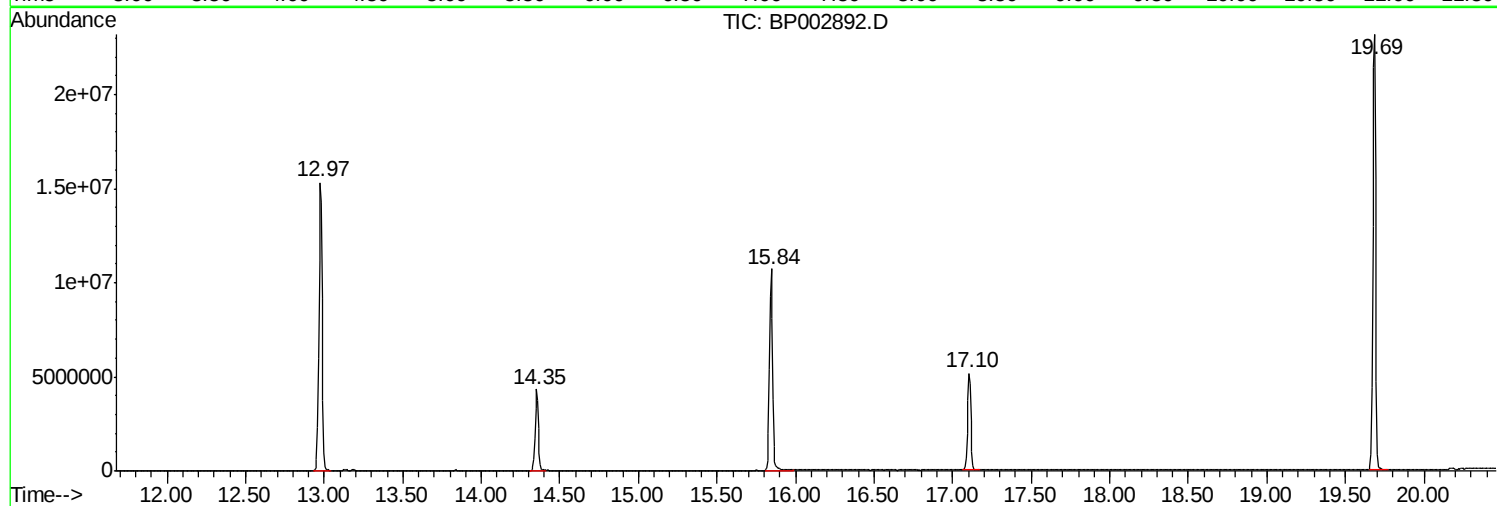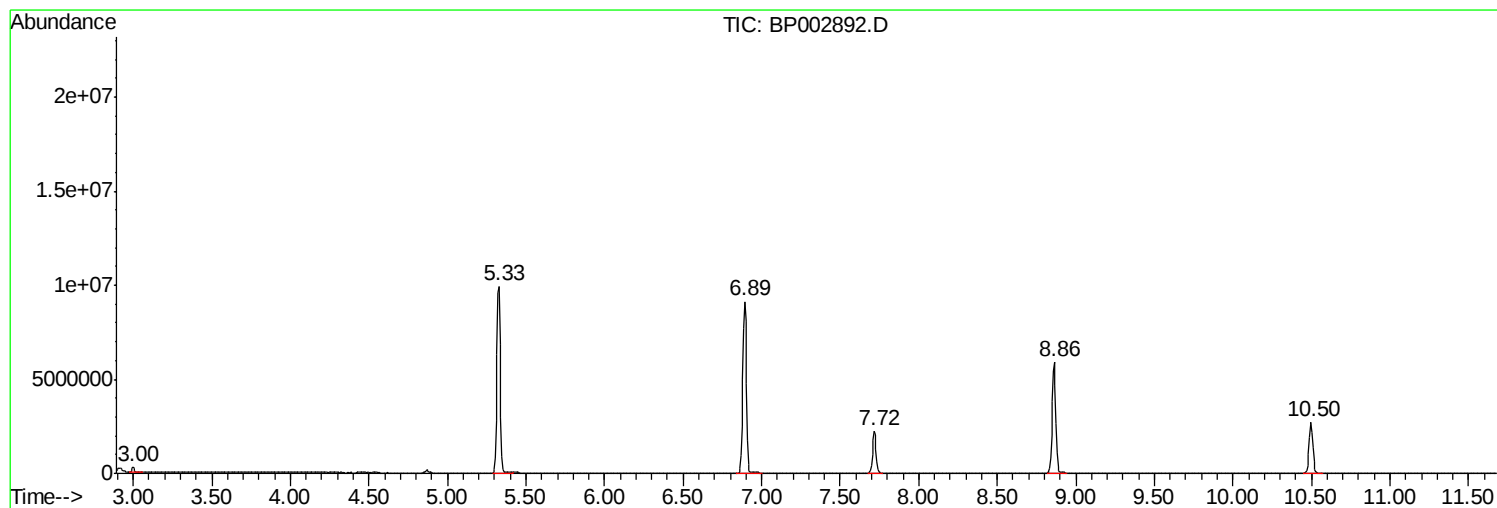

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP073120\
Data File : BP002892.D
Acq On : 31 Jul 2020 14:08
Operator : CG/JU
Sample : PB130646BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130646BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.00	2.06 ng	344916	1,4-Dichlorobenzene-d4	7.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3		Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
4		N-Ethylformamide	73	C3H7NO	000627-45-2	9
5		Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

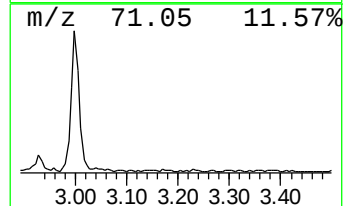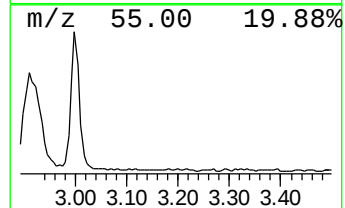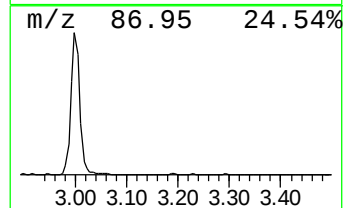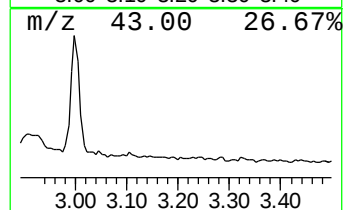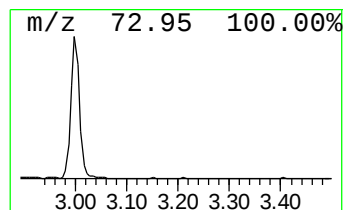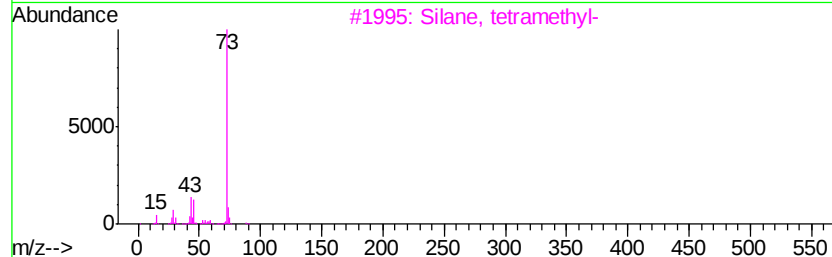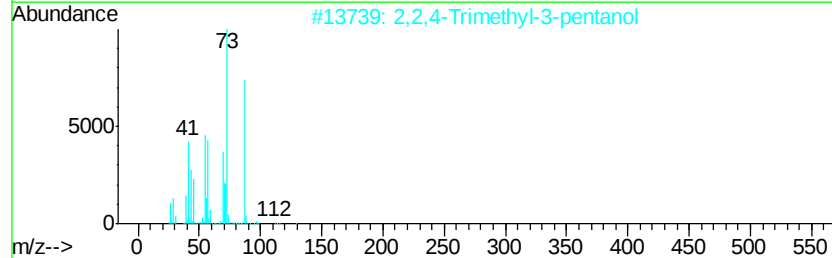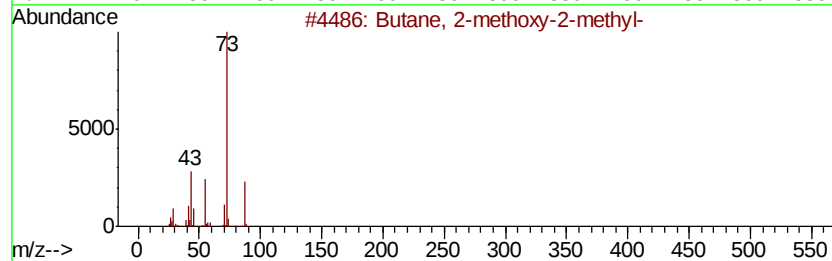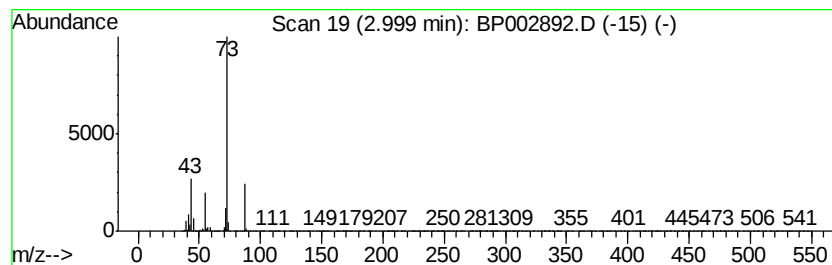

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP073120\
Data File : BP002892.D
Acq On : 31 Jul 2020 14:08
Operator : CG/JU
Sample : PB130646BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130646BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.00	2.1	ng	344916	1	7.72	3344110	20.0