


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073120\
 Data File : BP002887.D
 Acq On : 31 Jul 2020 10:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 15:30:34 2020

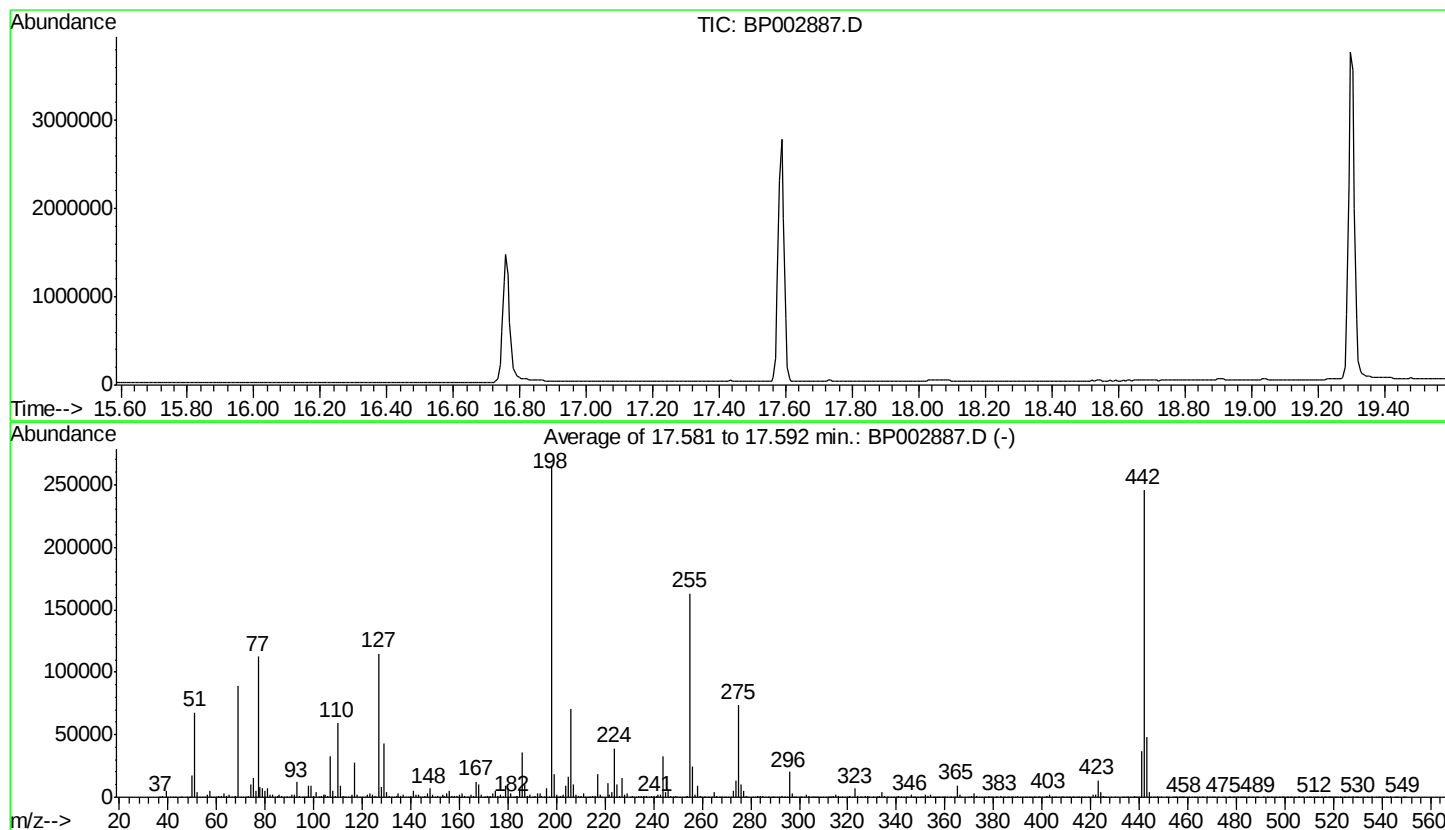

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	67912	PASS
68	69	0.00	2	1.6	1429	PASS
69	198	0.00	100	33.7	89367	PASS
70	69	0.00	2	0.5	418	PASS
127	198	10	80	43.4	115211	PASS
197	198	0.00	2	0.1	280	PASS
198	198	100	100	100.0	265249	PASS
199	198	5	9	6.9	18389	PASS
275	198	10	60	27.9	73955	PASS
365	198	1	100	3.5	9222	PASS
441	198	0.01	100	13.9	36898	PASS
442	198	50	100	92.7	245900	PASS
443	442	15	24	19.7	48442	PASS