




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011195.D
 Acq On : 01 Aug 2022 12:28
 Operator : CG/JU
 Sample : PB146543BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Manual IntegrationsAPPROVED

Quant Time: Aug 01 22:59:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

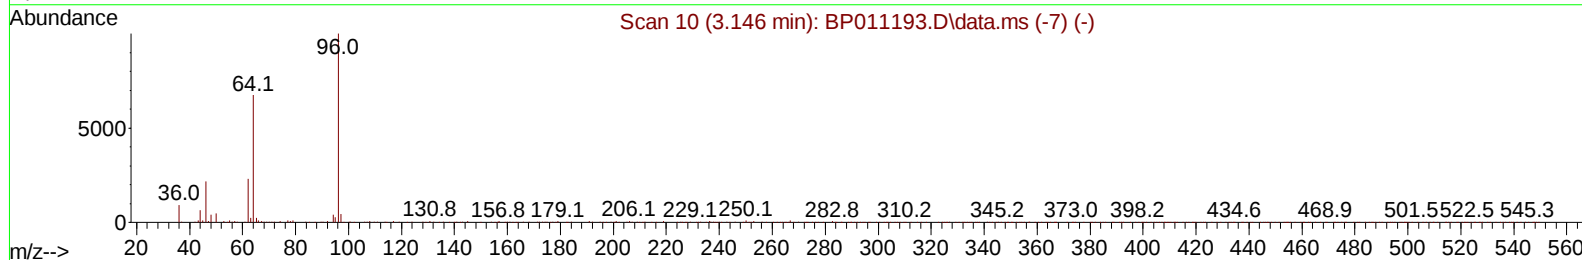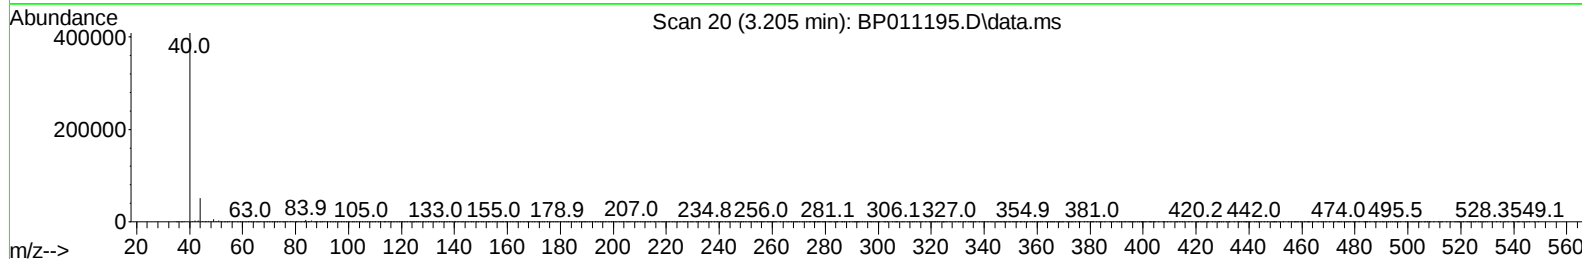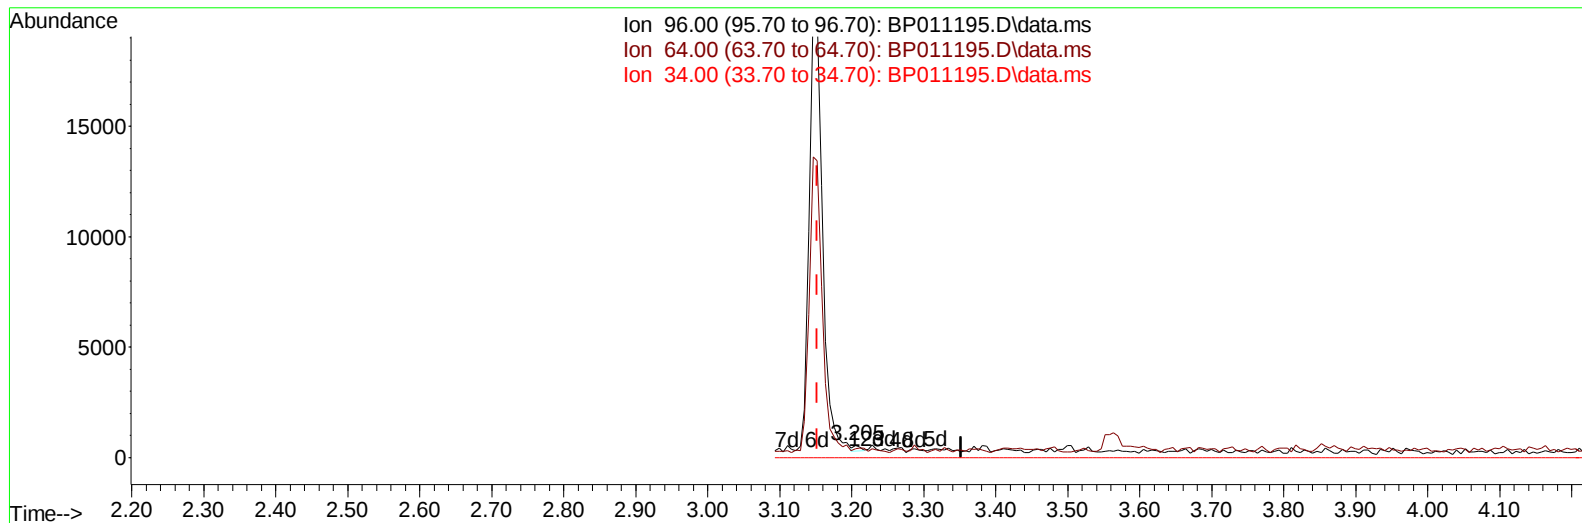

TIC: BP011195.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.205min (+ 0.053) 0.03 ng/uL

response 174

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.90	71.97
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011195.D
 Acq On : 01 Aug 2022 12:28
 Operator : CG/JU
 Sample : PB146543BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Manual IntegrationsAPPROVED

Quant Time: Aug 01 22:59:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

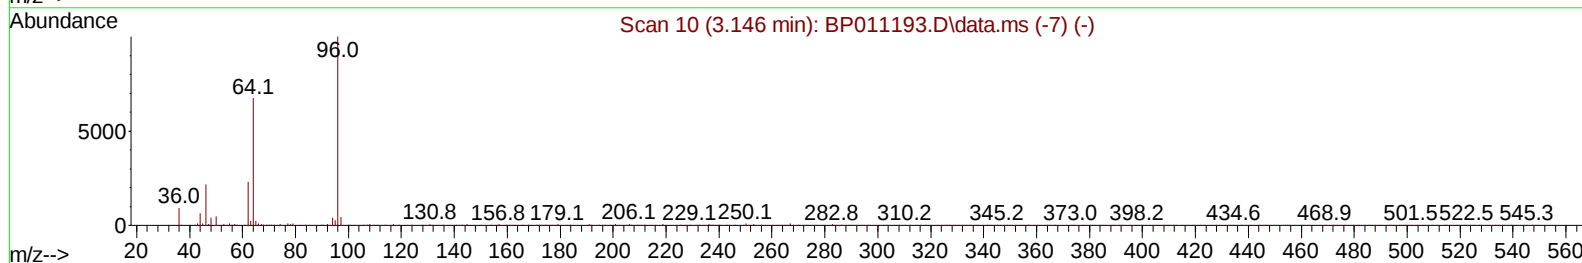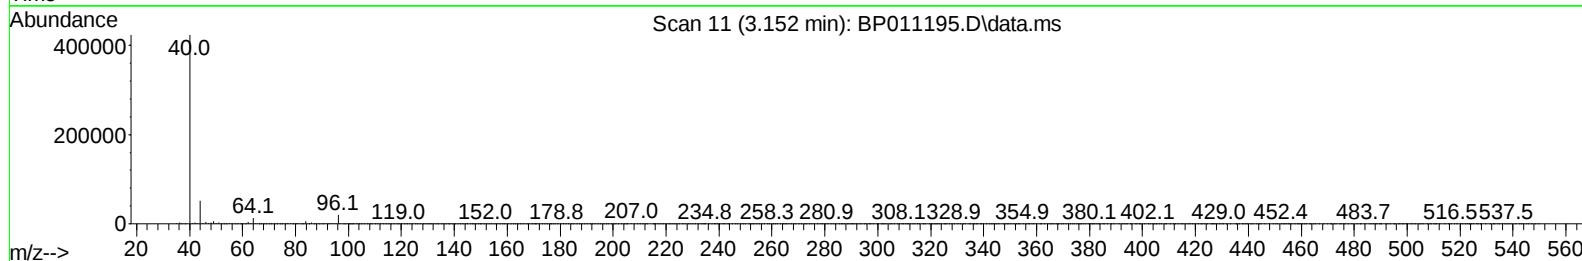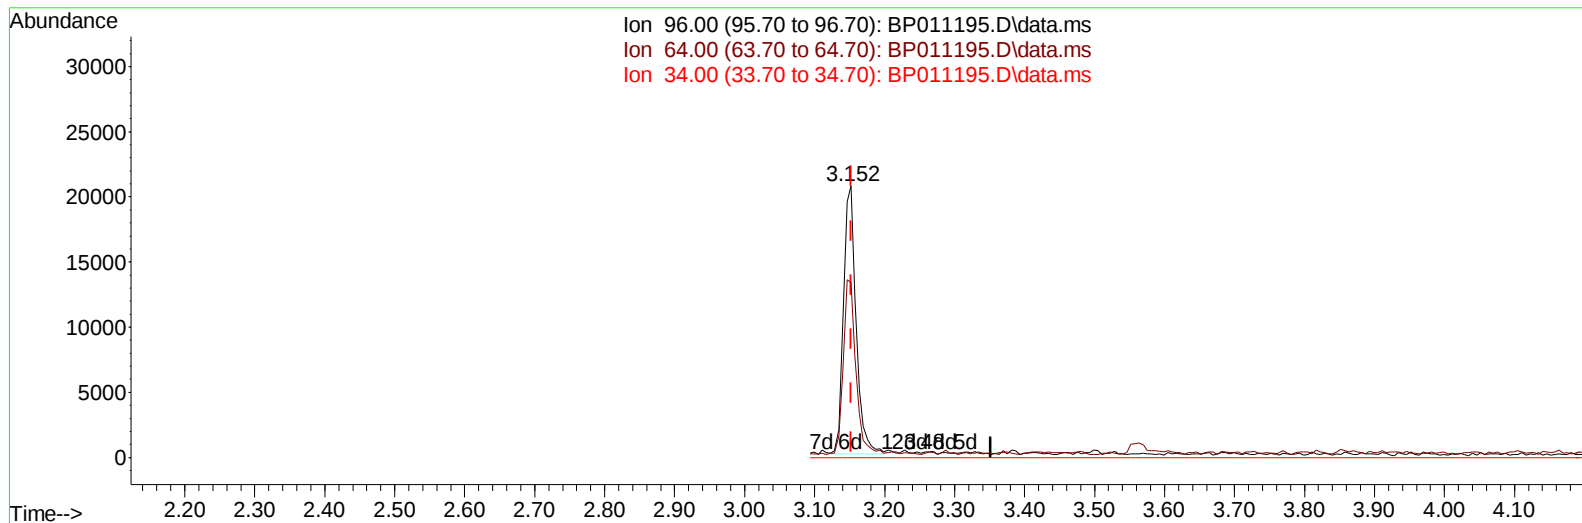

TIC: BP011195.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.152min (-0.000) 4.21 ng/uL m

response 25948

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.90	64.52#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011195.D
 Acq On : 01 Aug 2022 12:28
 Operator : CG/JU
 Sample : PB146543BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

Quant Time: Aug 01 22:59:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.646	152		282289	20.000	ng/ul	0.00
20) Naphthalene-d8	10.440	136		1220911	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.316	164		571698	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.086	188		927929	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.210	240		873438	20.000	ng/ul	# 0.00
88) Perylene-d12	23.557	264		993024	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.152	96		25948m	4.209	ng/uL	0.00
4) Pyridine-d5	3.558	84		392317	22.497	ng/ul	0.00
7) Phenol-d5	6.828	99		731010	29.668	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67		527384	30.270	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132		580720	29.907	ng/ul	0.00
15) 4-Methylphenol-d8	8.363	113		568382	28.200	ng/ul	0.00
21) Nitrobenzene-d5	8.810	128		291788	30.752	ng/ul	0.00
24) 2-Nitrophenol-d4	9.528	143		275512	30.313	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165		450049	28.098	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131		726118	27.964	ng/ul	0.00
46) Dimethylphthalate-d6	13.734	166		1210325	31.073	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160		1553374	31.736	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143		122438	17.476	ng/ul	0.00
60) Fluorene-d10	15.316	176		954743	29.170	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200		87842	18.779	ng/ul	0.00
73) Anthracene-d10	17.186	188		1300638	31.811	ng/ul	0.00
81) Pyrene-d10	19.445	212		1390418	29.625	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.404	264		1550560	31.437	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011195.D
Acq On : 01 Aug 2022 12:28
Operator : CG/JU
Sample : PB146543BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/02/2022
Supervised By :mohammad ahmed 08/03/2022

Quant Time: Aug 01 22:59:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 16:05:22 2022
Response via : Initial Calibration

