




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011199.D
 Acq On : 01 Aug 2022 14:45
 Operator : CG/JU
 Sample : N3790-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBUL3

Manual IntegrationsAPPROVED

Quant Time: Aug 01 23:00:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

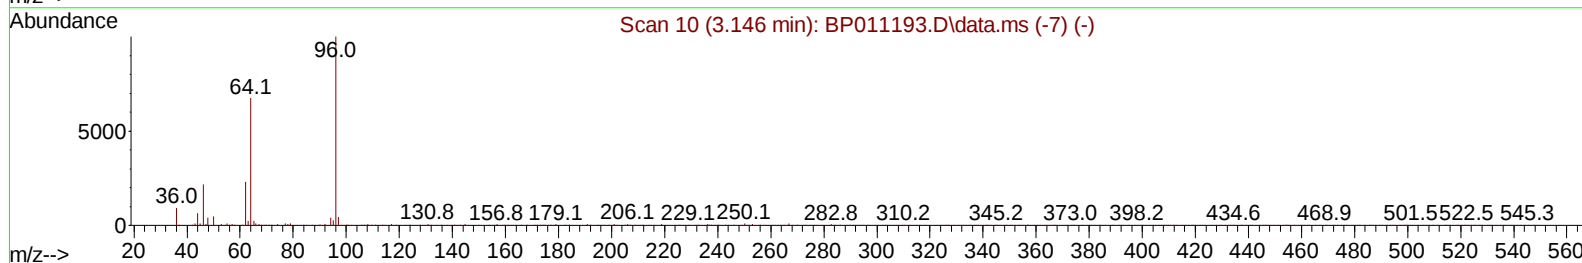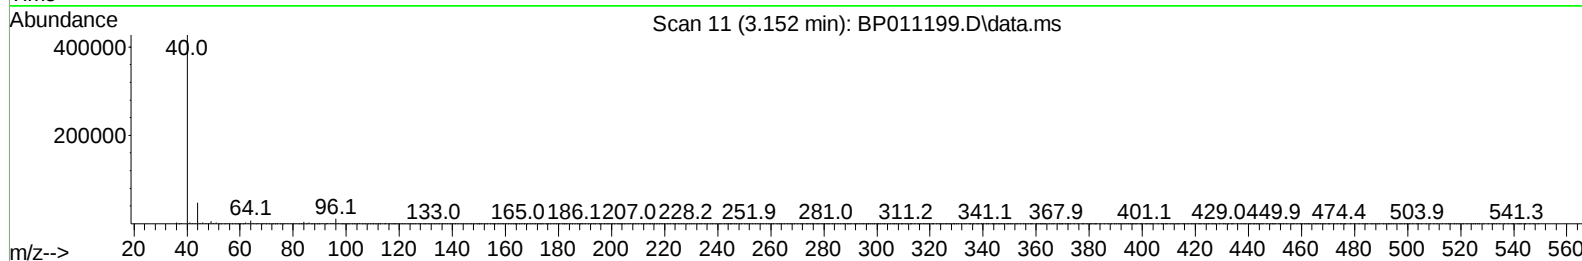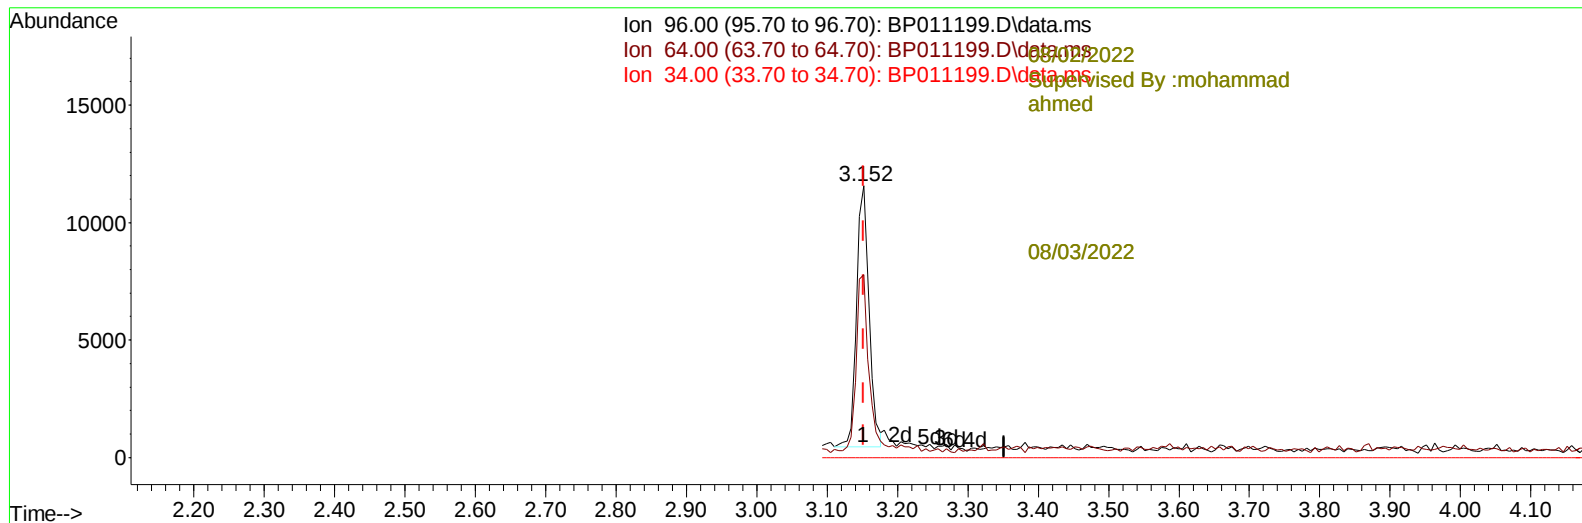

TIC: BP011199.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.152min (-0.000) 2.53 ng/uL

response 13633

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.90	67.36
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011199.D
 Acq On : 01 Aug 2022 14:45
 Operator : CG/JU
 Sample : N3790-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBUL3

Manual IntegrationsAPPROVED

Quant Time: Aug 01 23:00:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

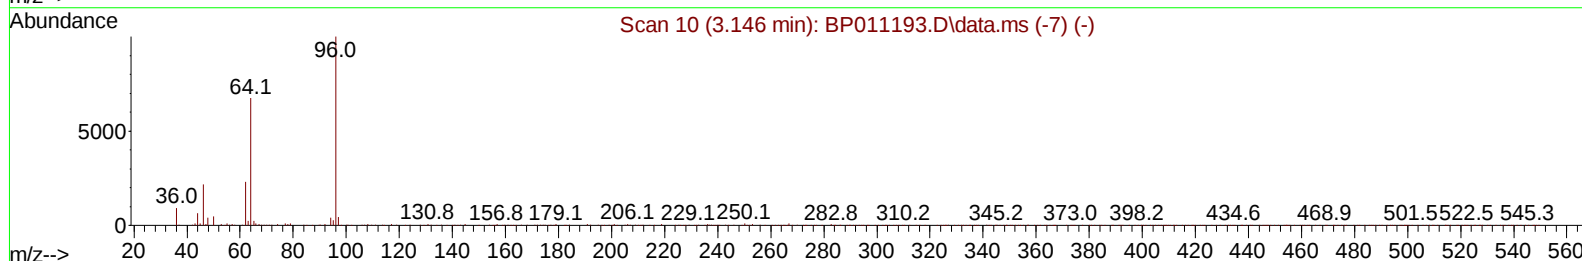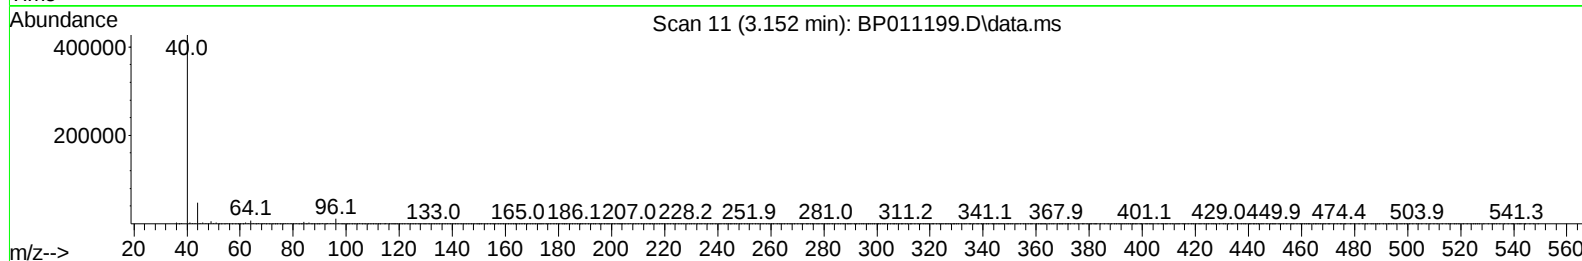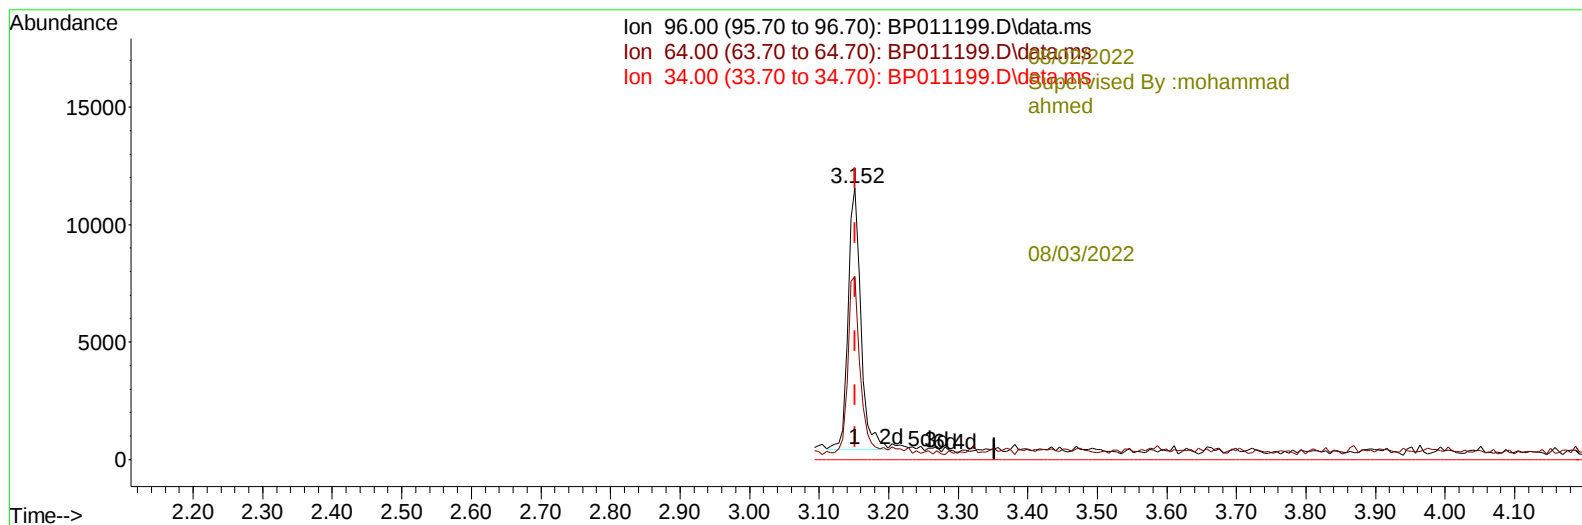

TIC: BP011199.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.152min (-0.000) 2.64 ng/uL m

response 14194

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.90	67.36
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011199.D
 Acq On : 01 Aug 2022 14:45
 Operator : CG/JU
 Sample : N3790-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBUL3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

Quant Time: Aug 01 23:00:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----08/02/2022						
Supervised By :mohammad ahmed						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	246376	20.000	ng/ul	0.00
20) Naphthalene-d8	10.440	136	1020127	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.310	164	511479	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.086	188	962381	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.210	240	984219	20.000	ng/ul	# 0.00
88) Perylene-d12	23.551	264	1066352	20.000	ng/ul	0.0008/03/2022
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.152	96	14194m	2.638	ng/uL	0.00
4) Pyridine-d5	3.569	84	61363	4.032	ng/ul	0.01
7) Phenol-d5	6.828	99	423435	19.690	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	293945	19.331	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	329924	19.468	ng/ul	0.00
15) 4-Methylphenol-d8	8.363	113	320258	18.205	ng/ul	0.00
21) Nitrobenzene-d5	8.810	128	155238	19.581	ng/ul	0.00
24) 2-Nitrophenol-d4	9.528	143	147792	19.461	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	257418	19.234	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	399418	18.410	ng/ul	0.00
46) Dimethylphthalate-d6	13.734	166	770787	22.119	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	960206	21.927	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	65496	10.449	ng/ul	0.00
60) Fluorene-d10	15.316	176	657572	22.456	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	48469	9.991	ng/ul	0.00
73) Anthracene-d10	17.180	188	1024565	24.161	ng/ul	0.00
81) Pyrene-d10	19.445	212	1195372	22.603	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.404	264	1253220	23.661	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011199.D
Acq On : 01 Aug 2022 14:45
Operator : CG/JU
Sample : N3790-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUL3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/02/2022
Supervised By :mohammad ahmed 08/03/2022

Quant Time: Aug 01 23:00:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 16:05:22 2022
Response via : Initial Calibration

